

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091123\
 Data File : VX037651.D
 Acq On : 11 Sep 2023 19:26
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Sep 12 09:15:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 09:13:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	155989	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	268809	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	236629	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	92024	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	106647	42.257	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	84.520%
35) Dibromofluoromethane	5.391	113	84805	44.509	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.020%
50) Toluene-d8	8.647	98	330698	46.021	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.040%
62) 4-Bromofluorobenzene	11.079	95	105744	40.789	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	81.580%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091123\
Data File : VX037651.D
Acq On : 11 Sep 2023 19:26
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Sep 12 09:15:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 09:13:03 2023
Response via : Initial Calibration




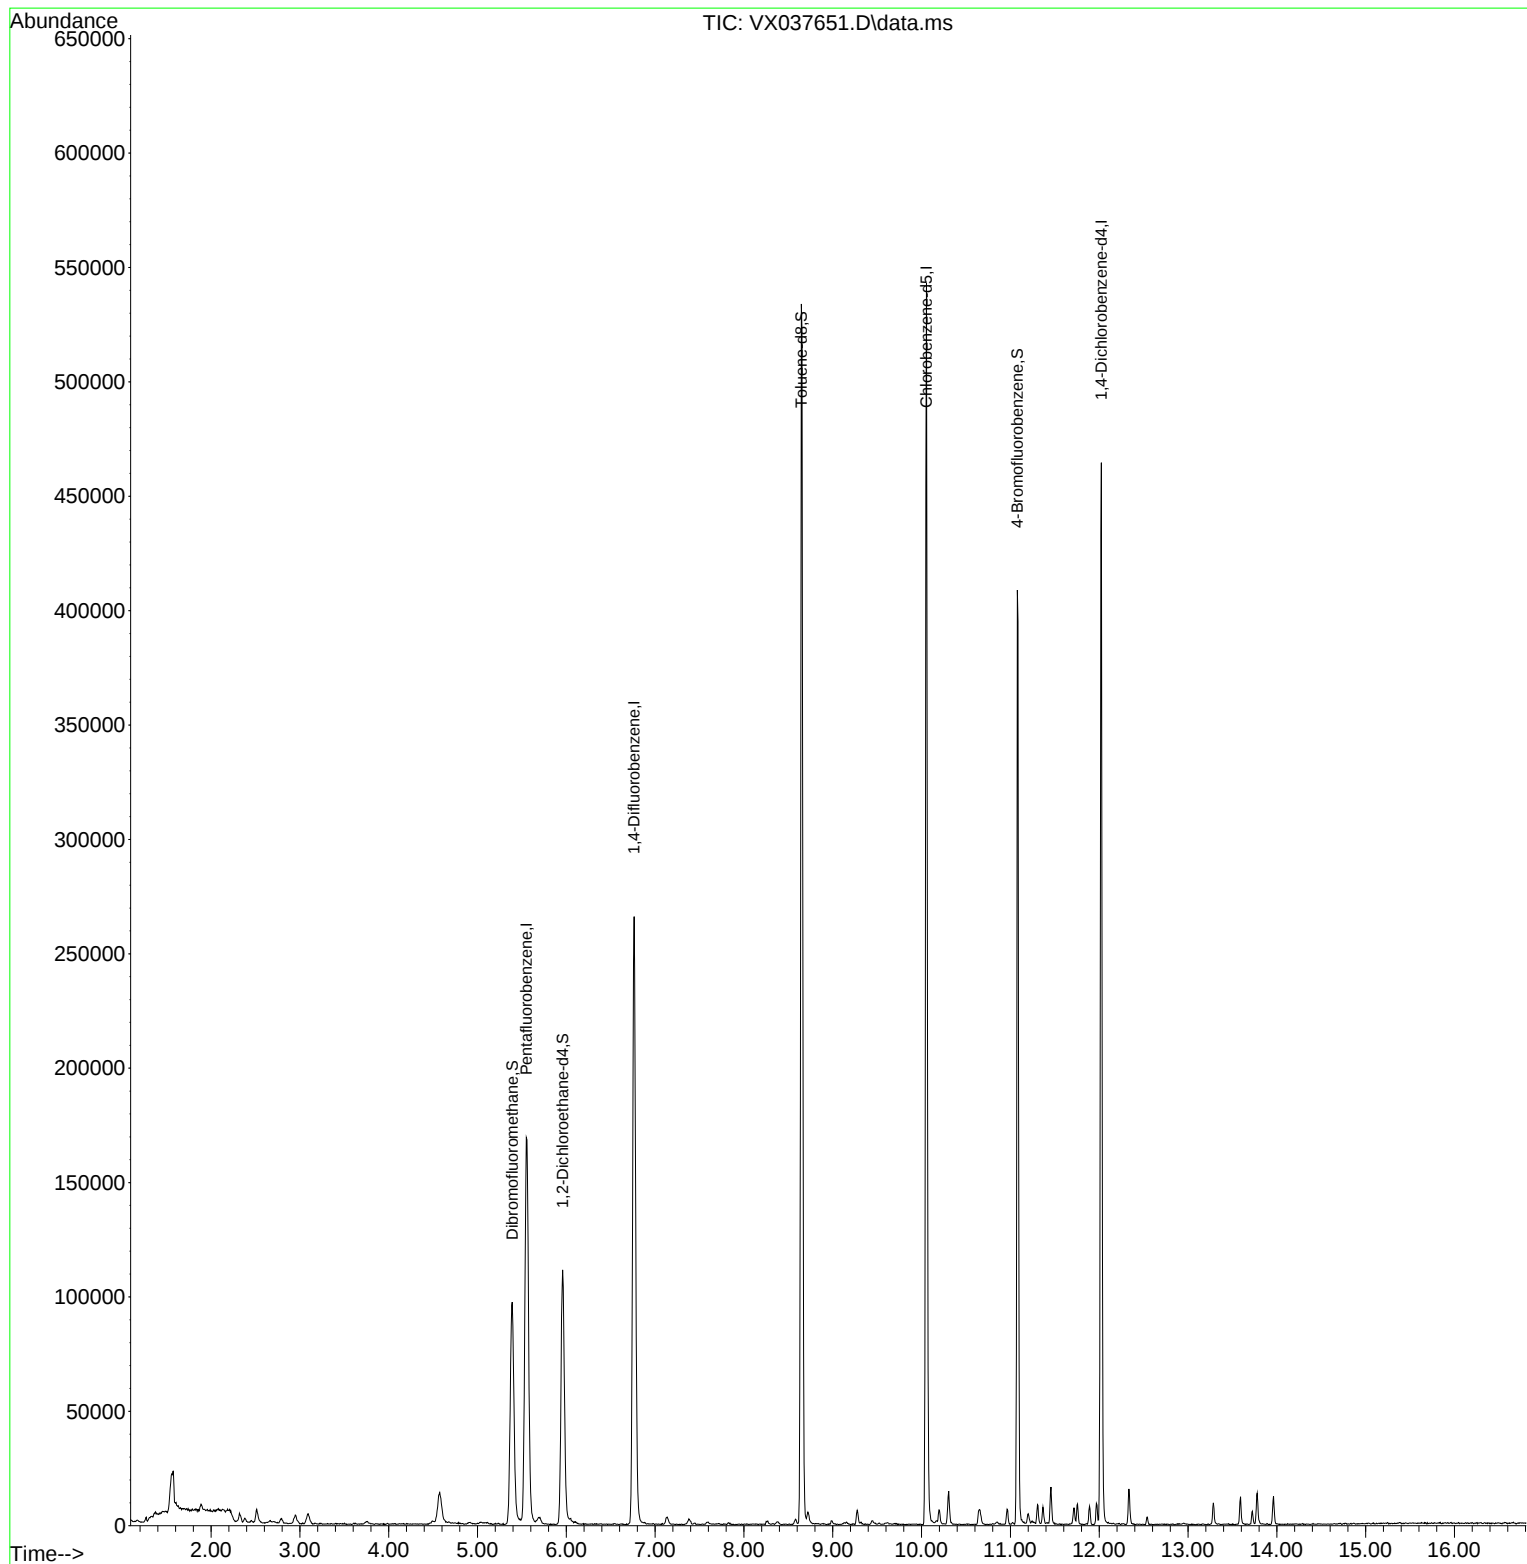


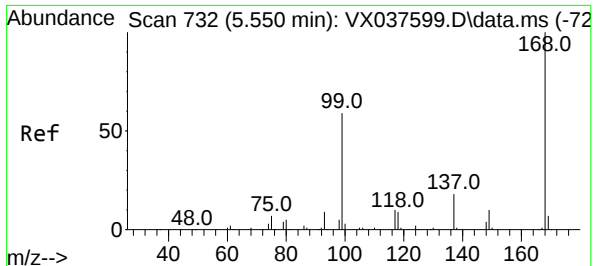

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX037651.D
Acq: 11 Sep 2023 19:26




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 155989
Ion Ratio Lower Upper
168 100
99 64.1 56.6 85.0

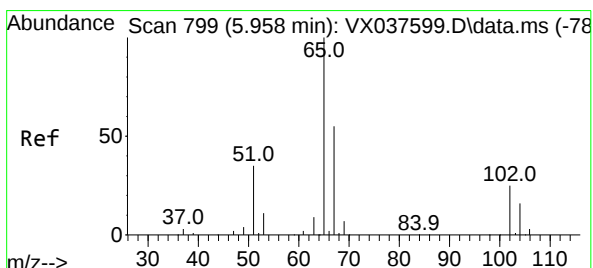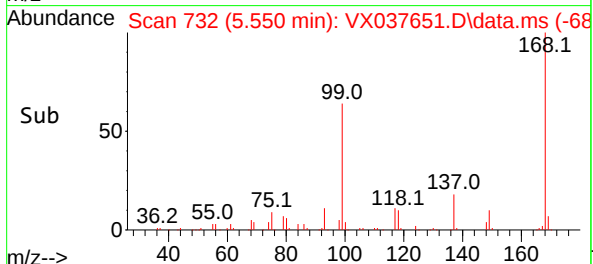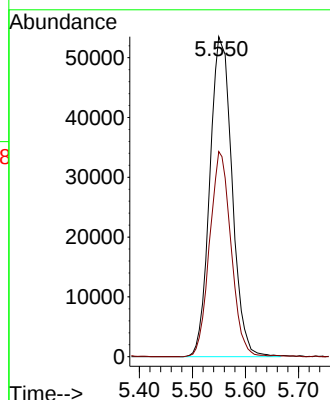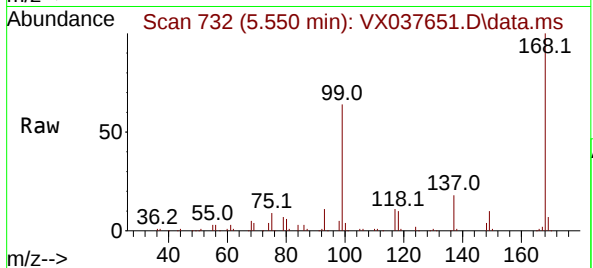

#33
1,2-Dichloroethane-d4
Concen: 42.257 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX037651.D
Acq: 11 Sep 2023 19:26

Tgt Ion: 65 Resp: 106647
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.2


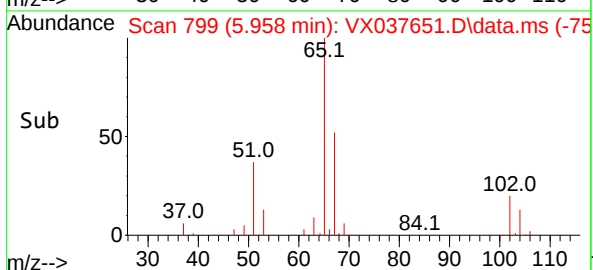
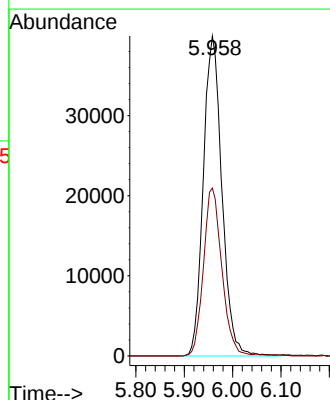
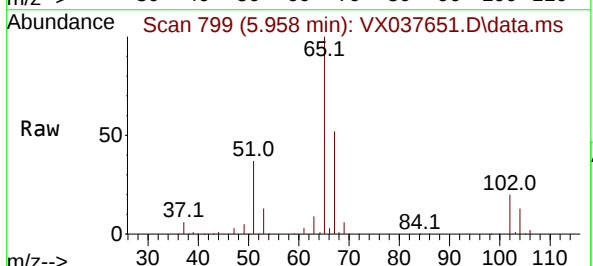


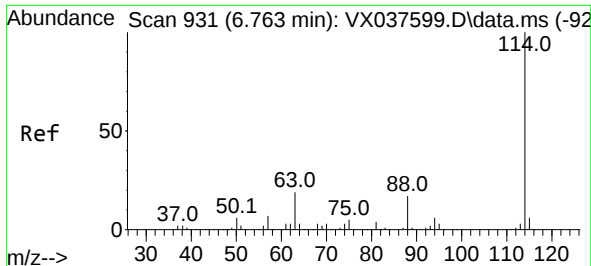

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX037651.D
Acq: 11 Sep 2023 19:26




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 268809
Ion Ratio Lower Upper
114 100
63 19.6 0.0 45.0
88 15.9 0.0 36.6

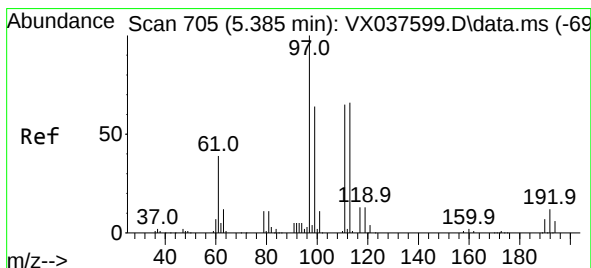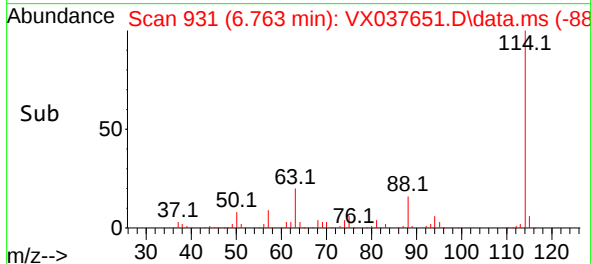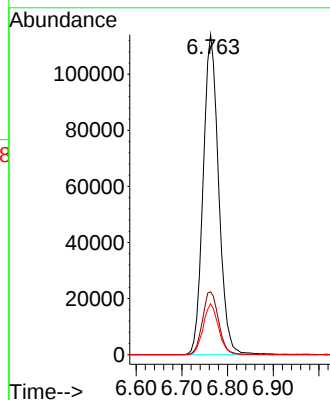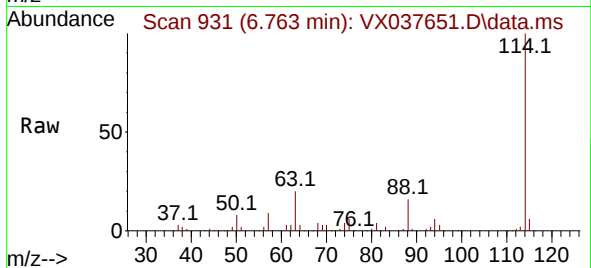

#35
Dibromofluoromethane
Concen: 44.509 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX037651.D
Acq: 11 Sep 2023 19:26

Tgt Ion:113 Resp: 84805
Ion Ratio Lower Upper
113 100
111 102.3 82.9 124.3
192 17.5 13.3 19.9

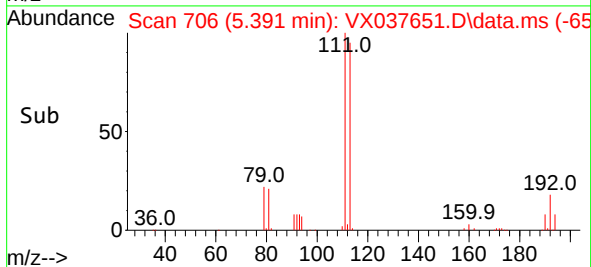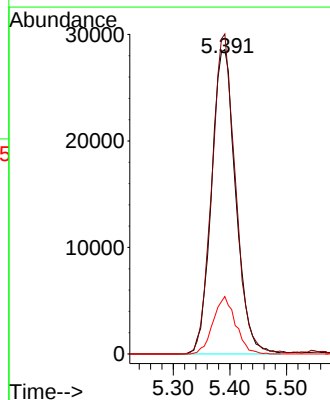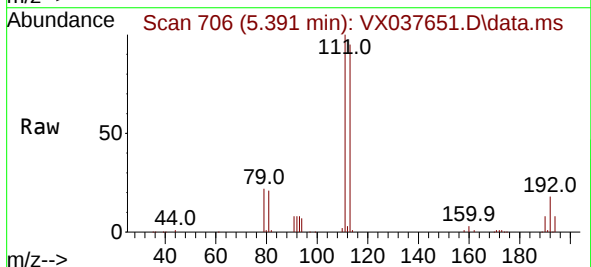

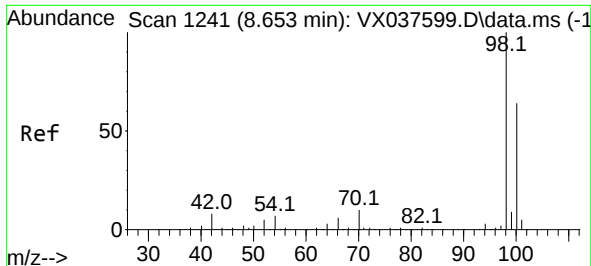

#50

Toluene-d8

Concen: 46.021 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 98 Resp: 330698

Ion Ratio Lower Upper

98 100

100 62.9 53.1 79.7

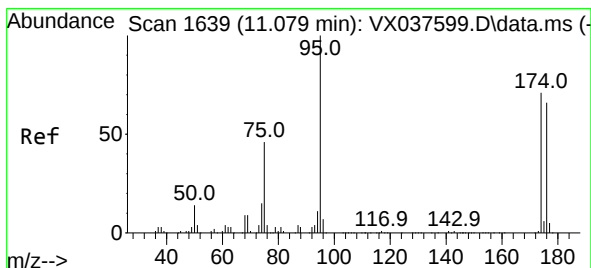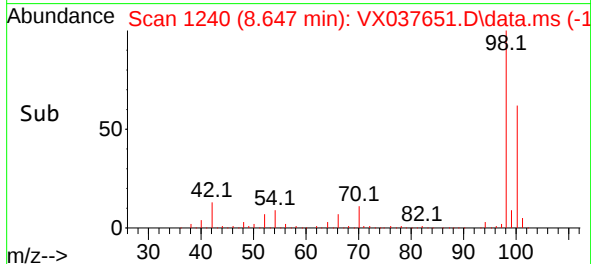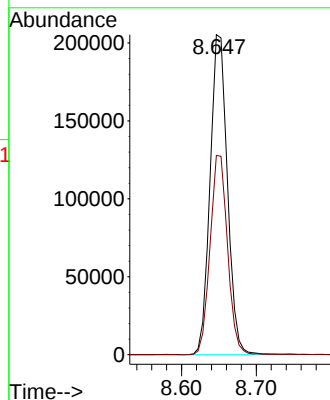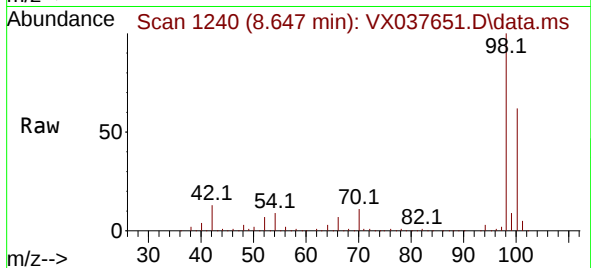

#62

4-Bromofluorobenzene

Concen: 40.789 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26




Tgt Ion: 95 Resp: 105744


Ion Ratio Lower Upper

95 100

174 76.9 0.0 135.6

176 74.3 0.0 131.0

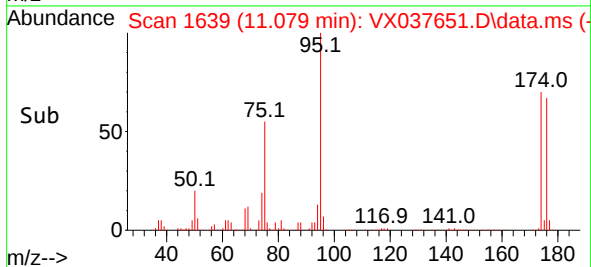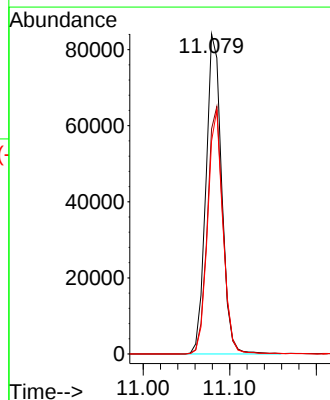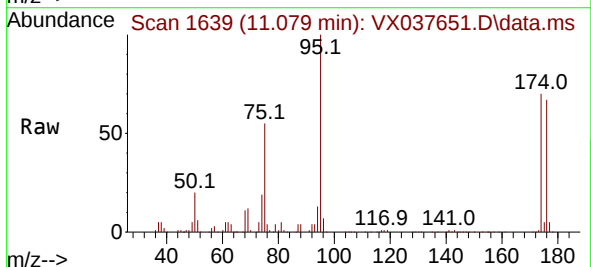

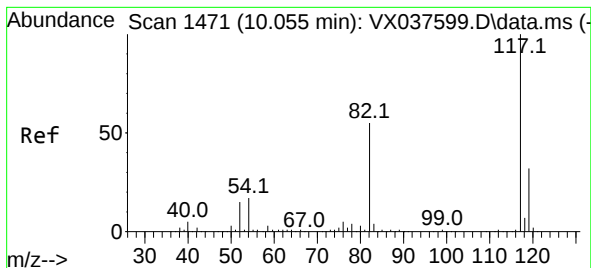

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:117 Resp: 236629

Ion Ratio Lower Upper

117 100

82 56.4 46.2 69.4

119 31.4 25.5 38.3

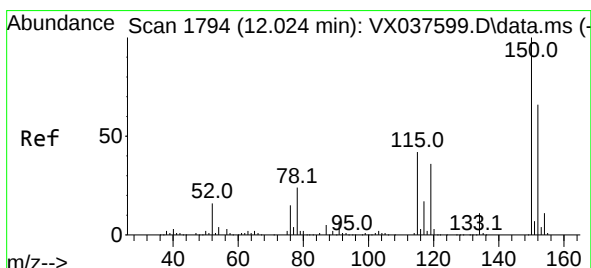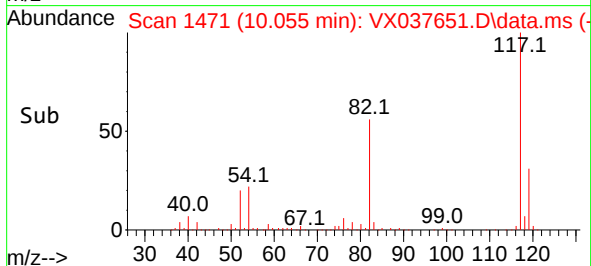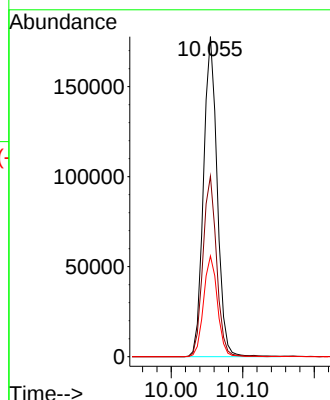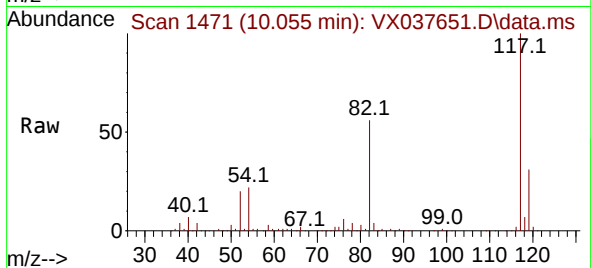

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Tgt Ion:152 Resp: 92024

Ion Ratio Lower Upper

152 100

115 62.8 43.3 129.9

150 161.2 0.0 345.0

