



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091123\
Data File : VX037642.D
Acq On : 11 Sep 2023 15:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 10:10:04 2023

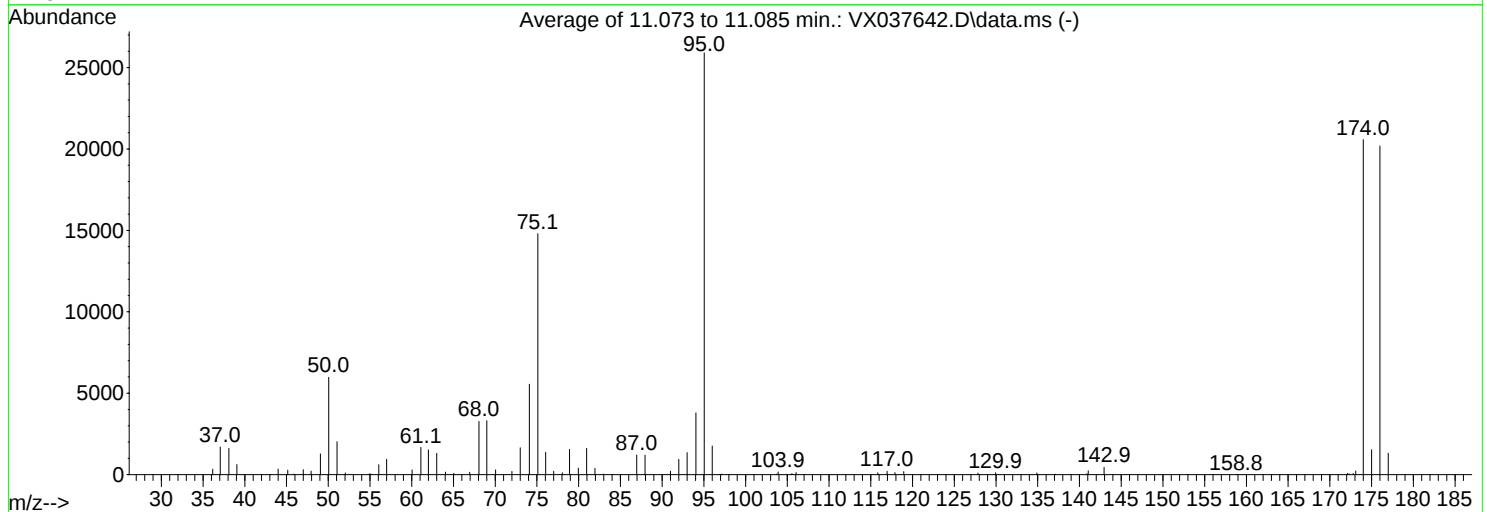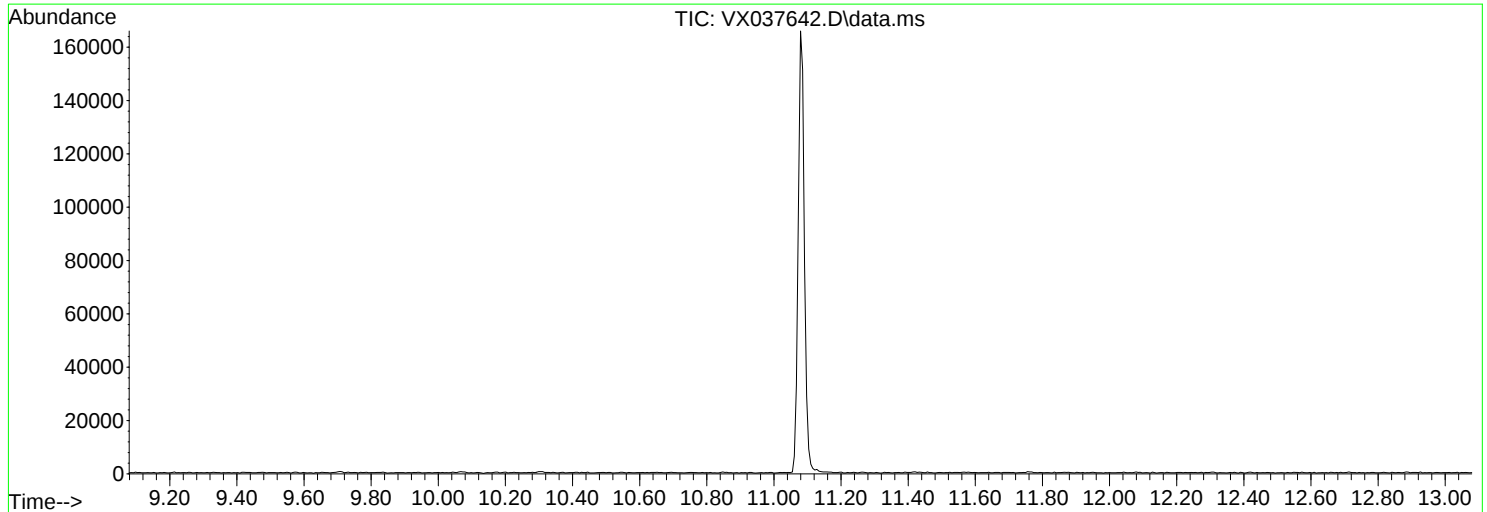

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	5979	PASS
75	95	30	60	57.1	14796	PASS
95	95	100	100	100.0	25904	PASS
96	95	5	9	6.8	1758	PASS
173	174	0.00	2	1.1	227	PASS
174	95	50	100	79.4	20575	PASS
175	174	5	9	7.5	1538	PASS
176	174	95	101	98.1	20185	PASS
177	176	5	9	6.5	1315	PASS