

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091219\
 Data File : VX012360.D
 Acq On : 12 Sep 2019 21:11
 Operator : SY/SP
 Sample : K4752-11
 Misc : 5.01g/5.0mL/MSVOA X/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-15-14.5-15.0

Quant Time: Sep 13 02:32:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 10 12:55:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	156017	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	271275	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	244895	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	118827	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	110079	49.90	ug/l	0.00
Spiked Amount			Recovery	=	99.80%	
35) Dibromofluoromethane	5.48	113	80104	46.06	ug/l	0.00
Spiked Amount			Recovery	=	92.12%	
50) Toluene-d8	8.71	98	321338	52.68	ug/l	0.00
Spiked Amount			Recovery	=	105.36%	
62) 4-Bromofluorobenzene	11.13	95	129640	45.85	ug/l	0.00
Spiked Amount			Recovery	=	91.70%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091219\
Data File : VX012360.D
Acq On : 12 Sep 2019 21:11
Operator : SY/SP
Sample : K4752-11
Misc : 5.01g/5.0mL/MSVOA X/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-15-14.5-15.0

Quant Time: Sep 13 02:32:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 10 12:55:26 2019
Response via : Initial Calibration

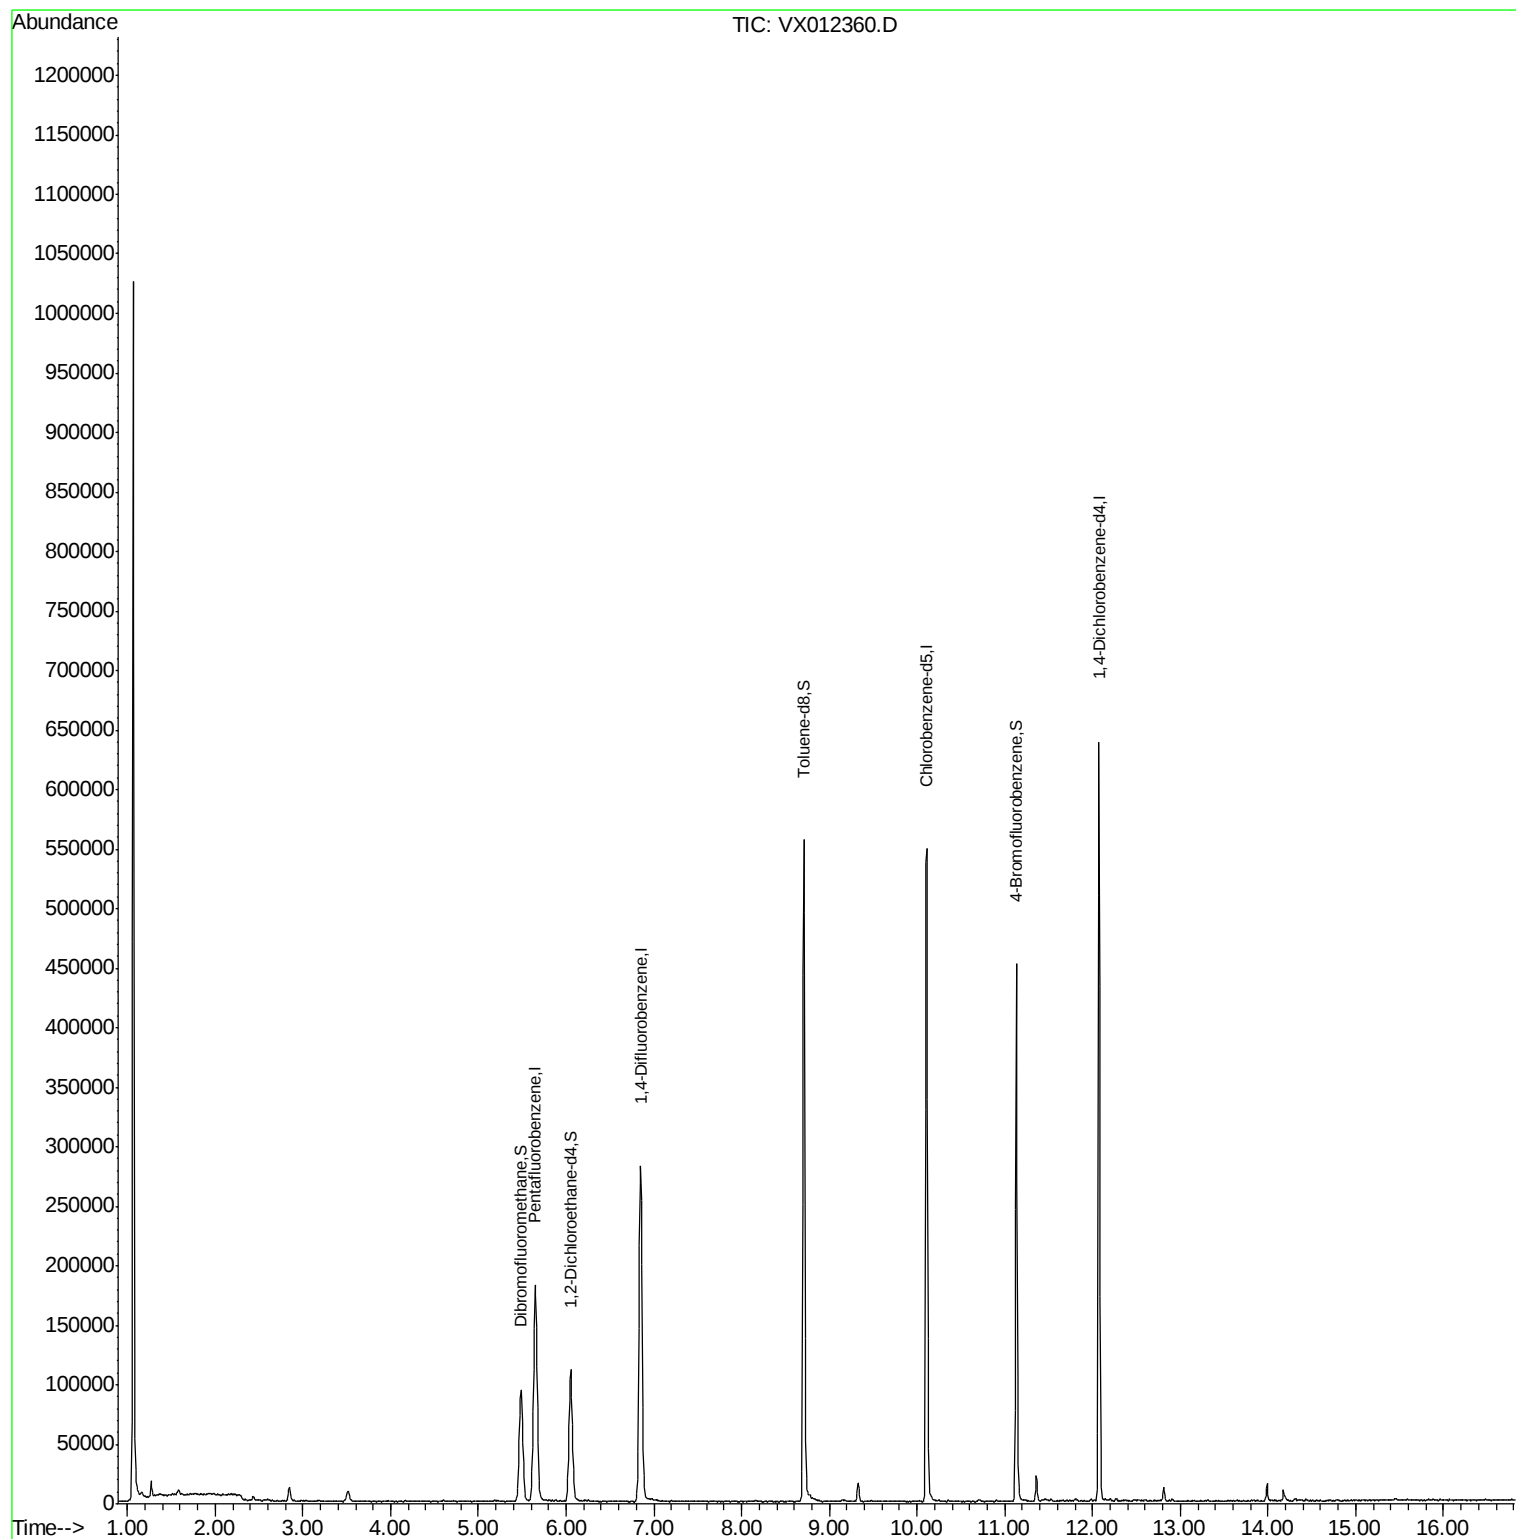

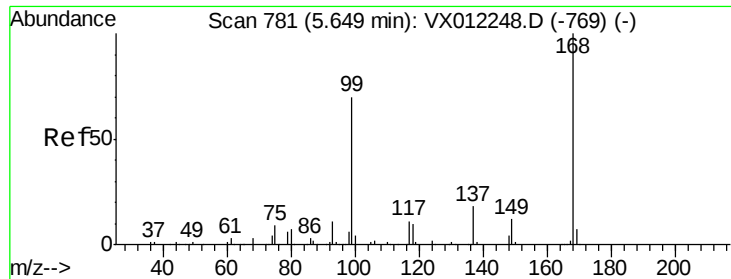

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX012360.D

Acq: 12 Sep 2019 21:11

Instrument :

MSVOA_X

ClientSampleId :


SB-15-14.5-15.0

Tot Ion:168 Resp: 156017

Ion Ratio Lower Upper




168 100

99 69.5 55.8 83.6

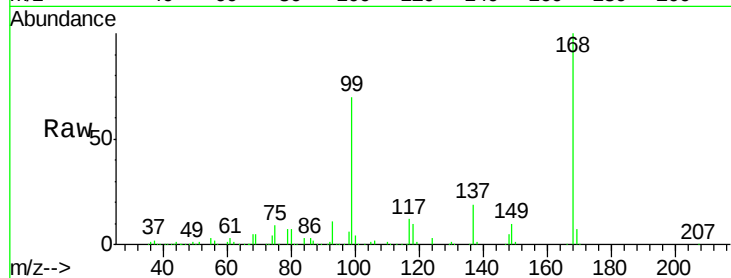

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

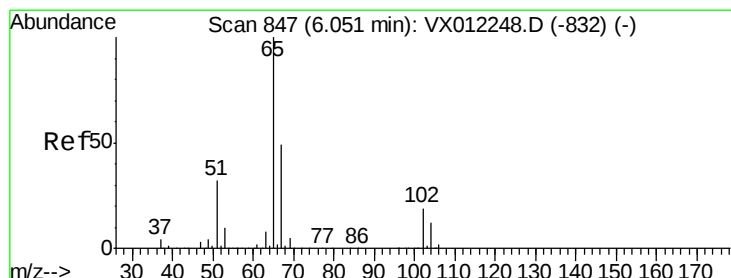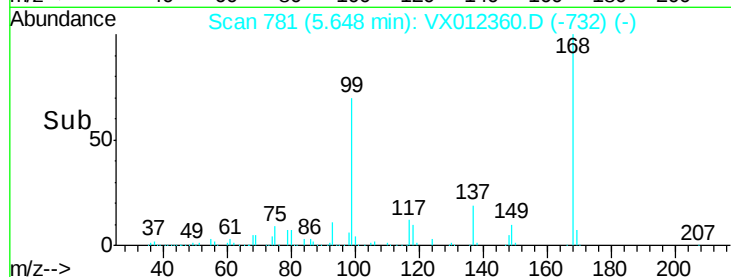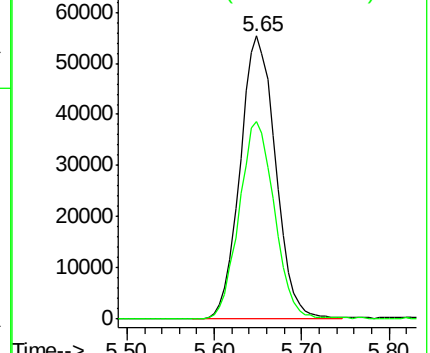

#33

1,2-Dichloroethane-d4

Concen: 49.905 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX012360.D


Acq: 12 Sep 2019 21:11

Tgt Ion: 65 Resp: 110079

Ion Ratio Lower Upper



65 100


67 50.0 0.0 99.8

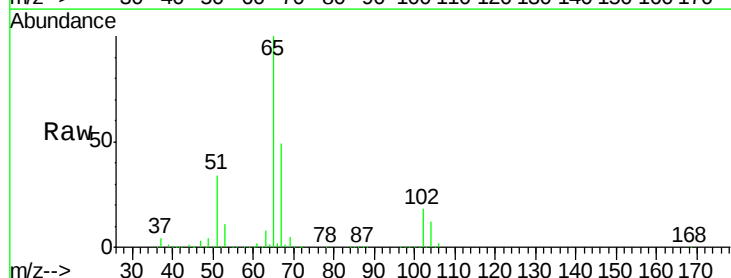

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

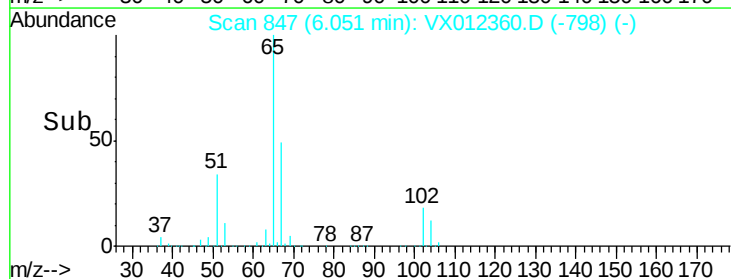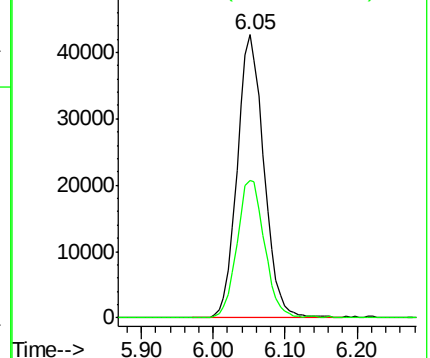

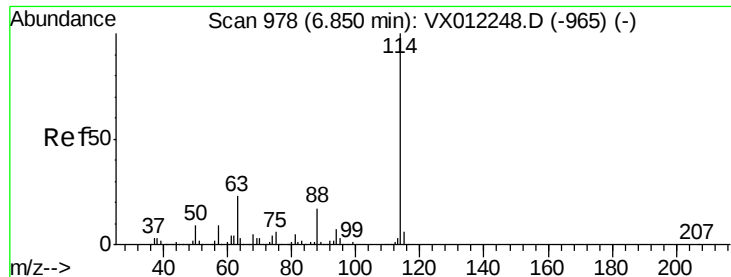

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX012360.D

Acq: 12 Sep 2019 21:11

Instrument :

MSVOA_X

ClientSampleId :

SB-15-14.5-15.0


Tot Ion:114 Resp: 271275

Ion Ratio Lower Upper

114 100

63 22.2 0.0 45.2




88 17.9 0.0 34.8

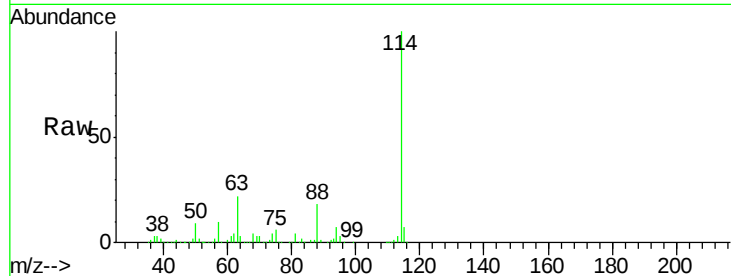

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

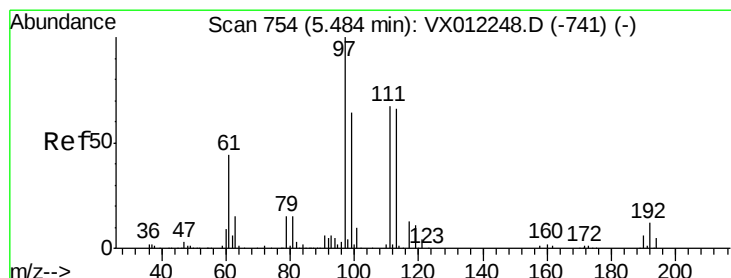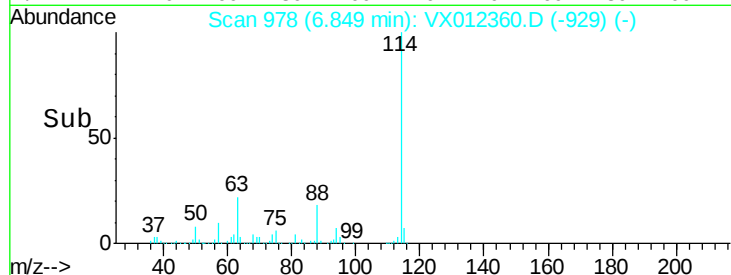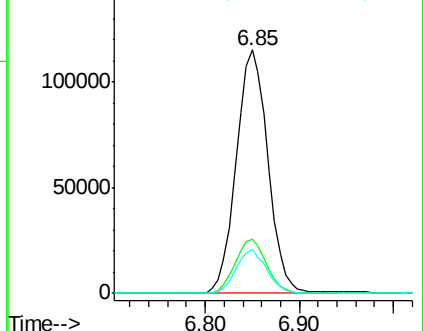

#35

Dibromofluoromethane

Concen: 46.063 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.00 min

Lab File: VX012360.D

Acq: 12 Sep 2019 21:11


Tgt Ion:113 Resp: 80104

Ion Ratio Lower Upper

113 100

111 103.6 83.0 124.6



192 18.1 14.3 21.5

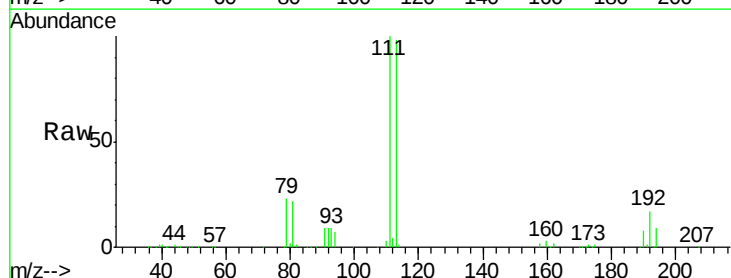


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



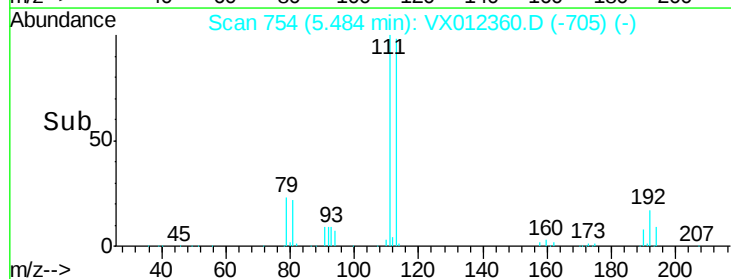
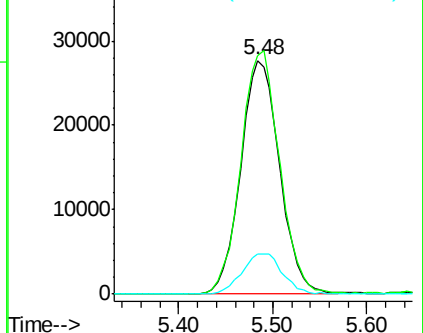


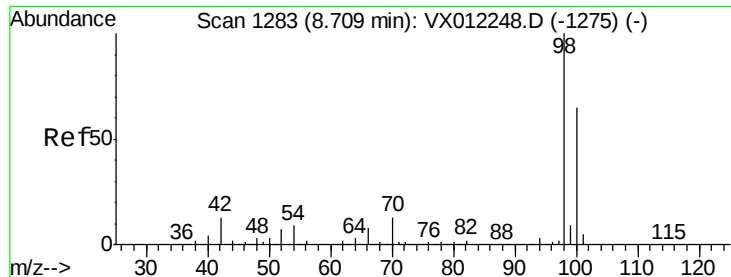

#50
Toluene-d8
Concen: 52.685 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX012360.D
Acq: 12 Sep 2019 21:11




Instrument :
MSVOA_X
ClientSampleId :
SB-15-14.5-15.0


Tot Ion: 98 Resp: 321338
Ion Ratio Lower Upper
98 100
100 67.1 54.1 81.1

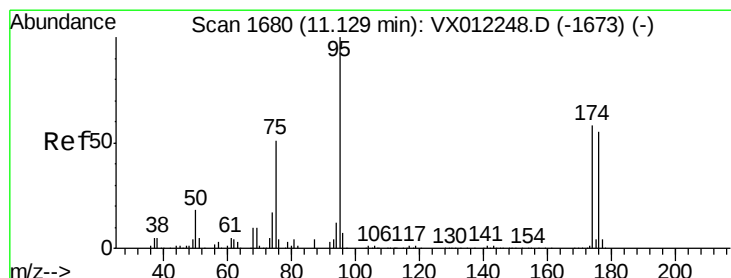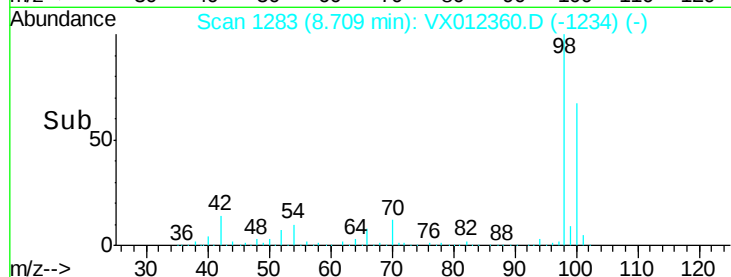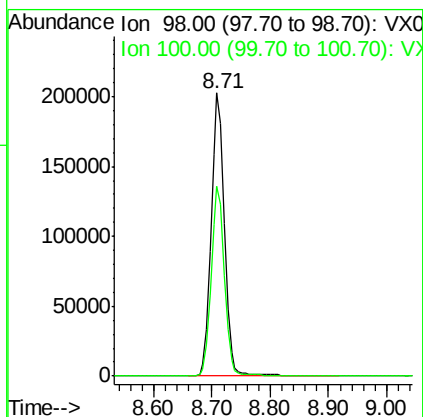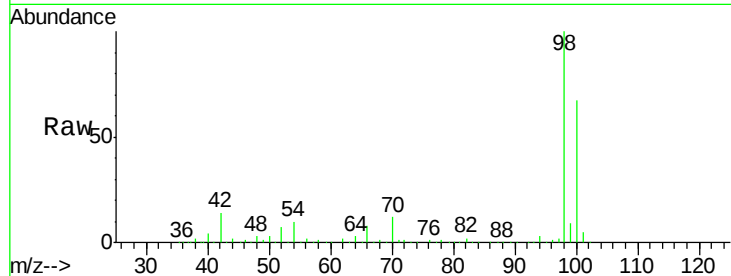

#62
4-Bromofluorobenzene
Concen: 45.848 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX012360.D
Acq: 12 Sep 2019 21:11

Tgt Ion: 95 Resp: 129640
Ion Ratio Lower Upper
95 100
174 68.0 0.0 127.0
176 65.0 0.0 125.8


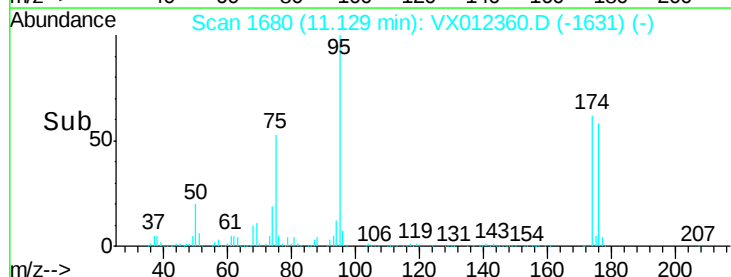
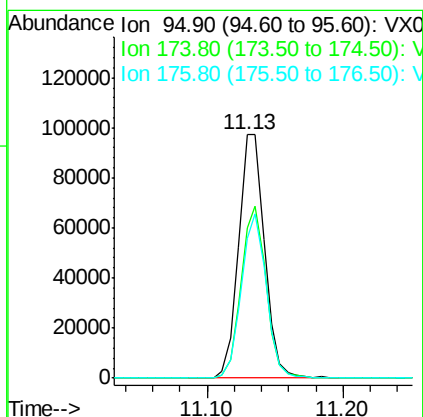
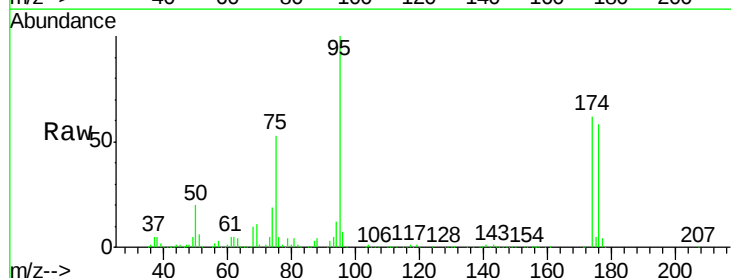


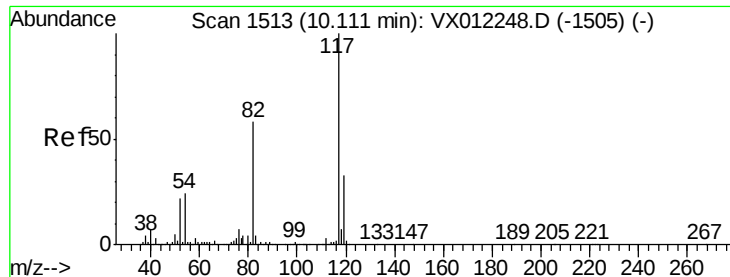

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX012360.D
Acq: 12 Sep 2019 21:11

Instrument :
MSVOA_X
ClientSampleId :
SB-15-14.5-15.0

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.5	46.4	69.6
119	31.6	26.6	39.8

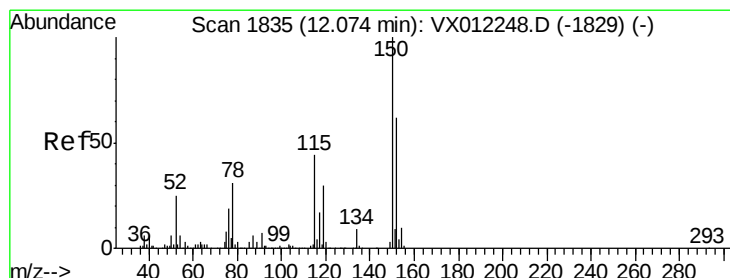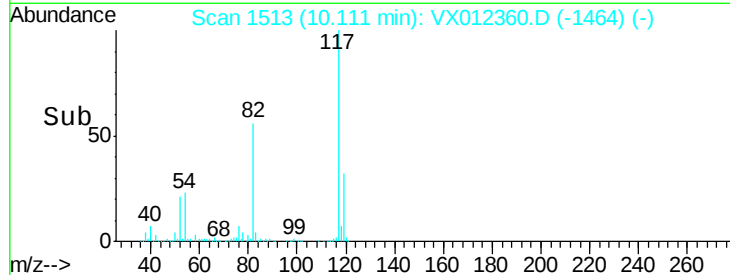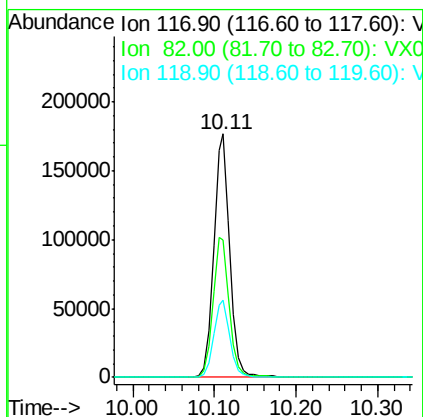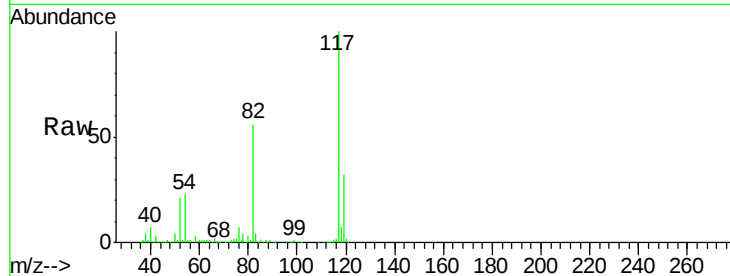

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX012360.D
Acq: 12 Sep 2019 21:11

Tgt Ion	Ratio	Lower	Upper
152	100		
115	62.6	45.5	136.4
150	152.9	0.0	346.4

