


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091219\
Data File : VX012350.D
Acq On : 12 Sep 2019 16:25
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Title : SW846 8260
Last Update : Tue Sep 10 12:55:26 2019

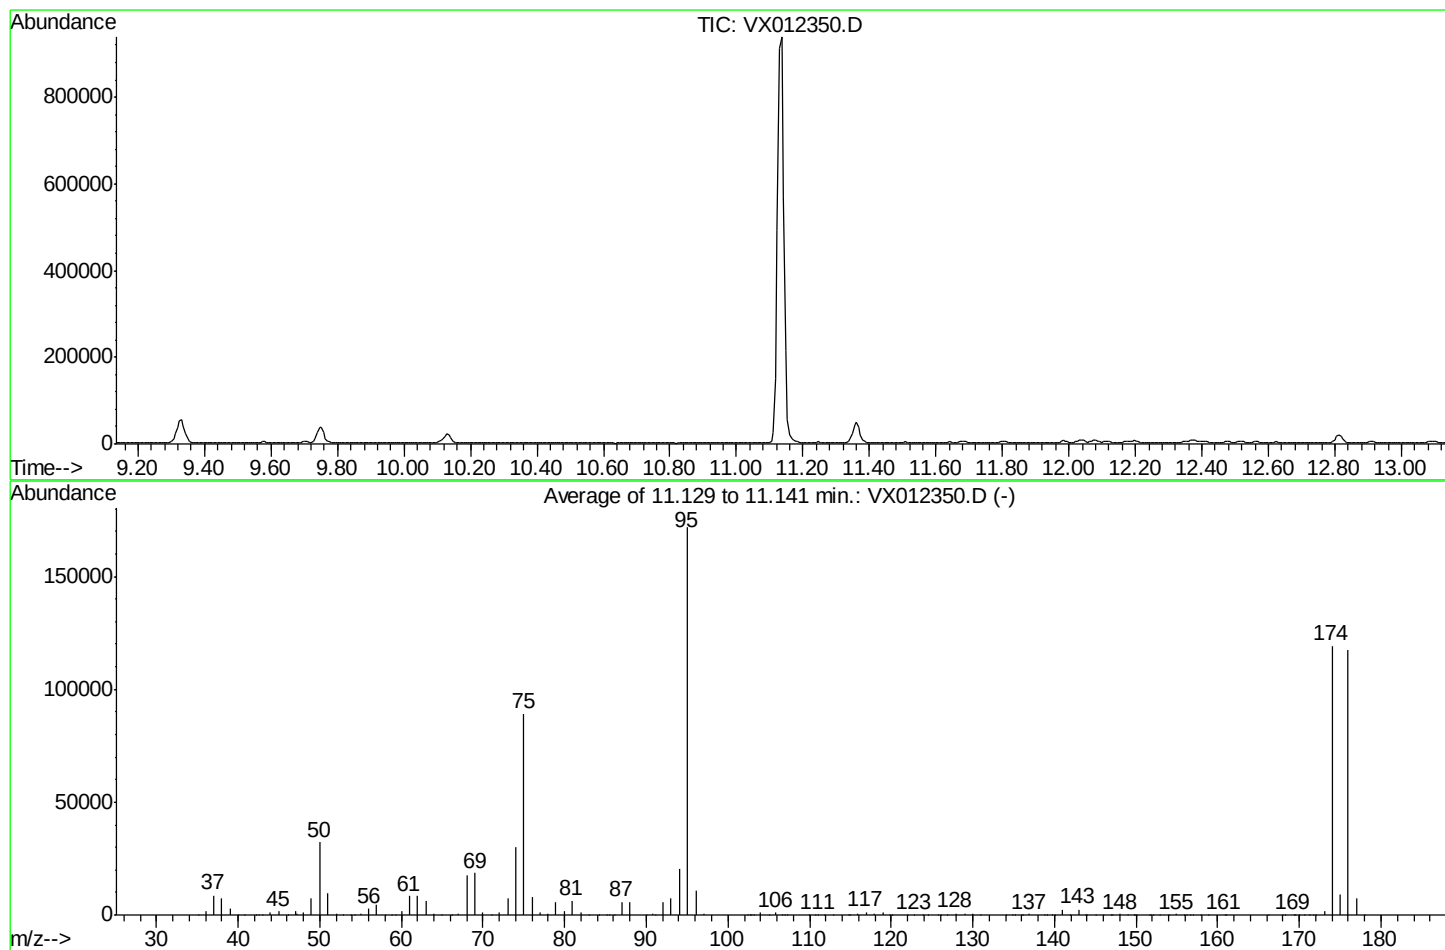

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	32205	PASS
75	95	30	60	51.9	89237	PASS
95	95	100	100	100.0	171805	PASS
96	95	5	9	6.4	11019	PASS
173	174	0.00	2	1.5	1831	PASS
174	95	50	100	69.3	119128	PASS
175	174	5	9	7.6	9055	PASS
176	174	95	101	98.4	117277	PASS
177	176	5	9	6.2	7235	PASS