

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091222\
 Data File : VX031285.D
 Acq On : 12 Sep 2022 19:47
 Operator : JC/MD
 Sample : N4298-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB01-20220822

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M

Title : SW846 8260

Signal : TIC: VX031285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	299	305	314	rBB	7426	16298	4.99%	0.762%
2	4.593	565	575	584	rBV2	4372	14445	4.43%	0.675%
3	5.391	695	706	721	rBV	65542	190881	58.48%	8.923%
4	5.562	723	734	749	rVB2	82575	233587	71.56%	10.919%
5	5.964	790	800	813	rBV2	71223	184237	56.44%	8.612%
6	6.769	922	932	944	rBV	112347	272422	83.46%	12.734%
7	8.653	1234	1241	1250	rBV	207965	326415	100.00%	15.258%
8	9.708	1409	1414	1419	rBV2	3069	4780	1.46%	0.223%
9	10.055	1466	1471	1483	rVB	219016	296796	90.93%	13.874%
10	11.085	1634	1640	1652	rBB	251714	315688	96.71%	14.757%
11	12.024	1789	1794	1802	rBV	235507	283739	86.93%	13.263%




Sum of corrected areas: 2139288

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091222\
Data File : VX031285.D
Acq On : 12 Sep 2022 19:47
Operator : JC/MD
Sample : N4298-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

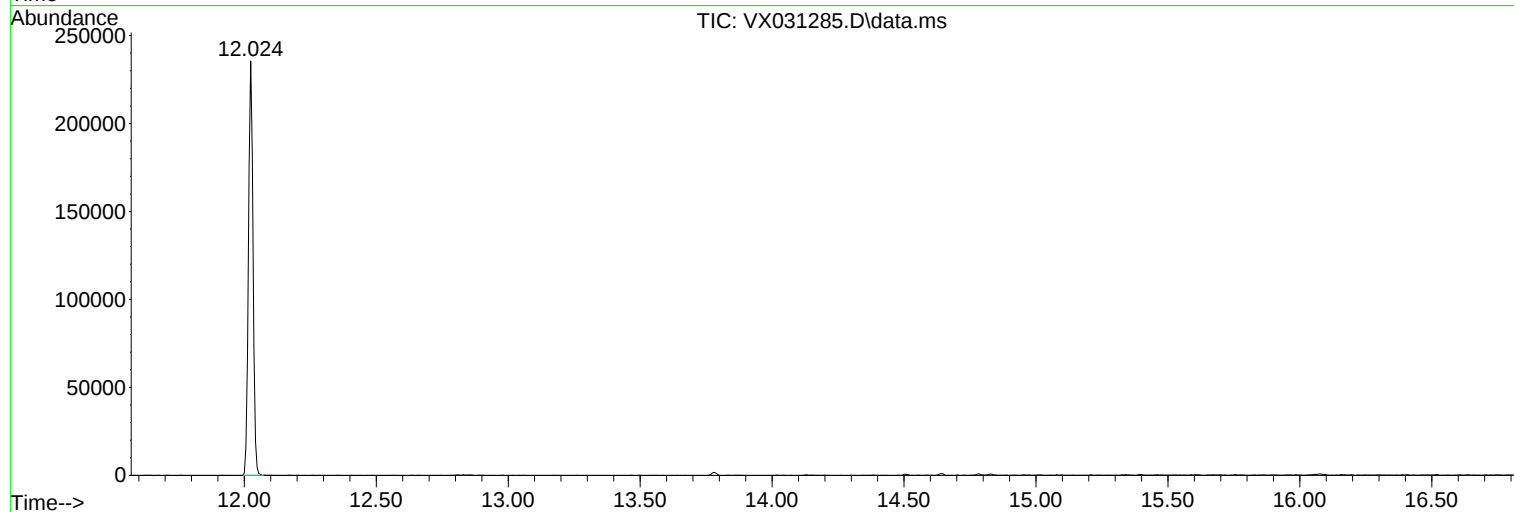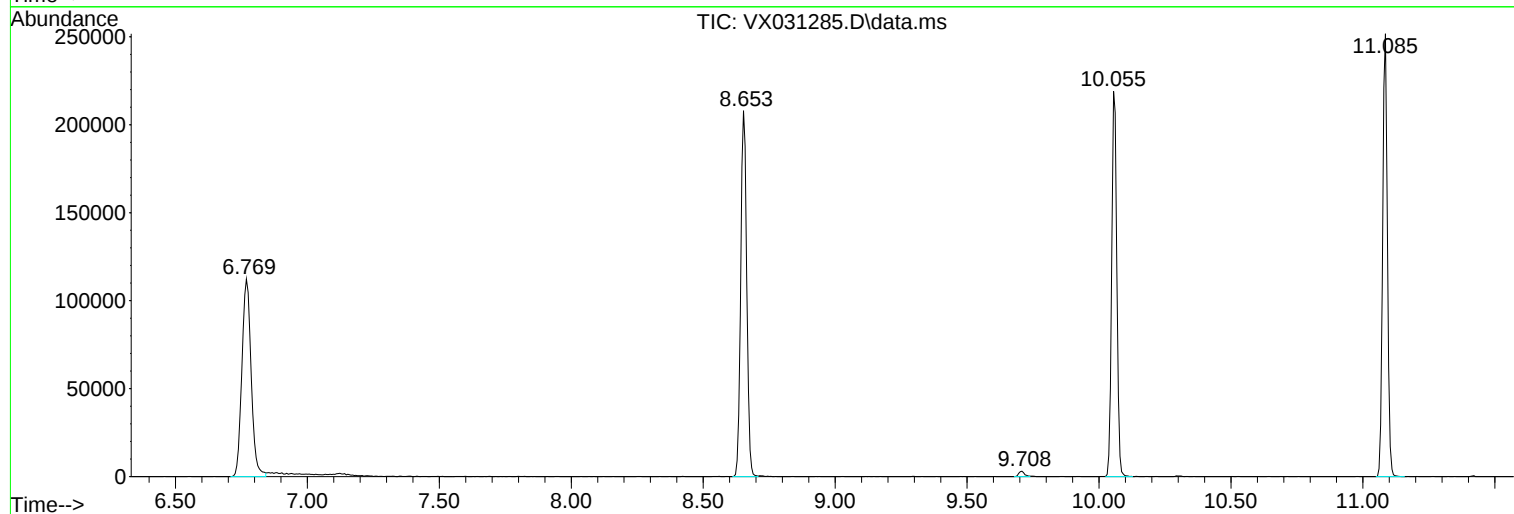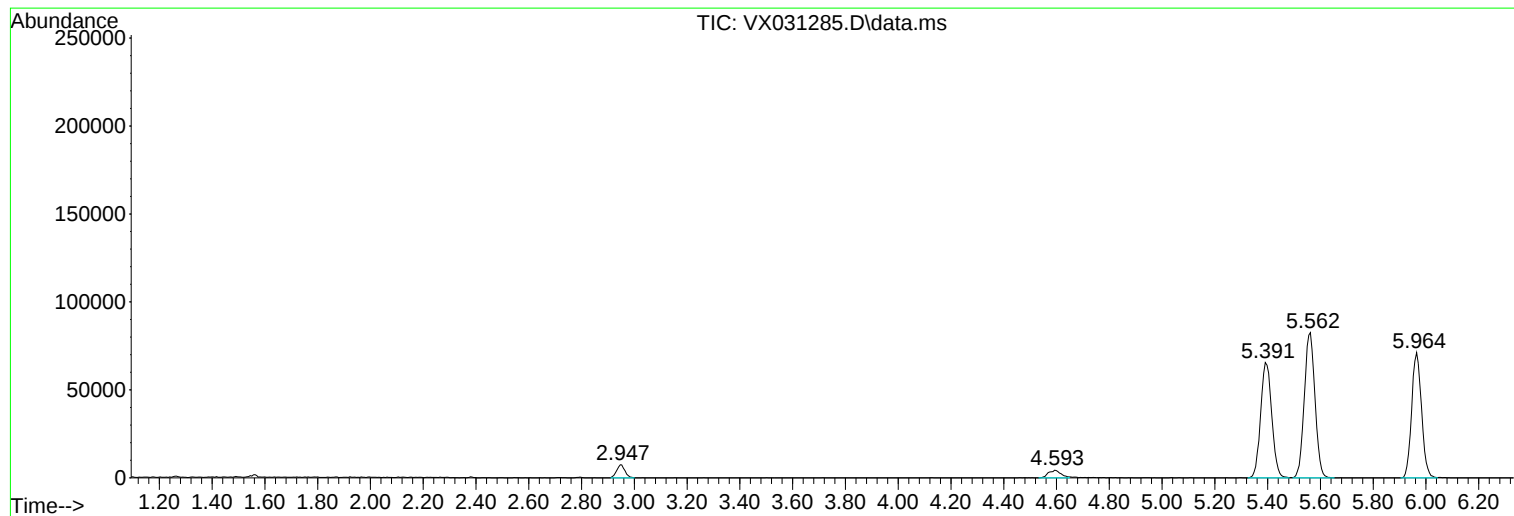

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091222\
Data File : VX031285.D
Acq On : 12 Sep 2022 19:47
Operator : JC/MD
Sample : N4298-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091222\
Data File : VX031285.D
Acq On : 12 Sep 2022 19:47
Operator : JC/MD
Sample : N4298-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc