
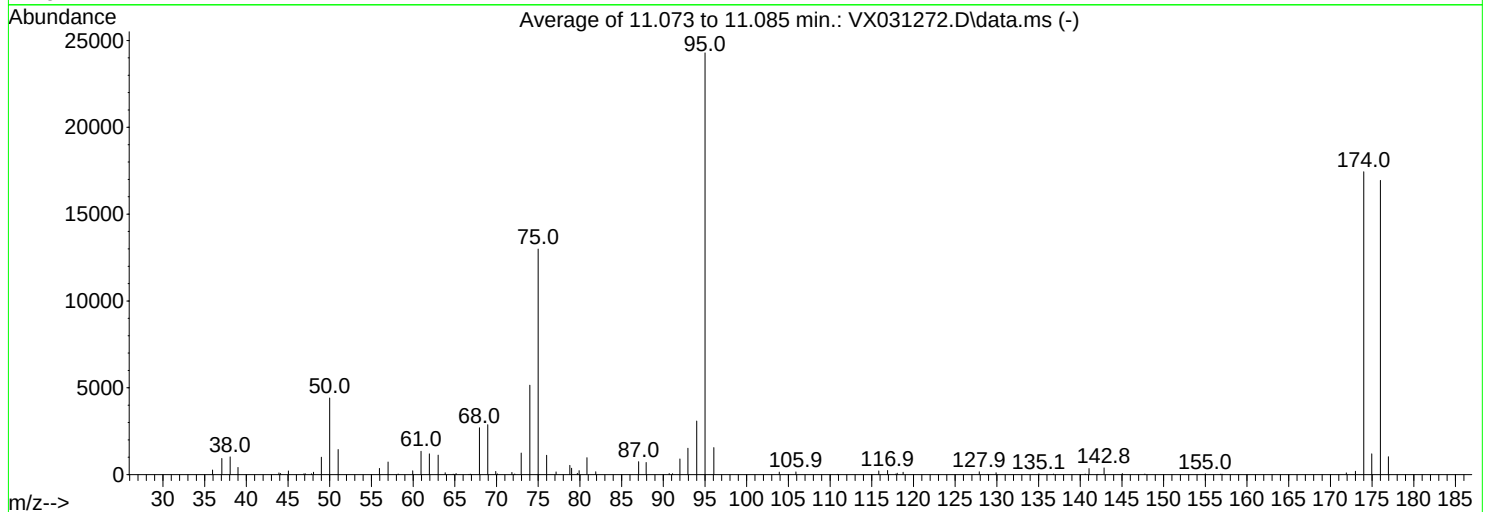


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091222\
Data File : VX031272.D
Acq On : 12 Sep 2022 11:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Title : SW846 8260
Last Update : Wed Sep 07 23:22:41 2022

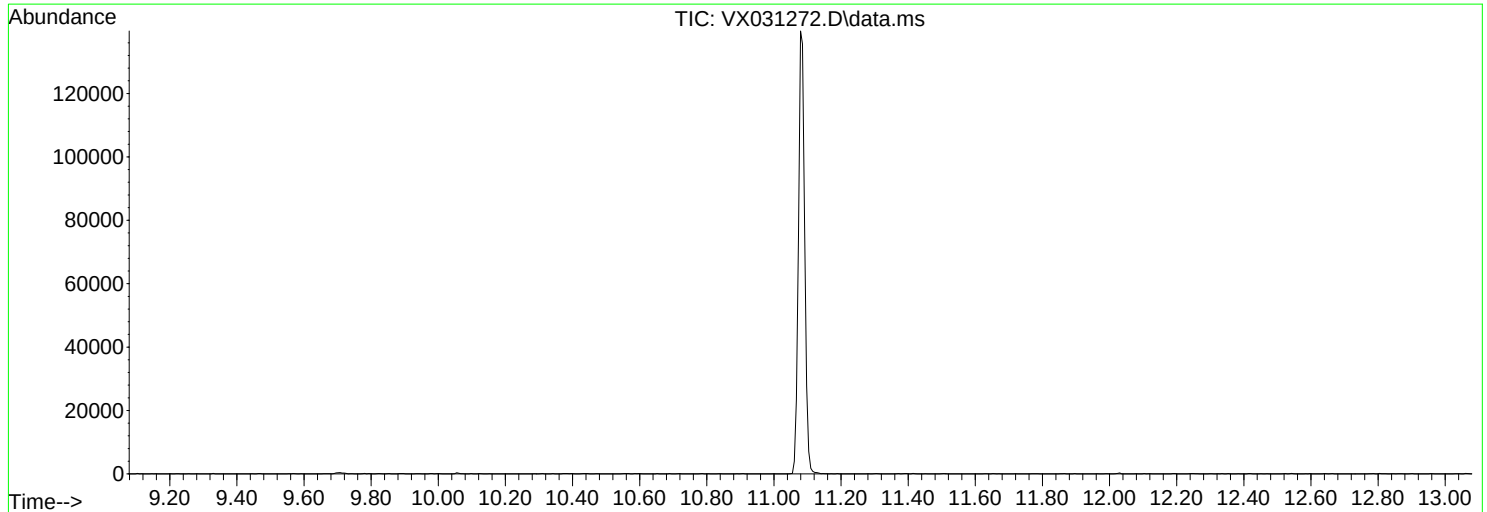

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	4415	PASS
75	95	30	60	53.5	12991	PASS
95	95	100	100	100.0	24288	PASS
96	95	5	9	6.4	1561	PASS
173	174	0.00	2	1.1	192	PASS
174	95	50	100	71.8	17442	PASS
175	174	5	9	6.9	1202	PASS
176	174	95	101	97.2	16947	PASS
177	176	5	9	6.1	1029	PASS