

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
 Data File : VX037662.D
 Acq On : 12 Sep 2023 12:33
 Operator : JC/MD
 Sample : 04296-03DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Sep 13 01:44:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 10:10:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	177416	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	304053	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	286266	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	136418	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	121598	42.362	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	84.720%		
35) Dibromofluoromethane	5.385	113	95824	44.463	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.920%		
50) Toluene-d8	8.647	98	378415	46.557	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	93.120%		
62) 4-Bromofluorobenzene	11.079	95	135866	46.333	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	92.660%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.940	59	3494	Below Cal	#	78
13) Acrolein	2.239	56	160	0.341	ug/l #	44
16) Acetone	2.386	43	2083	1.795	ug/l	96
20) Methylene Chloride	2.788	84	1007	Below Cal	#	74
25) 2-Butanone	4.580	43	1787	0.944	ug/l #	51
26) 2,2-Dichloropropane	4.574	77	1691	0.599	ug/l #	54
31) Cyclohexane	5.477	56	1314	0.398	ug/l	95
36) 1,1-Dichloropropene	5.556	75	15393	5.250	ug/l #	51
38) Carbon Tetrachloride	5.550	117	18652	6.227	ug/l #	15
39) Methylcyclohexane	7.385	83	3639	1.049	ug/l	95
55) 1,1,2-Trichloroethane	9.104	97	649	0.270	ug/l #	23
67) Ethyl Benzene	10.195	91	95279	8.775	ug/l	100
68) m/p-Xylenes	10.299	106	318924	77.029	ug/l	99
69) o-Xylene	10.640	106	125218	30.334	ug/l	99
70) Styrene	10.640	104	6532	0.970	ug/l #	1
73) Isopropylbenzene	10.963	105	18273	1.789	ug/l	97
76) 1,2,3-Trichloropropane	11.378	75	4038	1.346	ug/l #	1
78) n-propylbenzene	11.305	91	54788	4.663	ug/l	98
79) 2-Chlorotoluene	11.378	91	57723	7.980	ug/l #	43
80) 1,3,5-Trimethylbenzene	11.451	105	184508	21.495	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	71800	72.772	ug/l #	5
82) 4-Chlorotoluene	11.451	91	20933	2.533	ug/l #	49
83) tert-Butylbenzene	11.750	119	77840	9.027	ug/l #	59
84) 1,2,4-Trimethylbenzene	11.750	105	644385	74.461	ug/l	97
85) sec-Butylbenzene	11.750	105	644385	60.529	ug/l #	57
86) p-Isopropyltoluene	11.969	119	9001	1.032	ug/l	96
89) n-Butylbenzene	12.317	91	15839	2.005	ug/l #	15
90) Hexachloroethane	12.530	117	3580	2.432	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.957	75	388	0.494	ug/l #	9
93) 1,2,4-Trichlorobenzene	13.585	180	726	0.262	ug/l #	64
95) Naphthalene	13.774	128	158916	15.843	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037662.D
Acq On : 12 Sep 2023 12:33
Operator : JC/MD
Sample : 04296-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Sep 13 01:44:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 10:10:04 2023
Response via : Initial Calibration

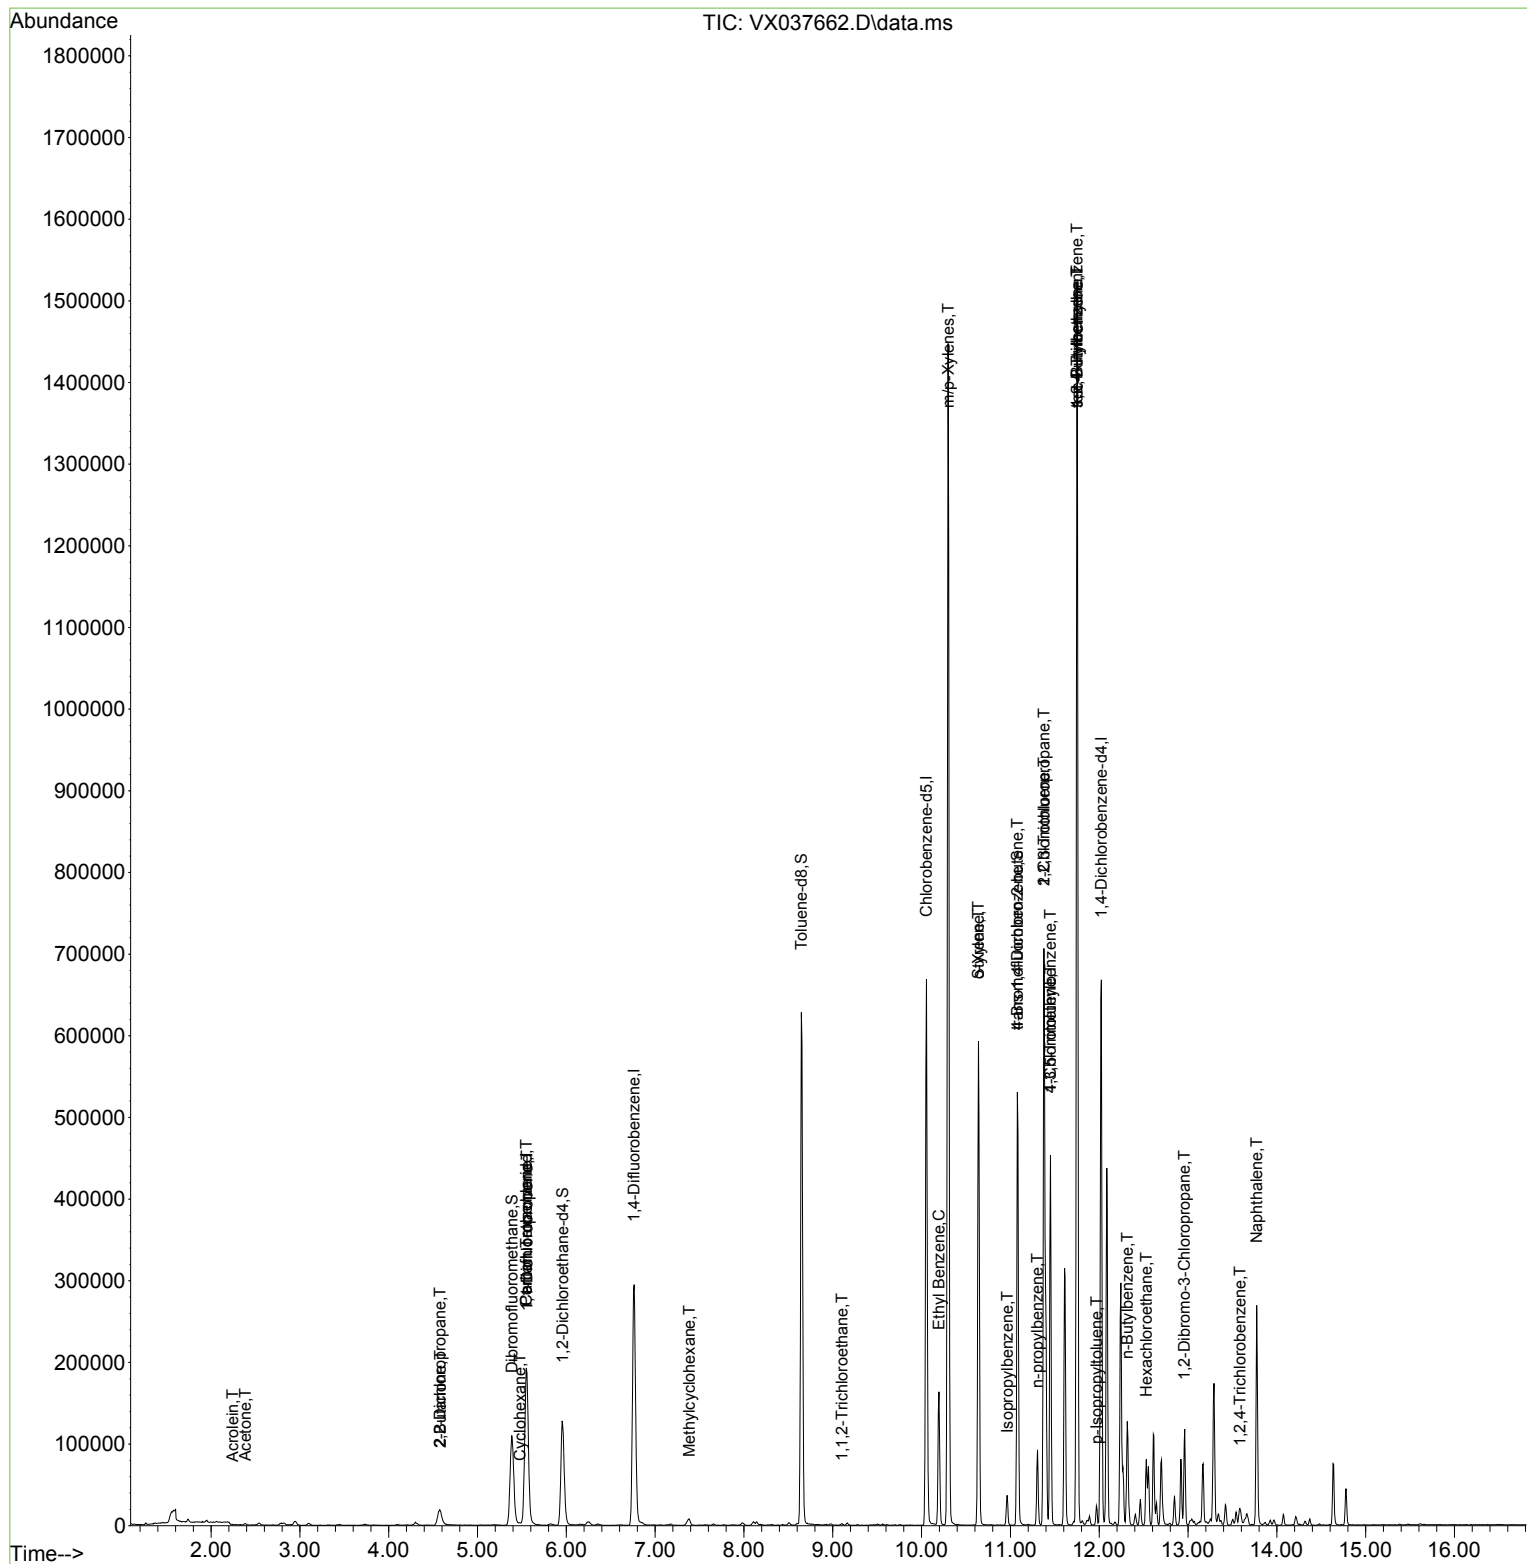



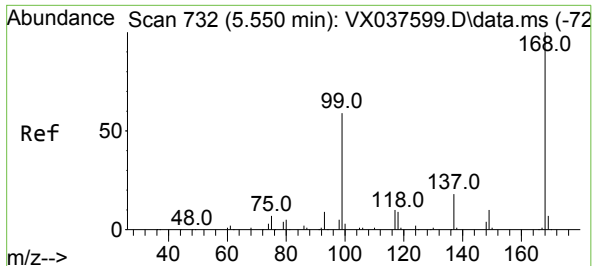


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Instrument :
MSVOA_X
ClientSampleId :



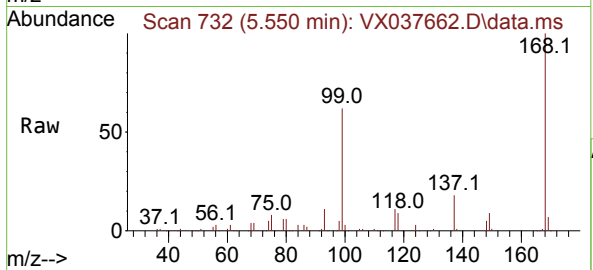



Tgt Ion:168 Resp: 177416
Ion Ratio Lower Upper
168 100
99 61.7 56.6 85.0

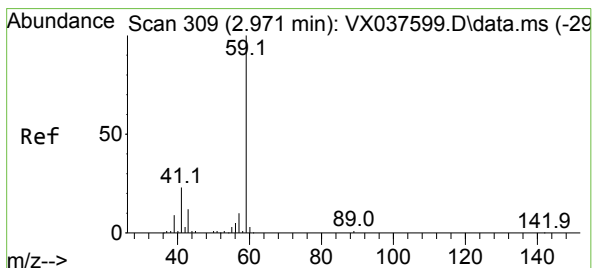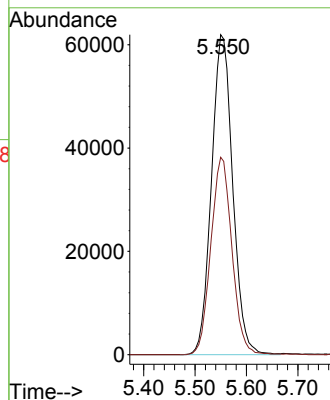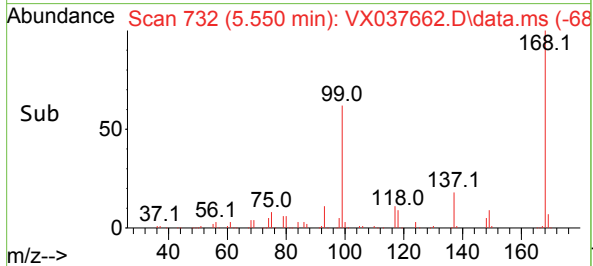

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.940 min Scan# 304
Delta R.T. -0.031 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33


Tgt Ion: 59 Resp: 3494
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

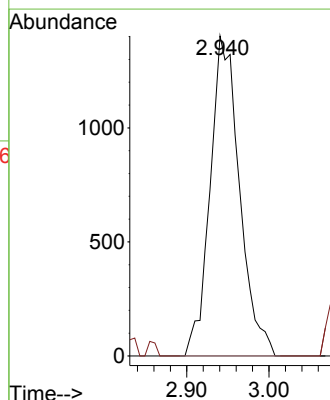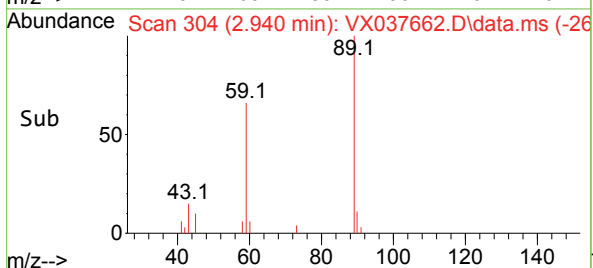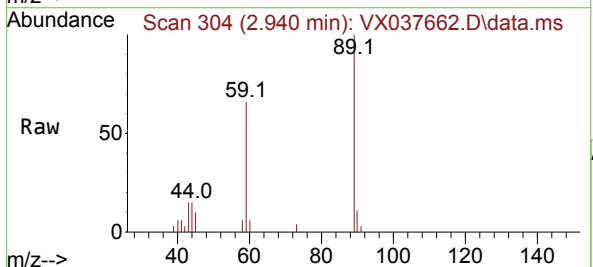



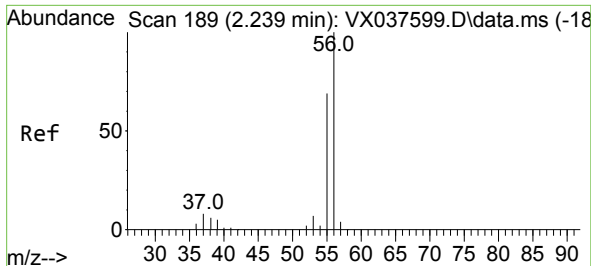


#13
Acrolein
Concen: 0.341 ug/l
RT: 2.239 min Scan# 118
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Instrument : MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 160
Ion Ratio Lower Upper
56 100
55 118.1 57.1 85.7#



#16
Acetone
Concen: 1.795 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33


Tgt Ion: 43 Resp: 2083
Ion Ratio Lower Upper
43 100
58 29.5 21.9 32.9

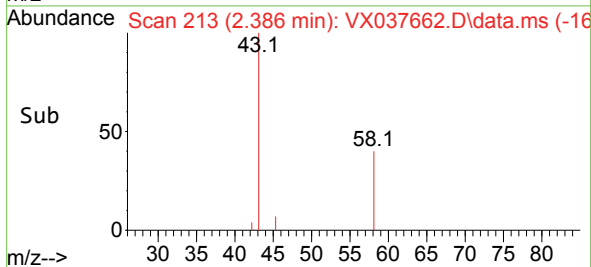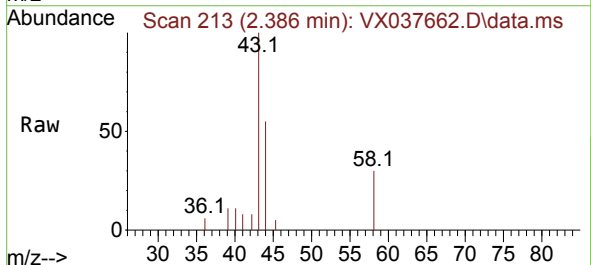

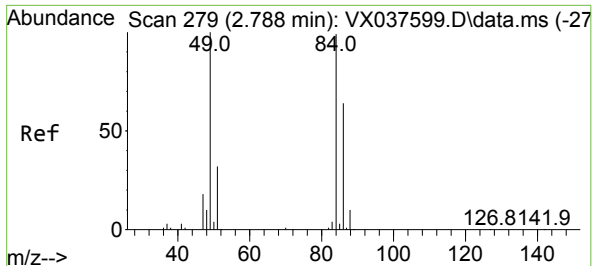




#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Instrument :
MSVOA_X
ClientSampleId :

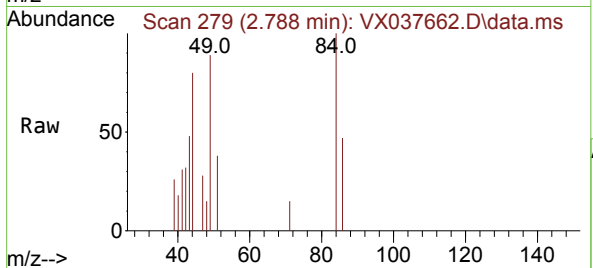

Tgt Ion: 84 Resp: 1007




Ion	Ratio	Lower	Upper
84	100		
49	88.6	103.6	155.4#
51	37.6	33.8	50.6
86	47.2	49.4	74.0#

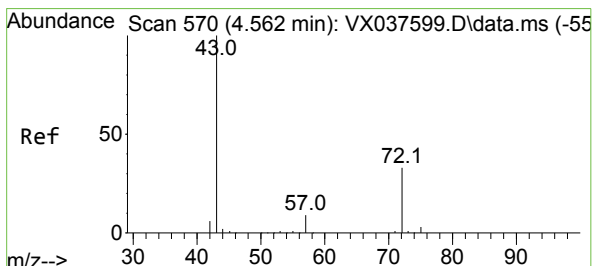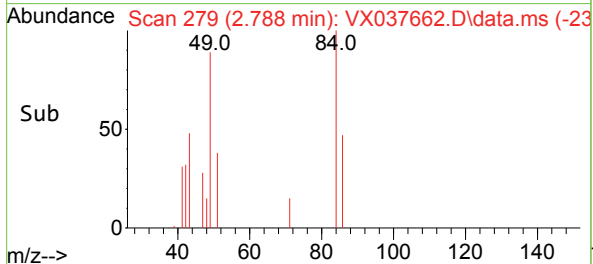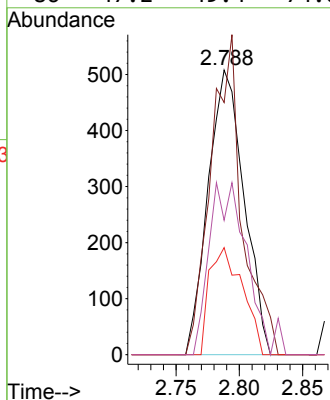


#25
2-Butanone
Concen: 0.944 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 43 Resp: 1787

Ion	Ratio	Lower	Upper
43	100		
72	0.0	19.4	29.2#


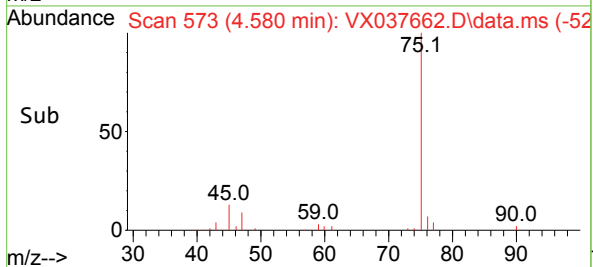
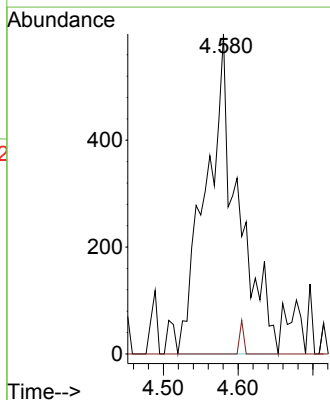
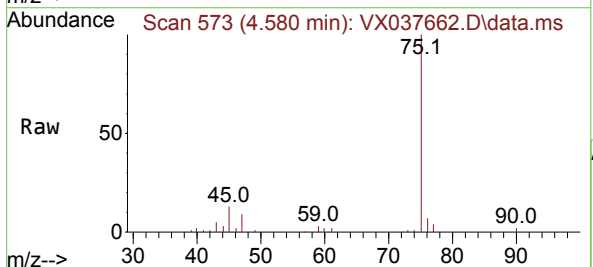




#26
2,2-Dichloropropane
Concen: 0.599 ug/l
RT: 4.574 min Scan# 51
Delta R.T. 0.097 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 77 Resp: 1691
Ion Ratio Lower Upper
77 100
97 0.0 10.8 32.3#



#31
Cyclohexane
Concen: 0.398 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 56 Resp: 1314
Ion Ratio Lower Upper
56 100
69 25.0 23.4 35.2
84 79.2 65.9 98.9


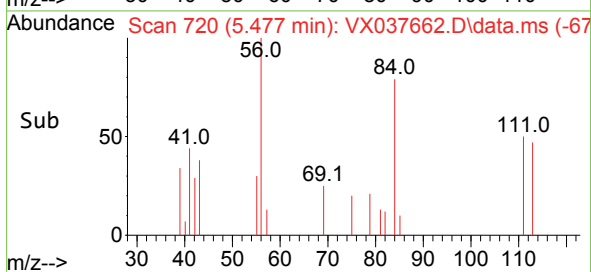

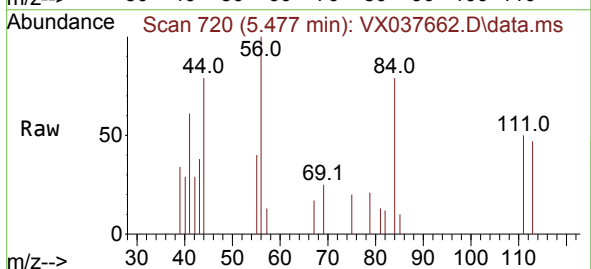




#33
1,2-Dichloroethane-d4
Concen: 42.362 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 65 Resp: 121598
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.2

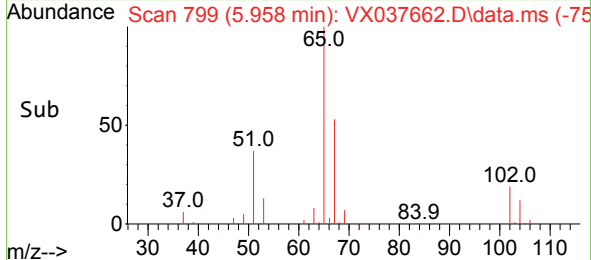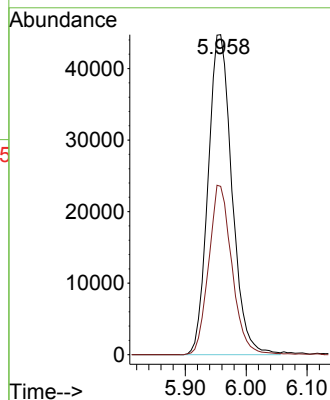

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33


Tgt Ion:114 Resp: 304053
Ion Ratio Lower Upper
114 100
63 20.6 0.0 45.0
88 15.6 0.0 36.6

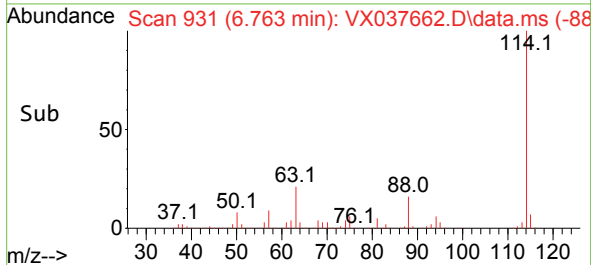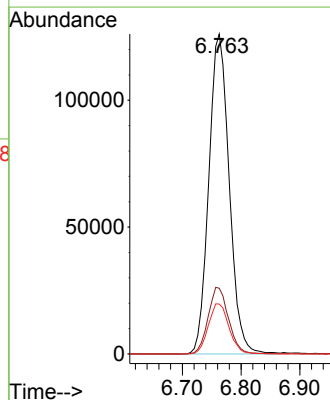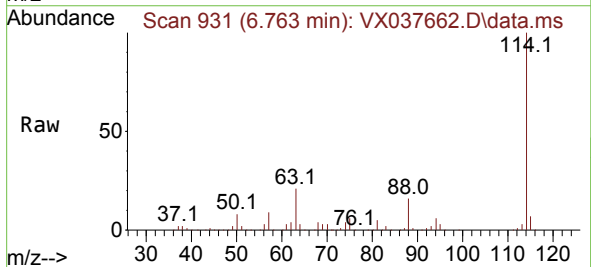

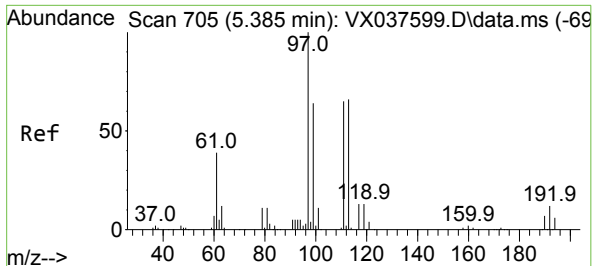




#35
 Dibromofluoromethane
 Concen: 44.463 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. -0.000 min
 Lab File: VX037662.D
 Acq: 12 Sep 2023 12:33

Instrument :
 MSVOA_X
 ClientSampleId :

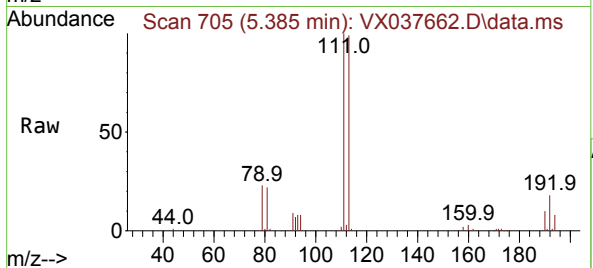

Tgt Ion:113 Resp: 95824




Ion	Ratio	Lower	Upper
113	100		
111	102.2	82.9	124.3
192	18.2	13.3	19.9

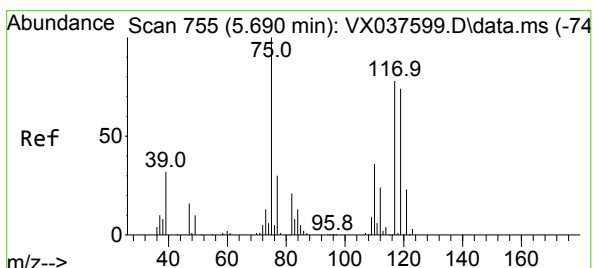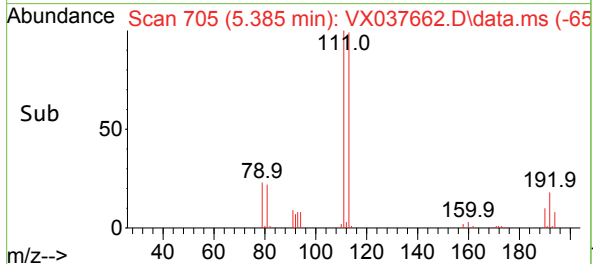


#36
 1,1-Dichloropropene
 Concen: 5.250 ug/l
 RT: 5.556 min Scan# 733
 Delta R.T. -0.134 min
 Lab File: VX037662.D
 Acq: 12 Sep 2023 12:33

Tgt Ion: 75 Resp: 15393


Ion	Ratio	Lower	Upper
75	100		
110	9.1	17.0	50.9#
77	0.0	24.7	37.1#

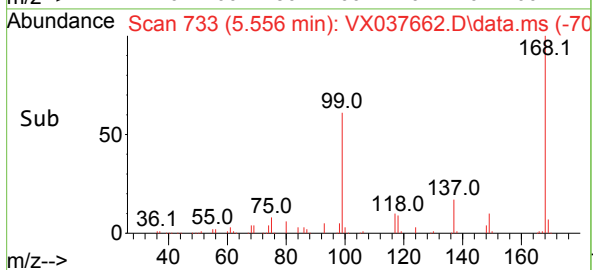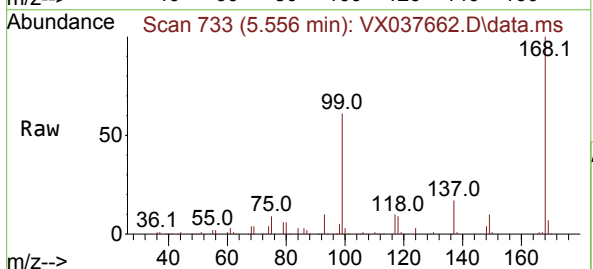



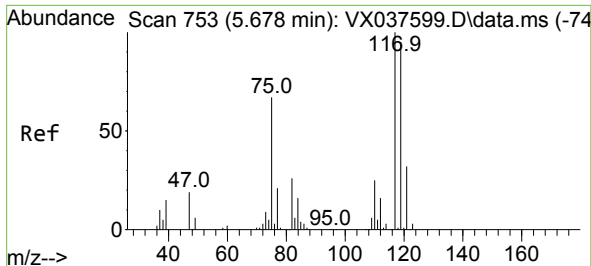


#38
Carbon Tetrachloride
Concen: 6.227 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 18652
Ion Ratio Lower Upper
117 100
119 4.3 78.2 117.2#
121 0.0 24.4 36.6#

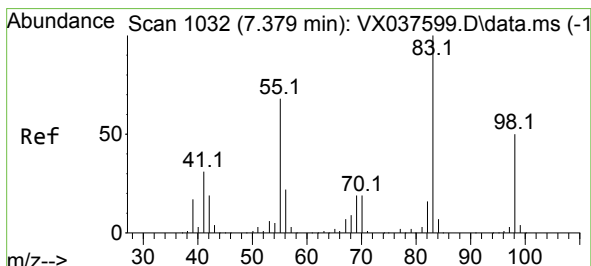

#39
Methylcyclohexane
Concen: 1.049 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.006 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 83 Resp: 3639
Ion Ratio Lower Upper
83 100
55 81.7 64.6 97.0
98 38.5 36.7 55.1









#50
Toluene-d8
Concen: 46.557 ug/l
RT: 8.647 min Scan# 1315
Delta R.T. -0.006 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 378415
Ion Ratio Lower Upper
98 100
100 63.4 53.1 79.7



#55
1,1,2-Trichloroethane
Concen: 0.270 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 97 Resp: 649
Ion Ratio Lower Upper
97 100
83 12.8 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#



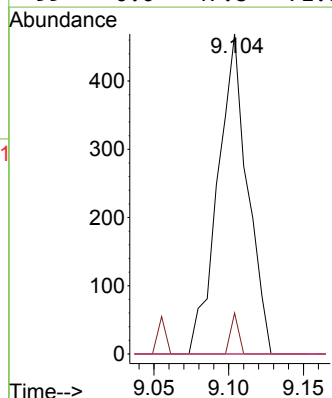
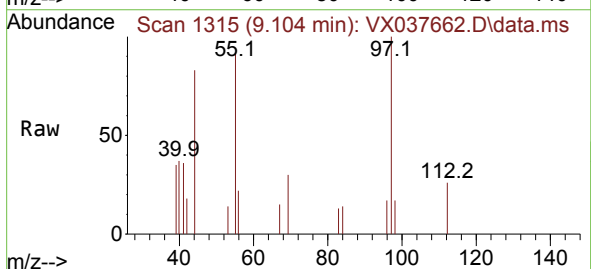


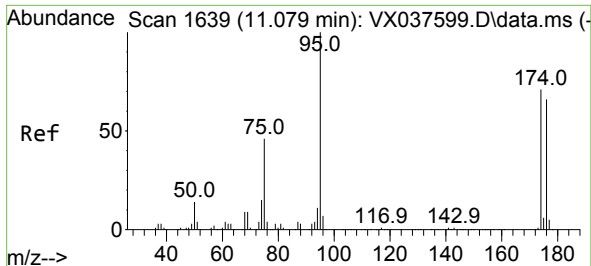

#62
4-Bromofluorobenzene
Concen: 46.333 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 135866
Ion Ratio Lower Upper
95 100
174 77.2 0.0 135.6
176 74.6 0.0 131.0

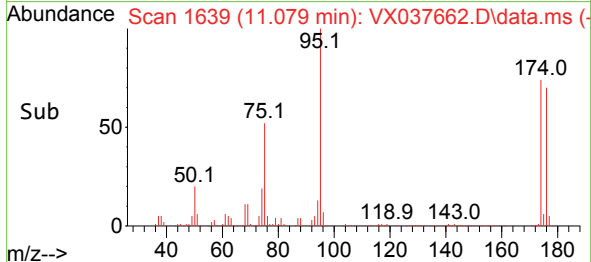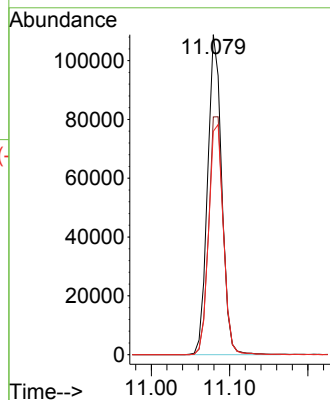

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 117 Resp: 286266
Ion Ratio Lower Upper
117 100
82 54.8 46.2 69.4
119 32.0 25.5 38.3


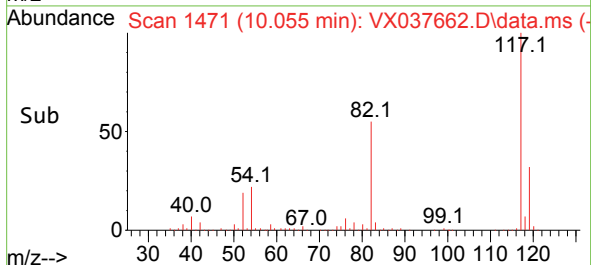
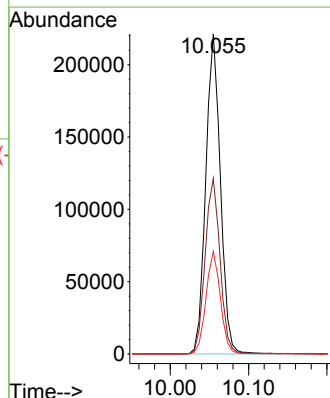
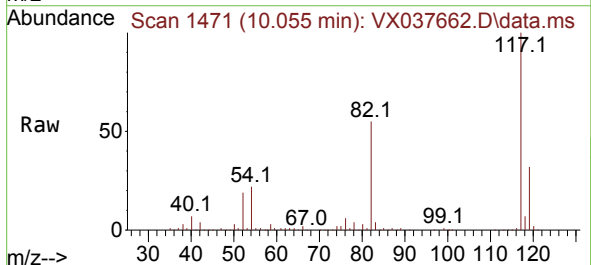




#67
Ethyl Benzene
Concen: 8.775 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 95279
Ion Ratio Lower Upper
91 100
106 31.0 24.9 37.3



#68
m/p-Xylenes
Concen: 77.029 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 106 Resp: 318924
Ion Ratio Lower Upper
106 100
91 205.5 165.5 248.3

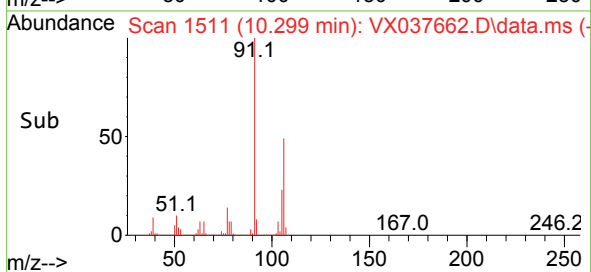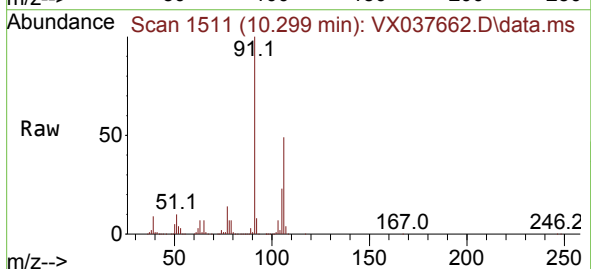



#69

o-Xylene

Concen: 30.334 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 125218

Ion Ratio Lower Upper

106 100

91 215.8 108.9 326.8



#70

Styrene

Concen: 0.970 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.019 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33




Tgt Ion:104 Resp: 6532


Ion Ratio Lower Upper

104 100

78 302.6 43.6 65.4#

103 275.1 43.6 65.4#


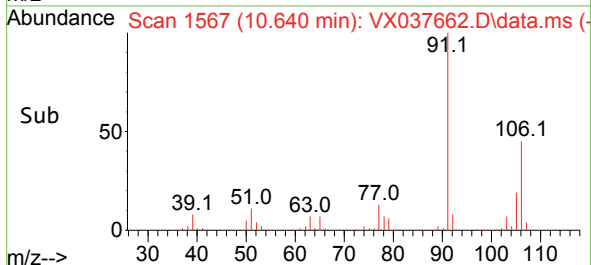
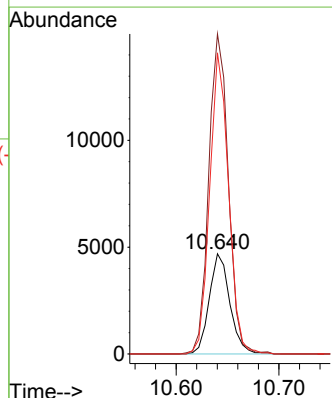
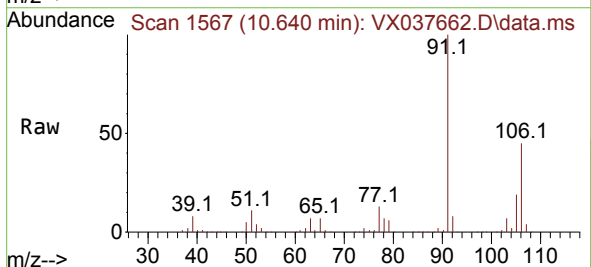




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 136418
Ion Ratio Lower Upper
152 100
115 61.0 43.3 129.9
150 157.5 0.0 345.0

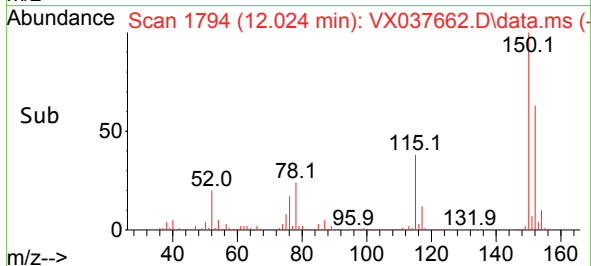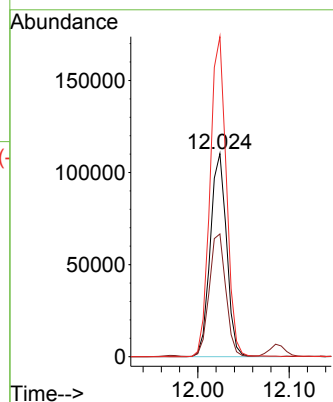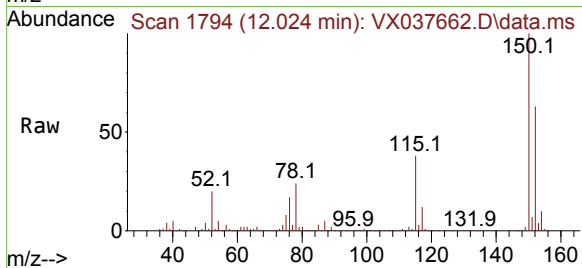

#73
Isopropylbenzene
Concen: 1.789 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion:105 Resp: 18273
Ion Ratio Lower Upper
105 100
120 27.2 12.9 38.6

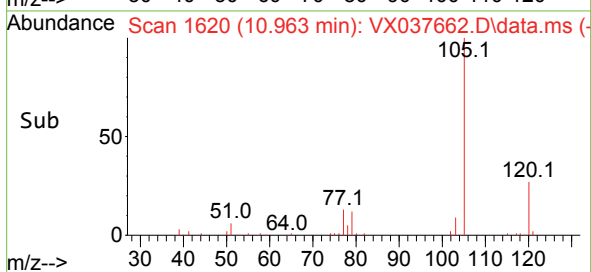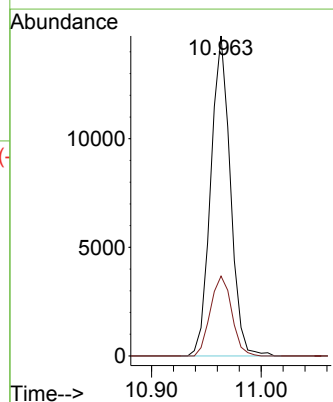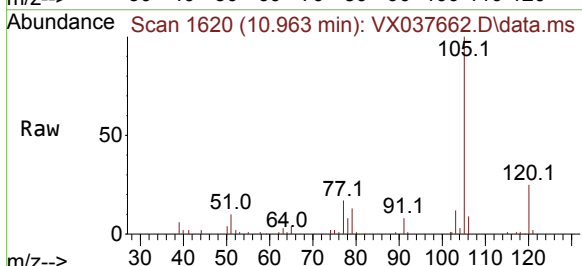



#76

1,2,3-Trichloropropane

Concen: 1.346 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.140 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 4038

Ion Ratio Lower Upper

75 100

77 1332.2 19.1 57.5#

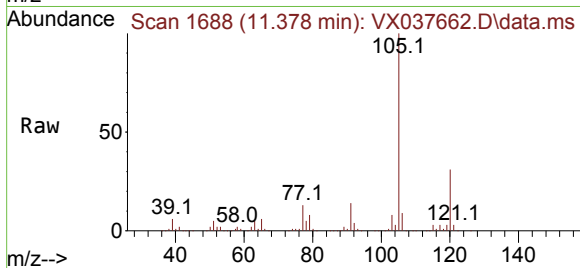

#78

n-propylbenzene

Concen: 4.663 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX037662.D




Acq: 12 Sep 2023 12:33


Tgt Ion: 91 Resp: 54788

Ion Ratio Lower Upper

91 100

120 22.0 11.5 34.4

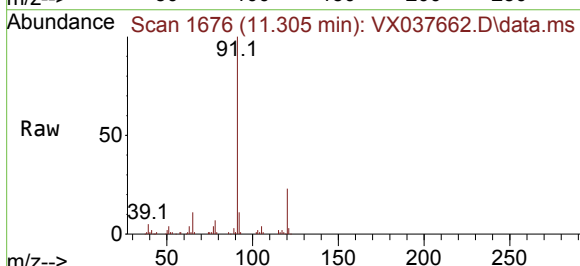



#79

2-Chlorotoluene

Concen: 7.980 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 57723

Ion Ratio Lower Upper

91 100

126 0.4 16.3 48.8#



#80

1,3,5-Trimethylbenzene

Concen: 21.495 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX037662.D




Acq: 12 Sep 2023 12:33


Tgt Ion:105 Resp: 184508

Ion Ratio Lower Upper

105 100

120 47.6 24.1 72.3




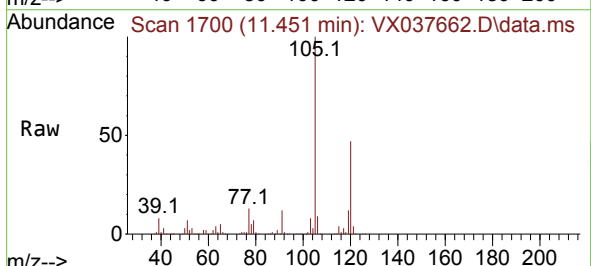




#81
trans-1,4-Dichloro-2-butene
Concen: 72.772 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 71800
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#



#82
4-Chlorotoluene
Concen: 2.533 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Tgt Ion: 91 Resp: 20933
Ion Ratio Lower Upper
91 100
126 1.4 14.2 42.6#

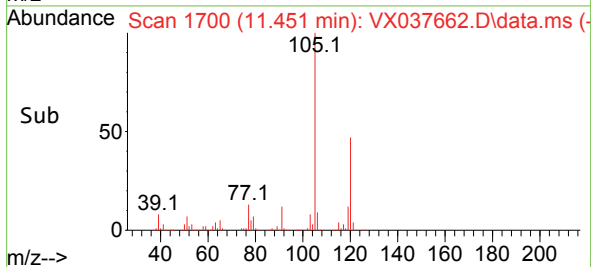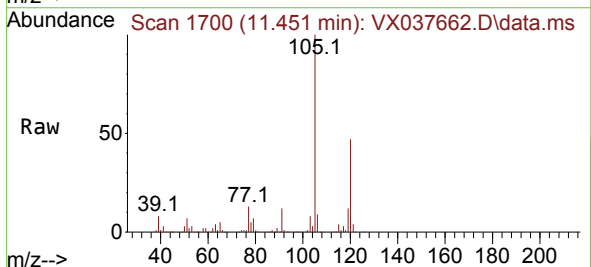



#83

tert-Butylbenzene

Concen: 9.027 ug/l

RT: 11.750 min Scan# 11

Delta R.T. 0.036 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 77840

Ion Ratio Lower Upper

119 100

91 92.1 31.2 93.6

134 0.0 11.7 35.0#

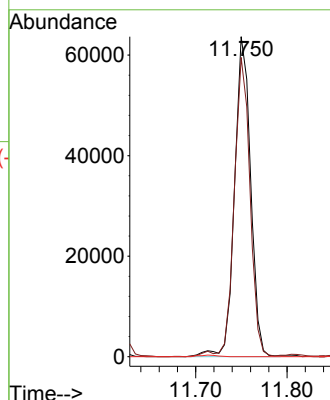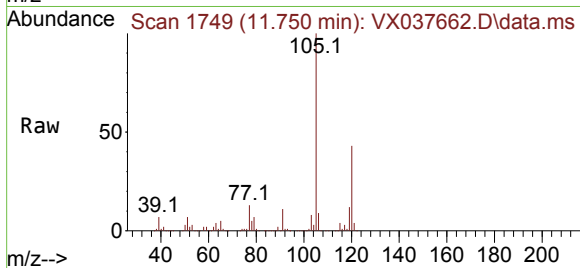

#84

1,2,4-Trimethylbenzene

Concen: 74.461 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.006 min

Lab File: VX037662.D




Acq: 12 Sep 2023 12:33


Tgt Ion:105 Resp: 644385

Ion Ratio Lower Upper

105 100

120 44.6 21.2 63.6

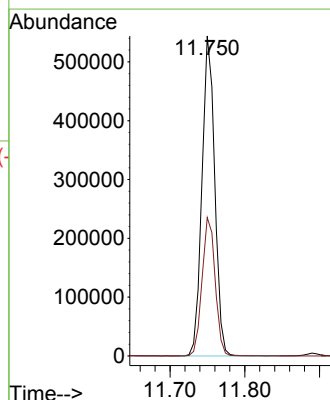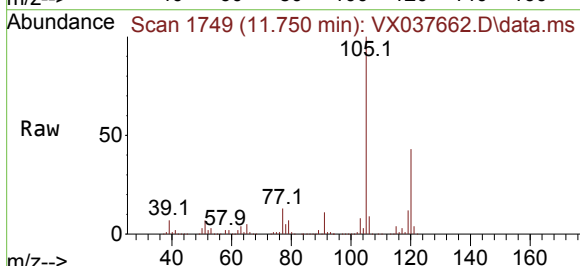



#85

sec-Butylbenzene

Concen: 60.529 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 644385

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#



#86

p-Isopropyltoluene

Concen: 1.032 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.043 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33




Tgt Ion:119 Resp: 9001


Ion Ratio Lower Upper

119 100

134 29.3 12.8 38.3

91 26.6 13.1 39.3

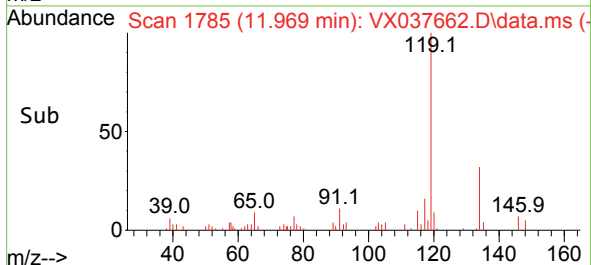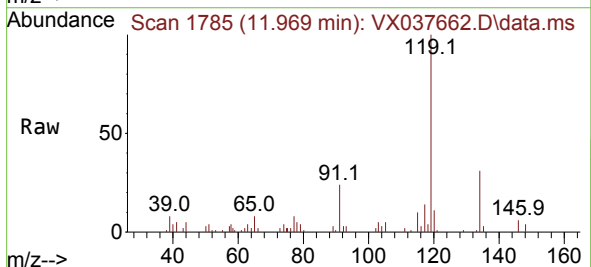

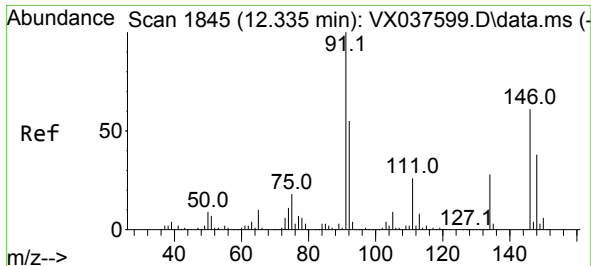

#89

n-Butylbenzene

Concen: 2.005 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. -0.018 min

Lab File: VX037662.D

Acq: 12 Sep 2023 12:33

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 91 Resp: 15839

Ion Ratio Lower Upper

91 100

92 27.4 27.4 82.0

134 119.6 12.6 37.8#

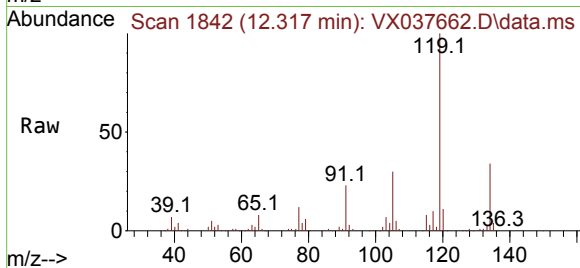

#90

Hexachloroethane

Concen: 2.432 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.012 min

Lab File: VX037662.D




Acq: 12 Sep 2023 12:33


Tgt Ion: 117 Resp: 3580

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#




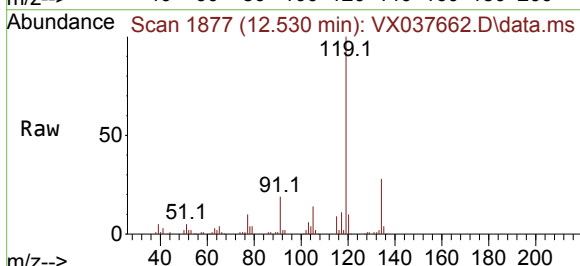


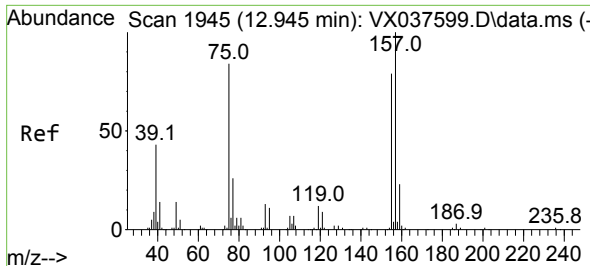

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.494 ug/l
RT: 12.957 min Scan# 1947
Delta R.T. 0.012 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 388
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 0.0 44.9 134.7#

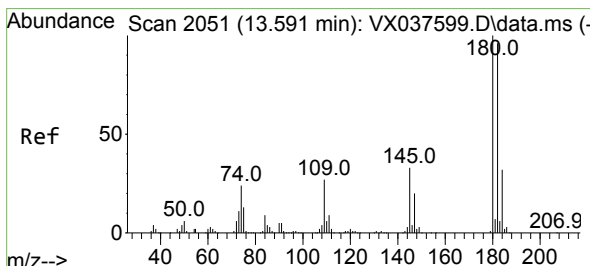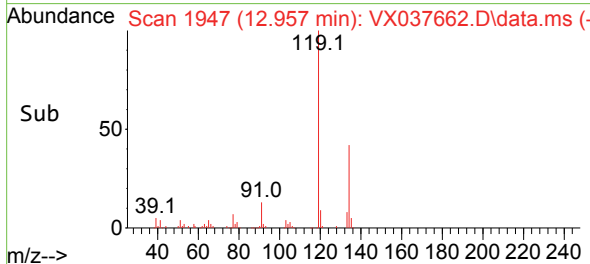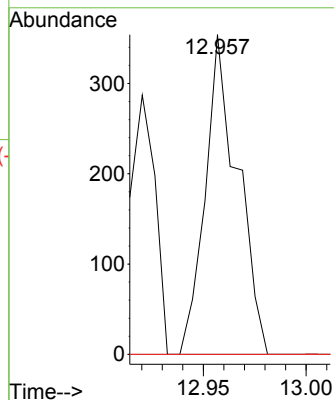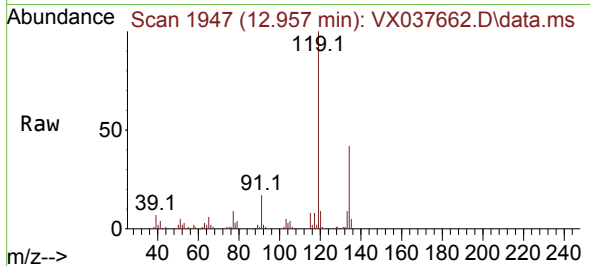

#93
1,2,4-Trichlorobenzene
Concen: 0.262 ug/l
RT: 13.585 min Scan# 2050
Delta R.T. -0.006 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33


Tgt Ion: 180 Resp: 726
Ion Ratio Lower Upper
180 100
182 85.7 48.3 144.8
145 95.7 18.0 54.0#

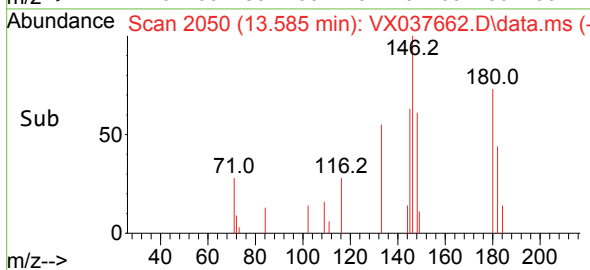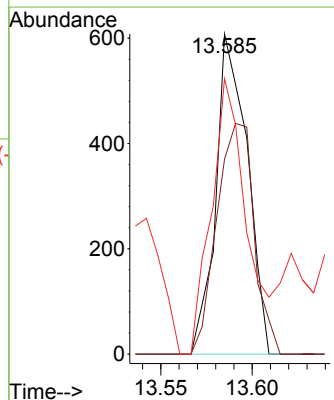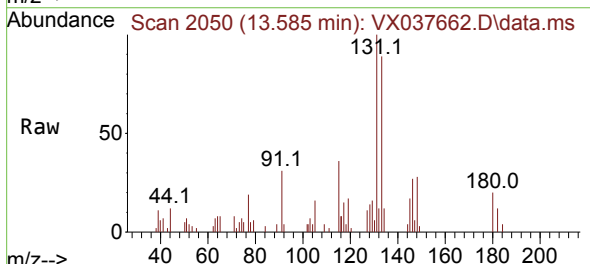



#95
Naphthalene
Concen: 15.843 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX037662.D
Acq: 12 Sep 2023 12:33

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion:128 Resp: 158916
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 10.9 8.8 13.2

