

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037661.D
Acq On : 12 Sep 2023 12:09
Operator : JC/MD
Sample : 04327-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-9.5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	68	83	87	rBV9	17760	84518	9.20%	1.706%
2	2.941	296	304	317	rVB	8034	19460	2.12%	0.393%
3	4.587	564	574	590	rVB	13977	48913	5.32%	0.987%
4	5.385	694	705	721	rBV	100649	297704	32.40%	6.009%
5	5.550	721	732	745	rBV	182436	519080	56.49%	10.477%
6	5.958	788	799	813	rBV	114464	312974	34.06%	6.317%
7	6.763	921	931	944	rBV	271741	670807	73.00%	13.540%
8	8.647	1233	1240	1249	rBV	581135	918931	100.00%	18.548%
9	10.055	1465	1471	1486	rBV	594304	800576	87.12%	16.159%
10	11.079	1634	1639	1650	rBV	455557	581907	63.32%	11.745%
11	12.018	1788	1793	1807	rVB	533969	699487	76.12%	14.119%




Sum of corrected areas: 4954357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037661.D
Acq On : 12 Sep 2023 12:09
Operator : JC/MD
Sample : 04327-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-9.5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

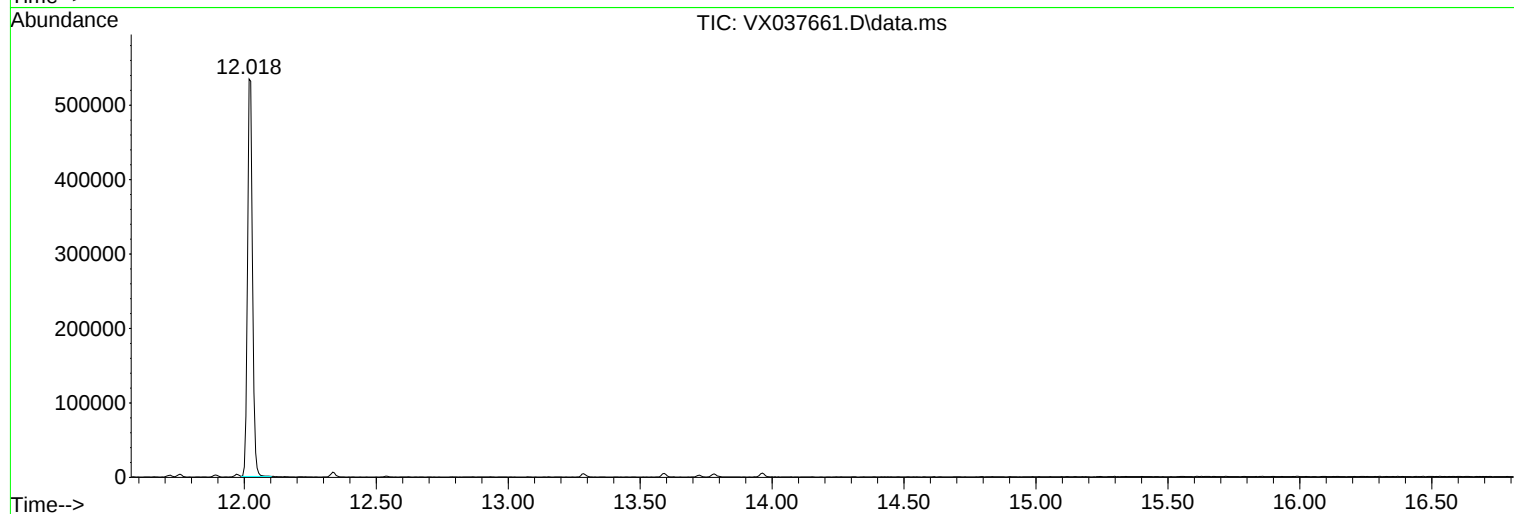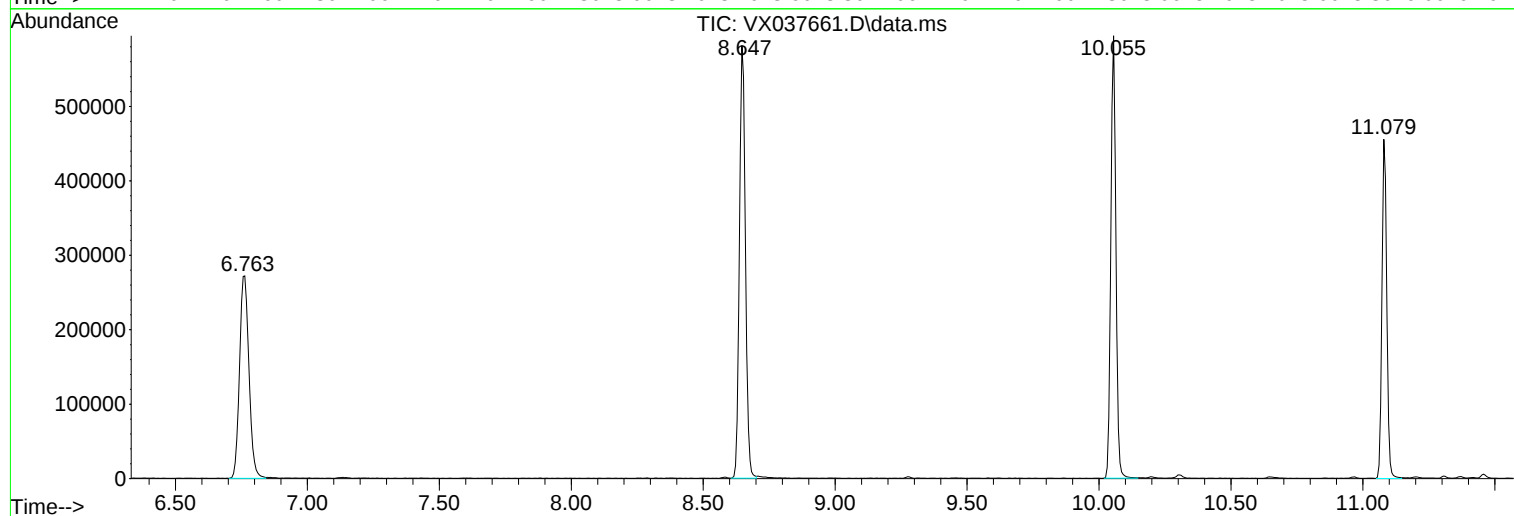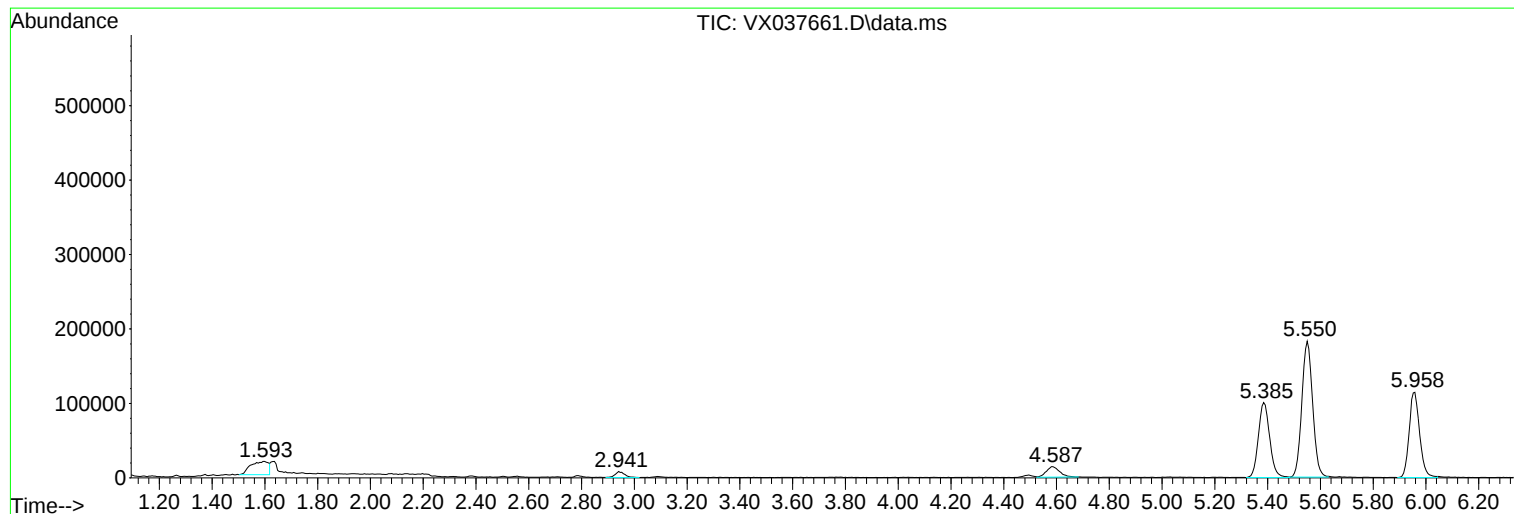

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037661.D
Acq On : 12 Sep 2023 12:09
Operator : JC/MD
Sample : 04327-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-9.5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.593 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.593	8.14 ug/l	84518	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxalyl chloride	126	C2Cl2O2	000079-37-8	32
2			Methylene chloride	84	CH2Cl2	000075-09-2	10
3			bis(chloromethyl) carbonate	158	C3H4Cl2O3	1000404-37-0	10
4			Methane, bromochloro-	128	CH2BrCl	000074-97-5	10
5			2-Chloroethyl methyl sulfone	142	C3H7ClO2S	050890-51-2	9

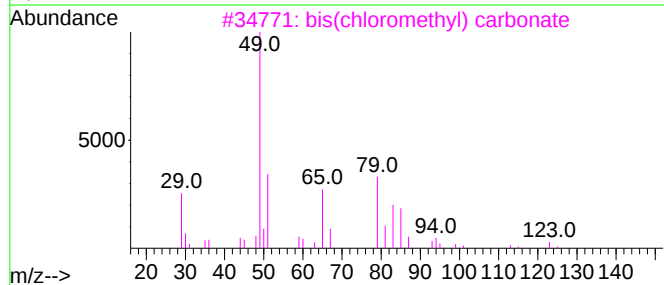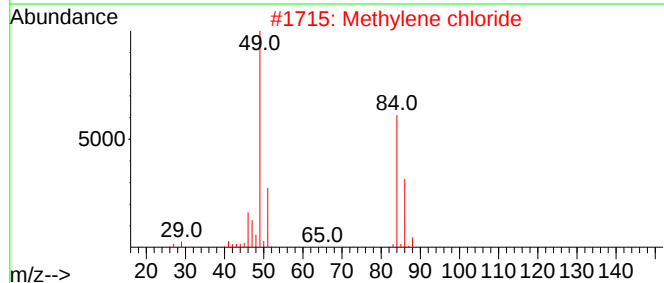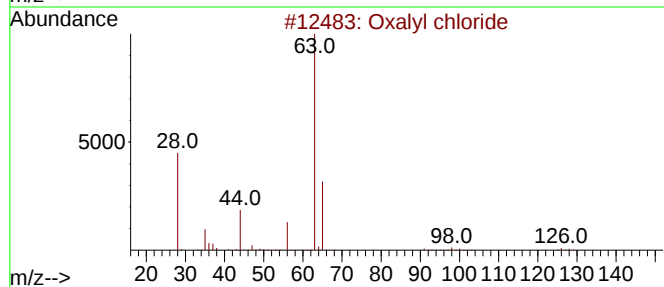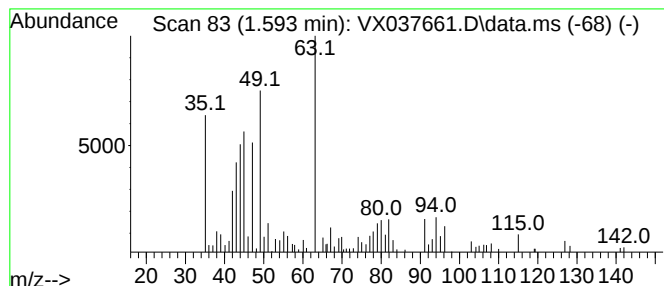

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037661.D
Acq On : 12 Sep 2023 12:09
Operator : JC/MD
Sample : 04327-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-9.5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.593	1.593	8.1	ug/l	84518	1	5.550	519080	50.0