

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091223\  
 Data File : VX037665.D  
 Acq On : 12 Sep 2023 13:46  
 Operator : JC/MD  
 Sample : 04297-04  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 1731-DRIP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
 Title : SW846 8260

Signal : TIC: VX037665.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.557       | 66            | 77          | 78           | rBV3     | 22285          | 49612         | 4.83%           | 0.889%        |
| 2         | 2.380       | 206           | 212         | 223          | rVV      | 28828          | 48489         | 4.72%           | 0.869%        |
| 3         | 2.965       | 298           | 308         | 316          | rBV2     | 4545           | 10785         | 1.05%           | 0.193%        |
| 4         | 4.239       | 507           | 517         | 525          | rBV4     | 5560           | 16443         | 1.60%           | 0.295%        |
| 5         | 4.580       | 565           | 573         | 580          | rBV2     | 3567           | 11074         | 1.08%           | 0.198%        |
| 6         | 5.385       | 693           | 705         | 721          | rBV      | 116348         | 340341        | 33.11%          | 6.100%        |
| 7         | 5.550       | 721           | 732         | 748          | rVB      | 201701         | 573804        | 55.82%          | 10.285%       |
| 8         | 5.958       | 788           | 799         | 824          | rBV      | 132071         | 356518        | 34.68%          | 6.390%        |
| 9         | 6.763       | 921           | 931         | 949          | rBV      | 320029         | 753671        | 73.32%          | 13.509%       |
| 10        | 8.647       | 1234          | 1240        | 1251         | rBV      | 648527         | 1027976       | 100.00%         | 18.425%       |
| 11        | 9.031       | 1297          | 1303        | 1313         | rBV      | 11257          | 20746         | 2.02%           | 0.372%        |
| 12        | 10.055      | 1465          | 1471        | 1484         | rBV      | 671331         | 902911        | 87.83%          | 16.184%       |
| 13        | 11.079      | 1634          | 1639        | 1647         | rBV      | 527320         | 664288        | 64.62%          | 11.907%       |
| 14        | 12.024      | 1788          | 1794        | 1802         | rBV      | 625842         | 802531        | 78.07%          | 14.384%       |




Sum of corrected areas: 5579189

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091223\  
Data File : VX037665.D  
Acq On : 12 Sep 2023 13:46  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

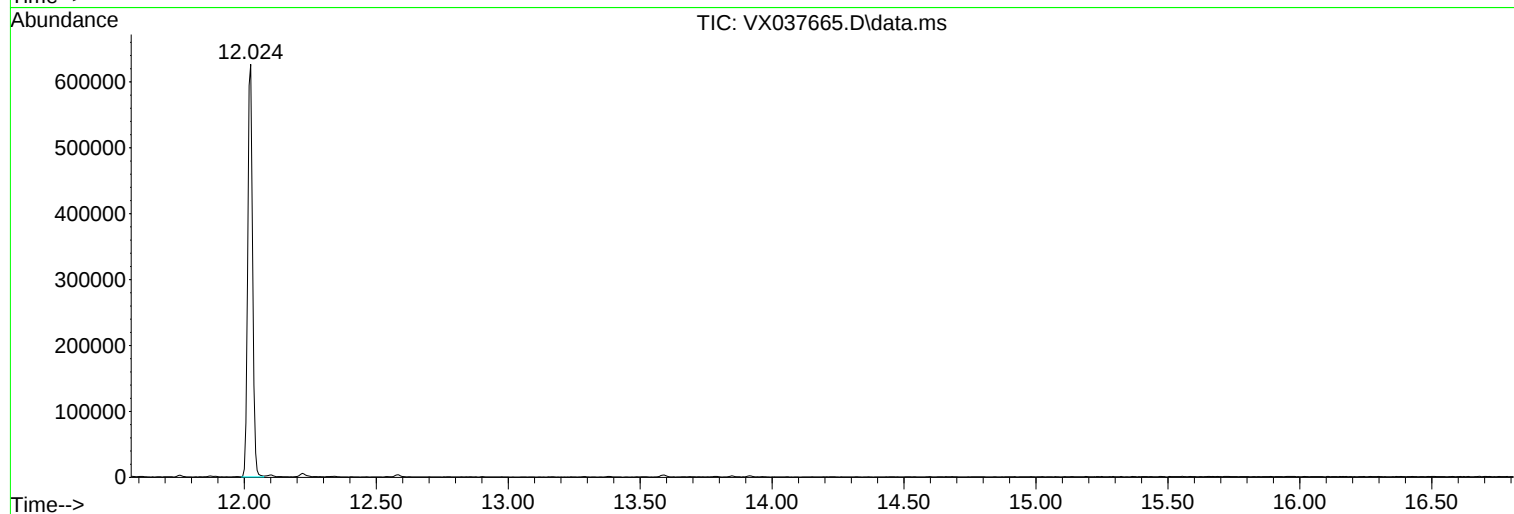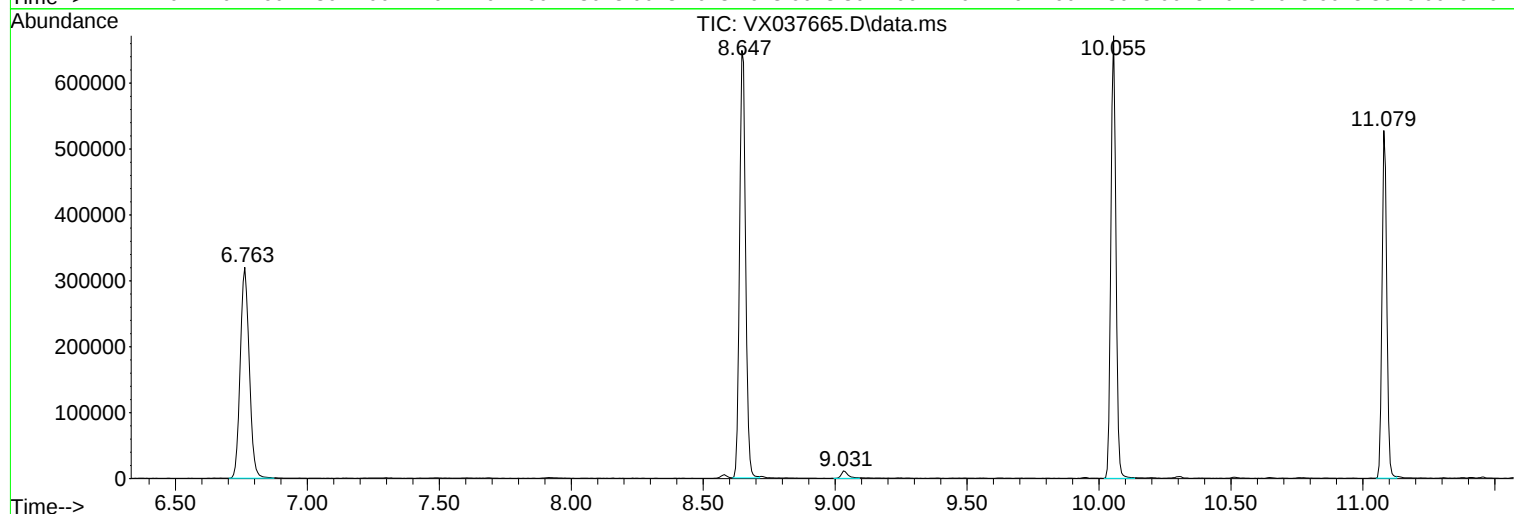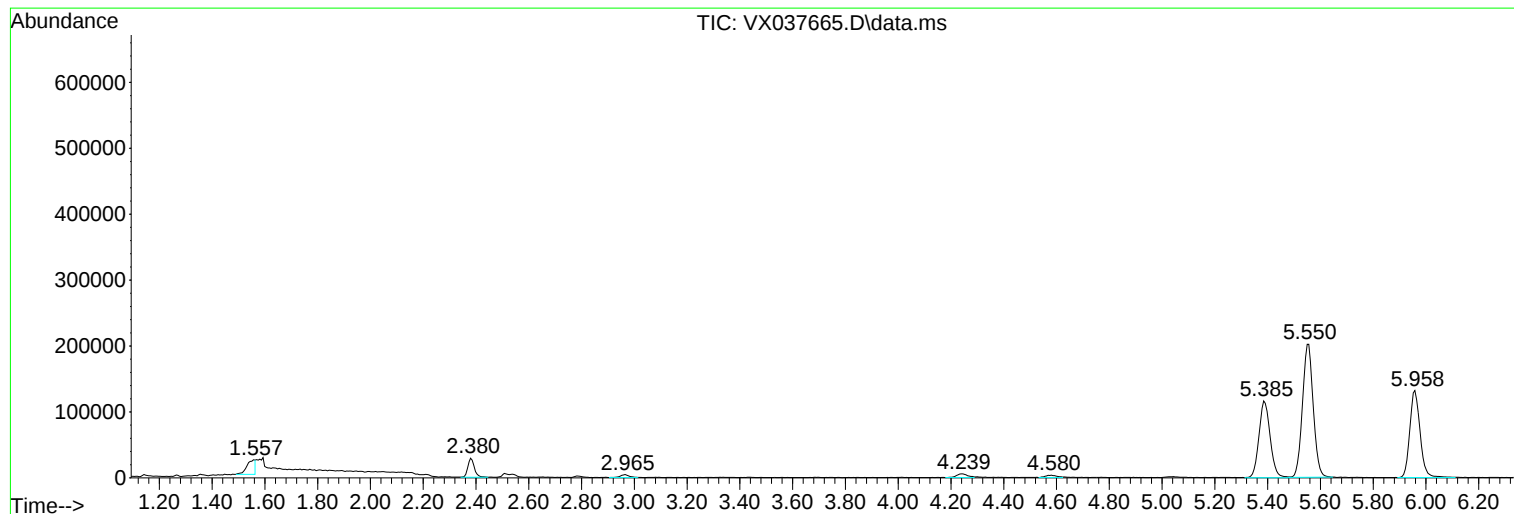

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091223\  
Data File : VX037665.D  
Acq On : 12 Sep 2023 13:46  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091223\  
Data File : VX037665.D  
Acq On : 12 Sep 2023 13:46  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|