

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
 Data File : VX037673.D
 Acq On : 12 Sep 2023 17:02
 Operator : JC/MD
 Sample : 04394-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB9/8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	68	80	81	rBV4	15205	45620	4.08%	0.738%
2	2.940	295	304	316	rBV2	12389	30463	2.73%	0.493%
3	3.440	377	386	400	rBV	110492	247058	22.11%	3.995%
4	5.385	695	705	719	rBV2	126989	369869	33.10%	5.981%
5	5.550	721	732	747	rVB	210315	600908	53.77%	9.718%
6	5.952	789	798	820	rBV	146847	397612	35.58%	6.430%
7	6.763	920	931	945	rBV	342972	814600	72.89%	13.173%
8	8.647	1234	1240	1256	rBV	692490	1117549	100.00%	18.073%
9	9.275	1337	1343	1351	rVB2	26784	39087	3.50%	0.632%
10	10.055	1465	1471	1489	rBV	724672	976346	87.36%	15.789%
11	11.079	1634	1639	1654	rBV	546364	711829	63.70%	11.511%
12	12.024	1788	1794	1805	rBV	660953	832693	74.51%	13.466%




Sum of corrected areas: 6183634

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037673.D
Acq On : 12 Sep 2023 17:02
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

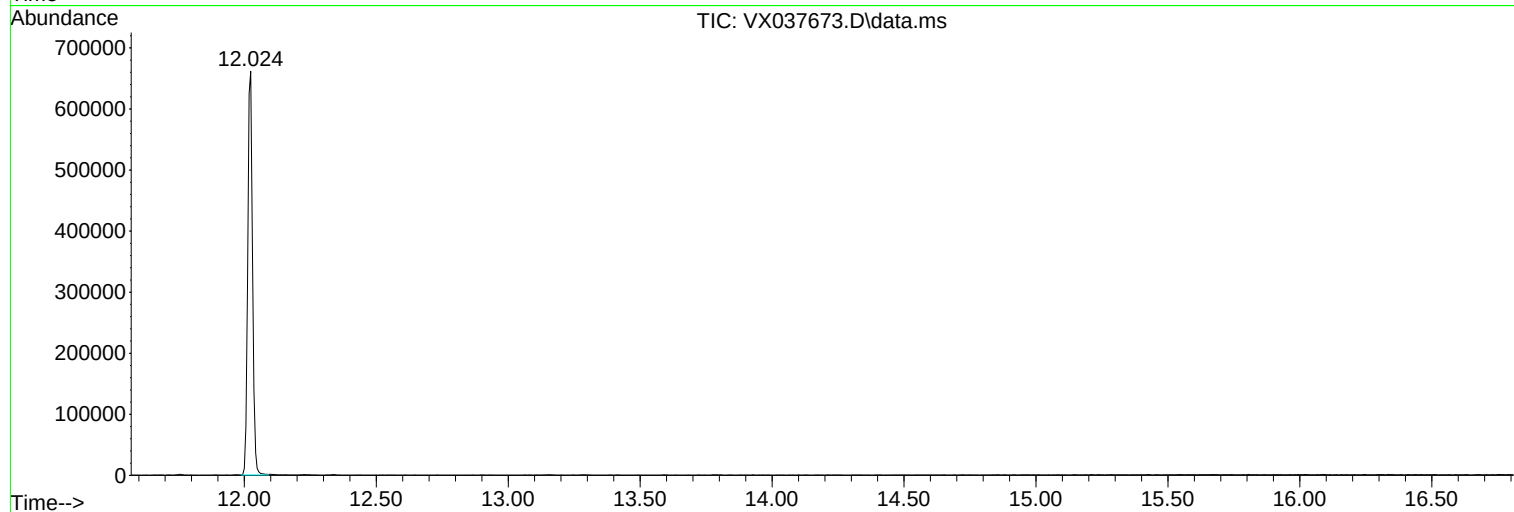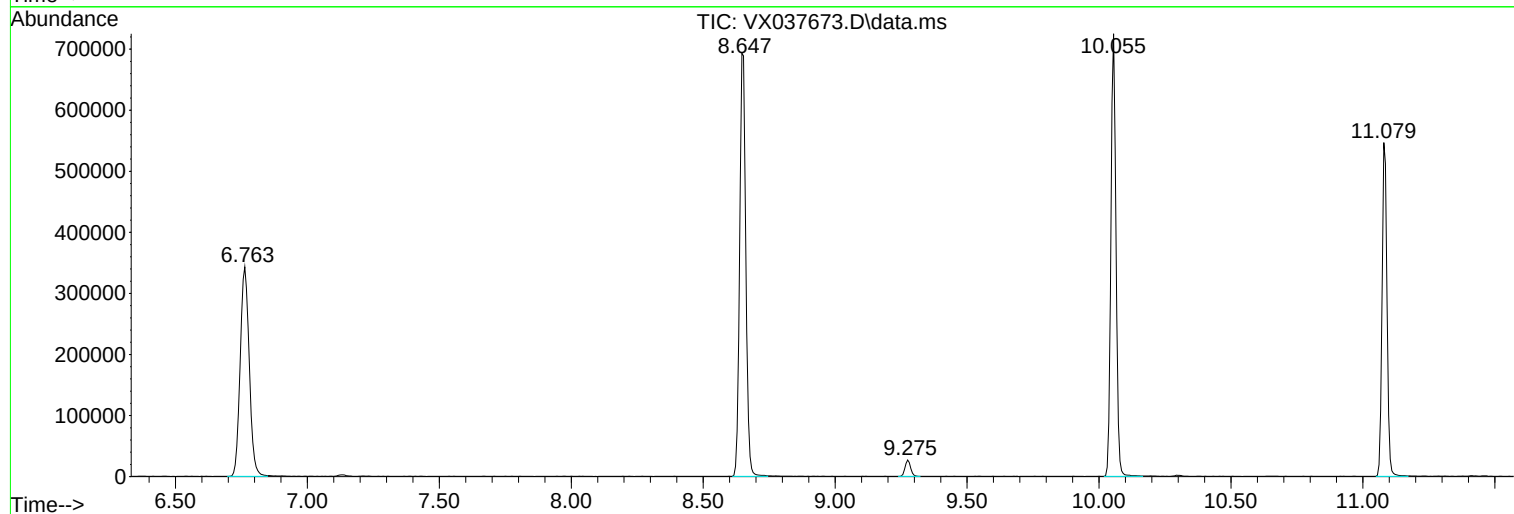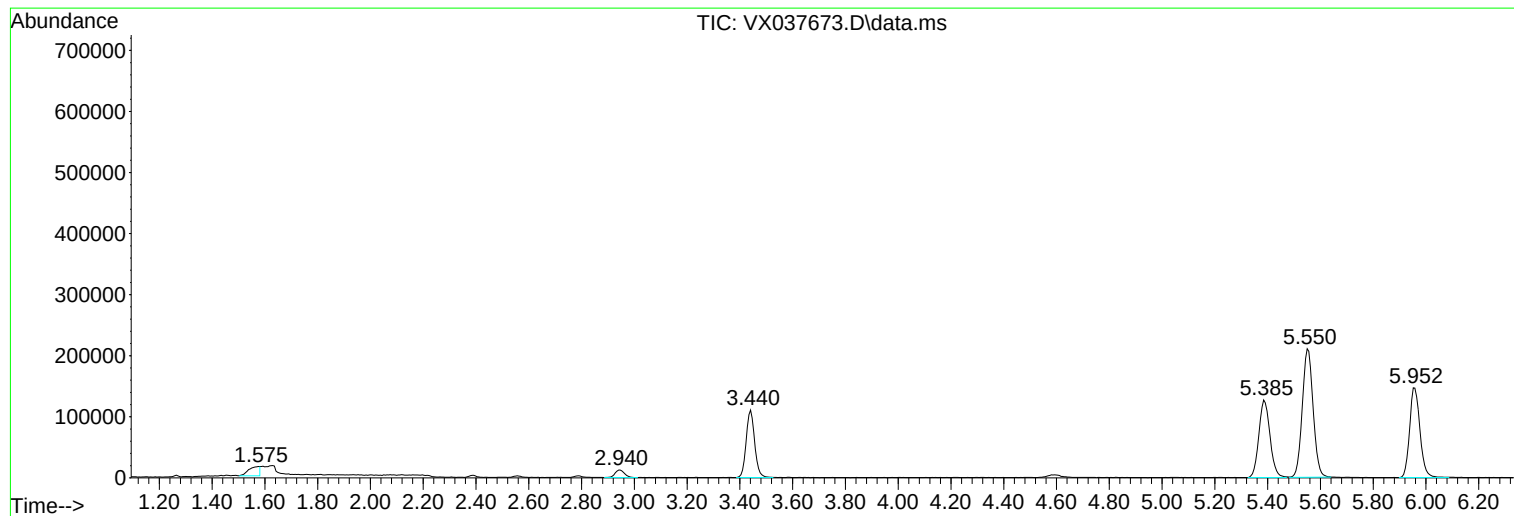

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037673.D
Acq On : 12 Sep 2023 17:02
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.440	20.56 ug/l	247058	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Hexane	86	C6H14	000110-54-3	91
2			2-Ethyl-oxetane	86	C5H10O	1010386-40-2	83
3			Pentane, 2,2,3,4-tetramethyl-	128	C9H20	001186-53-4	50
4			Propanal, 2,2-dimethyl-	86	C5H10O	000630-19-3	38
5			Hydroperoxide, hexyl	118	C6H14O2	004312-76-9	38

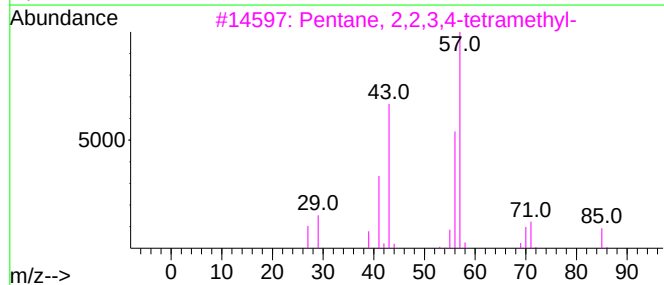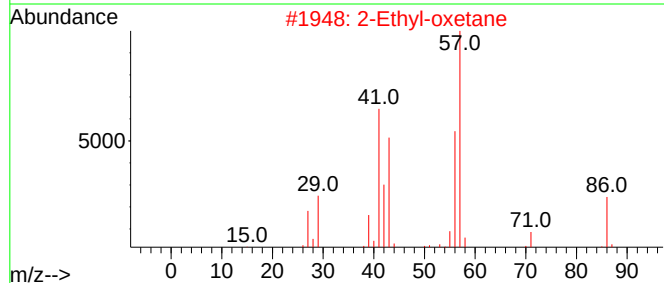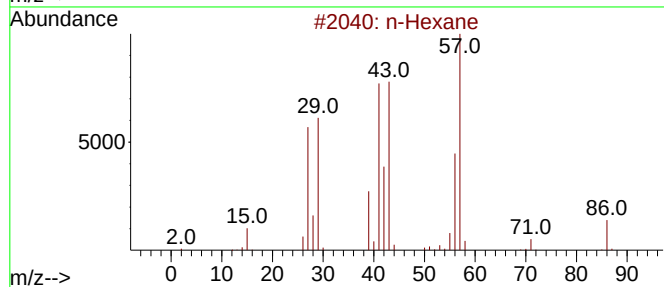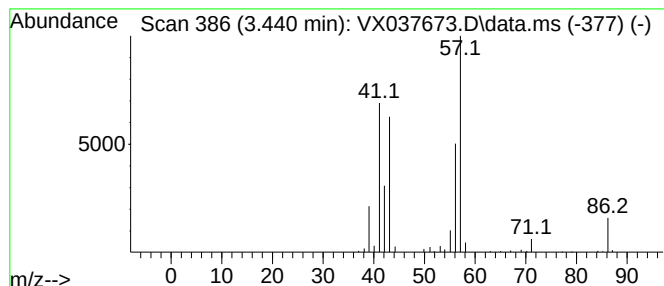

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037673.D
Acq On : 12 Sep 2023 17:02
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexane	3.440	20.6	ug/l	247058	1	5.550	600908	50.0