

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
 Data File : VX037674.D
 Acq On : 12 Sep 2023 17:26
 Operator : JC/MD
 Sample : 04394-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	70	79	86	rBV3	12064	29248	2.65%	0.452%
2	2.538	231	238	249	rVB	8459	17483	1.58%	0.270%
3	2.788	273	279	290	rVB3	7056	14109	1.28%	0.218%
4	3.446	373	387	401	rBV	358046	795771	72.08%	12.292%
5	5.391	694	706	721	rBV	128190	370571	33.57%	5.724%
6	5.556	721	733	746	rVV	215021	612649	55.49%	9.463%
7	5.958	789	799	815	rBV	146319	388201	35.16%	5.996%
8	6.763	921	931	955	rBV	339149	810097	73.38%	12.513%
9	8.653	1234	1241	1253	rBV	695977	1104010	100.00%	17.053%
10	10.055	1465	1471	1484	rBV	685373	924969	83.78%	14.288%
11	11.079	1634	1639	1650	rBV	497514	656000	59.42%	10.133%
12	12.024	1788	1794	1803	rBV	592405	750708	68.00%	11.596%




Sum of corrected areas: 6473816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037674.D
Acq On : 12 Sep 2023 17:26
Operator : JC/MD
Sample : 04394-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

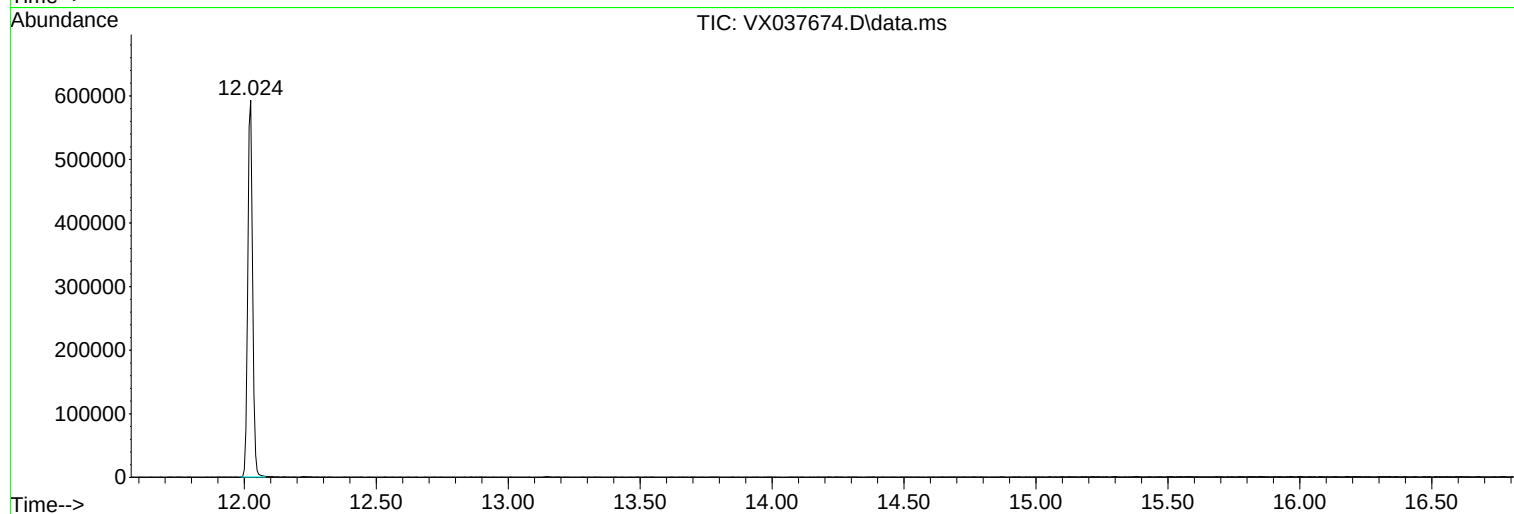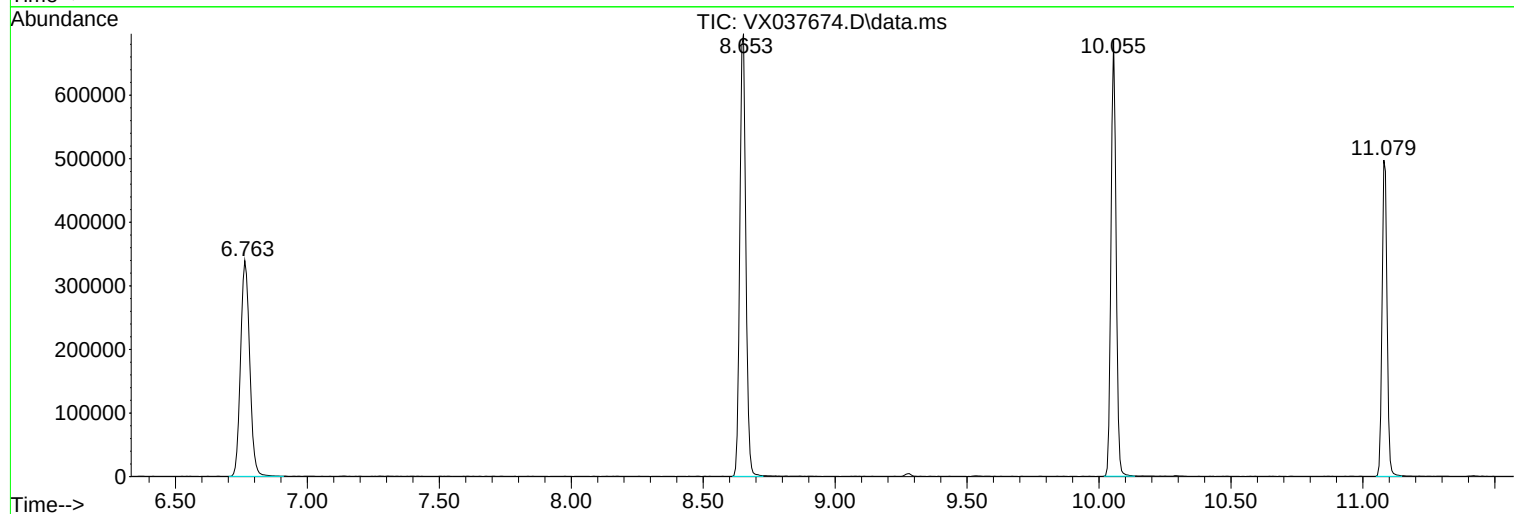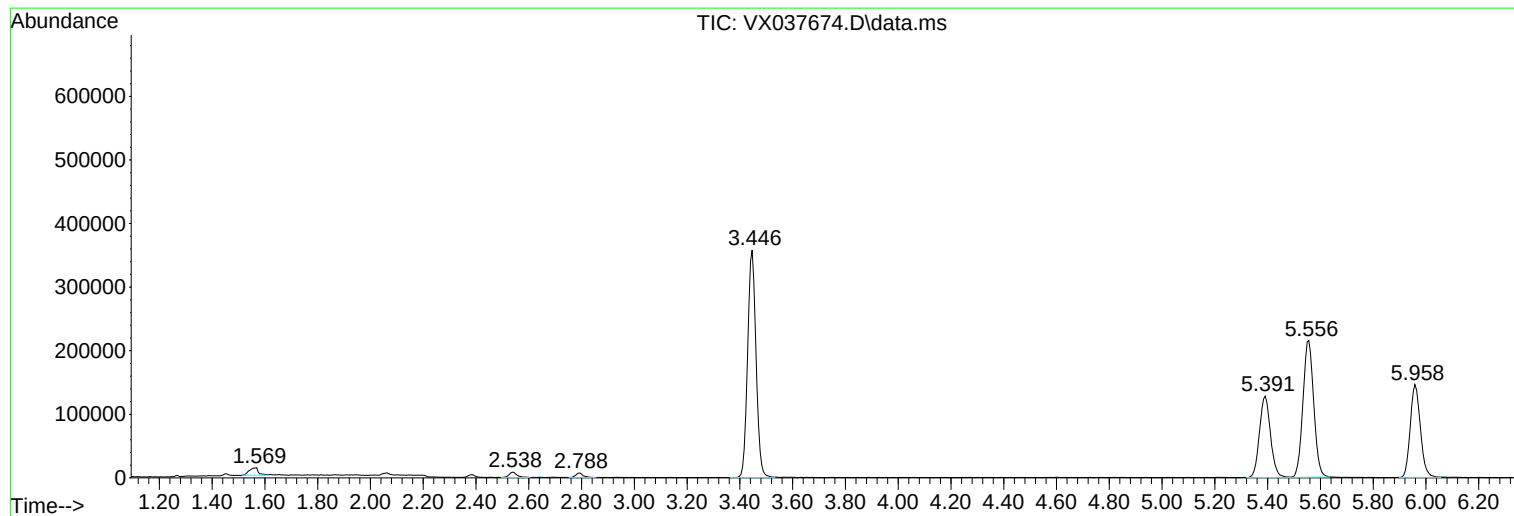

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037674.D
Acq On : 12 Sep 2023 17:26
Operator : JC/MD
Sample : 04394-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.446	64.95 ug/l	795771	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Hexane	86	C6H14	000110-54-3	91
2			2-Ethyl-oxetane	86	C5H10O	1010386-40-2	78
3			Furan, tetrahydro-3-methyl-	86	C5H10O	013423-15-9	47
4			Pentane, 2,2,3,4-tetramethyl-	128	C9H20	001186-53-4	40
5			Hydroperoxide, hexyl	118	C6H14O2	004312-76-9	38

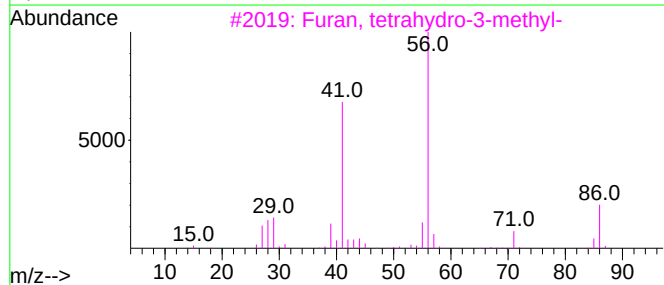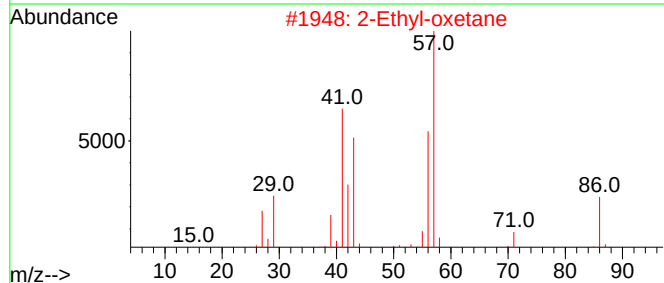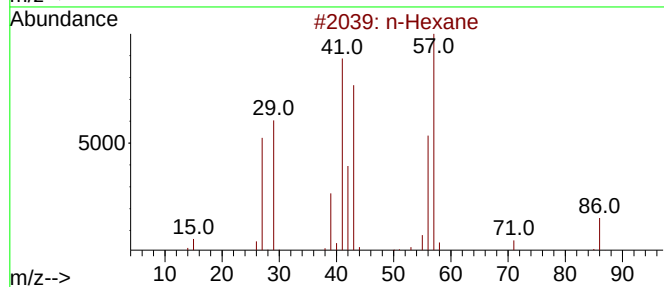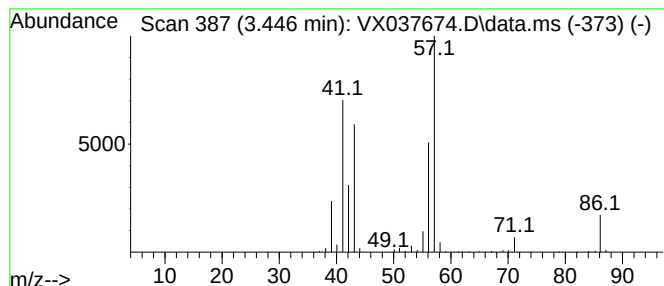

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091223\
Data File : VX037674.D
Acq On : 12 Sep 2023 17:26
Operator : JC/MD
Sample : 04394-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexane	3.446	65.0	ug/l	795771	1	5.556	612649	50.0