


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091318\
 Data File : VX004505.D
 Acq On : 13 Sep 2018 09:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
 Title : SW846 8260
 Last Update : Wed Sep 12 02:17:23 2018

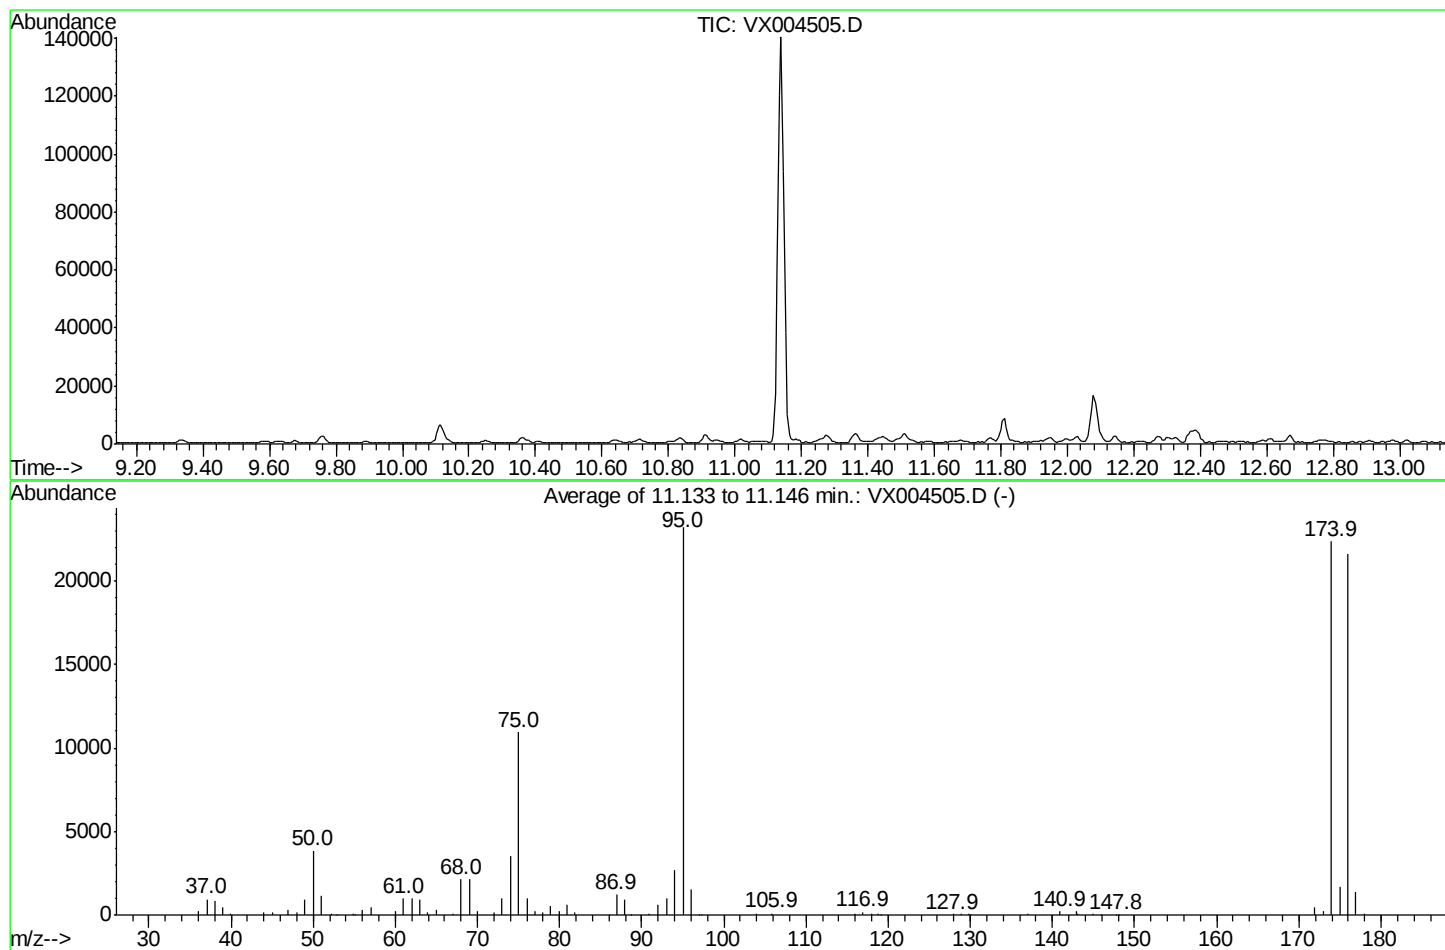

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	3850	PASS
75	95	30	60	47.2	10951	PASS
95	95	100	100	100.0	23205	PASS
96	95	5	9	6.7	1565	PASS
173	174	0.00	2	1.1	242	PASS
174	95	50	100	96.3	22352	PASS
175	174	5	9	7.7	1710	PASS
176	174	95	101	96.6	21600	PASS
177	176	5	9	6.2	1344	PASS