

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091319\
 Data File : VX012391.D
 Acq On : 13 Sep 2019 17:18
 Operator : SY/SP
 Sample : K4695-12
 Misc : 5.03g/5.0mL/MSVOA X/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T5-3-(2.5)

Quant Time: Sep 14 00:42:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 10 12:55:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	152189	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	256628	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	223004	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	96936	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	94222	43.79	ug/l	0.00
Spiked Amount			Recovery	=	87.58%	
35) Dibromofluoromethane	5.49	113	73202	44.50	ug/l	0.00
Spiked Amount			Recovery	=	89.00%	
50) Toluene-d8	8.71	98	303748	52.64	ug/l	0.00
Spiked Amount			Recovery	=	105.28%	
62) 4-Bromofluorobenzene	11.14	95	112123	41.92	ug/l	0.00
Spiked Amount			Recovery	=	83.84%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091319\
Data File : VX012391.D
Acq On : 13 Sep 2019 17:18
Operator : SY/SP
Sample : K4695-12
Misc : 5.03g/5.0mL/MSVOA X/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T5-3-(2.5)

Quant Time: Sep 14 00:42:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 10 12:55:26 2019
Response via : Initial Calibration

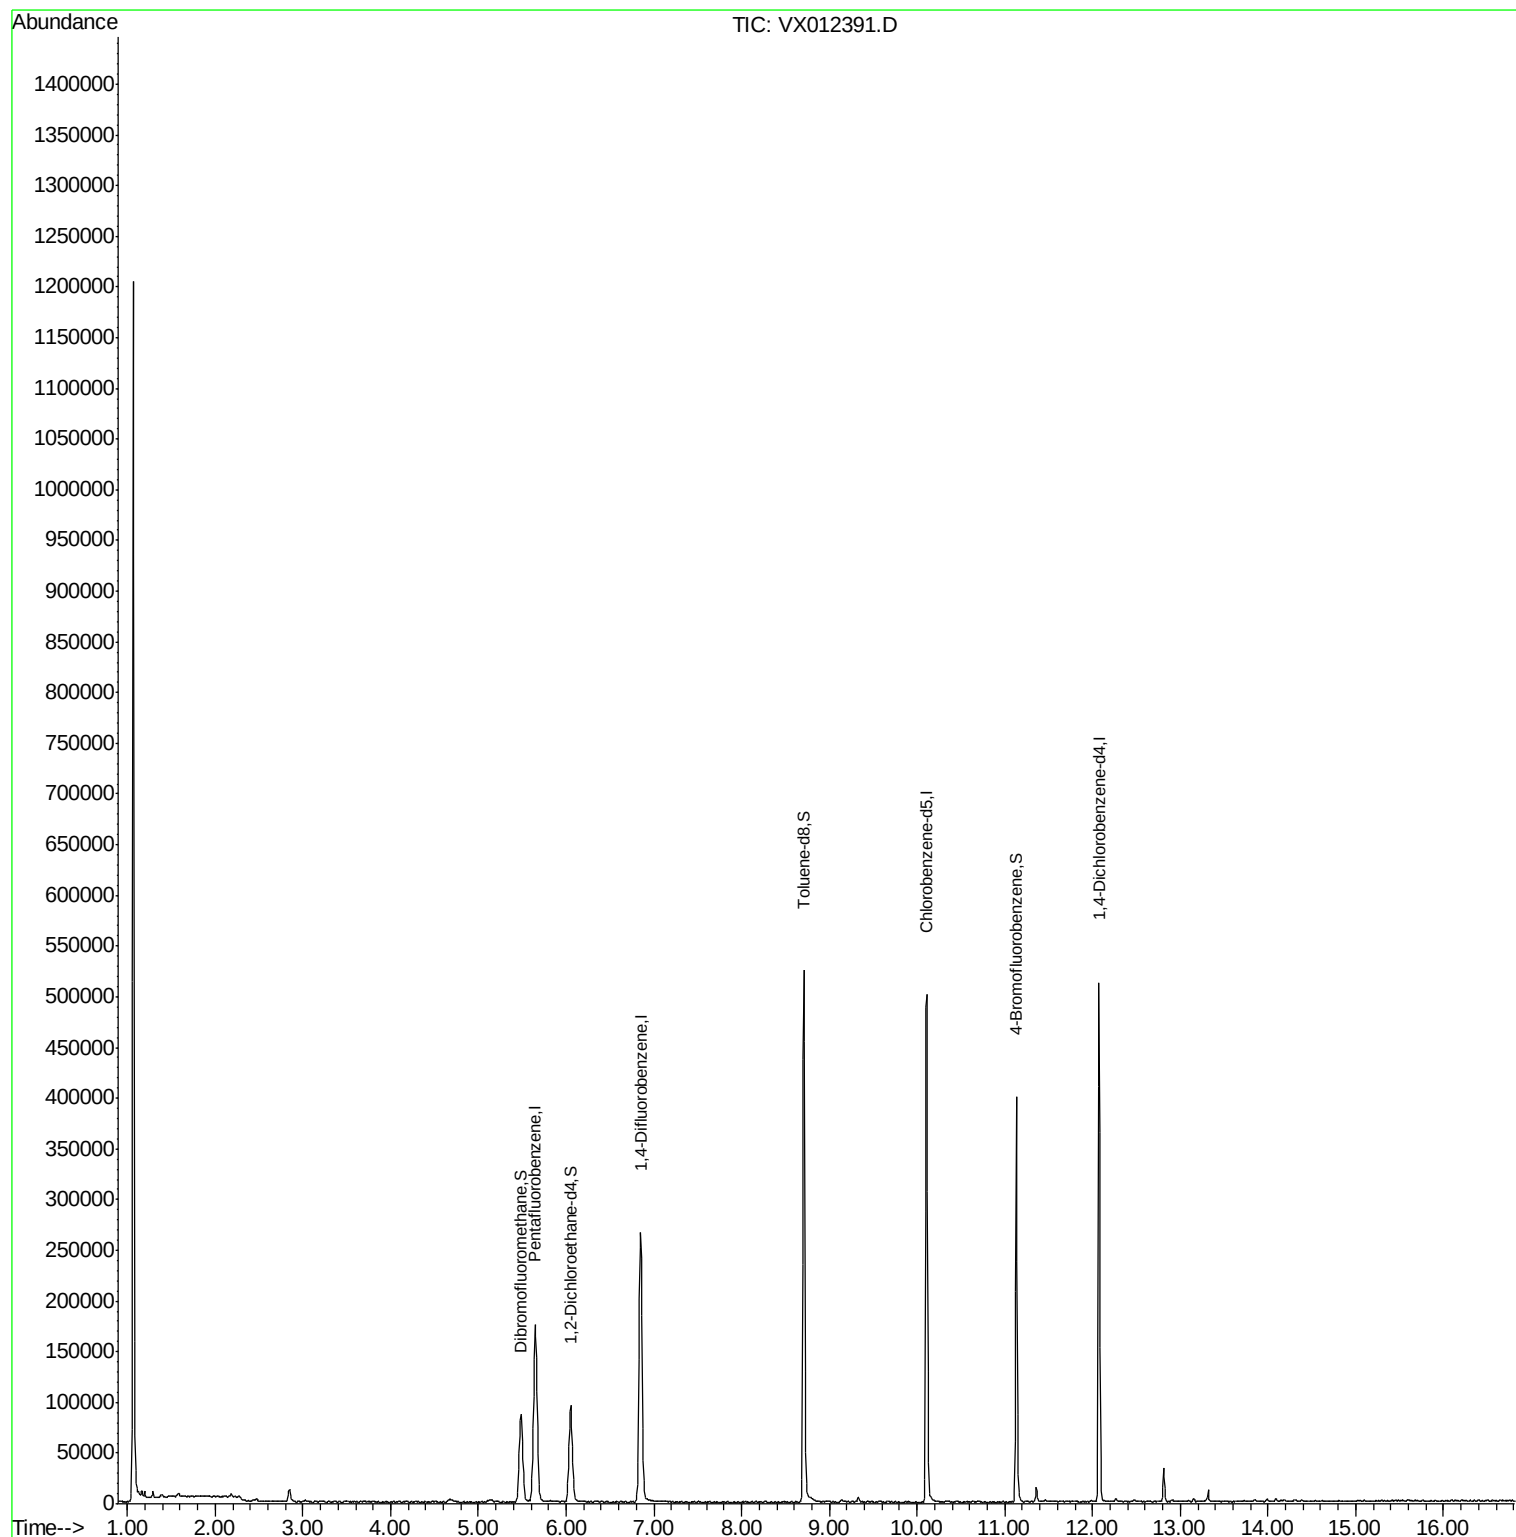

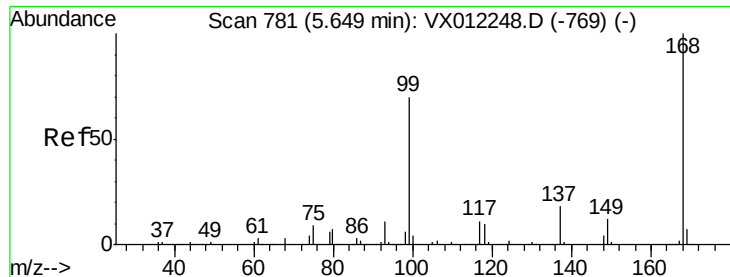

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX012391.D

Acq: 13 Sep 2019 17:18

Instrument :

MSVOA_X

ClientSampleId :


T5-3-(2.5)

Tot Ion:168 Resp: 152189

Ion Ratio Lower Upper

168 100

99 64.5 55.8 83.6

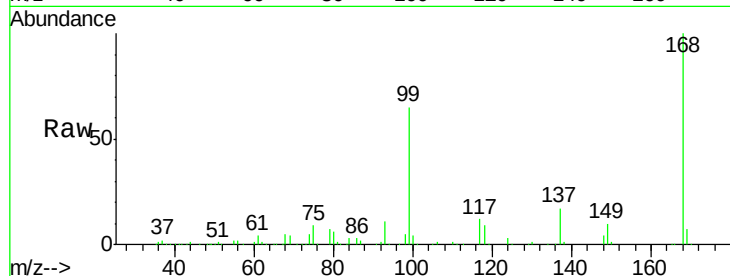

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

60000

50000

40000



30000

20000

10000

0

Time--> 5.50 5.60 5.70

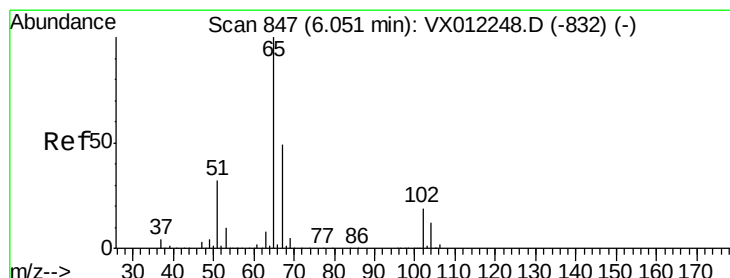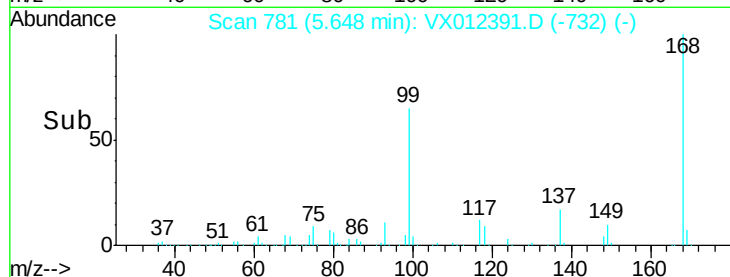

#33

1,2-Dichloroethane-d4

Concen: 43.790 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX012391.D


Acq: 13 Sep 2019 17:18

Tgt Ion: 65 Resp: 94222

Ion Ratio Lower Upper

65 100

67 50.5 0.0 99.8

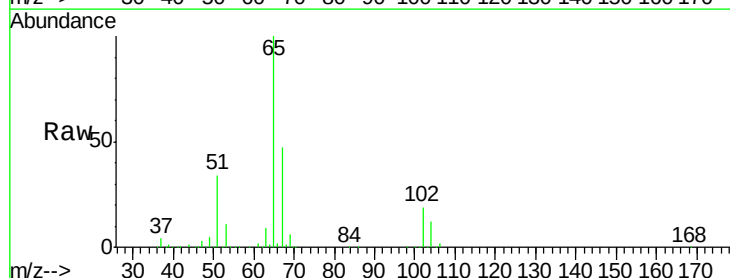

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05

40000


30000


20000

10000

0

Time--> 5.90 6.00 6.10 6.20




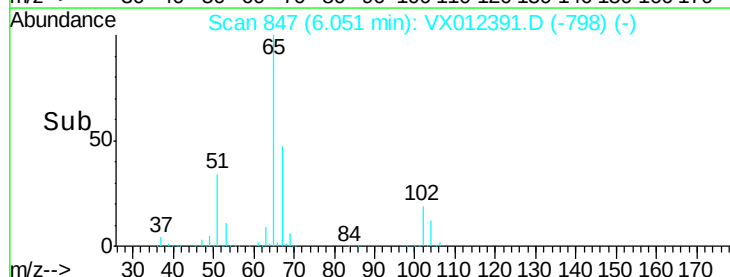


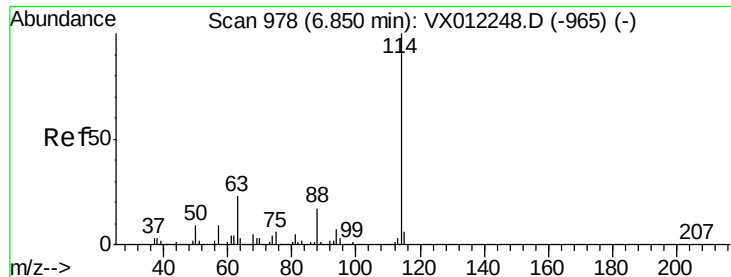

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. -0.00 min
 Lab File: VX012391.D
 Acq: 13 Sep 2019 17:18




Instrument :
 MSVOA_X
 ClientSampleId :
 T5-3-(2.5)


Tot Ion	Ratio	Lower	Upper
114	100		
63	22.7	0.0	45.2
88	17.4	0.0	34.8

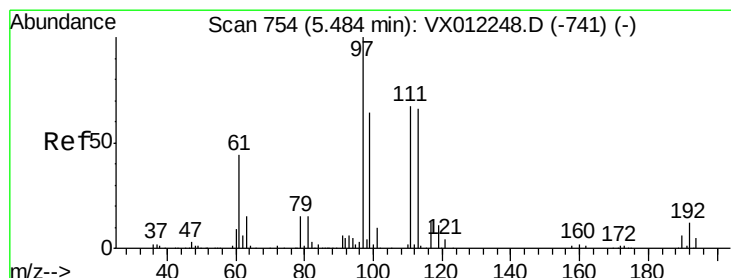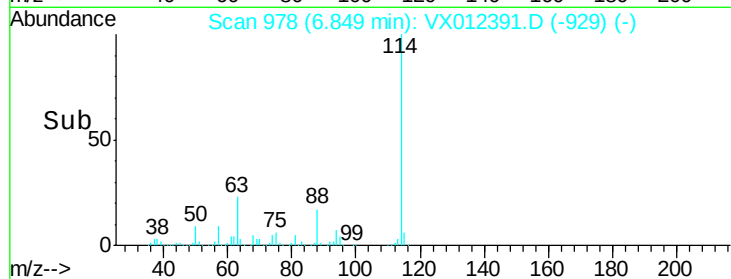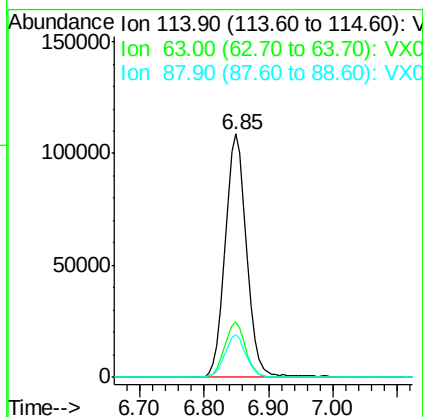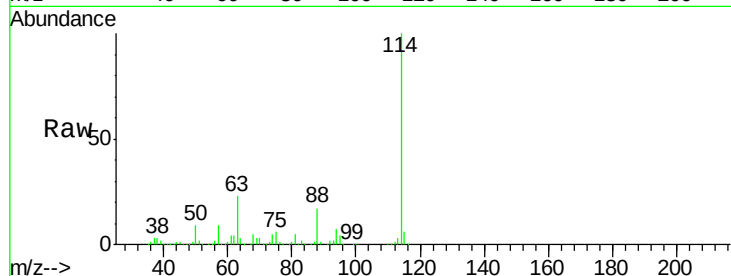

#35
 Dibromofluoromethane
 Concen: 44.497 ug/l
 RT: 5.49 min Scan# 755
 Delta R.T. 0.01 min
 Lab File: VX012391.D
 Acq: 13 Sep 2019 17:18

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.4	83.0	124.6
192	18.7	14.3	21.5


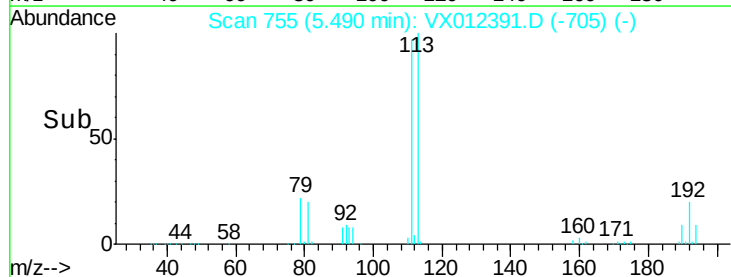
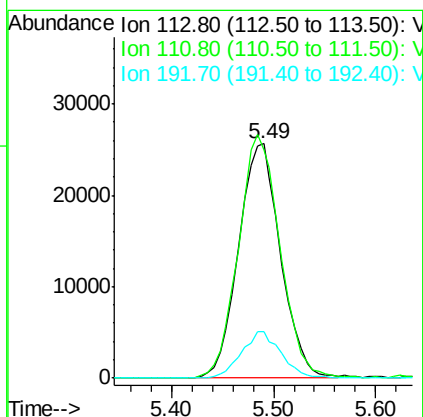
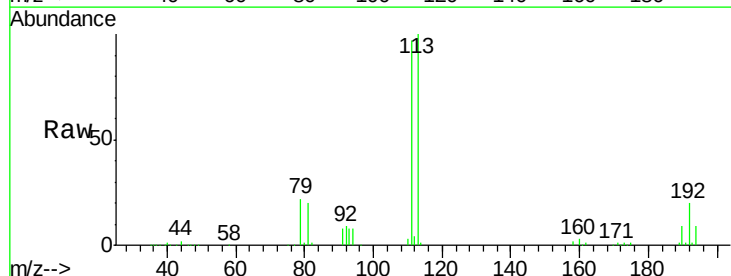


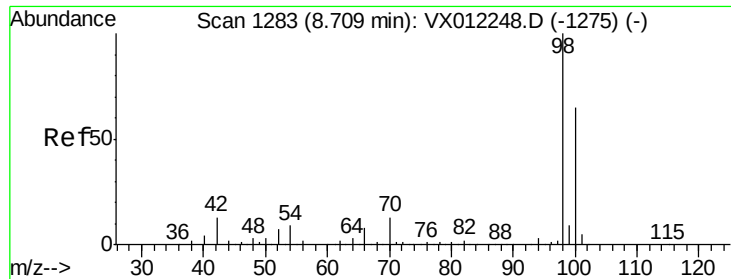

#50
Toluene-d8
Concen: 52.643 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX012391.D
Acq: 13 Sep 2019 17:18




Instrument :
MSVOA_X
ClientSampleId :
T5-3-(2.5)


Tot Ion: 98 Resp: 303748
Ion Ratio Lower Upper
98 100
100 67.1 54.1 81.1

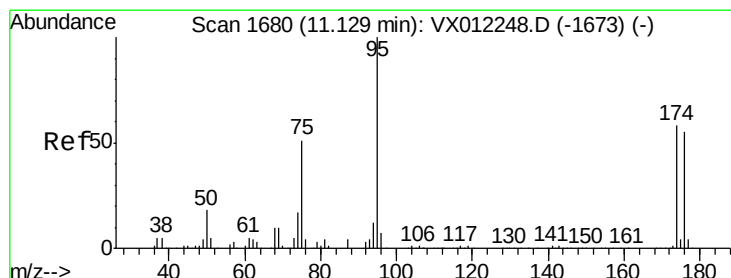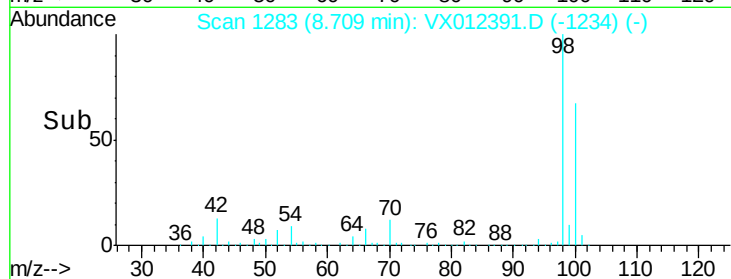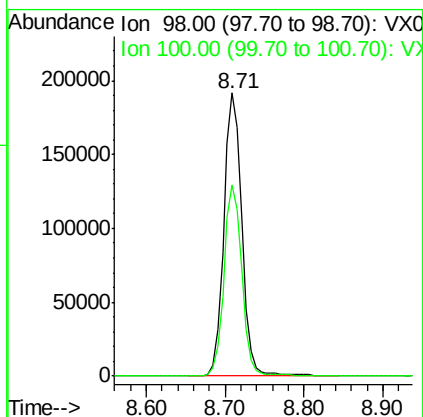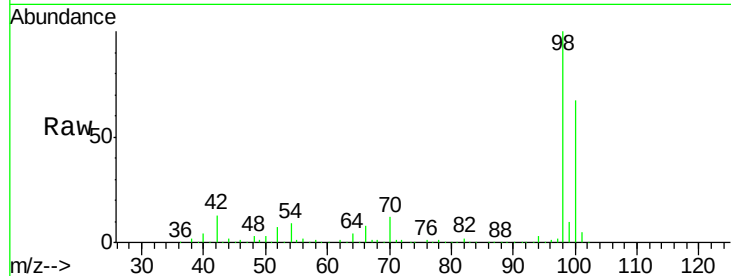

#62
4-Bromofluorobenzene
Concen: 41.916 ug/l
RT: 11.14 min Scan# 1681
Delta R.T. 0.01 min
Lab File: VX012391.D
Acq: 13 Sep 2019 17:18

Tgt Ion: 95 Resp: 112123
Ion Ratio Lower Upper
95 100
174 69.0 0.0 127.0
176 66.8 0.0 125.8


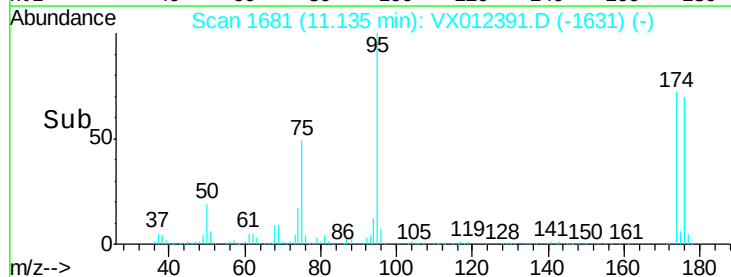
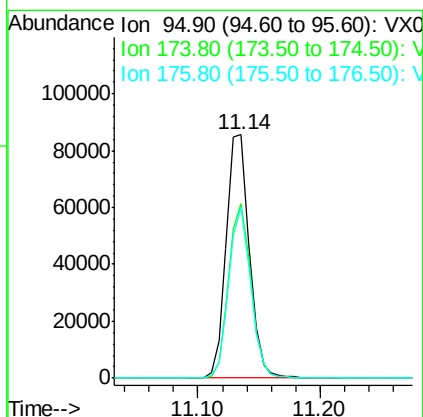
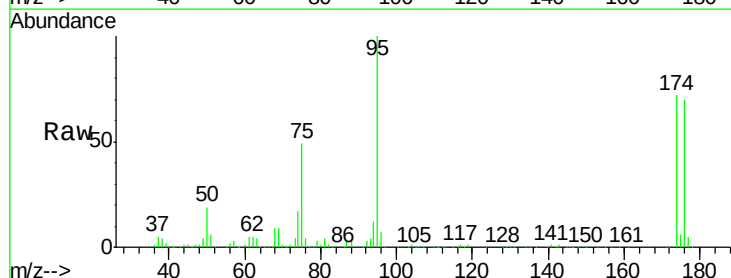


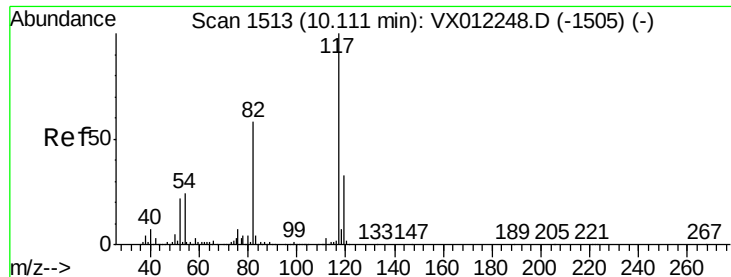

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX012391.D
Acq: 13 Sep 2019 17:18

Instrument :
MSVOA_X
ClientSampleId :
T5-3-(2.5)

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.1	46.4	69.6
119	32.3	26.6	39.8

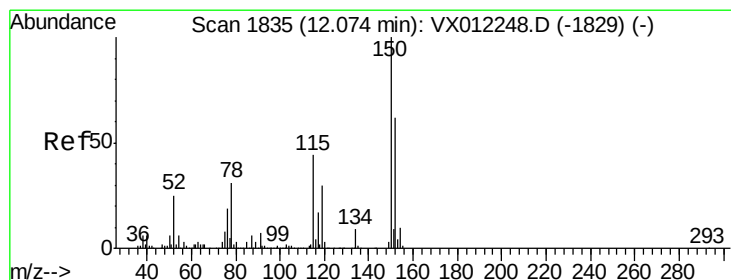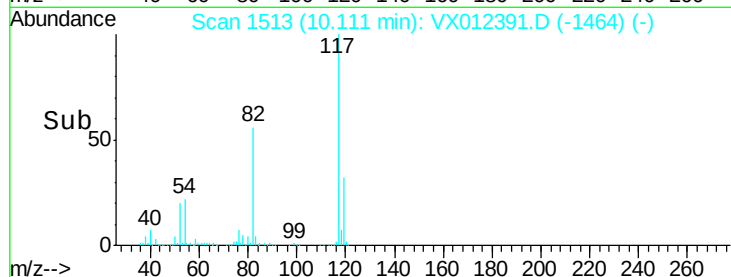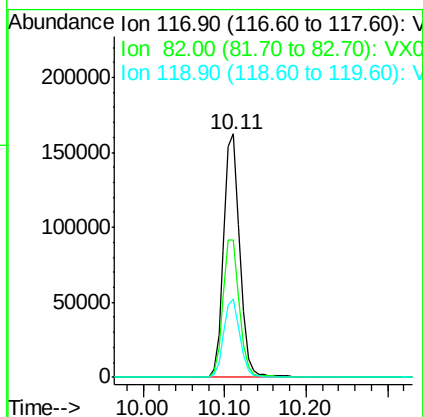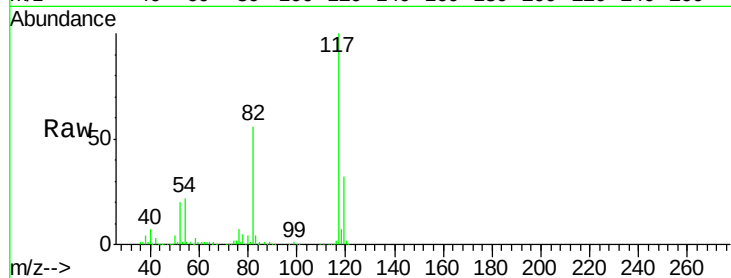

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX012391.D
Acq: 13 Sep 2019 17:18

Tgt Ion	Ratio	Lower	Upper
152	100		
115	62.6	45.5	136.4
150	157.0	0.0	346.4

