


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091319\  
Data File : VX012374.D  
Acq On : 13 Sep 2019 09:19  
Operator : SY/SP  
Sample : BFB  
Misc : 5.00µ/5.0mL/MSVOA X/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X091019S.M  
Title : SW846 8260  
Last Update : Tue Sep 10 12:55:26 2019

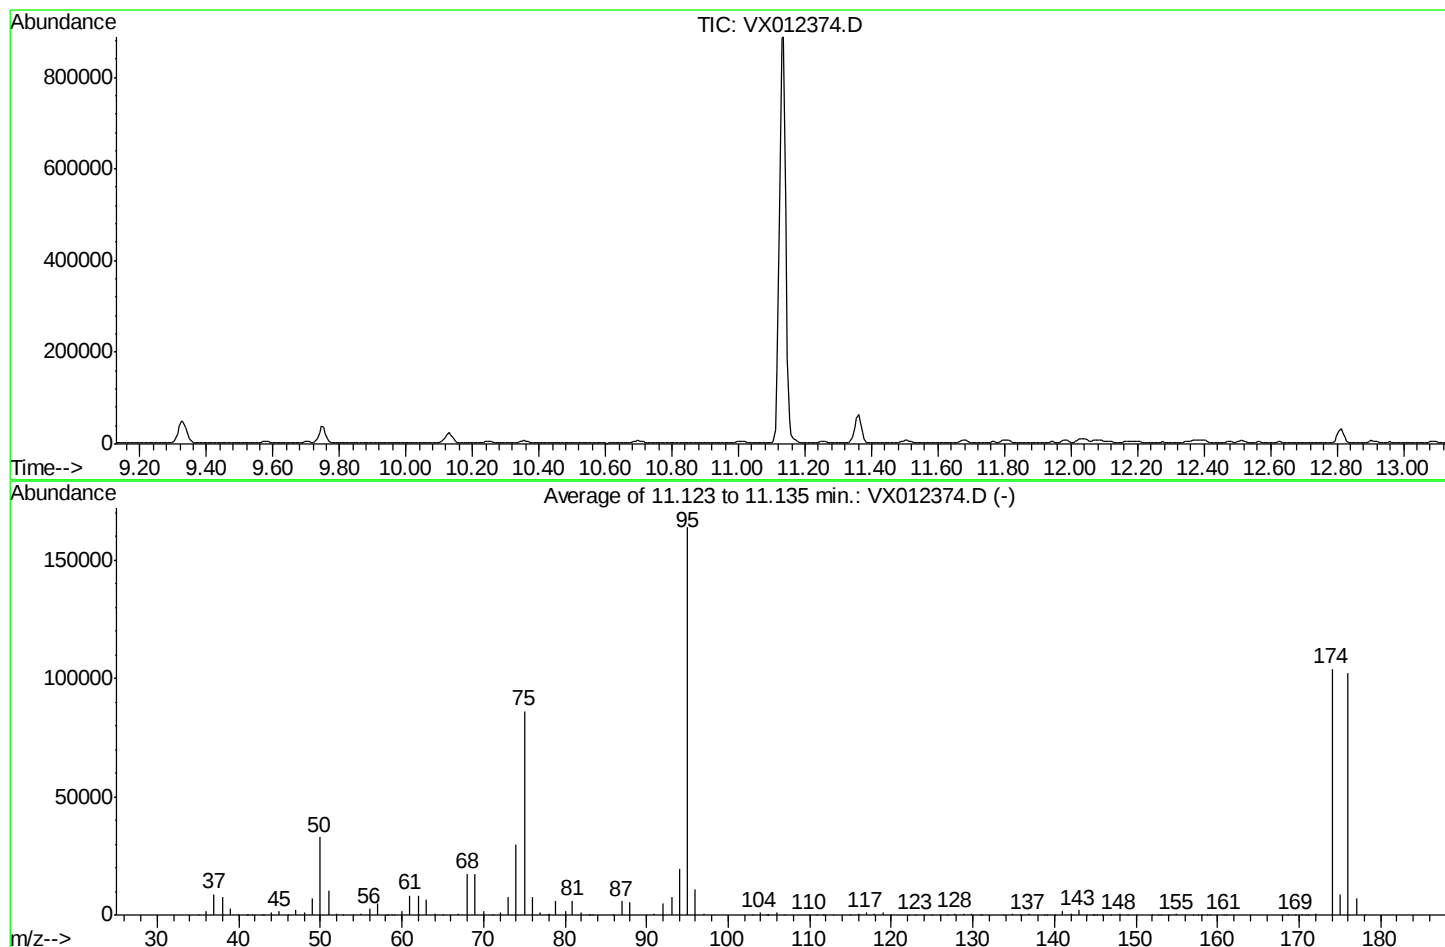

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.0      | 32824   | PASS             |
| 75          | 95           | 30           | 60           | 52.6      | 86269   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 163960  | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 11103   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 63.5      | 104069  | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 8421    | PASS             |
| 176         | 174          | 95           | 101          | 98.1      | 102101  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 6854    | PASS             |