


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091319\
Data File : VX012399.D
Acq On : 13 Sep 2019 21:27
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Title : SW846 8260
Last Update : Tue Sep 10 12:55:26 2019

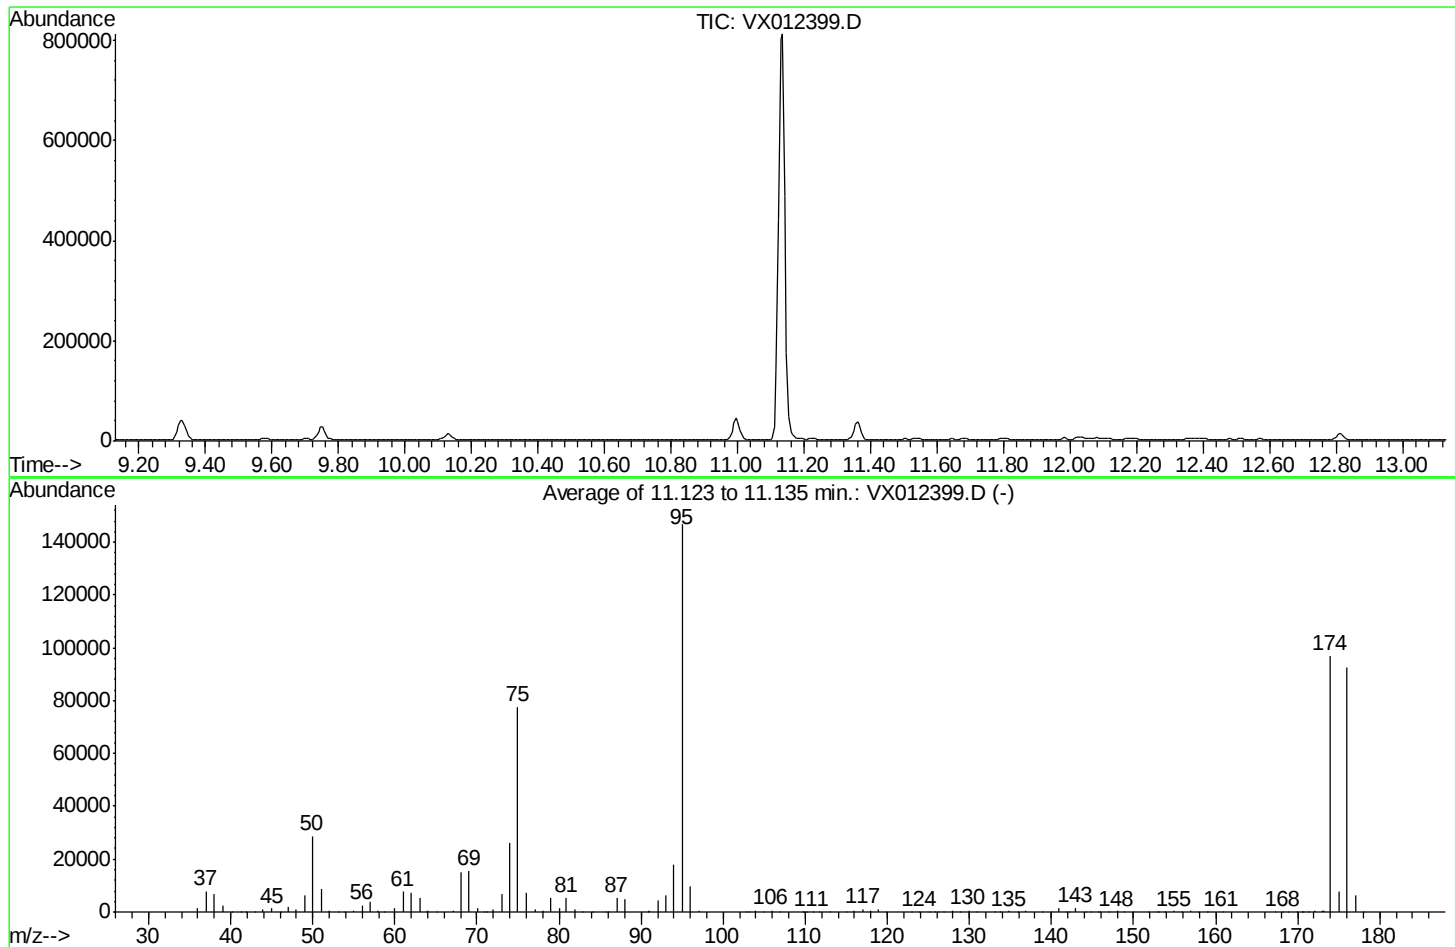

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	28684	PASS
75	95	30	60	53.0	77724	PASS
95	95	100	100	100.0	146744	PASS
96	95	5	9	6.6	9747	PASS
173	174	0.00	2	0.6	562	PASS
174	95	50	100	66.2	97085	PASS
175	174	5	9	7.9	7717	PASS
176	174	95	101	95.5	92677	PASS
177	176	5	9	6.7	6216	PASS