


Methylene Chloride

Response Ratio

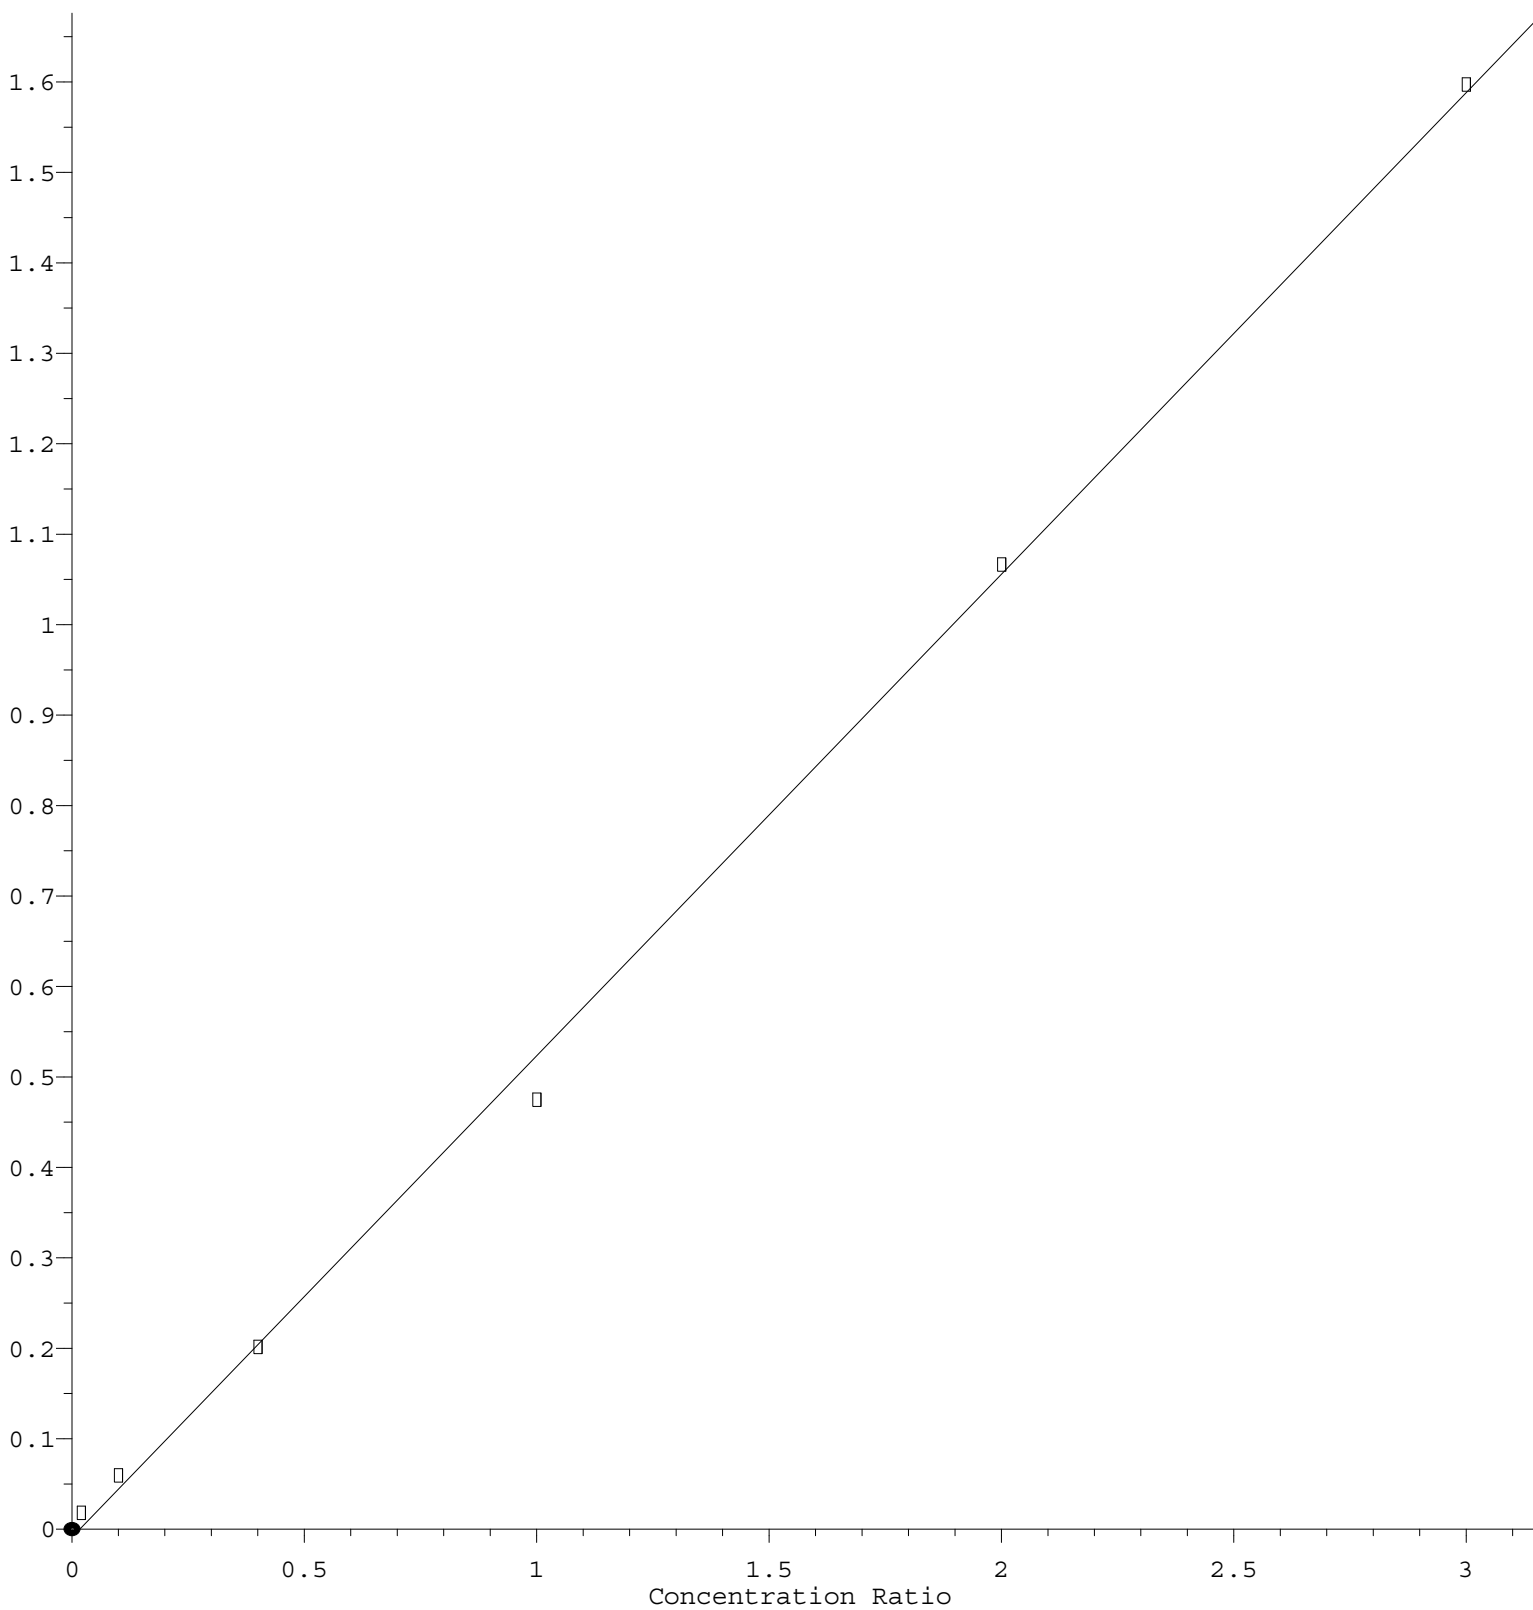

$$\text{Response} = 5.324\text{e-}001 * \text{Amt} - 9.017\text{e-}003$$


Coef of Det (r^2) = 0.998480 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091321W.M

Calibration Table Last Updated: Mon Sep 13 12:27:19 2021

Chloromethane

Response Ratio

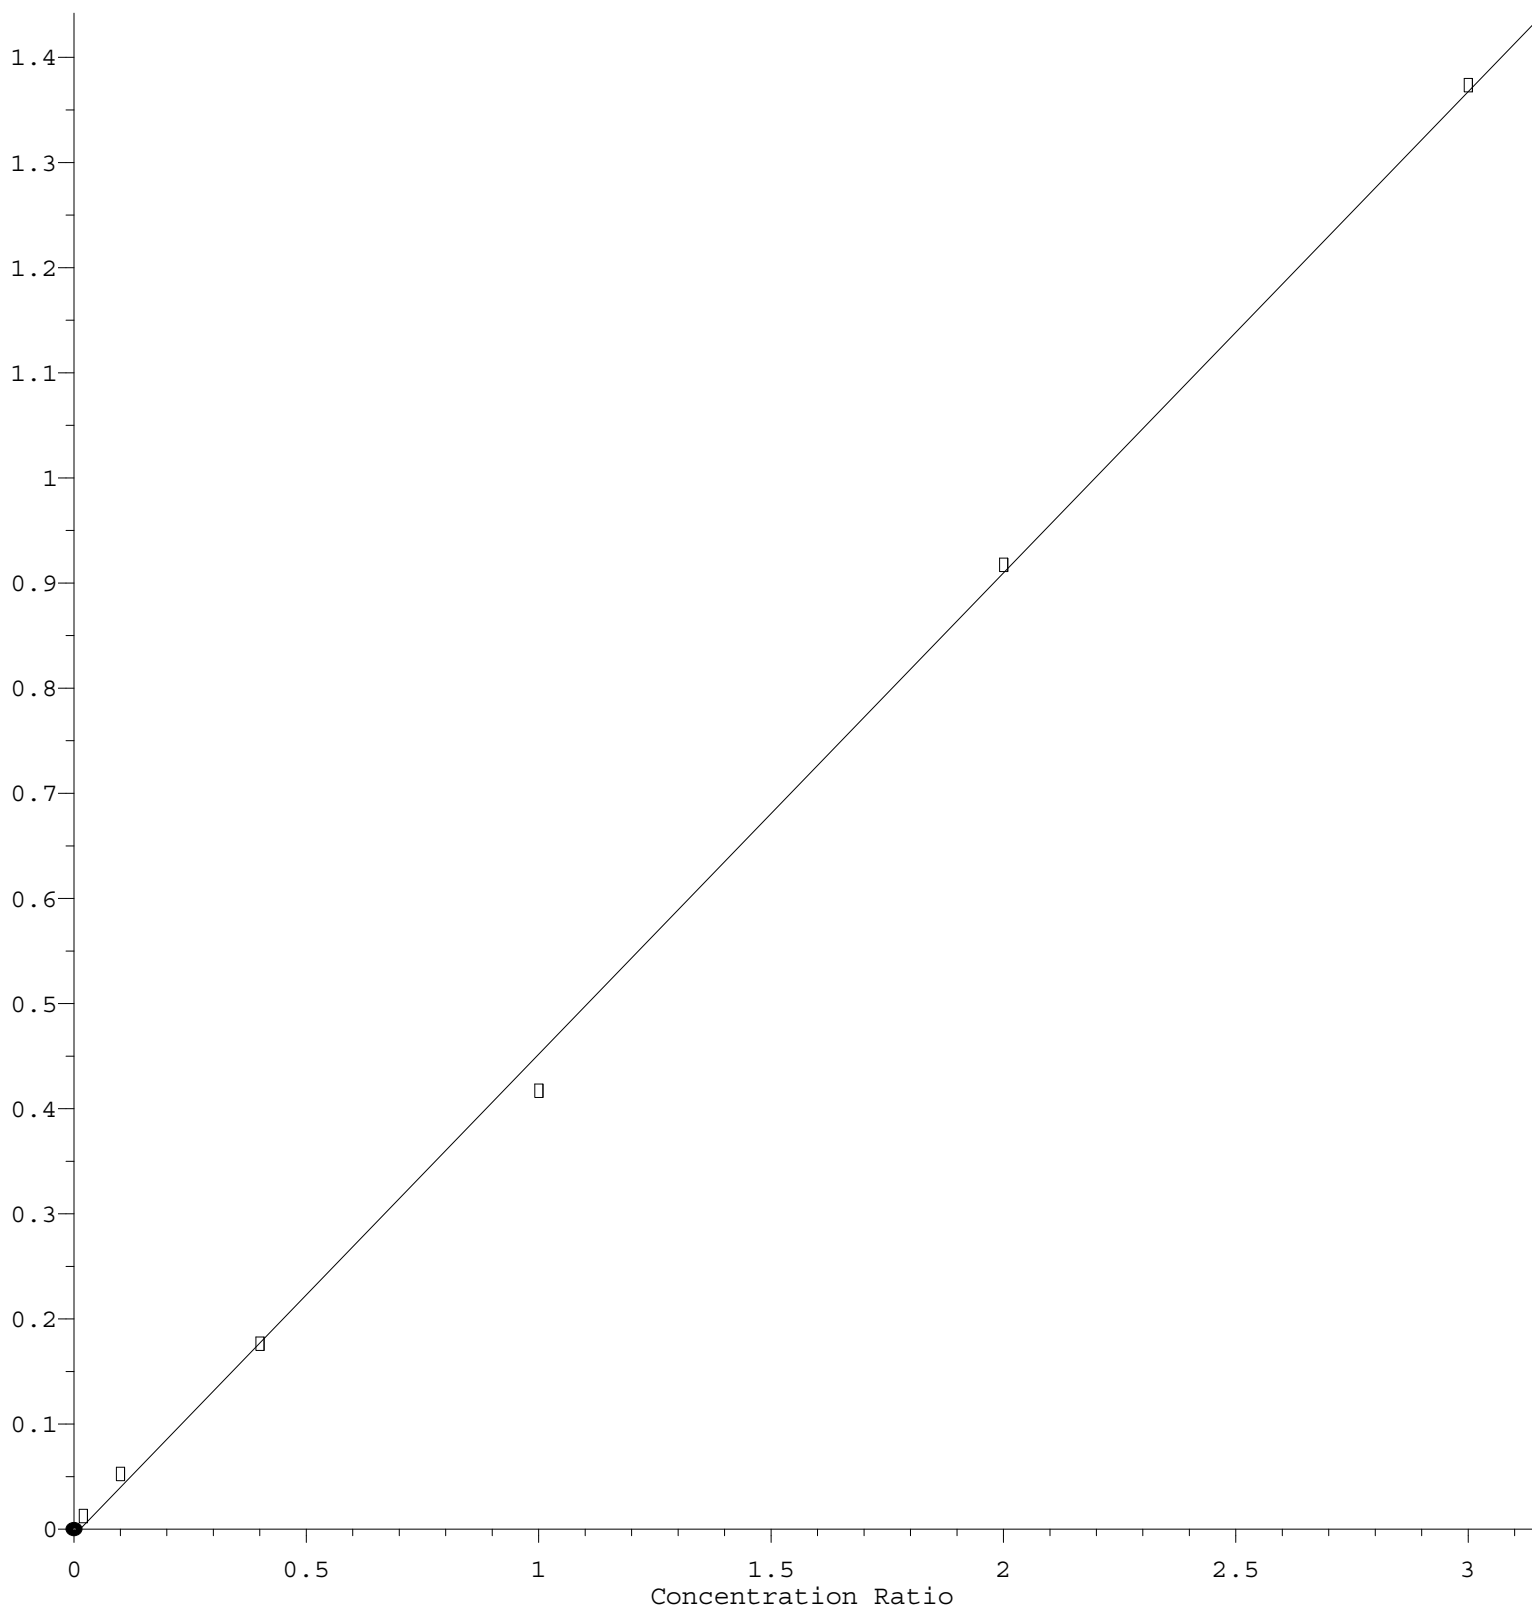

$$\text{Response} = 4.578\text{e-}001 * \text{Amt} - 5.922\text{e-}003$$


Coef of Det (r^2) = 0.998949 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091321W.M

Calibration Table Last Updated: Mon Sep 13 12:27:19 2021

Tert butyl alcohol

Response Ratio

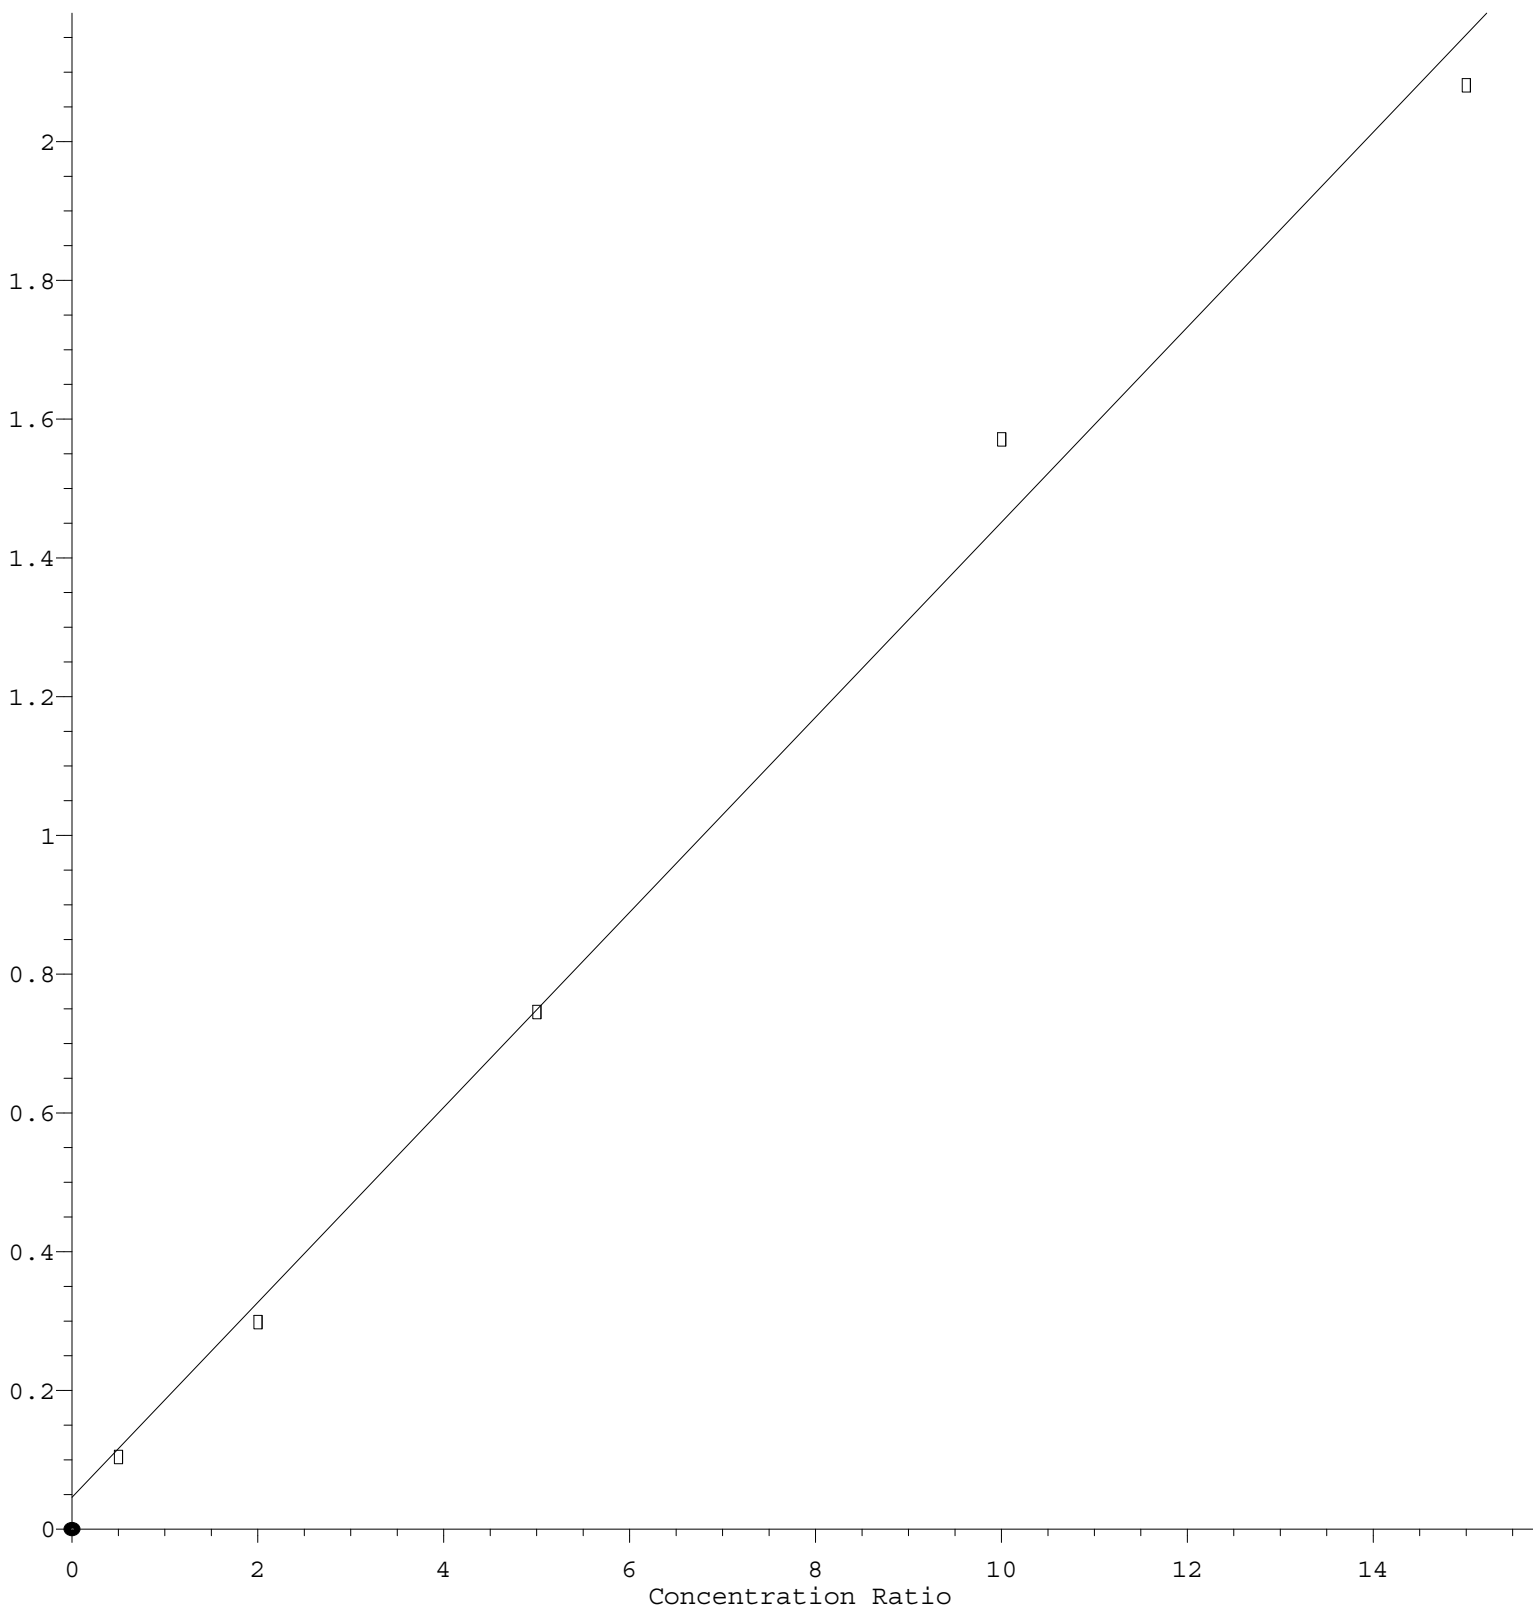

$$\text{Response} = 1.406\text{e-}001 * \text{Amt} + 4.621\text{e-}002$$


Coef of Det (r^2) = 0.992782 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091321W.M

Calibration Table Last Updated: Mon Sep 13 12:27:19 2021

Acetone

Response Ratio

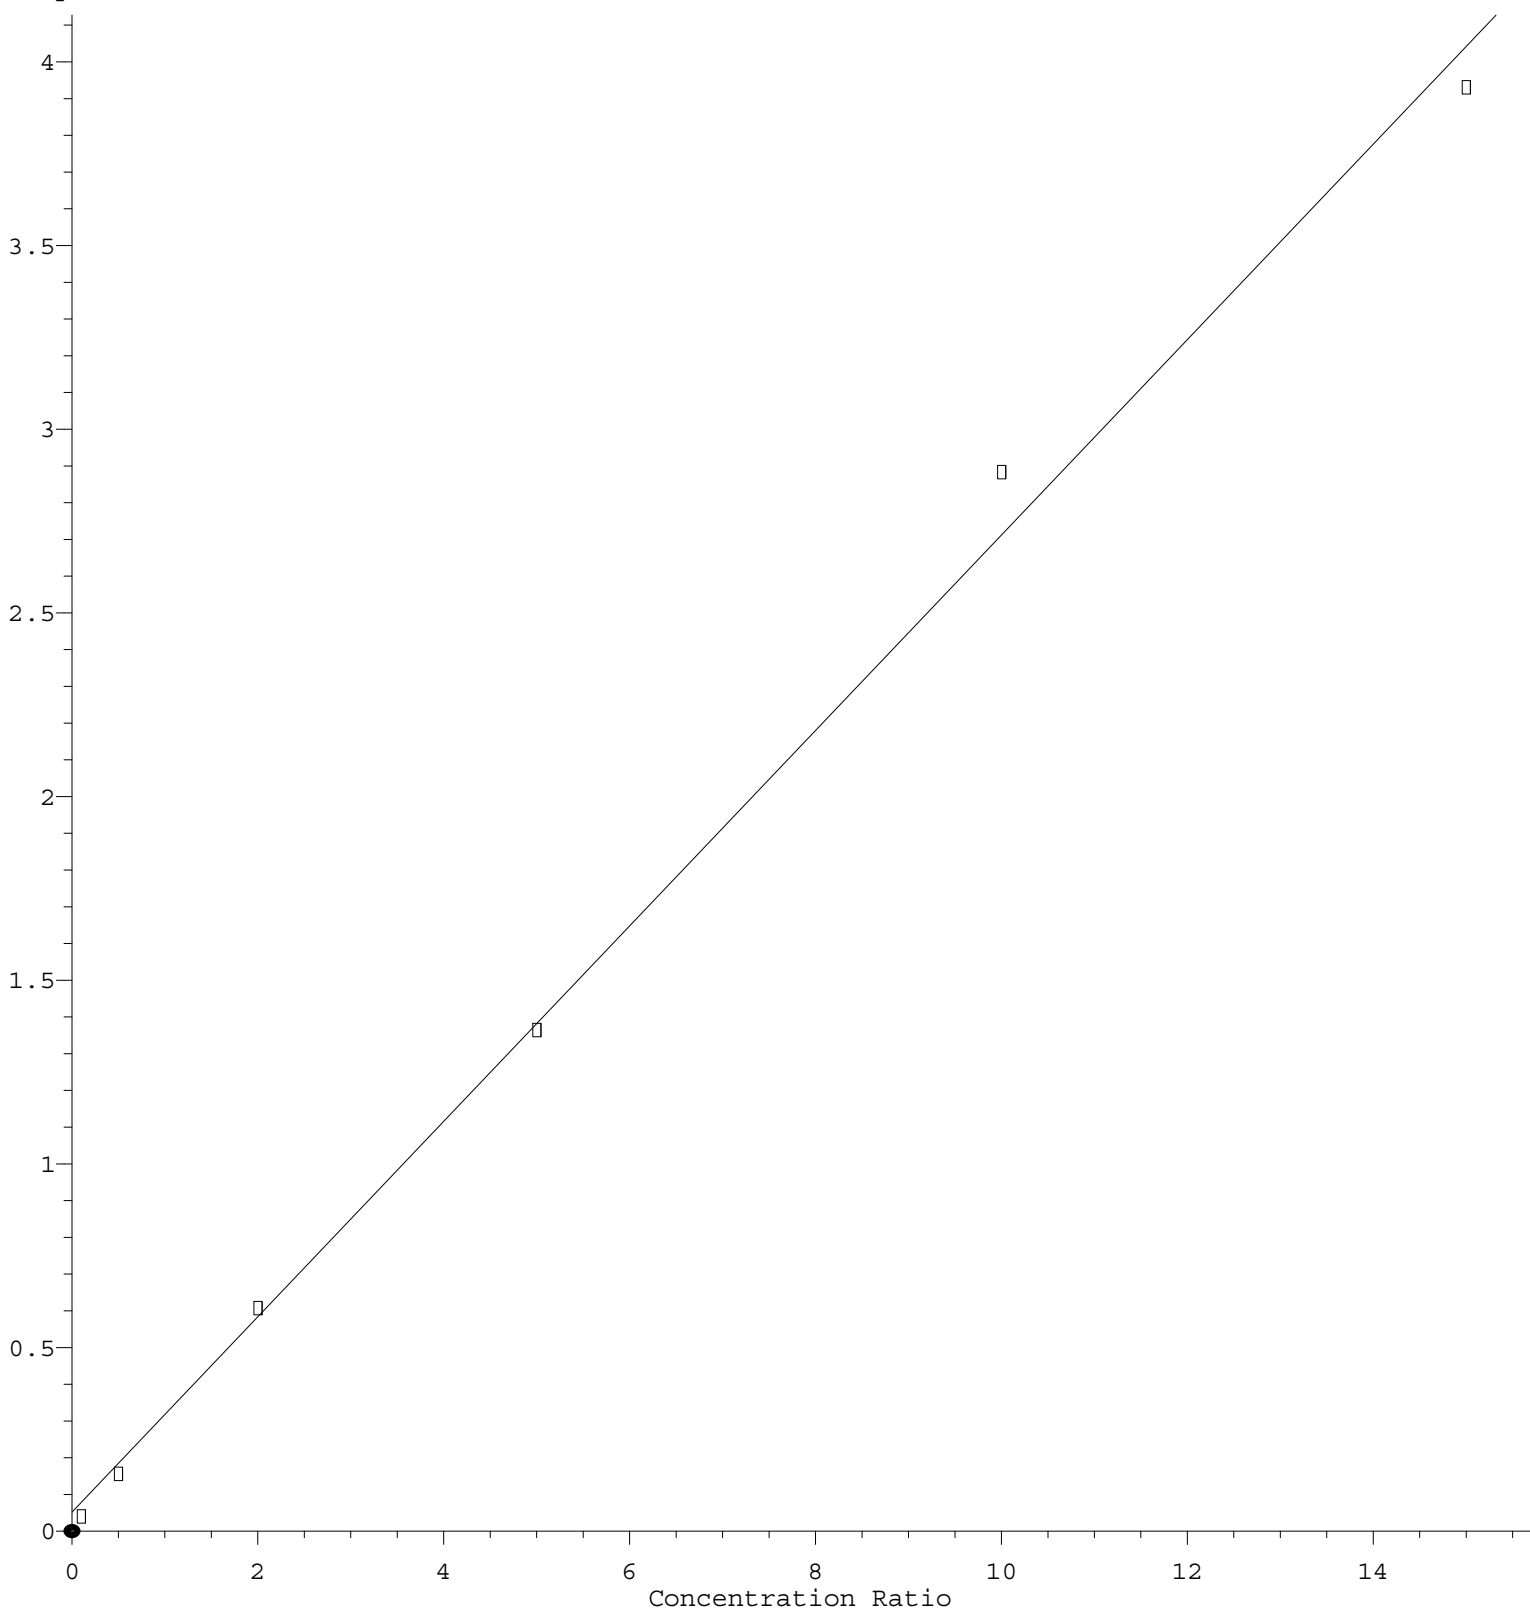

$\text{Response} = 2.660\text{e-}001 * \text{Amt} + 5.186\text{e-}002$
 Coef of Det (r^2) = 0.996431 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091321W.M
 Calibration Table Last Updated: Mon Sep 13 12:27:19 2021