
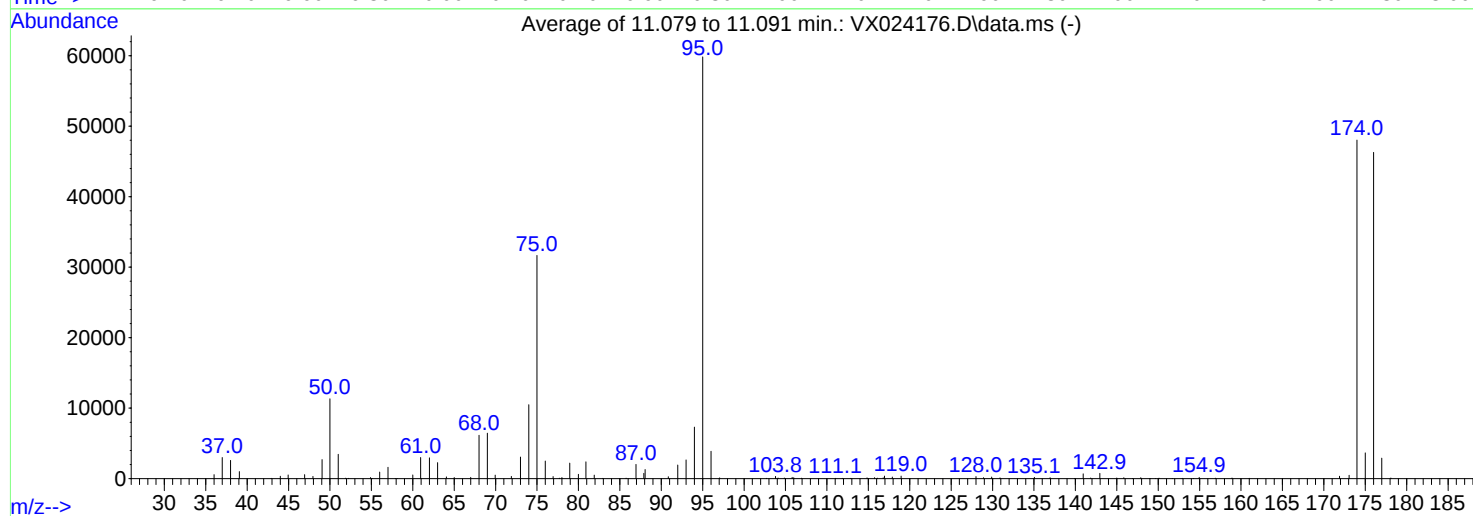


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091321\
 Data File : VX024176.D
 Acq On : 13 Sep 2021 09:22
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091321W.M
 Title : SW846 8260
 Last Update : Mon Sep 13 12:27:19 2021

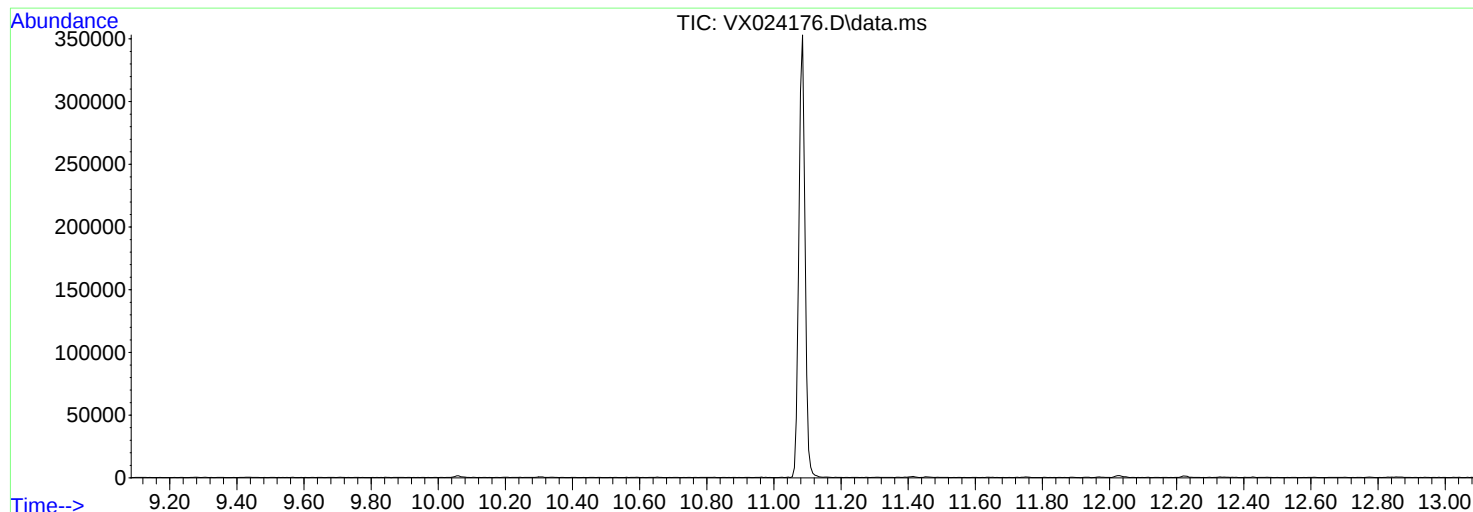

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	11321	PASS
75	95	30	60	52.9	31659	PASS
95	95	100	100	100.0	59837	PASS
96	95	5	9	6.5	3891	PASS
173	174	0.00	2	1.0	475	PASS
174	95	50	100	80.3	48037	PASS
175	174	5	9	7.6	3662	PASS
176	174	95	101	96.3	46277	PASS
177	176	5	9	6.3	2915	PASS