


1,1-Dichloroethene

Response Ratio

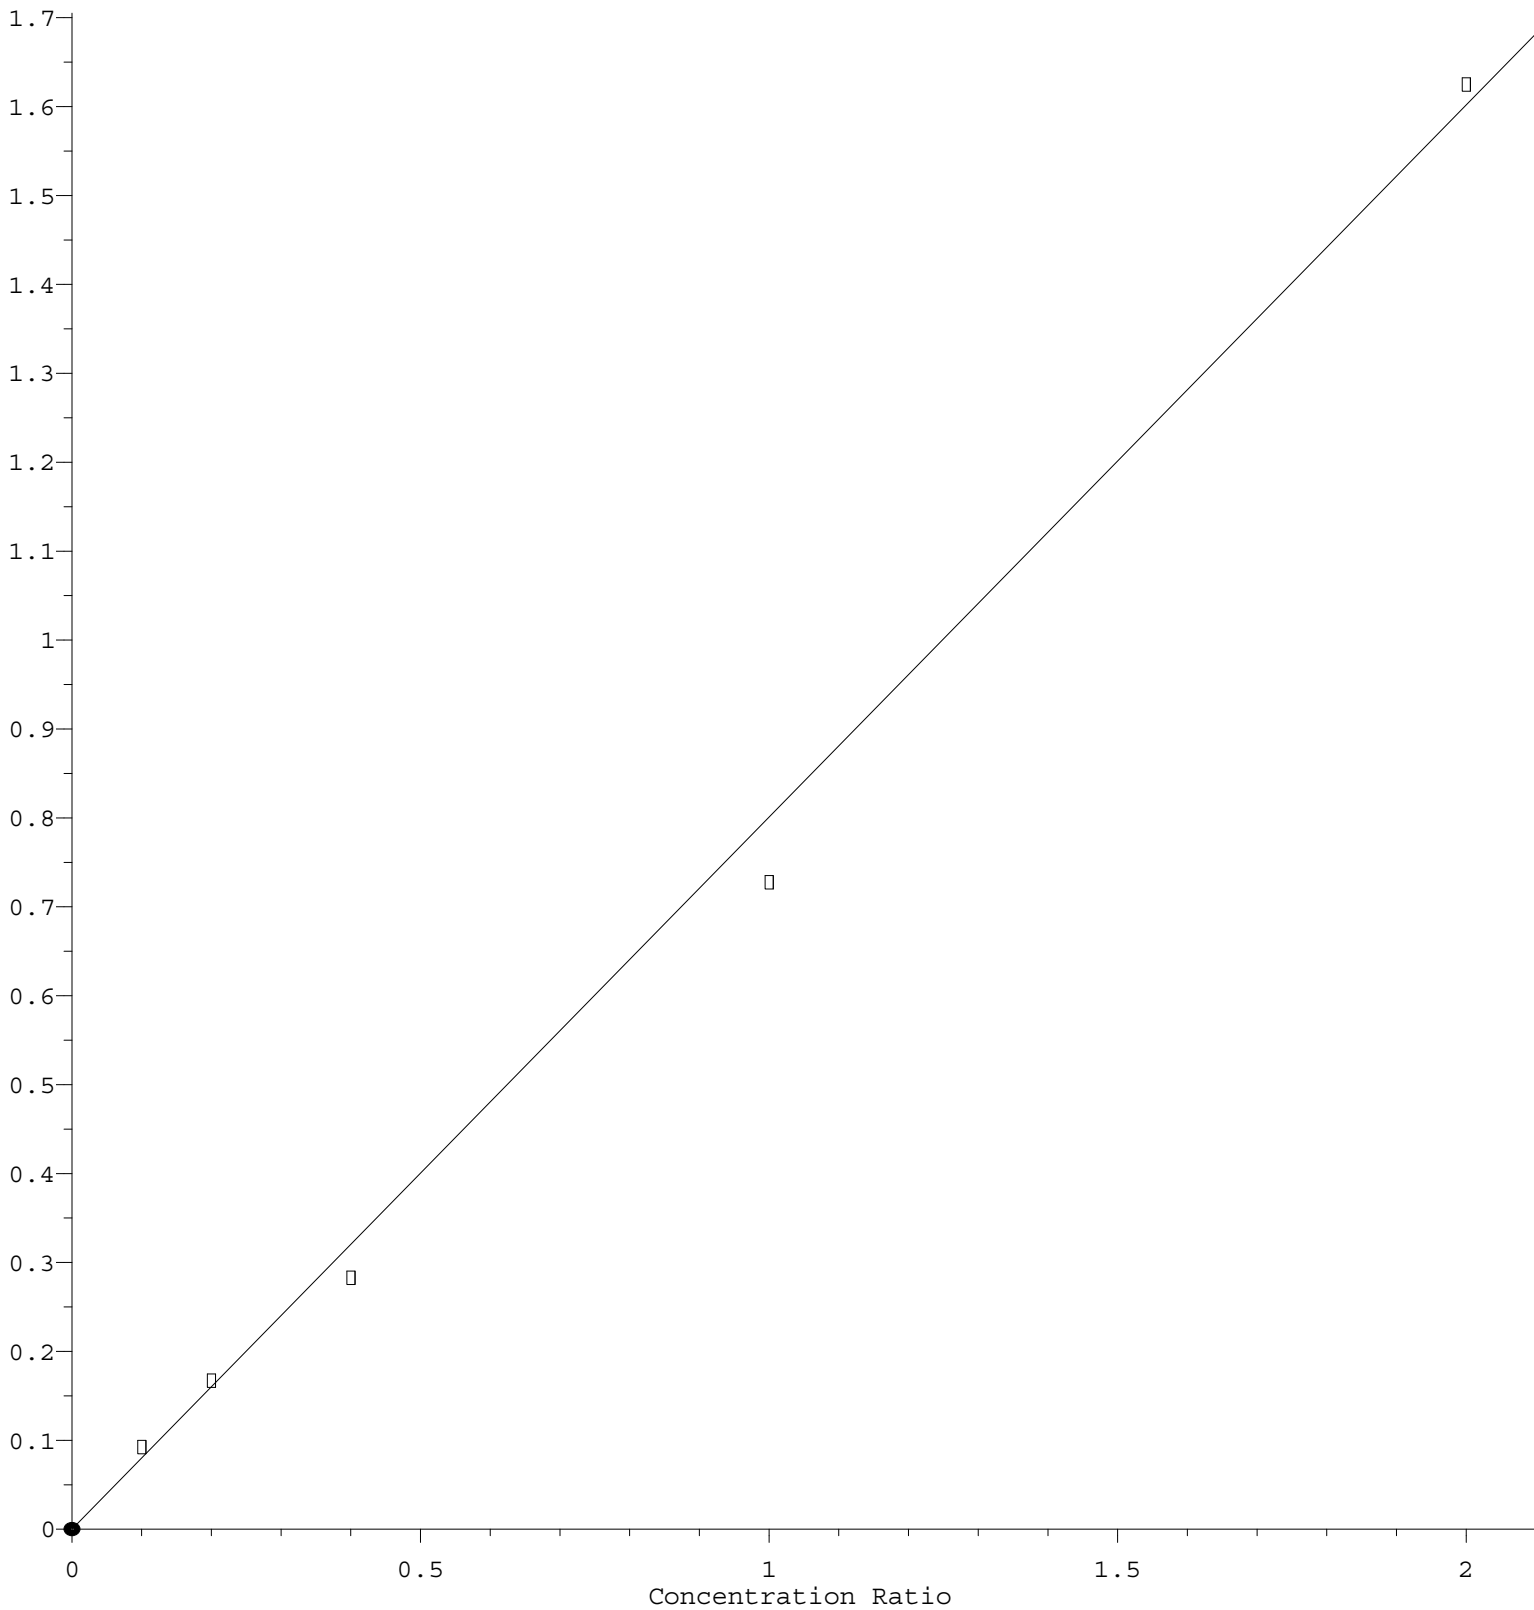


$$\text{Response} = 8.009\text{e-}001 * \text{Amt}$$

RF Rel Std Dev = 10.871% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091322W.M

Calibration Table Last Updated: Wed Sep 14 14:21:29 2022


1,2-Dibromo-3-Chloropropane

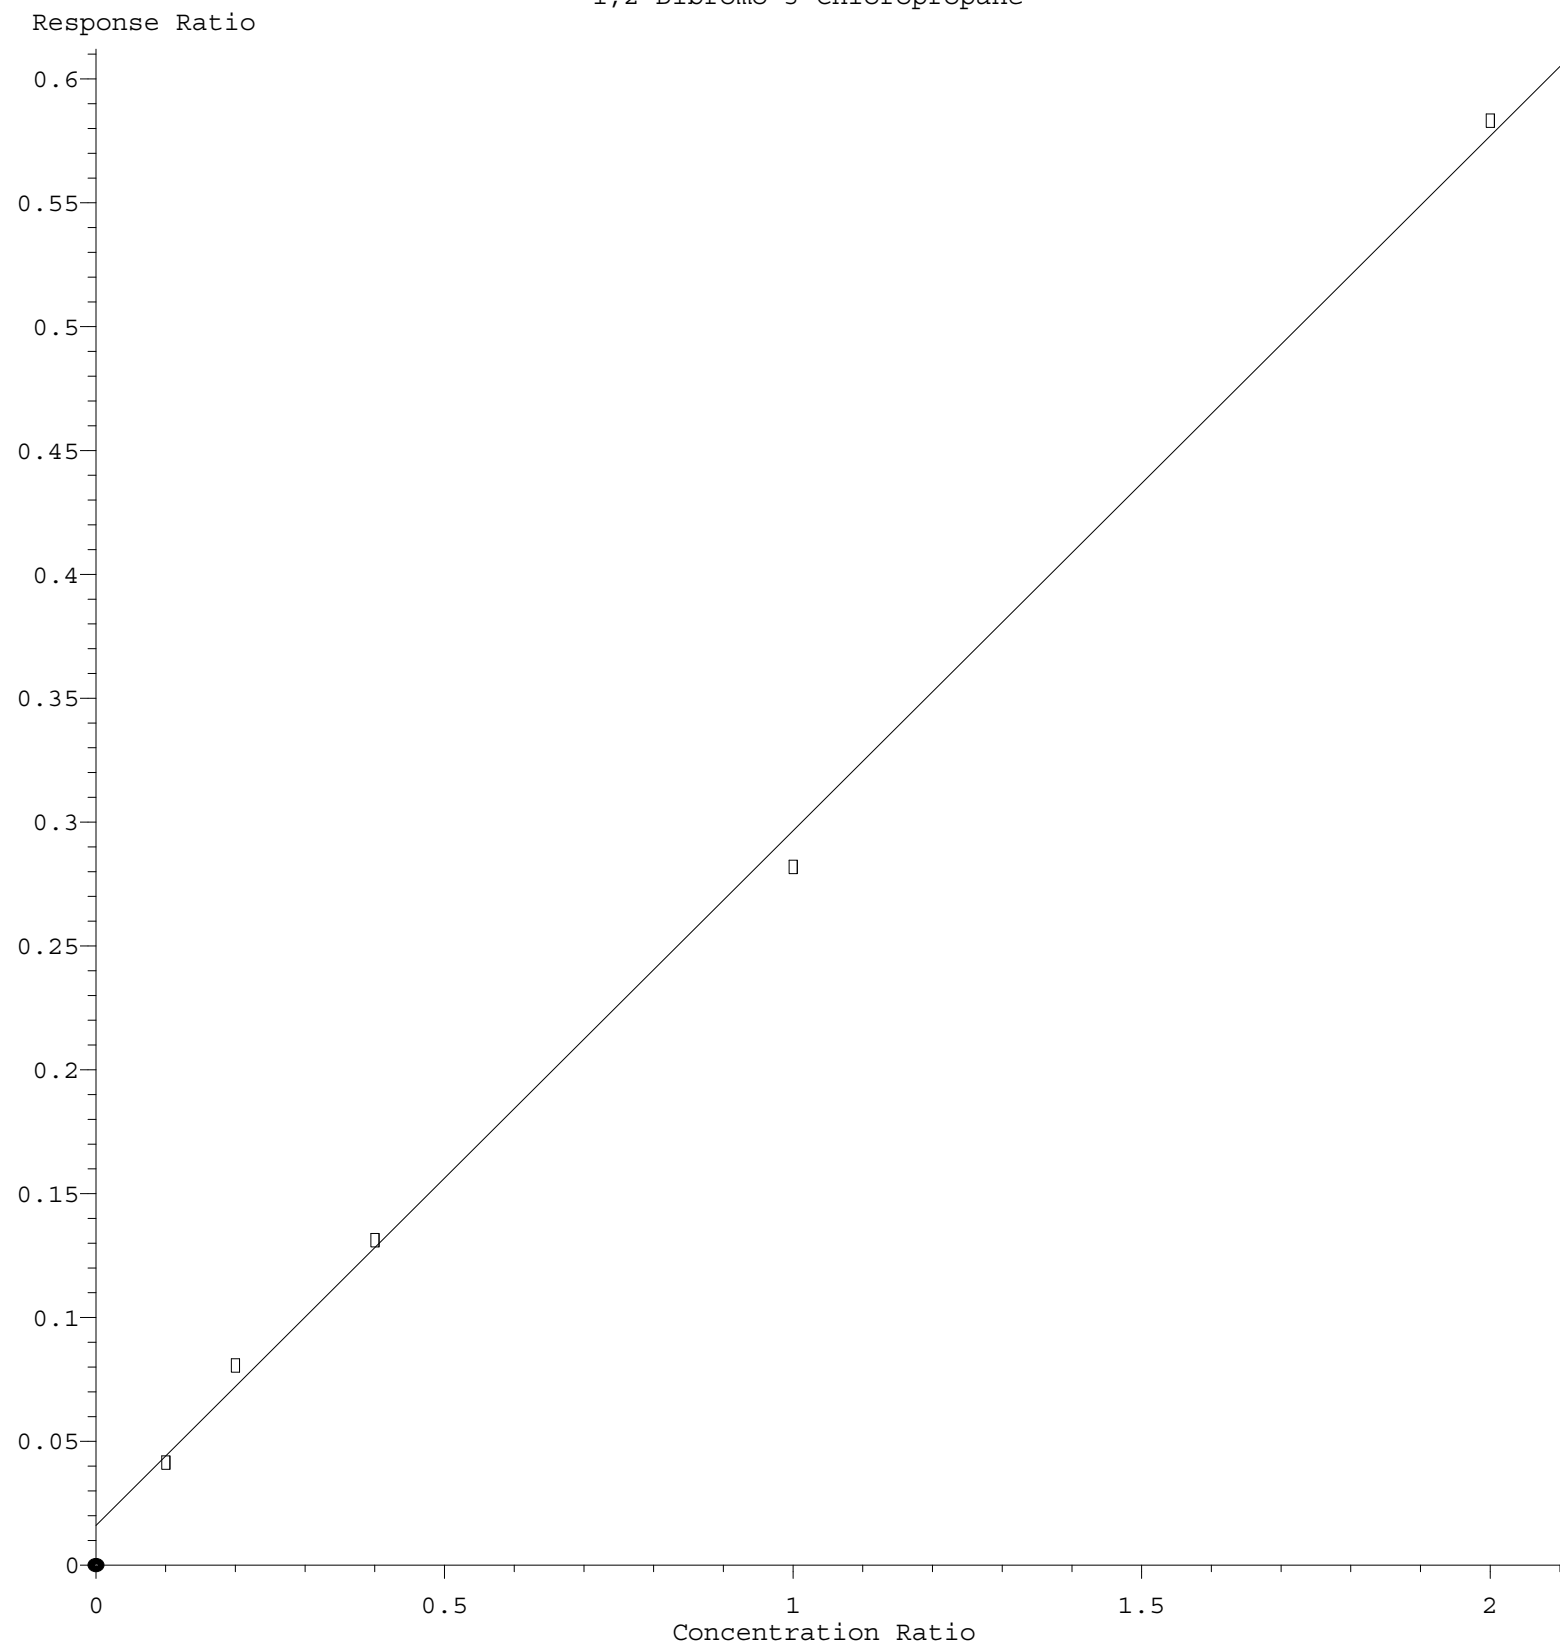

$\text{Response} = 2.805\text{e-}001 * \text{Amt} + 1.608\text{e-}002$
 Coef of Det (r^2) = 0.998253 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091322W.M
 Calibration Table Last Updated: Wed Sep 14 14:21:29 2022

Carbon Disulfide

Response Ratio

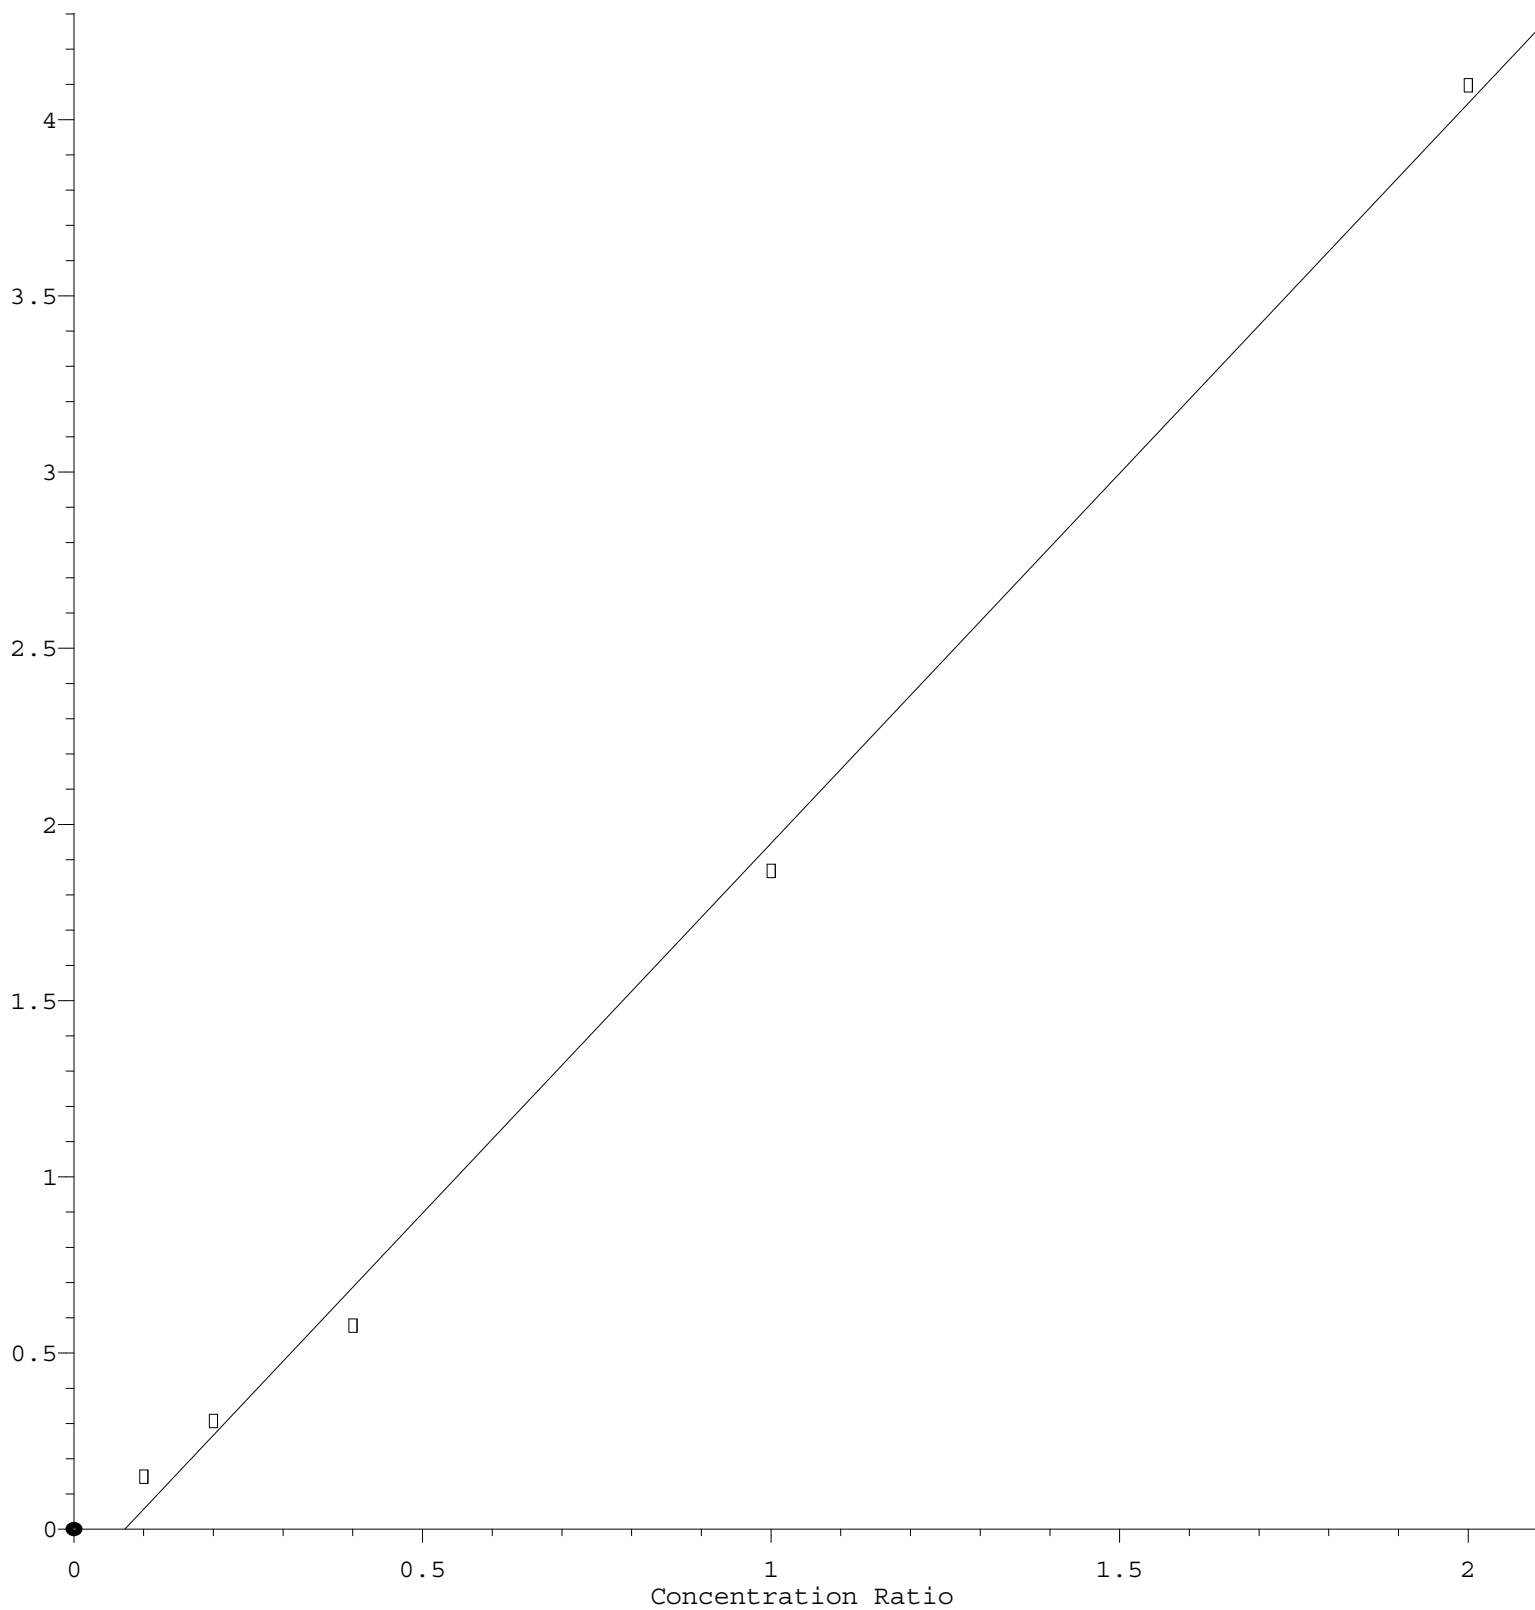

$$\text{Response} = 2.100\text{e}+000 * \text{Amt} - 1.541\text{e}-001$$


Coef of Det (r^2) = 0.997179 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091322W.M

Calibration Table Last Updated: Wed Sep 14 14:21:29 2022

Toluene-d8

Response Ratio

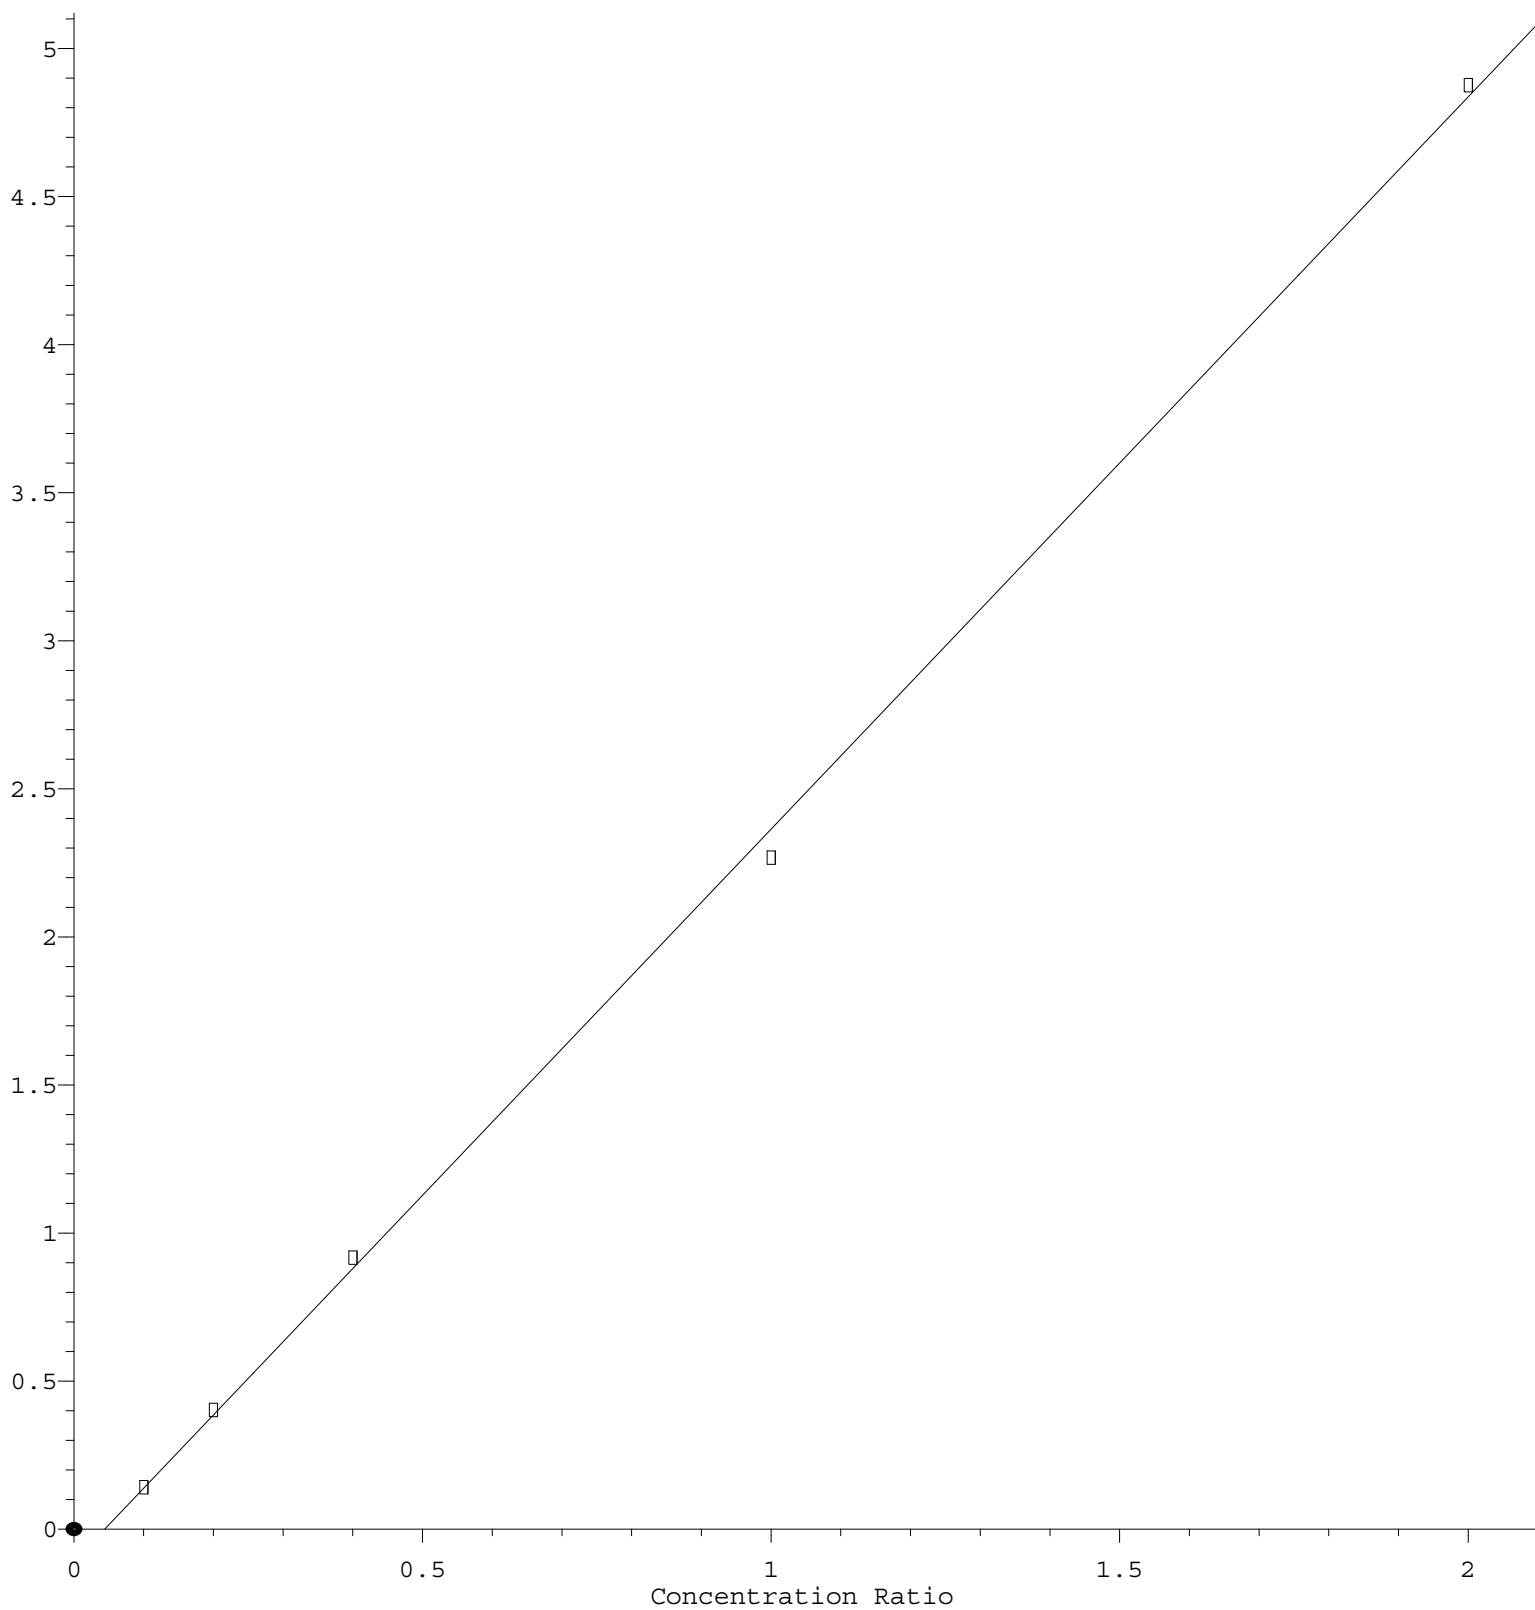

$$\text{Response} = 2.473\text{e}+000 * \text{Amt} - 1.095\text{e}-001$$

Coef of Det (r^2) = 0.999177 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091322W.M

Calibration Table Last Updated: Wed Sep 14 14:21:29 2022