
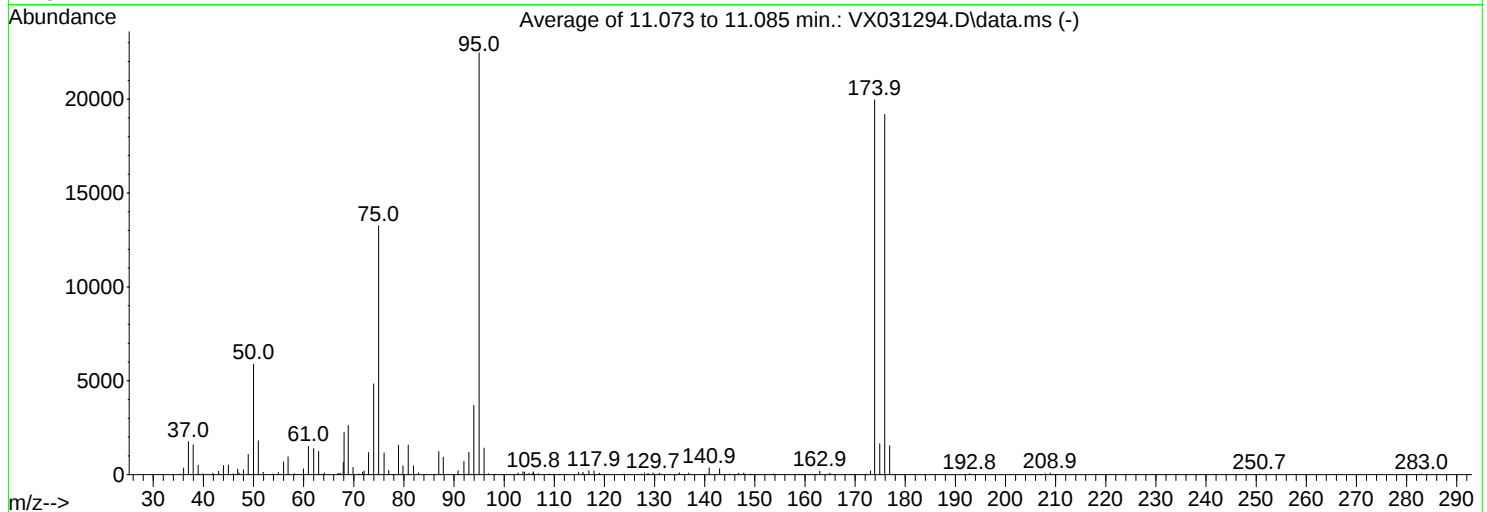


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091322\
Data File : VX031294.D
Acq On : 13 Sep 2022 16:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091322W.M
Title : SW846 8260
Last Update : Wed Sep 14 14:21:29 2022

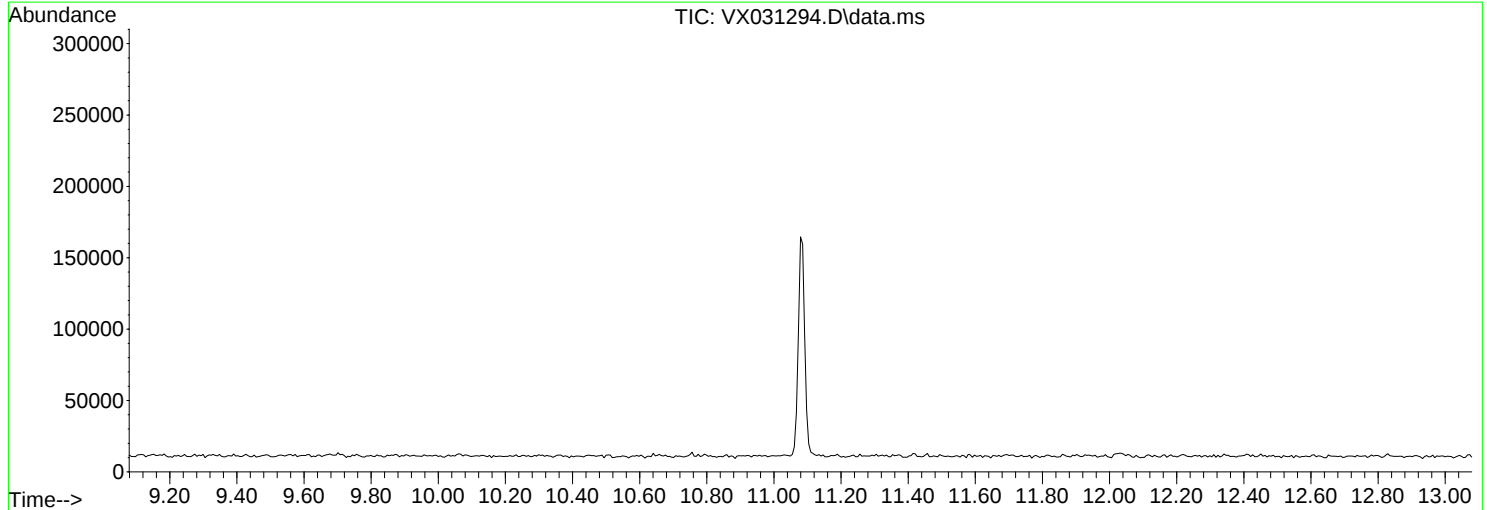

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.2	5892	PASS
75	95	30	60	59.0	13263	PASS
95	95	100	100	100.0	22464	PASS
96	95	5	9	6.3	1418	PASS
173	174	0.00	2	1.0	209	PASS
174	95	50	100	88.8	19955	PASS
175	174	5	9	8.3	1647	PASS
176	174	95	101	96.1	19180	PASS
177	176	5	9	8.1	1544	PASS