

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
 Data File : VX037691.D
 Acq On : 13 Sep 2023 13:40
 Operator : JC/MD
 Sample : 04394-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB9/8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	69	78	79	rBV3	14234	31029	2.45%	0.447%
2	2.940	296	304	315	rBV2	7983	20122	1.59%	0.290%
3	3.440	377	386	401	rBV	86639	197661	15.59%	2.849%
4	4.587	564	574	587	rBV	14391	49994	3.94%	0.721%
5	5.385	693	705	721	rBV	146252	435931	34.39%	6.284%
6	5.550	721	732	750	rVB	237989	684298	53.98%	9.864%
7	5.952	788	798	817	rBV	173699	462303	36.47%	6.664%
8	6.763	921	931	956	rBV	383234	928554	73.25%	13.385%
9	8.647	1234	1240	1254	rBV	804197	1267707	100.00%	18.274%
10	10.055	1465	1471	1486	rBV	831165	1113874	87.87%	16.057%
11	11.079	1634	1639	1654	rBV	620966	805407	63.53%	11.610%
12	12.024	1788	1794	1807	rBV	747597	940190	74.16%	13.553%




Sum of corrected areas: 6937070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037691.D
Acq On : 13 Sep 2023 13:40
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

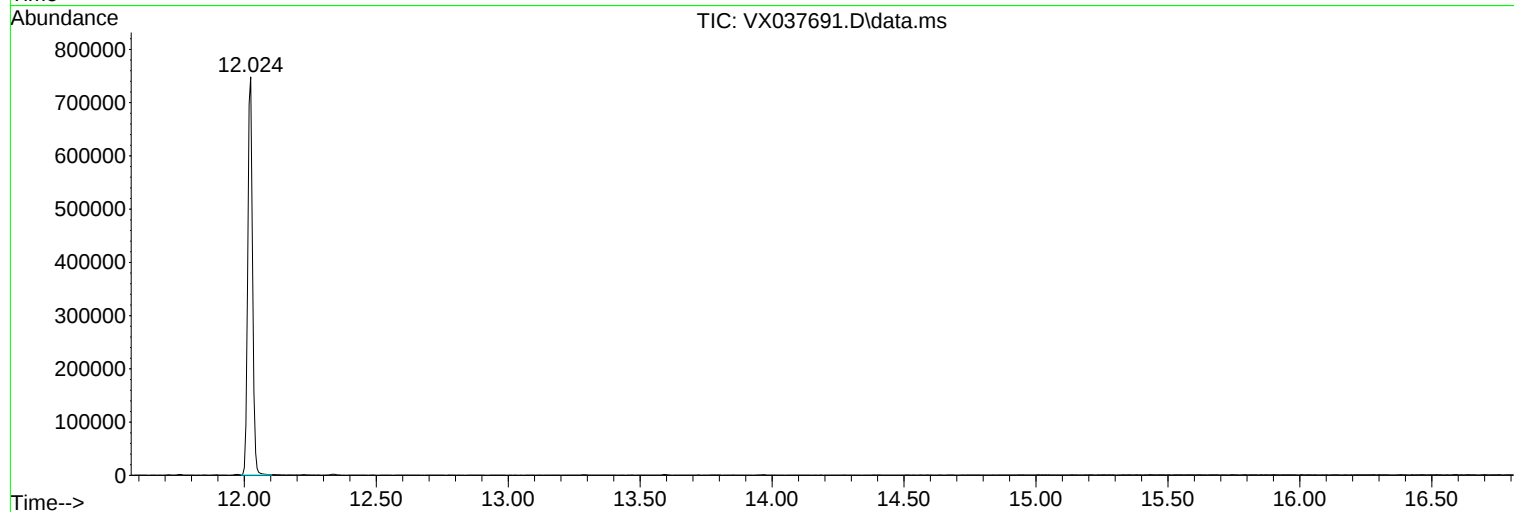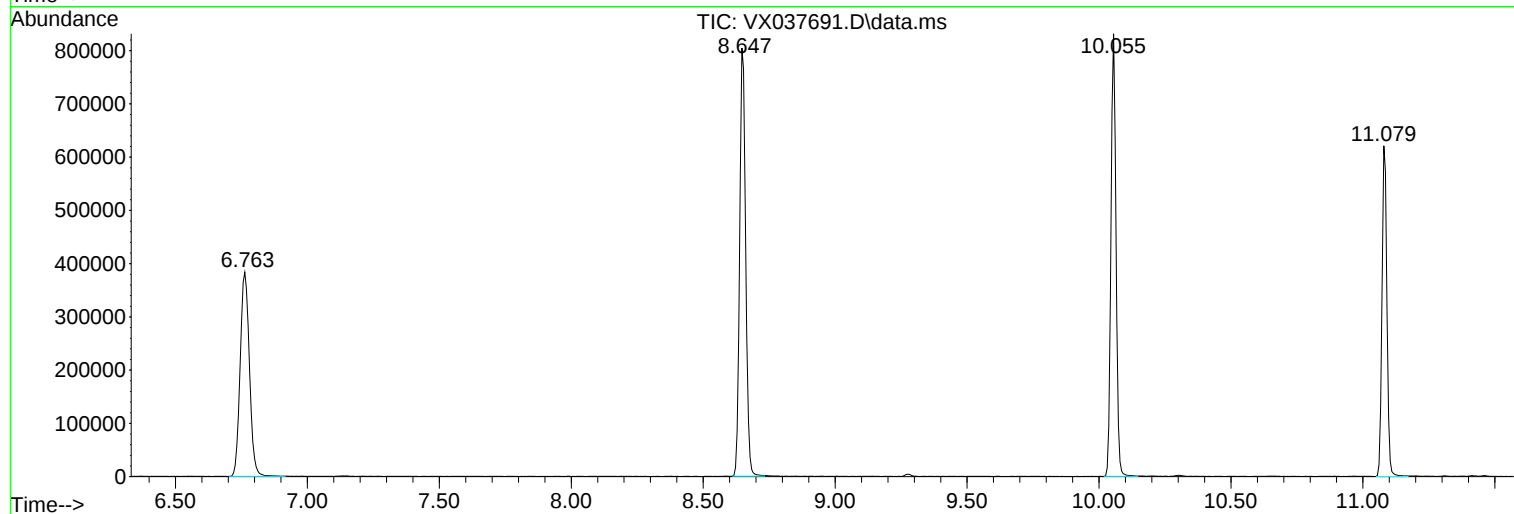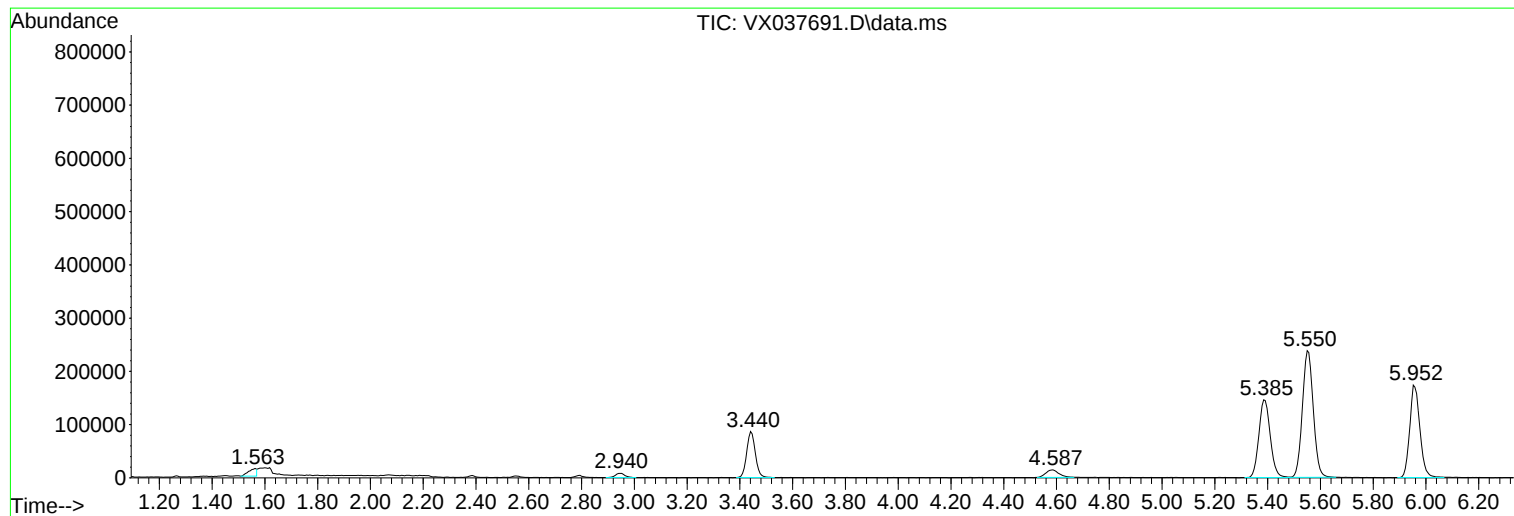

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037691.D
Acq On : 13 Sep 2023 13:40
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.440	14.44 ug/l	197661	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Hexane	86	C6H14	000110-54-3	90
2			Pentane, 2,2,3,4-tetramethyl-	128	C9H20	001186-53-4	50
3			Furan, tetrahydro-3-methyl-	86	C5H10O	013423-15-9	49
4			2-Ethyl-oxetane	86	C5H10O	1010386-40-2	43
5			Pentane, 3-methyl-	86	C6H14	000096-14-0	42

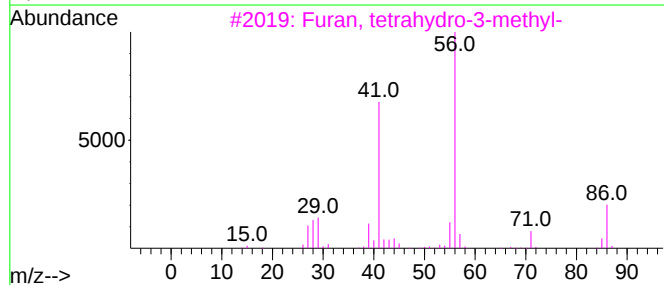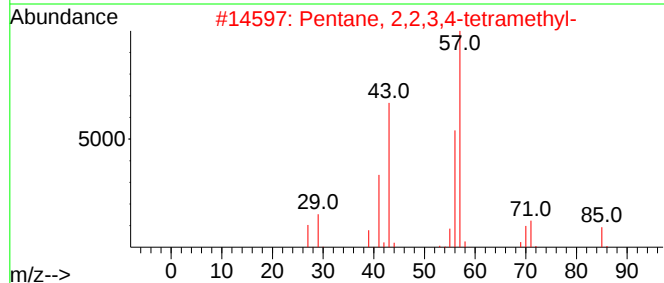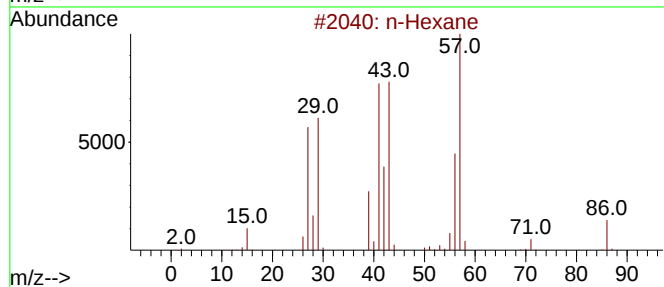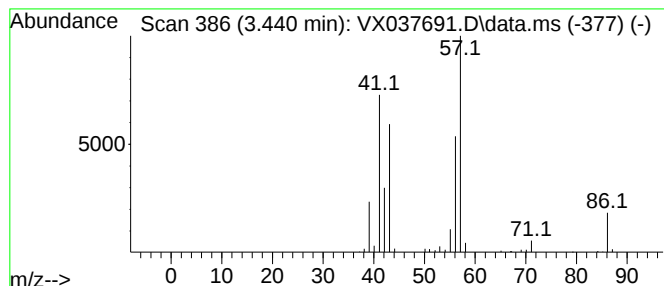

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037691.D
Acq On : 13 Sep 2023 13:40
Operator : JC/MD
Sample : 04394-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB9/8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexane	3.440	14.4	ug/l	197661	1	5.556	684298	50.0