

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
 Data File : VX037693.D
 Acq On : 13 Sep 2023 14:29
 Operator : JC/MD
 Sample : 04352-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-02-090723

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	6	10	21	rVB	12549	20404	1.70%	0.319%
2	1.557	70	77	78	rBV3	13682	26912	2.25%	0.421%
3	5.093	646	657	670	rBV3	4728	15225	1.27%	0.238%
4	5.385	693	705	721	rBV	139292	408608	34.09%	6.396%
5	5.550	721	732	751	rVB	227714	649723	54.21%	10.171%
6	5.958	788	799	814	rBV	158914	426990	35.63%	6.684%
7	6.763	920	931	946	rBV	362951	874050	72.93%	13.682%
8	8.647	1233	1240	1250	rBV	758821	1198551	100.00%	18.762%
9	10.055	1465	1471	1484	rBV	797366	1054766	88.00%	16.511%
10	11.079	1634	1639	1653	rBV	604770	777154	64.84%	12.166%
11	12.024	1788	1794	1806	rBV	697509	923071	77.02%	14.450%
12	13.780	2078	2082	2086	rBV2	9683	12718	1.06%	0.199%




Sum of corrected areas: 6388172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037693.D
Acq On : 13 Sep 2023 14:29
Operator : JC/MD
Sample : 04352-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-090723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

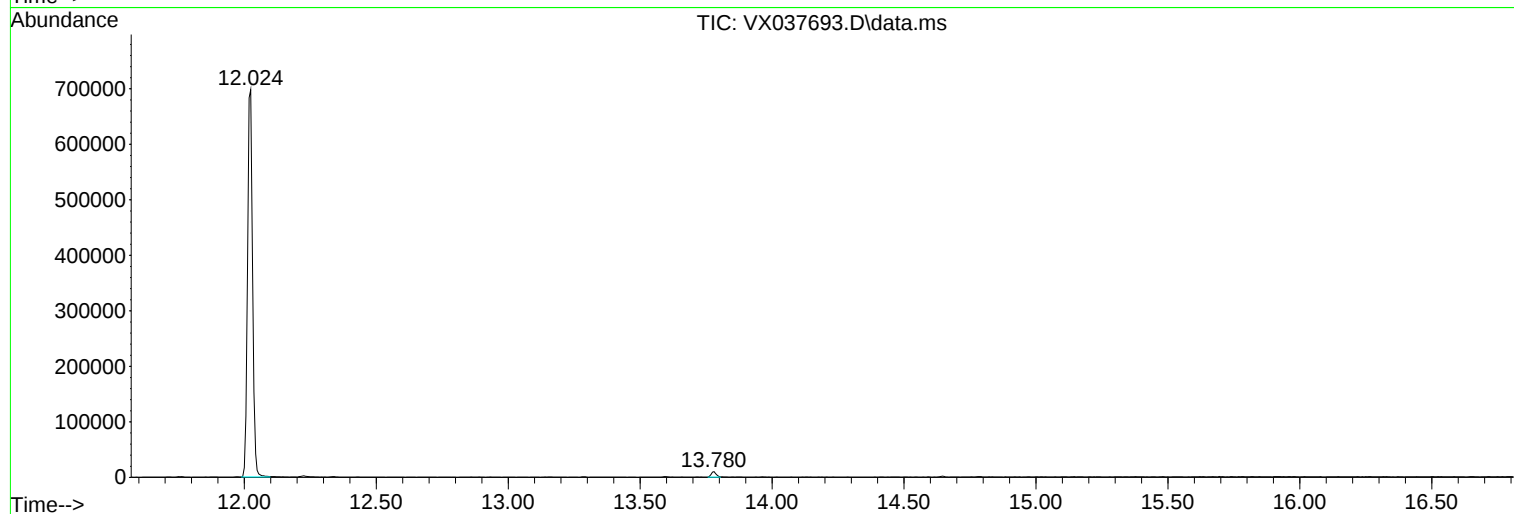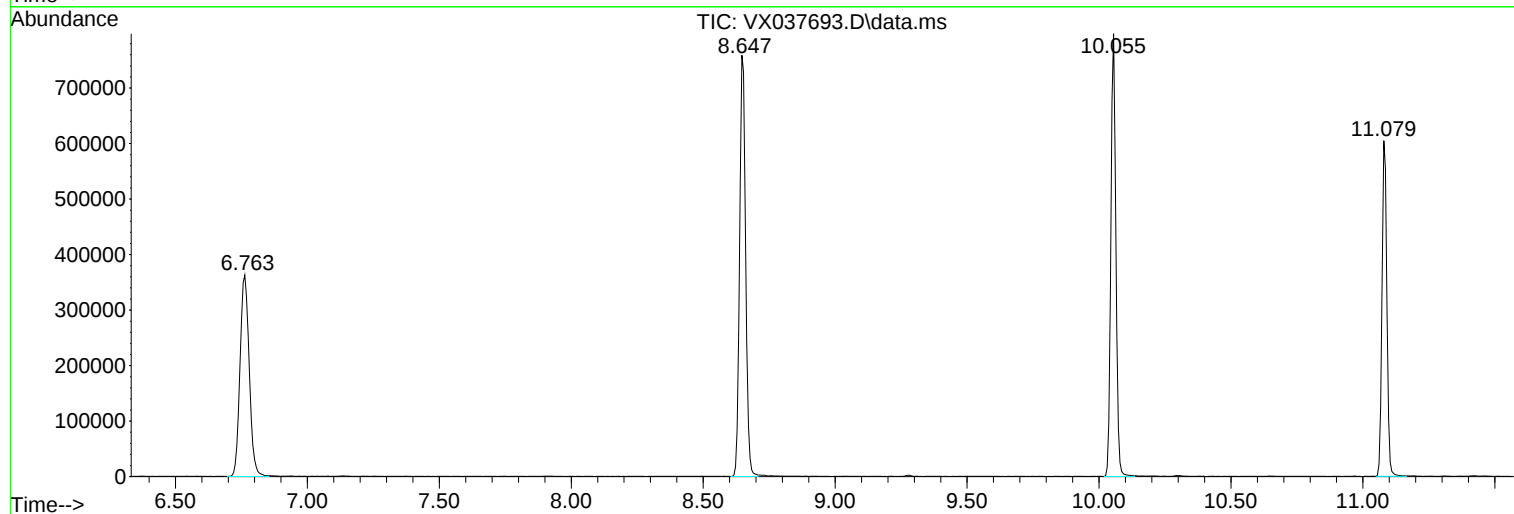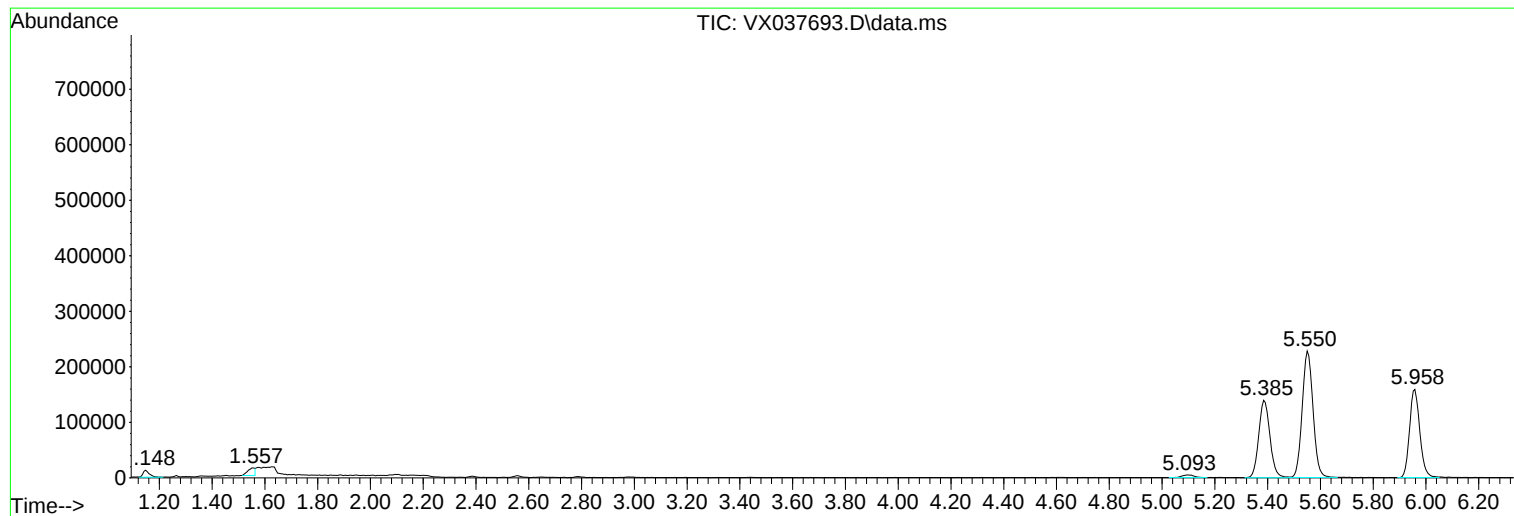

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037693.D
Acq On : 13 Sep 2023 14:29
Operator : JC/MD
Sample : 04352-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-090723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037693.D
Acq On : 13 Sep 2023 14:29
Operator : JC/MD
Sample : 04352-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-090723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc