

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
 Data File : VX037700.D
 Acq On : 13 Sep 2023 17:20
 Operator : JC/MD
 Sample : 04351-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M

Title : SW846 8260

Signal : TIC: VX037700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.557	68	77	78	rBV3	12859	24599	2.10%	0.375%
2	2.947	297	305	314	rVB	6677	16283	1.39%	0.248%
3	3.440	374	386	407	rVB	179159	405220	34.54%	6.171%
4	4.587	561	574	588	rBV2	10823	38013	3.24%	0.579%
5	5.385	693	705	721	rBV	135743	400586	34.14%	6.101%
6	5.550	721	732	751	rVB	223345	638600	54.43%	9.726%
7	5.958	789	799	814	rBV	156256	421159	35.90%	6.414%
8	6.763	920	931	945	rBV	360945	859661	73.27%	13.093%
9	8.647	1234	1240	1251	rBV	748361	1173300	100.00%	17.869%
10	10.055	1465	1471	1481	rBV	760500	1015789	86.58%	15.470%
11	11.079	1634	1639	1653	rBV	562477	731804	62.37%	11.145%
12	12.024	1788	1794	1804	rBV	656013	841024	71.68%	12.809%




Sum of corrected areas: 6566038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037700.D
Acq On : 13 Sep 2023 17:20
Operator : JC/MD
Sample : 04351-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

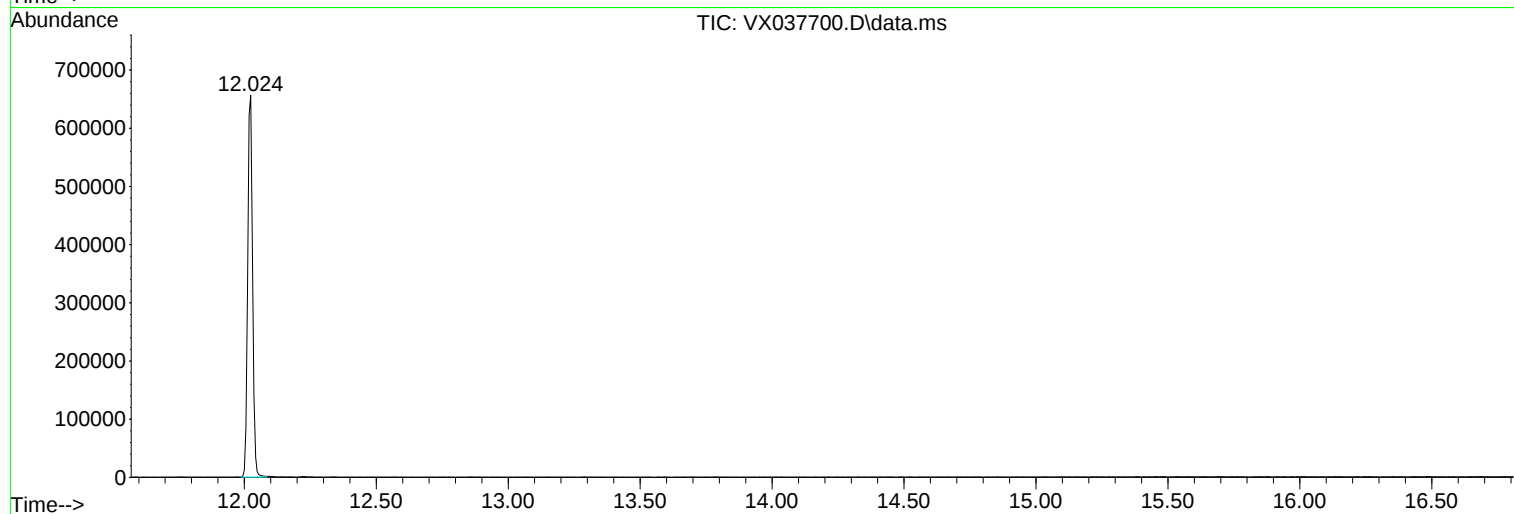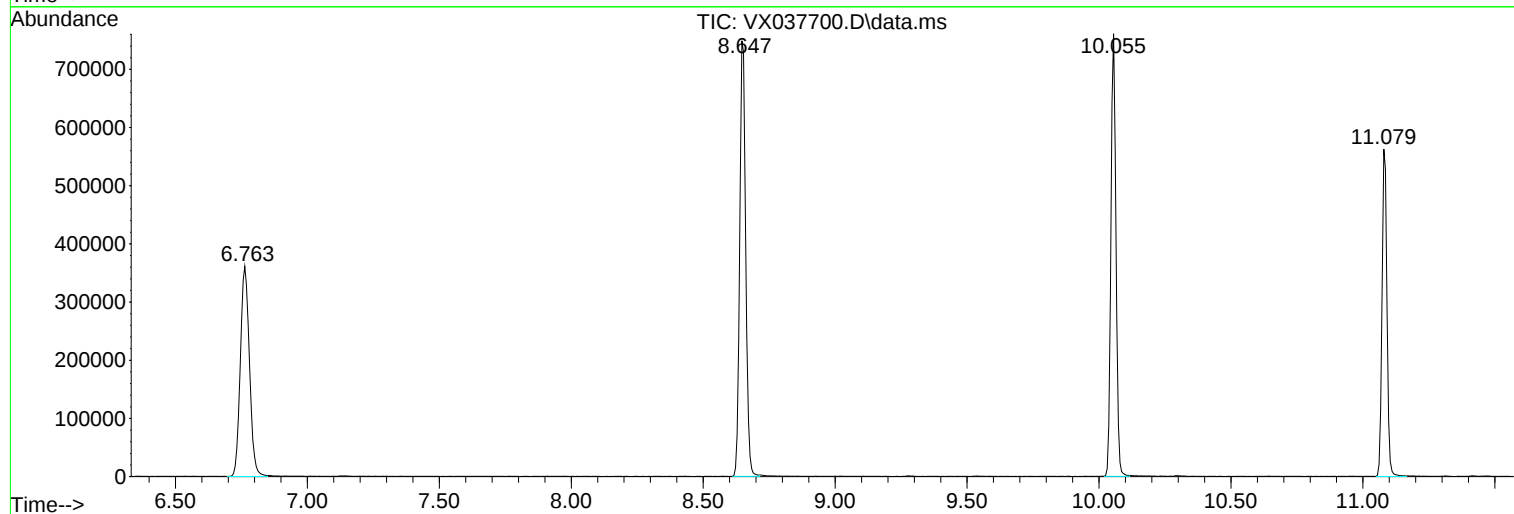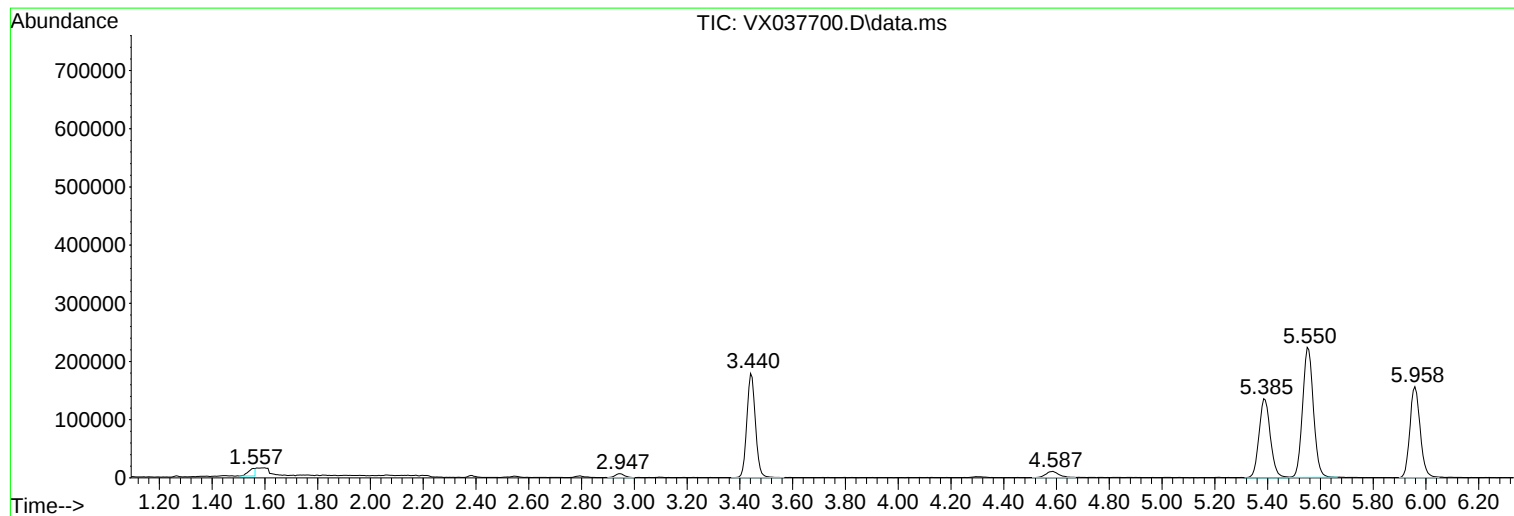

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037700.D
Acq On : 13 Sep 2023 17:20
Operator : JC/MD
Sample : 04351-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.440	31.73 ug/l	405220	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Hexane	86	C6H14	000110-54-3	91
2			2-Ethyl-oxetane	86	C5H10O	1010386-40-2	78
3			Pentane, 2,2,3,4-tetramethyl-	128	C9H20	001186-53-4	50
4			Hydroperoxide, hexyl	118	C6H14O2	004312-76-9	38
5			Methane, isocyanato-	57	C2H3NO	000624-83-9	32

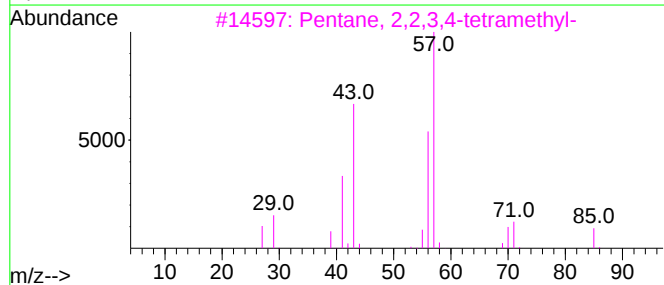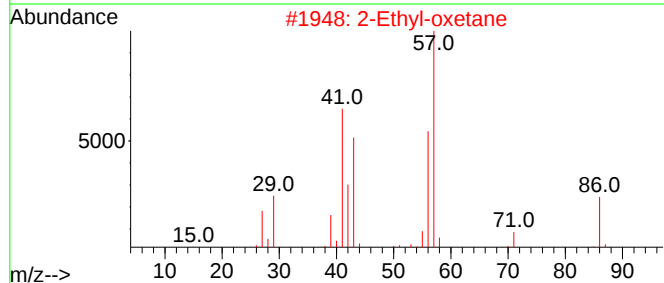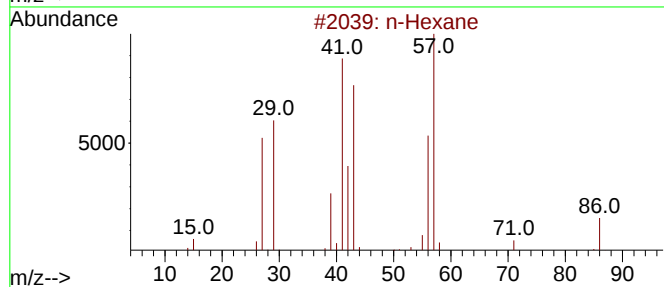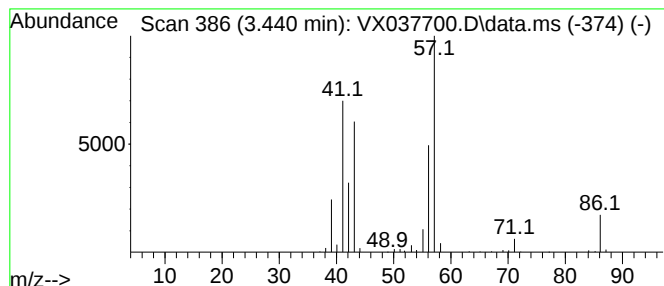

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037700.D
Acq On : 13 Sep 2023 17:20
Operator : JC/MD
Sample : 04351-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexane	3.440	31.7	ug/l	405220	1	5.556	638600	50.0