


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091323\
Data File : VX037708.D
Acq On : 14 Sep 2023 02:10
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 10:10:04 2023

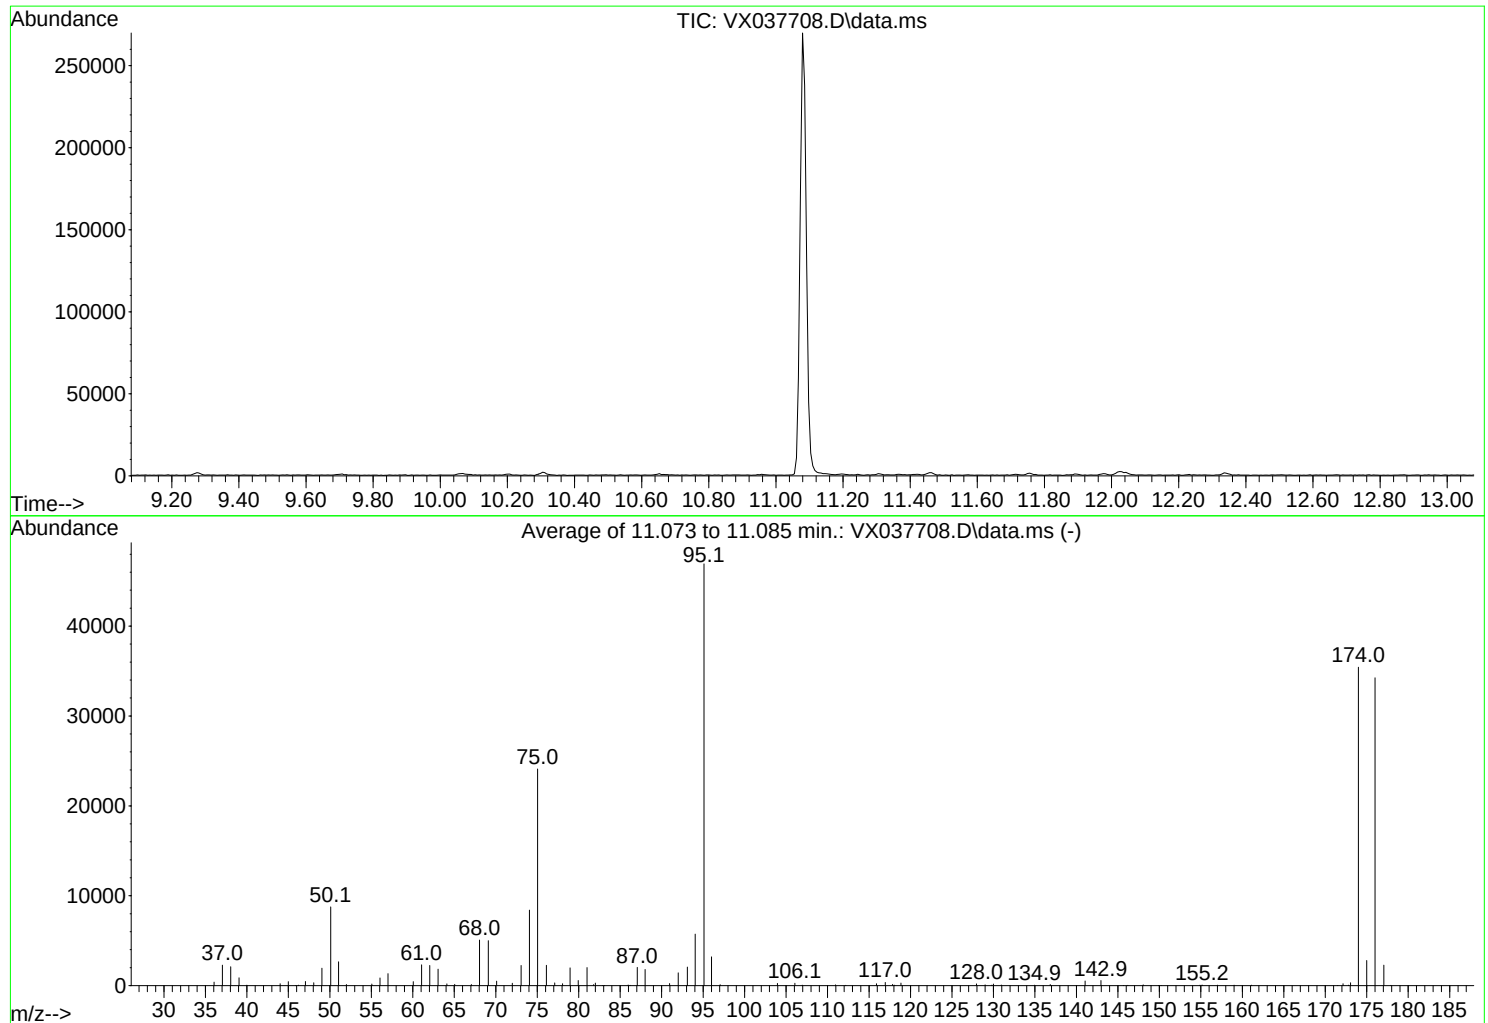

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	8766	PASS
75	95	30	60	51.4	24099	PASS
95	95	100	100	100.0	46928	PASS
96	95	5	9	6.8	3208	PASS
173	174	0.00	2	0.9	325	PASS
174	95	50	100	75.5	35429	PASS
175	174	5	9	7.9	2802	PASS
176	174	95	101	96.7	34259	PASS
177	176	5	9	6.7	2283	PASS