

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091418\
 Data File : VX004544.D
 Acq On : 14 Sep 2018 17:07
 Operator : JC/MD
 Sample : J4897-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-CLASS-DRUMS

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.605	67	74	77	rVB5	7529	15045	1.04%	0.172%
2	2.446	207	212	221	rVB	12749	20623	1.43%	0.236%
3	5.500	702	713	726	rBV	187948	528870	36.58%	6.042%
4	5.665	729	740	761	rVB	261264	739846	51.18%	8.453%
5	6.067	795	806	826	rBV2	193446	509228	35.23%	5.818%
6	6.860	926	936	955	rBV	370452	878213	60.75%	10.033%
7	8.719	1234	1241	1248	rBV	932648	1445617	100.00%	16.516%
8	8.787	1248	1252	1263	rVB	16755	30237	2.09%	0.345%
9	10.116	1464	1470	1484	rBV	775454	1044375	72.24%	11.932%
10	10.359	1505	1510	1517	rVB	22130	29165	2.02%	0.333%
11	11.140	1632	1638	1649	rBV	798367	989950	68.48%	11.310%
12	11.810	1742	1748	1752	rBV	11726	17075	1.18%	0.195%
13	12.079	1786	1792	1799	rBV	1006898	1212063	83.84%	13.848%
14	12.371	1836	1840	1848	rVB5	8341	16539	1.14%	0.189%
15	12.469	1851	1856	1861	rBV	23254	30332	2.10%	0.347%
16	12.639	1869	1884	1885	rBV8	7504	21527	1.49%	0.246%
17	12.719	1893	1897	1904	rVB2	7781	14898	1.03%	0.170%
18	13.145	1953	1967	1988	rVB3	94548	488119	33.77%	5.577%
19	13.834	2070	2080	2086	rBV	269264	366355	25.34%	4.186%
20	14.328	2149	2161	2167	rBV4	26108	91833	6.35%	1.049%
21	14.377	2167	2169	2176	rVB4	10353	16857	1.17%	0.193%
22	14.694	2216	2221	2226	rBV	48573	65242	4.51%	0.745%
23	14.840	2240	2245	2250	rBV	32318	43966	3.04%	0.502%
24	15.273	2313	2316	2321	rVB	12248	17259	1.19%	0.197%
25	15.547	2357	2361	2371	rVB5	14449	32092	2.22%	0.367%
26	15.688	2377	2384	2387	rBV2	11722	21078	1.46%	0.241%
27	16.175	2458	2464	2469	rBV	25113	43264	2.99%	0.494%
28	16.413	2496	2503	2512	rBV	12176	23254	1.61%	0.266%


Sum of corrected areas: 8752922

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091418\
Data File : VX004544.D
Acq On : 14 Sep 2018 17:07
Operator : JC/MD
Sample : J4897-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-CLASS-DRUMS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

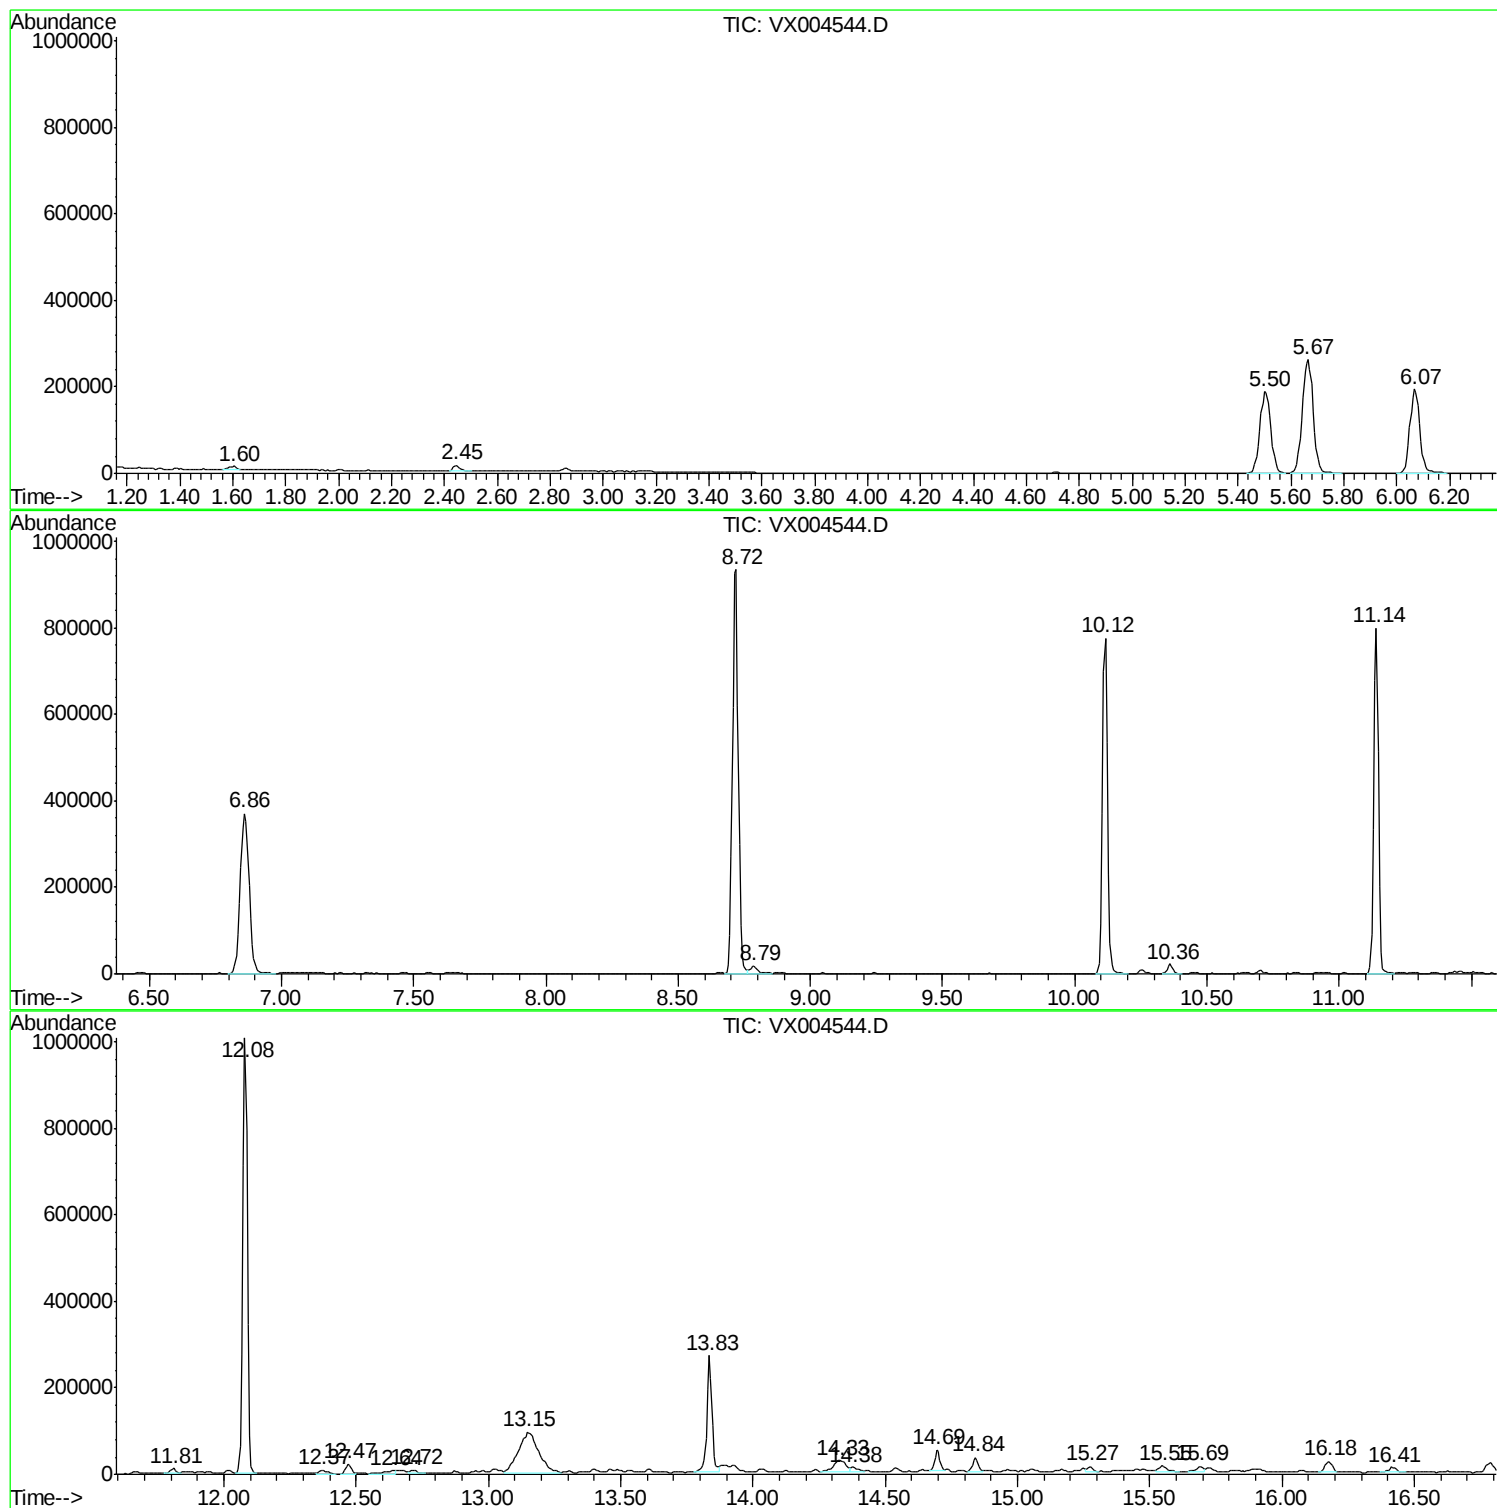

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091418\
Data File : VX004544.D
Acq On : 14 Sep 2018 17:07
Operator : JC/MD
Sample : J4897-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-CLASS-DRUMS










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.15	20.14 ug/l	488119	1,4-Dichlorobenzene-d4	12.08

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Fluorene	166	C13H10	000086-73-7	95
2		3-Trifluoromethylbenzhydryl chlo...	270	C14H10ClF3	067240-79-3	72
3		1H-Phenylene	166	C13H10	000203-80-5	53
4		Benzaldehyde, 2,4-dihydroxy-3,6-...	166	C9H10O3	034883-14-2	38
5		Spiro[4.5]decane-6,10-dione	166	C10H14O2	006684-66-8	22

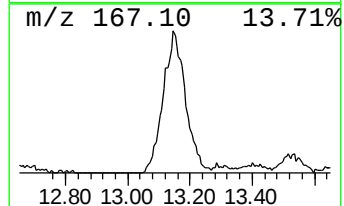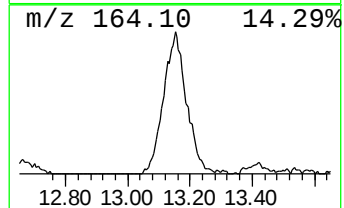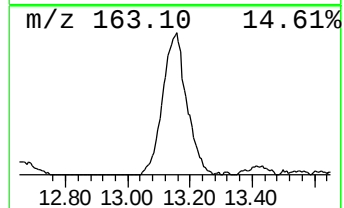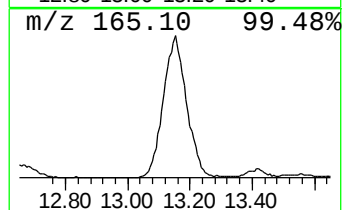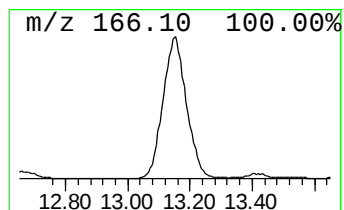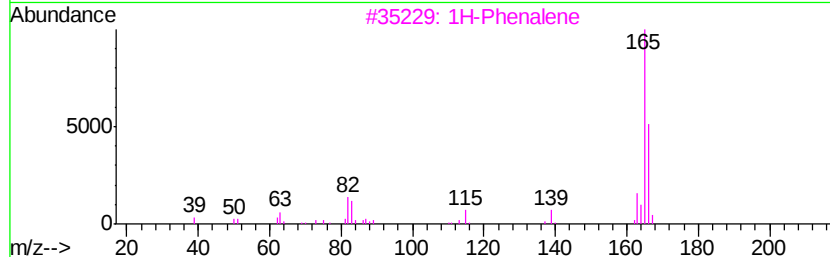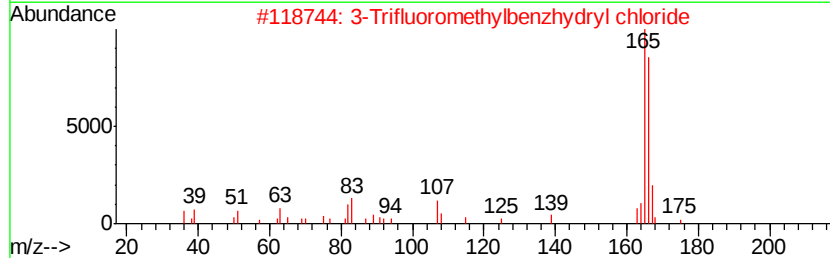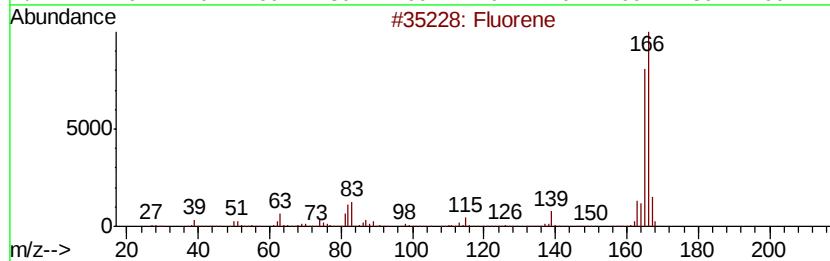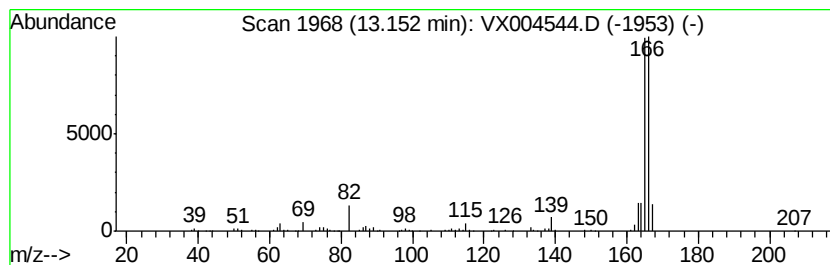

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX091418\
Data File : VX004544.D
Acq On : 14 Sep 2018 17:07
Operator : JC/MD
Sample : J4897-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-CLASS-DRUMS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorene	13.15	20.1	ug/l	488119	4	12.08	1212060	50.0