

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
 Data File : VX024228.D
 Acq On : 15 Sep 2021 00:08
 Operator : JC/MD
 Sample : PB139075ZHE#01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB139075ZHE#01

Quant Time: Sep 15 02:00:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	133474	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	228144	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	220407	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90123	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	99677	52.371	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.740%			
35) Dibromofluoromethane	5.397	113	77528	50.671	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.340%			
50) Toluene-d8	8.653	98	285655	51.249	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.500%			
62) 4-Bromofluorobenzene	11.085	95	102517	47.261	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 94.520%			
Target Compounds						Qvalue
3) Chloromethane	1.301	50	268	0.200	ug/l #	42
5) Bromomethane	1.618	94	618	0.779	ug/l	81
6) Chloroethane	1.697	64	209	2.187	ug/l #	43
10) Methyl Iodide	2.465	142	1003	0.552	ug/l #	89
11) Tert butyl alcohol	2.971	59	1660	Below Cal	#	82
13) Acrolein	2.252	56	121	0.965	ug/l	85
16) Acetone	2.386	43	46513	57.314	ug/l #	85
17) Carbon Disulfide	2.514	76	731	0.237	ug/l #	75
18) Methyl Acetate	2.715	43	990	0.389	ug/l #	78
20) Methylene Chloride	2.794	84	19070	12.237	ug/l	90
25) 2-Butanone	4.574	43	8387	7.017	ug/l	95
29) Tetrahydrofuran	5.038	42	966	1.291	ug/l #	91
31) Cyclohexane	5.562	56	3067	1.378	ug/l #	22
36) 1,1-Dichloropropene	5.562	75	10447	4.981	ug/l #	49
38) Carbon Tetrachloride	5.562	117	14304	6.059	ug/l #	16
41) Methacrylonitrile	5.044	41	836	0.641	ug/l #	35
43) Isopropyl Acetate	6.348	43	18865	4.849	ug/l	95
48) Methyl methacrylate	7.806	41	110605	56.977	ug/l #	37
49) 1,4-Dioxane	7.806	88	193	4.748	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	70635	28.491	ug/l #	46
54) cis-1,3-Dichloropropene	8.555	75	29158	11.496	ug/l #	69
56) Ethyl methacrylate	9.013	69	126	1.406	ug/l #	29
57) 1,3-Dichloropropane	9.488	76	19564	7.154	ug/l #	42
59) 2-Hexanone	9.488	43	279798	144.838	ug/l #	43
60) Dibromochloromethane	9.281	129	86	1.770	ug/l #	11
74) N-amyl acetate	10.768	43	984	0.348	ug/l #	39
76) 1,2,3-Trichloropropane	11.085	75	54974	26.528	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	54974	78.019	ug/l #	12
95) Naphthalene	13.786	128	433	1.353	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
Data File : VX024228.D
Acq On : 15 Sep 2021 00:08
Operator : JC/MD
Sample : PB139075ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01

Quant Time: Sep 15 02:00:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 14 12:18:04 2021
Response via : Initial Calibration




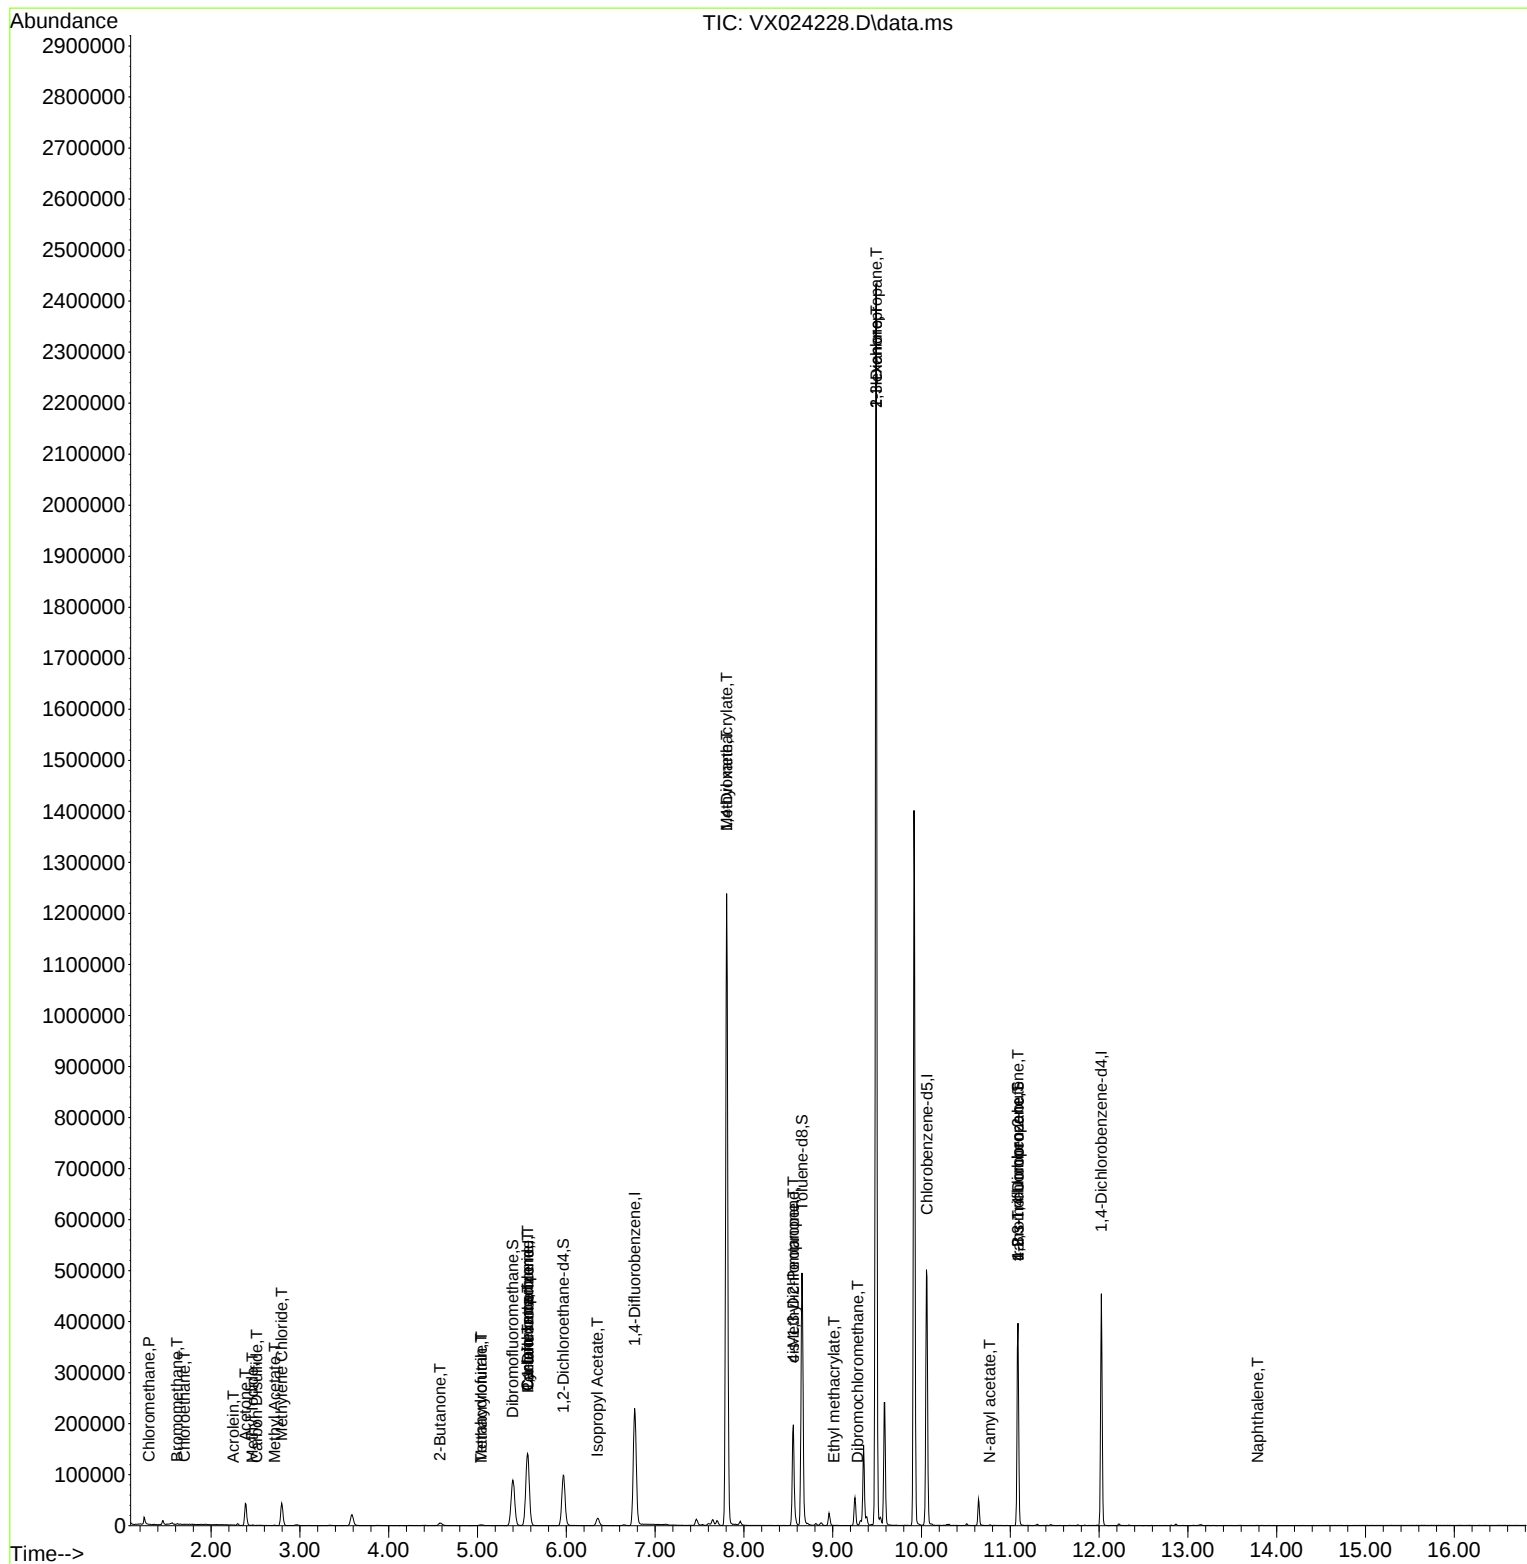


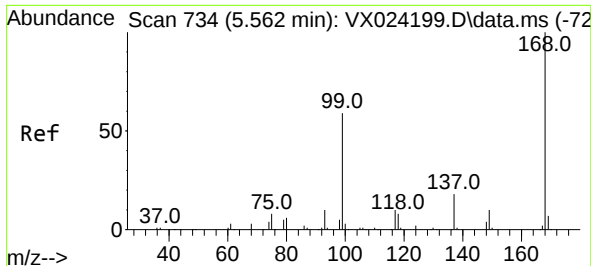

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.006 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion:168 Resp: 133474
Ion Ratio Lower Upper
168 100
99 56.6 45.8 68.6

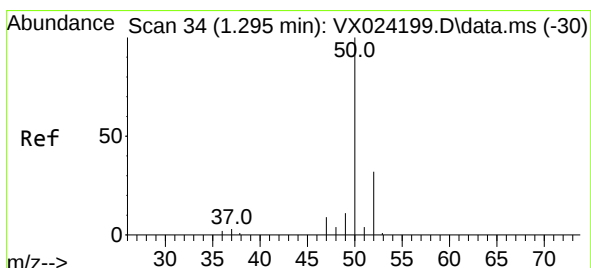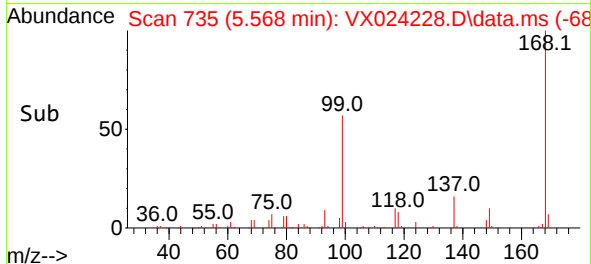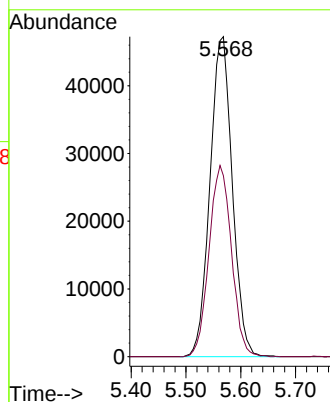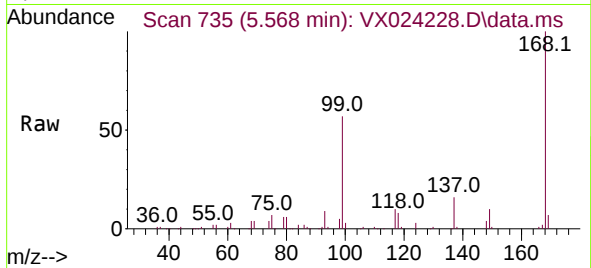

#3
Chloromethane
Concen: 0.200 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 50 Resp: 268
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#


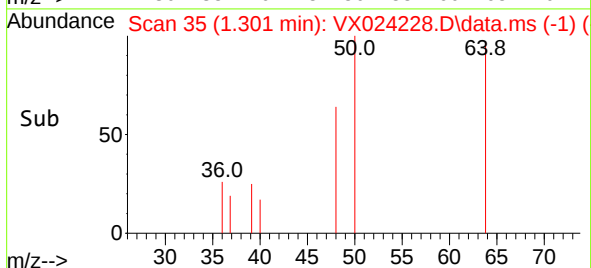

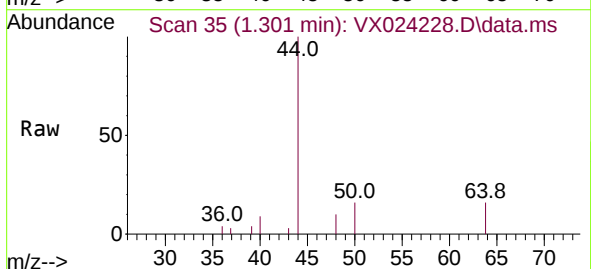


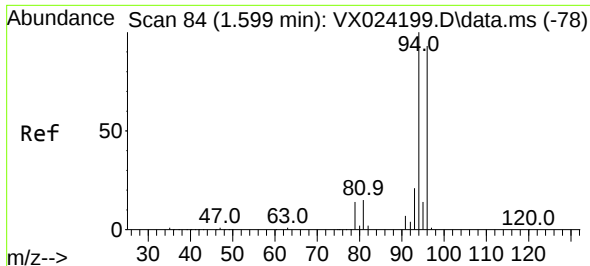

#5
Bromomethane
Concen: 0.779 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 94 Resp: 618
Ion Ratio Lower Upper
94 100
96 77.3 76.4 114.6

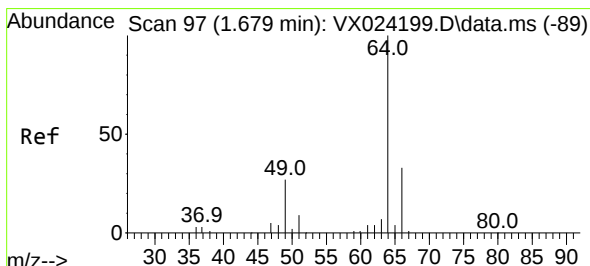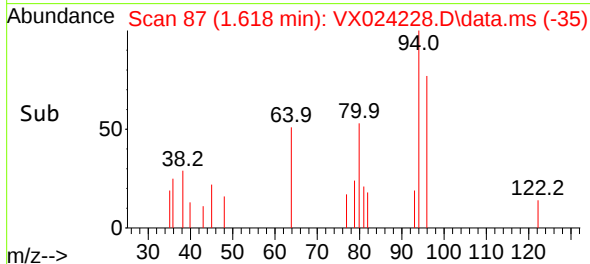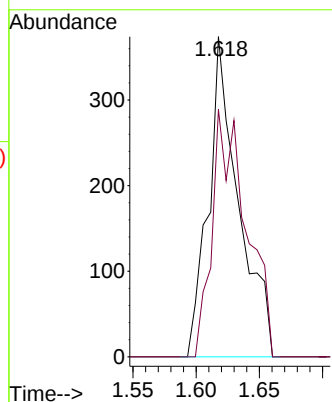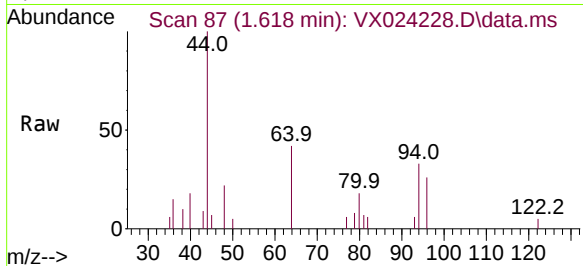

#6
Chloroethane
Concen: 2.187 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.018 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08


Tgt Ion: 64 Resp: 209
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

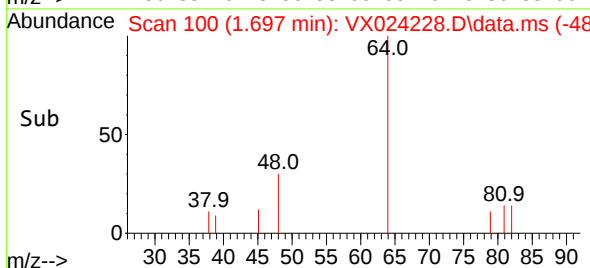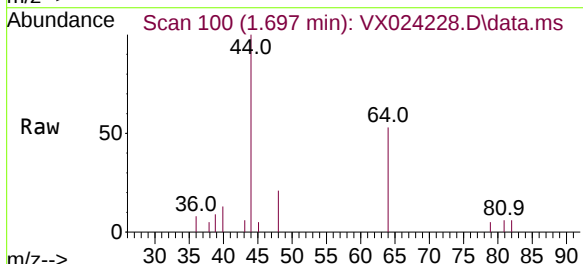






#10
Methyl Iodide
Concen: 0.552 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08


Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01

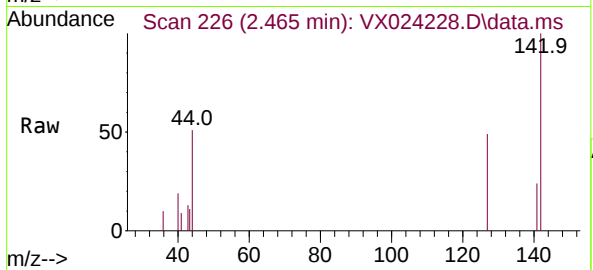



Tgt Ion:142 Resp: 1003
Ion Ratio Lower Upper
142 100
127 49.3 33.3 49.9
141 11.0 11.4 17.0#

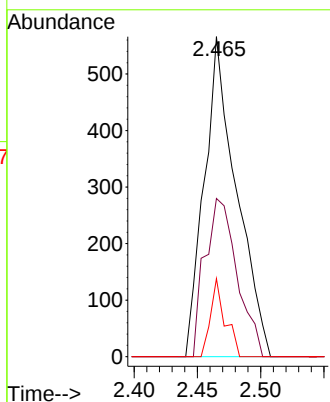


#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

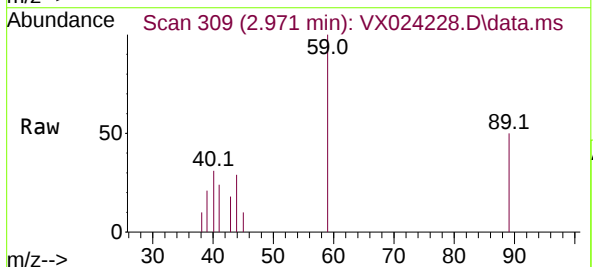

Tgt Ion: 59 Resp: 1660
Ion Ratio Lower Upper
59 100
57 3.1 7.8 11.8#









#13
Acrolein
Concen: 0.965 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.006 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 56 Resp: 121
Ion Ratio Lower Upper
56 100
55 57.9 56.4 84.6

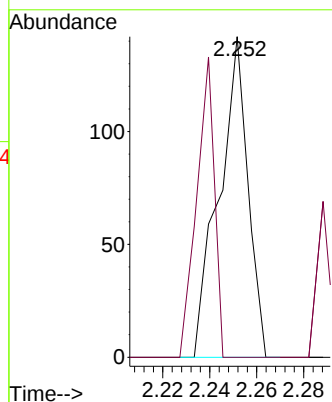

#16
Acetone
Concen: 57.314 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 43 Resp: 46513
Ion Ratio Lower Upper
43 100
58 26.1 27.8 41.8#

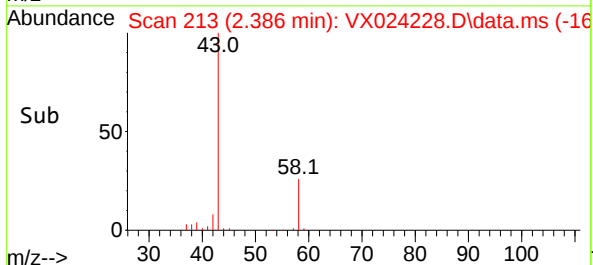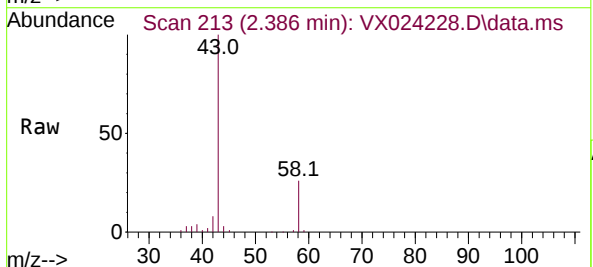



#17

Carbon Disulfide

Concen: 0.237 ug/l

RT: 2.514 min Scan# 234

Delta R.T. -0.000 min

Lab File: VX024228.D





Acq: 15 Sep 2021 00:08

Tgt Ion: 76 Resp: 731

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#

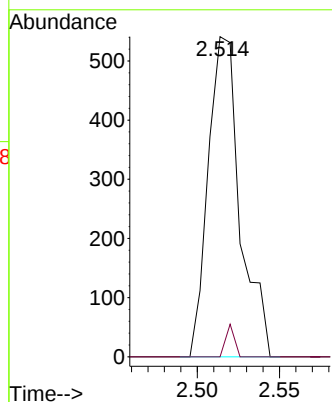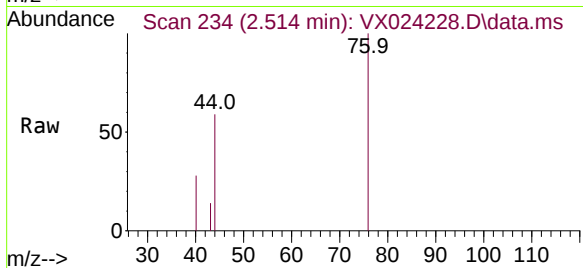

#18

Methyl Acetate

Concen: 0.389 ug/l

RT: 2.715 min Scan# 267

Delta R.T. 0.000 min

Lab File: VX024228.D




Acq: 15 Sep 2021 00:08


Tgt Ion: 43 Resp: 990

Ion Ratio Lower Upper

43 100

74 16.0 21.9 32.9#

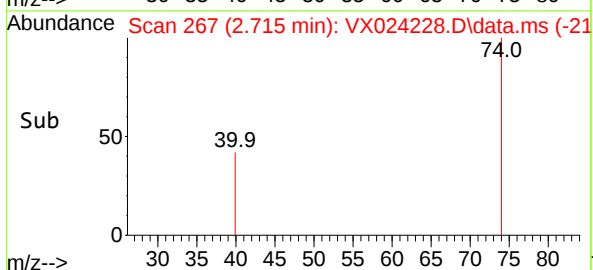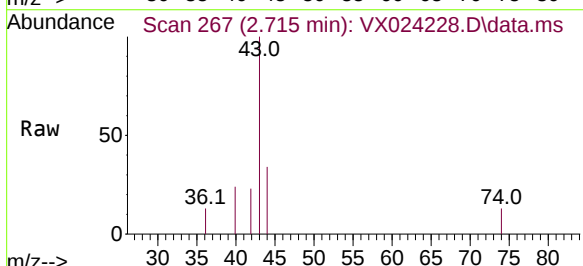

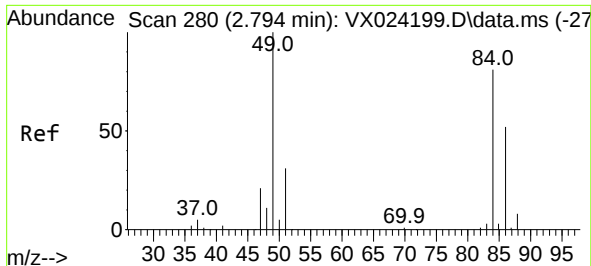

#20

Methylene Chloride

Concen: 12.237 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.000 min

Lab File: VX024228.D

Acq: 15 Sep 2021 00:08

Instrument :

MSVOA_X

ClientSampleId :

PB139075ZHE#01

Tgt Ion: 84 Resp: 19070





Ion Ratio Lower Upper

84 100

49 127.2 88.6 132.8

51 38.6 27.0 40.6

86 62.1 50.3 75.5

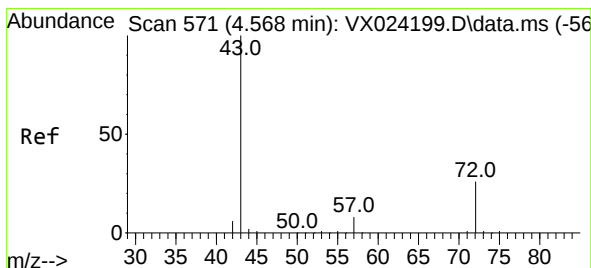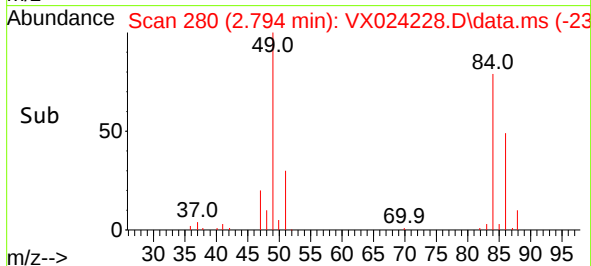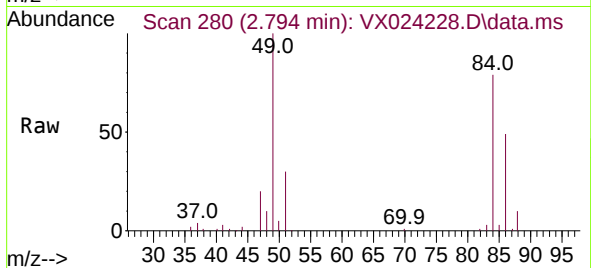

#25

2-Butanone

Concen: 7.017 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.006 min

Lab File: VX024228.D




Acq: 15 Sep 2021 00:08


Tgt Ion: 43 Resp: 8387

Ion Ratio Lower Upper

43 100

72 26.7 23.7 35.5

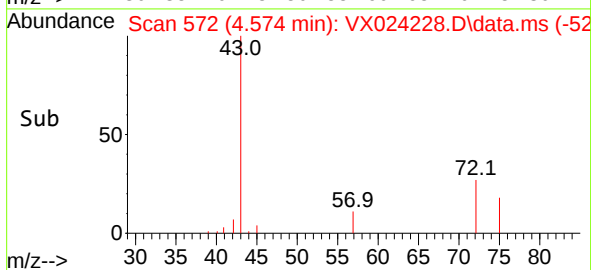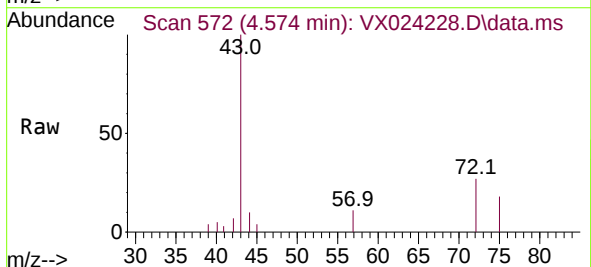



#29

Tetrahydrofuran

Concen: 1.291 ug/l

RT: 5.038 min Scan# 648

Delta R.T. 0.019 min

Lab File: VX024228.D

Acq: 15 Sep 2021 00:08





Instrument :

MSVOA_X

ClientSampleId :

PB139075ZHE#01

Tgt Ion:	42	Resp:	966
Ion	Ratio	Lower	Upper
42	100		
72	54.6	41.7	62.5
71	37.5	38.4	57.6#

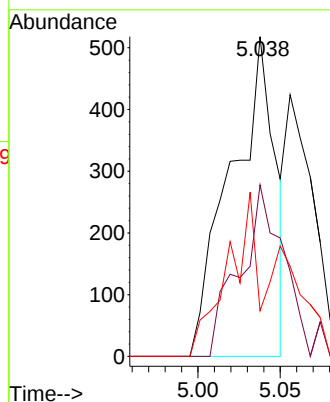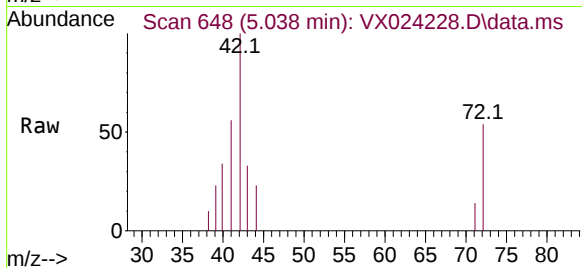

#31

Cyclohexane

Concen: 1.378 ug/l




RT: 5.562 min Scan# 734


Delta R.T. 0.085 min

Lab File: VX024228.D

Acq: 15 Sep 2021 00:08

Tgt Ion:	56	Resp:	3067
Ion	Ratio	Lower	Upper
56	100		
69	159.2	25.3	37.9#
84	111.5	71.4	107.0#

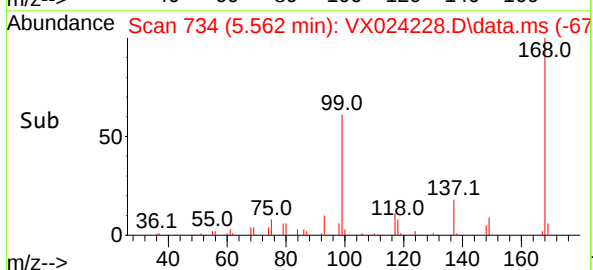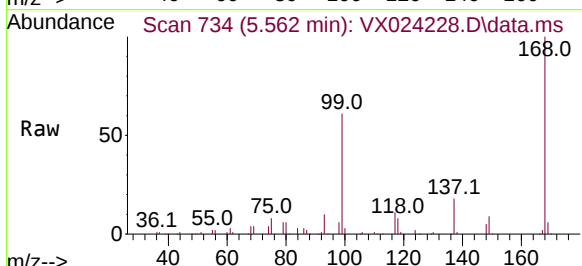



#33

1,2-Dichloroethane-d4

Concen: 52.371 ug/l

RT: 5.964 min Scan# 800

Delta R.T. -0.007 min

Lab File: VX024228.D





Acq: 15 Sep 2021 00:08

Tgt Ion: 65 Resp: 99677

Ion Ratio Lower Upper

65 100

67 50.4 0.0 105.4

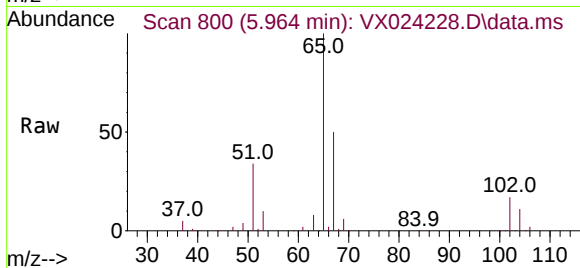

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX024228.D

Acq: 15 Sep 2021 00:08




Tgt Ion: 114 Resp: 228144


Ion Ratio Lower Upper

114 100

63 20.0 0.0 40.8

88 16.0 0.0 32.8


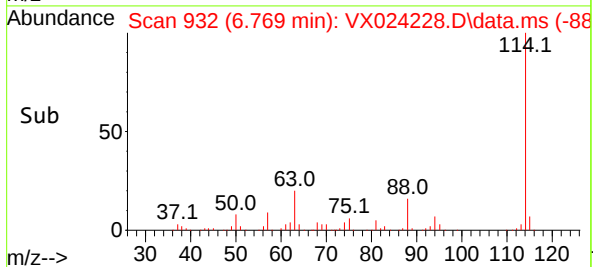

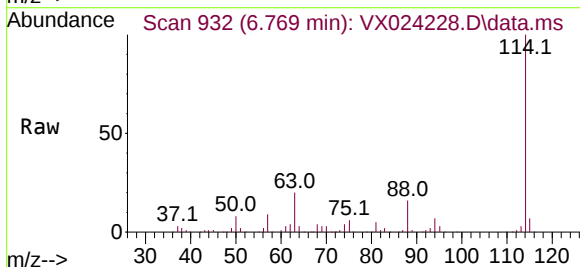




#35
Dibromofluoromethane
Concen: 50.671 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion:113 Resp: 77528
Ion Ratio Lower Upper
113 100
111 102.1 81.9 122.9
192 19.6 16.7 25.1

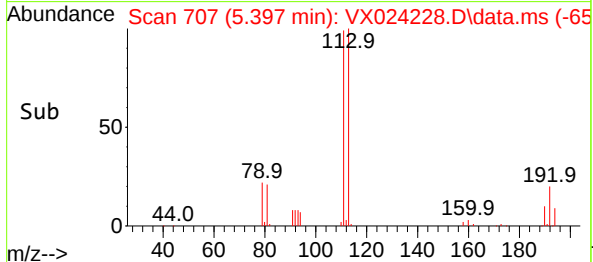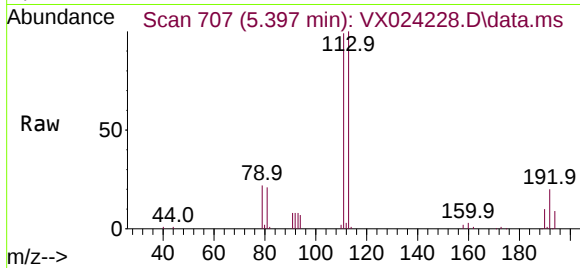

#36
1,1-Dichloropropene
Concen: 4.981 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08


Tgt Ion: 75 Resp: 10447
Ion Ratio Lower Upper
75 100
110 8.8 18.1 54.4#
77 0.0 25.3 37.9#

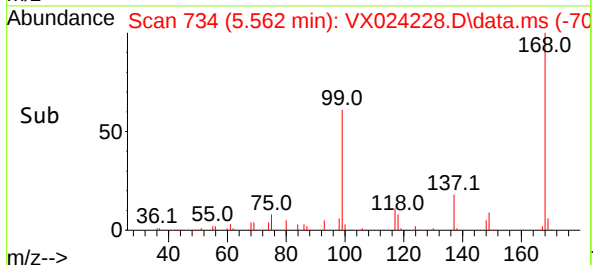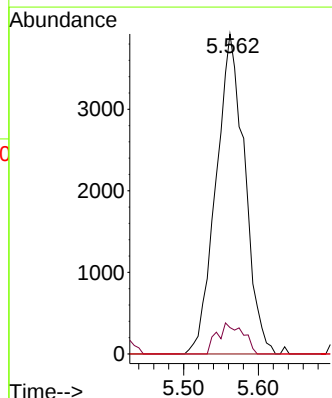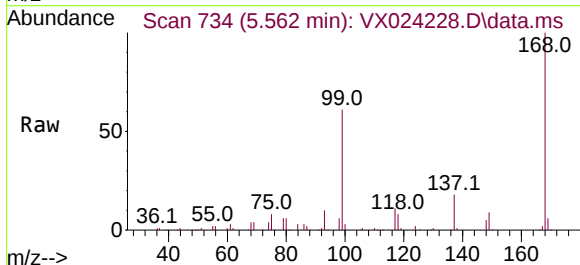






#38
Carbon Tetrachloride
Concen: 6.059 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08


Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01

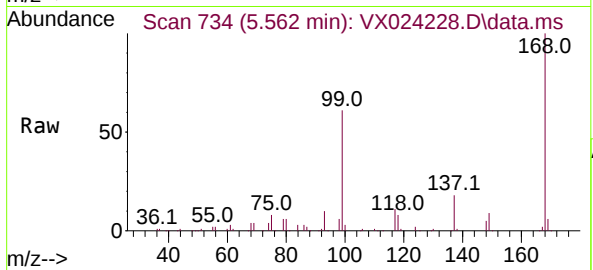



Tgt Ion: 117 Resp: 14304
Ion Ratio Lower Upper
117 100
119 4.8 76.2 114.2#
121 0.0 24.8 37.2#

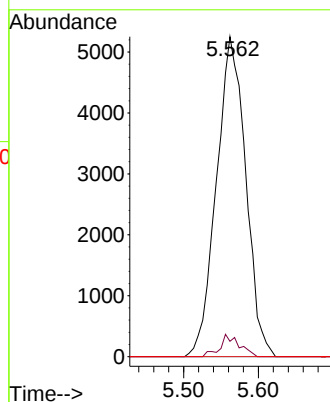


#41
Methacrylonitrile
Concen: 0.641 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.110 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

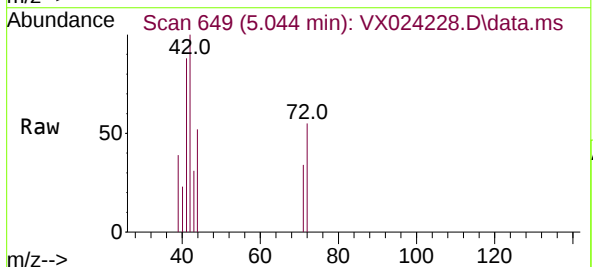

Tgt Ion: 41 Resp: 836
Ion Ratio Lower Upper
41 100
39 32.2 42.5 63.7#
67 0.0 65.0 97.6#
52 0.0 25.3 37.9#



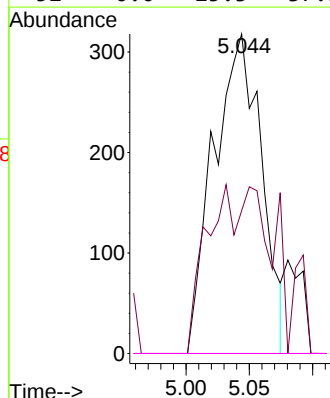





#43
Isopropyl Acetate
Concen: 4.849 ug/l
RT: 6.348 min Scan# 863
Delta R.T. -0.001 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion:	43	Resp:	18865
Ion	Ratio	Lower	Upper
43	100		
61	19.9	18.2	27.4
87	14.3	12.5	18.7

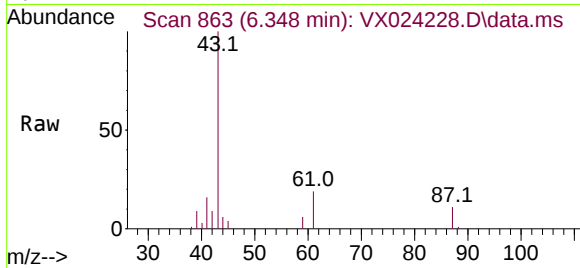

#48
Methyl methacrylate
Concen: 56.977 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.104 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion:	41	Resp:	110605
Ion	Ratio	Lower	Upper
41	100		
69	0.2	76.0	114.0#
39	53.5	44.6	67.0


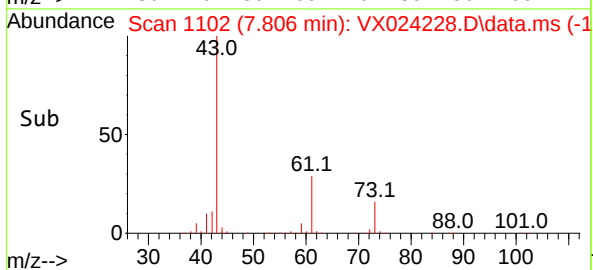

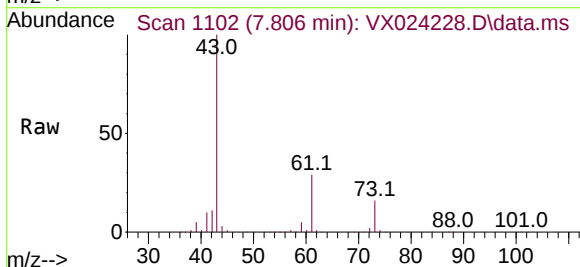




#49
1,4-Dioxane
Concen: 4.748 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.141 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 88 Resp: 193
Ion Ratio Lower Upper
88 100
43 571435.8 23.2 34.8#
58 2447.7 55.0 82.4#

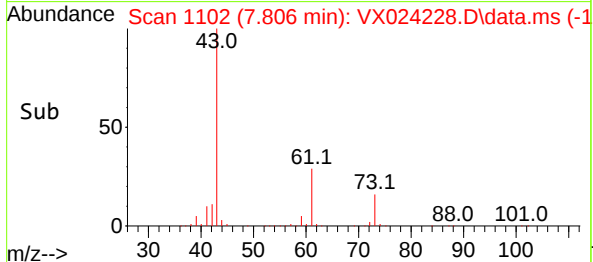

#50
Toluene-d8
Concen: 51.249 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 98 Resp: 285655
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9


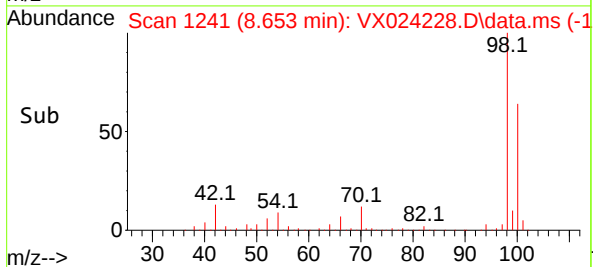

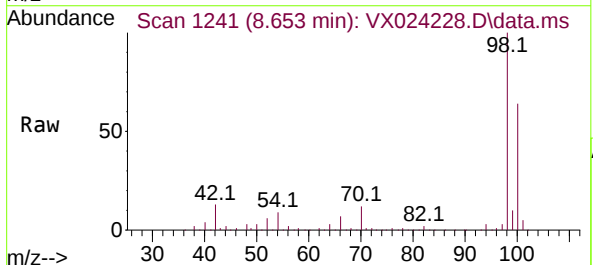




#51
4-Methyl-2-Pentanone
Concen: 28.491 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 43 Resp: 70635
Ion Ratio Lower Upper
43 100
58 9.1 35.4 53.0#

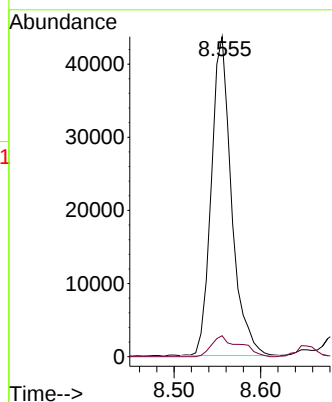

#54
cis-1,3-Dichloropropene
Concen: 11.496 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.182 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 75 Resp: 29158
Ion Ratio Lower Upper
75 100
77 0.7 25.7 38.5#
39 35.9 35.1 52.7


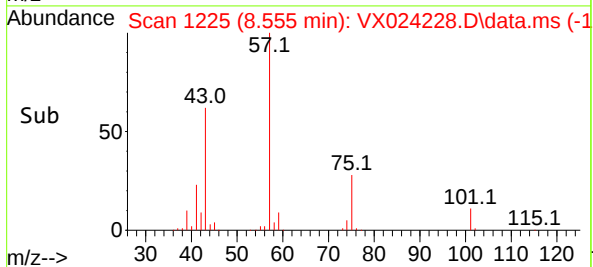
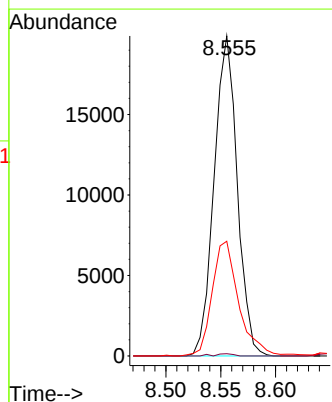
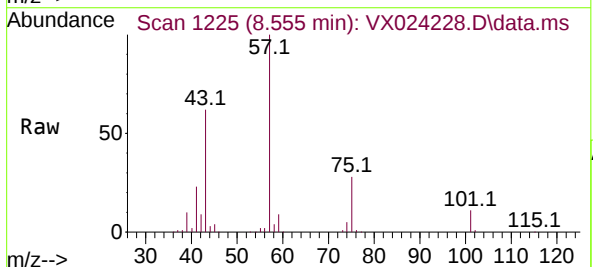




#56
Ethyl methacrylate
Concen: 1.406 ug/l
RT: 9.013 min Scan# 1300
Delta R.T. -0.109 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 69 Resp: 126
Ion Ratio Lower Upper
69 100
41 0.0 46.8 70.2#
39 0.0 24.7 37.1#

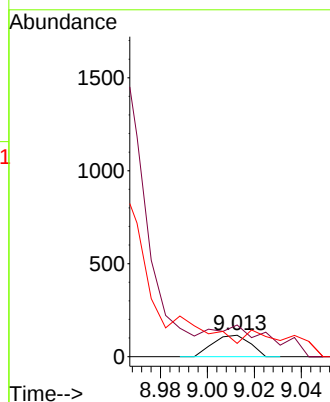

#57
1,3-Dichloropropane
Concen: 7.154 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 76 Resp: 19564
Ion Ratio Lower Upper
76 100
78 0.3 26.2 39.2#









#59
2-Hexanone
Concen: 144.838 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.055 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 43 Resp: 279798
Ion Ratio Lower Upper
43 100
58 17.7 30.9 92.8#

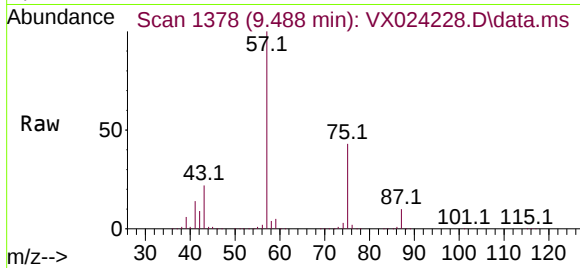

#60
Dibromochloromethane
Concen: 1.770 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.244 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 129 Resp: 86
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


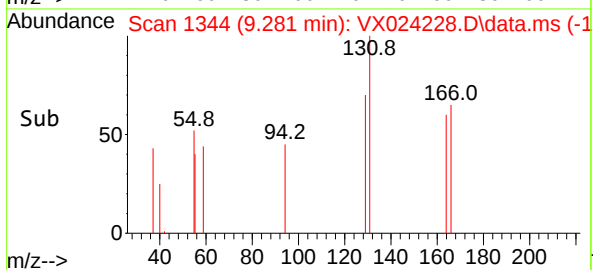

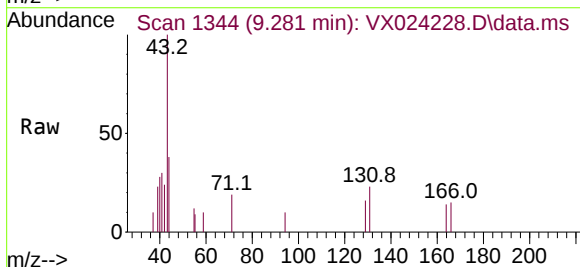


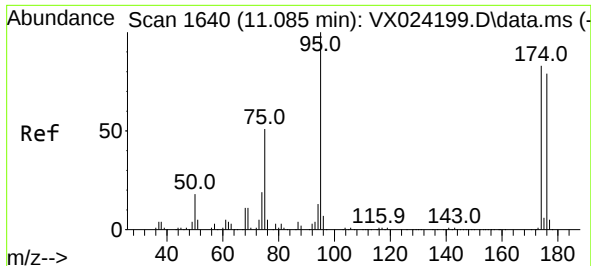

#62
4-Bromofluorobenzene
Concen: 47.261 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 95 Resp: 102517
Ion Ratio Lower Upper
95 100
174 79.2 0.0 154.6
176 76.0 0.0 155.8

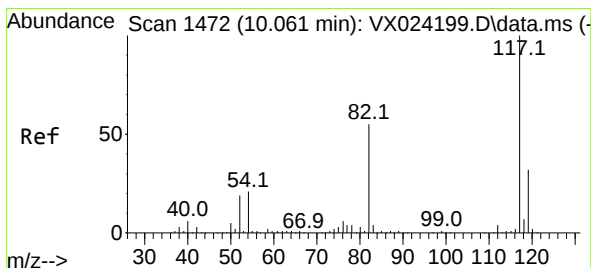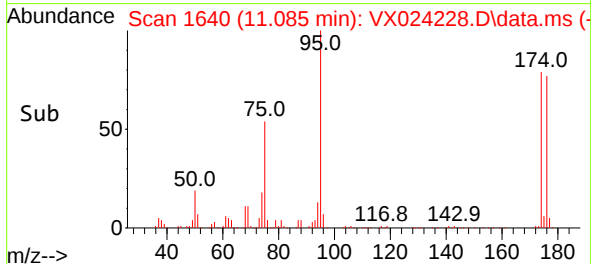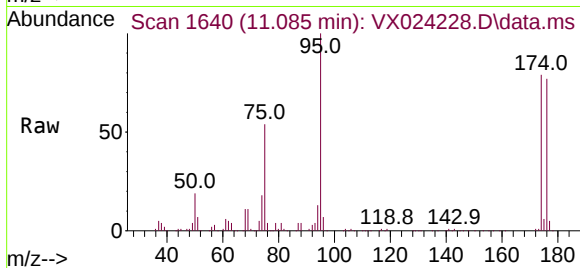

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 117 Resp: 220407
Ion Ratio Lower Upper
117 100
82 55.9 47.4 71.2
119 32.3 26.6 39.8


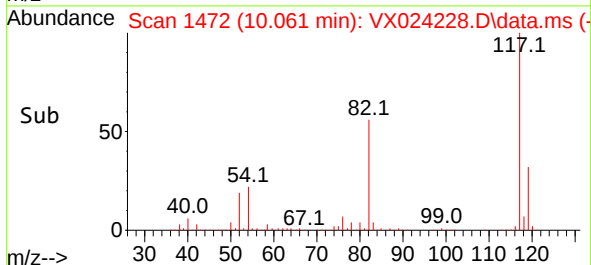
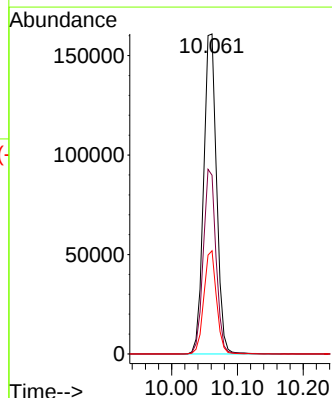
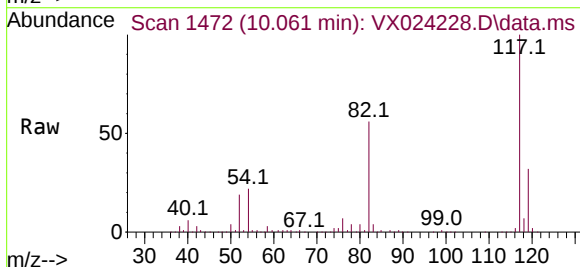


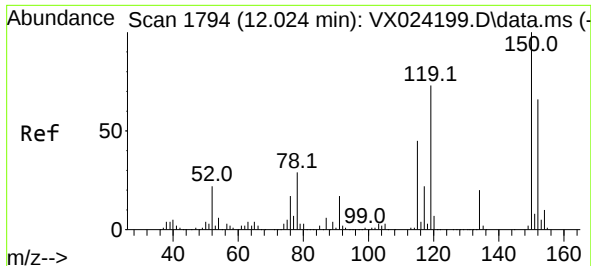

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion:152 Resp: 90123
Ion Ratio Lower Upper
152 100
115 60.9 41.1 123.3
150 158.5 0.0 349.0

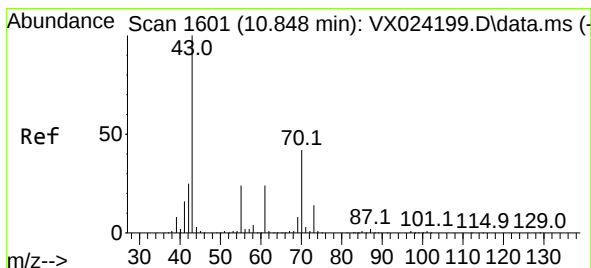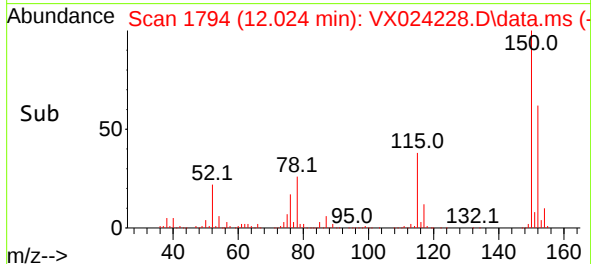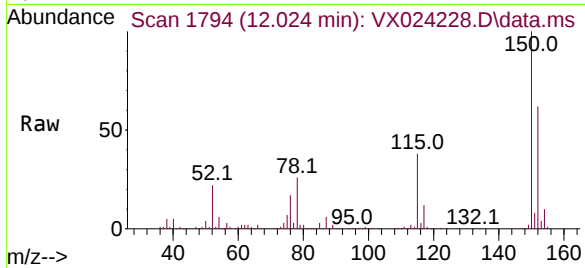

#74
N-ethyl acetate
Concen: 0.348 ug/l
RT: 10.768 min Scan# 1588
Delta R.T. -0.080 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Tgt Ion: 43 Resp: 984
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 1.9 21.5 32.3#
61 0.0 22.1 33.1#


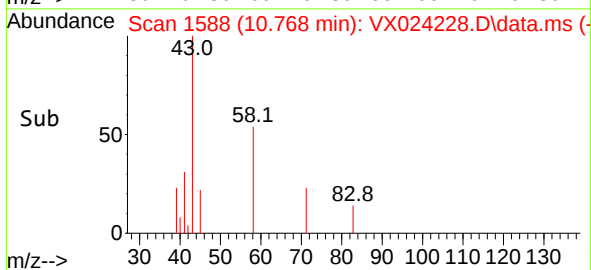

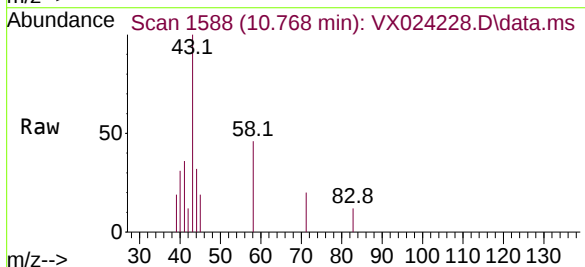


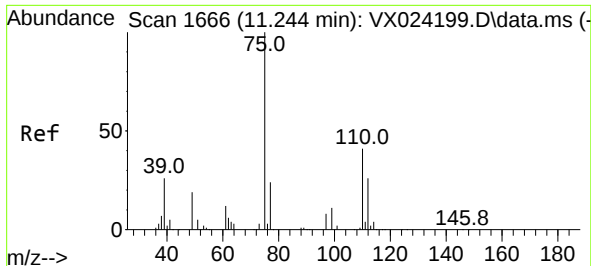

#76
1,2,3-Trichloropropane
Concen: 26.528 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08




Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01


Tgt Ion: 75 Resp: 54974
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#

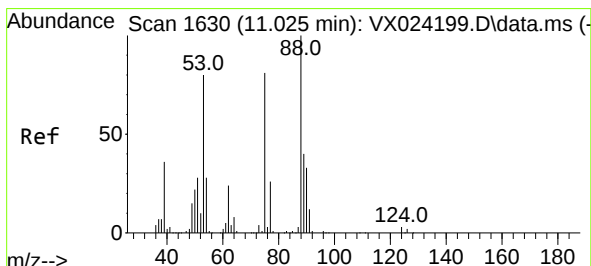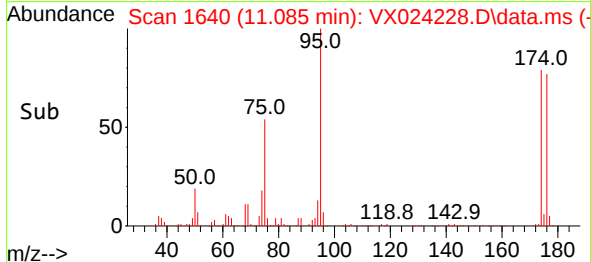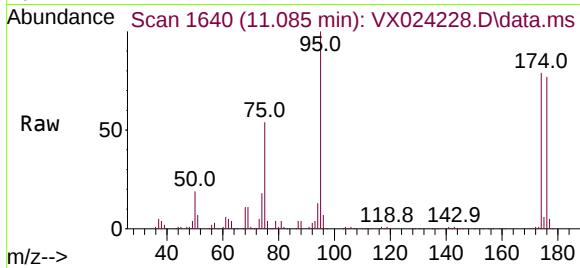

#81
trans-1,4-Dichloro-2-butene
Concen: 78.019 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08


Tgt Ion: 75 Resp: 54974
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

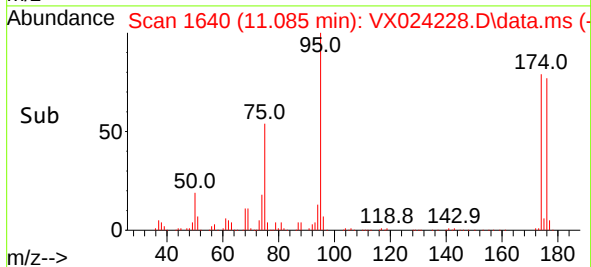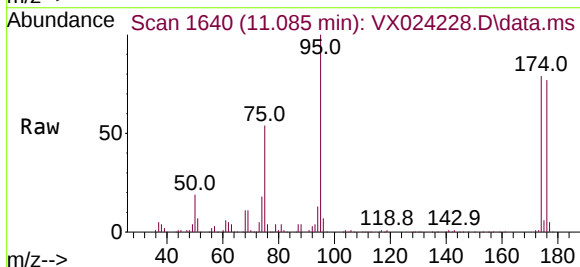

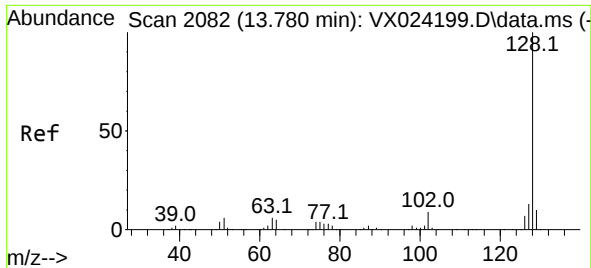

#95
Naphthalene
Concen: 1.353 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX024228.D
Acq: 15 Sep 2021 00:08

Instrument :
MSVOA_X
ClientSampleId :
PB139075ZHE#01

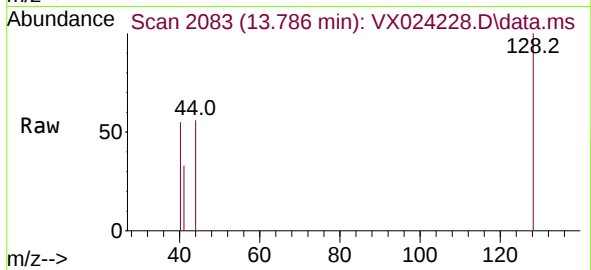

Tgt Ion:128 Resp: 433
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

