


Tert butyl alcohol

Response Ratio

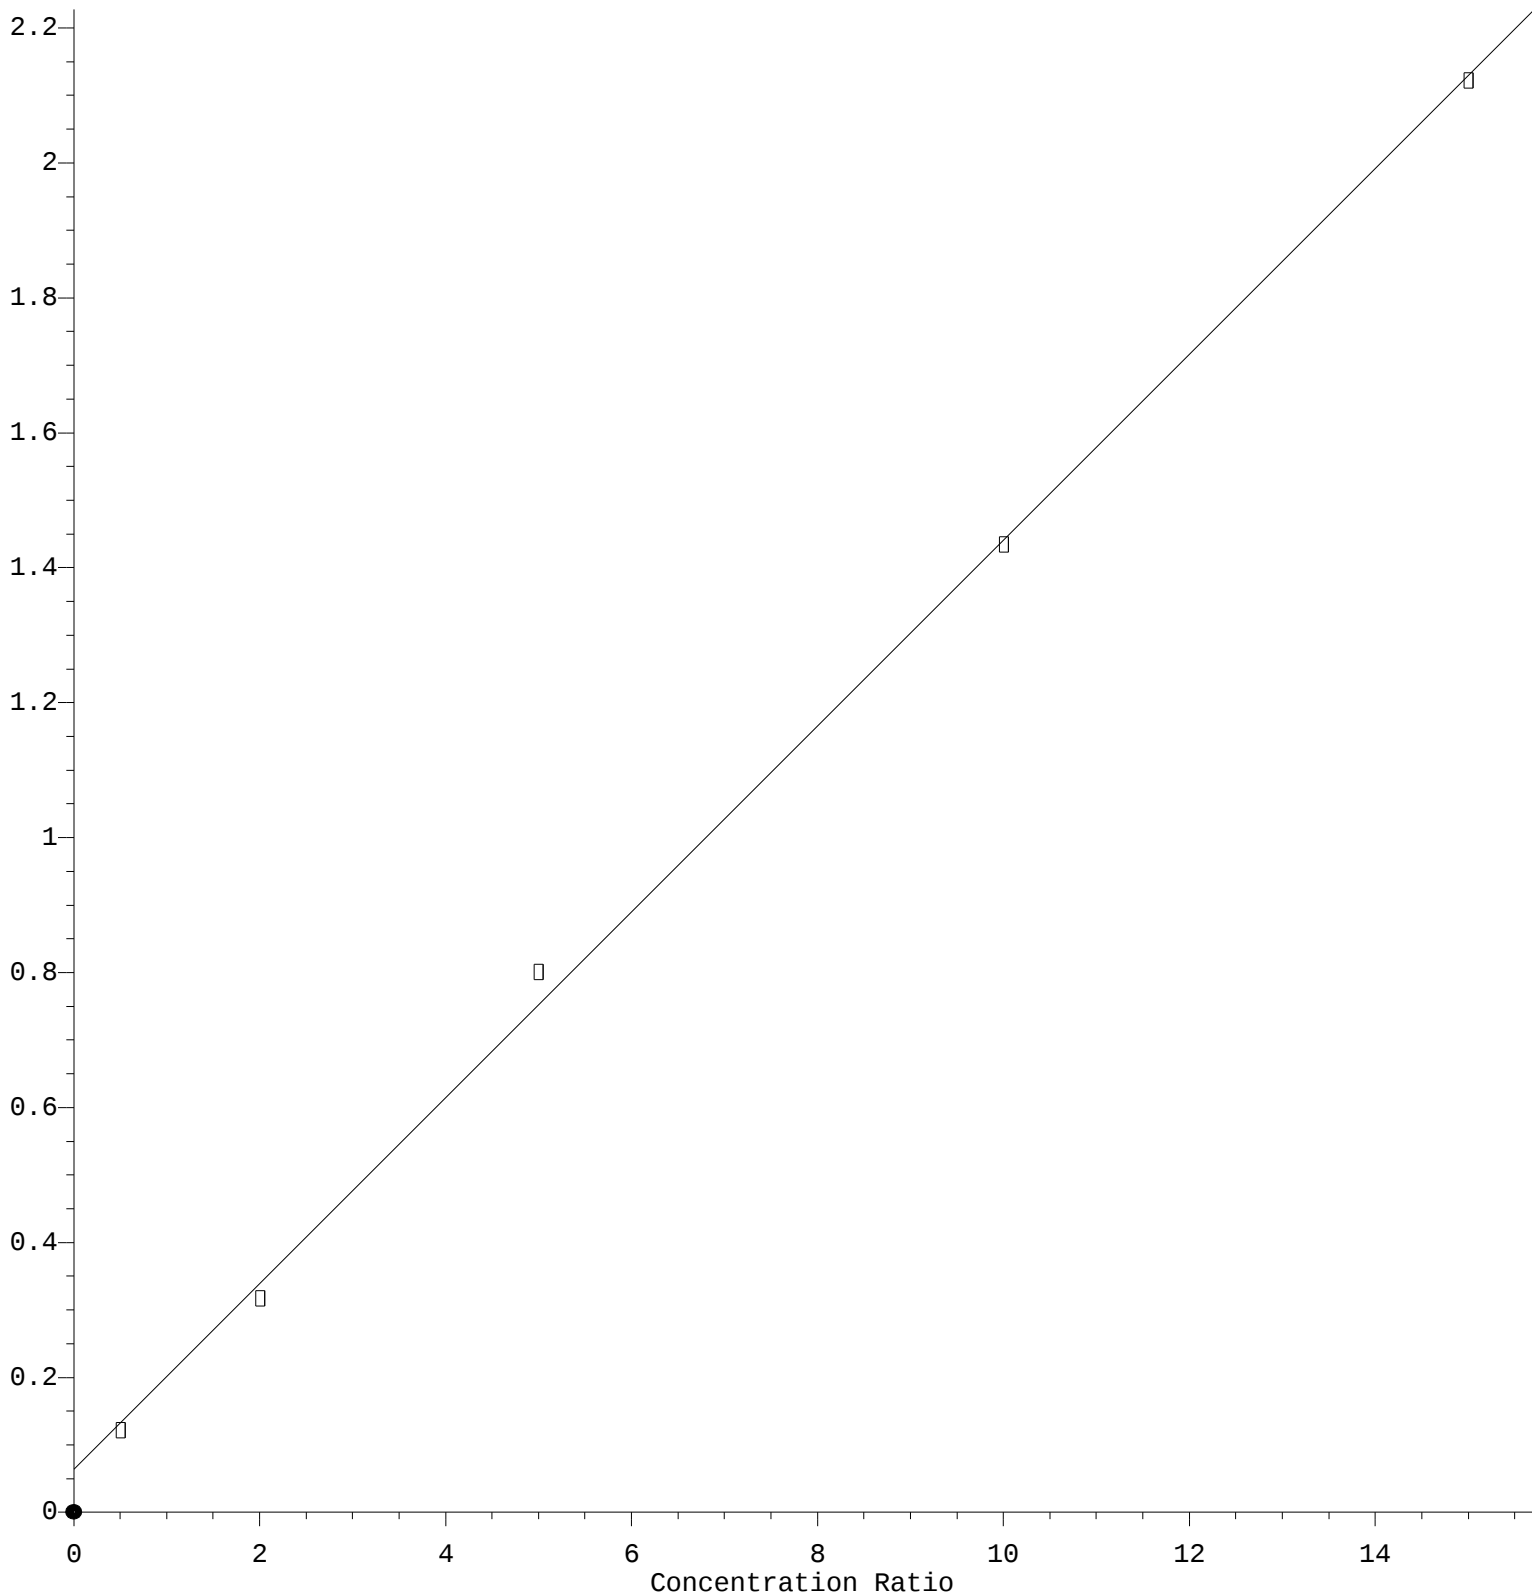

$$\text{Response} = 1.378\text{e-}001 * \text{Amt} + 6.354\text{e-}002$$


Coef of Det (r^2) = 0.998876 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Calibration Table Last Updated: Tue Sep 14 12:18:04 2021

Ethyl methacrylate

Response Ratio

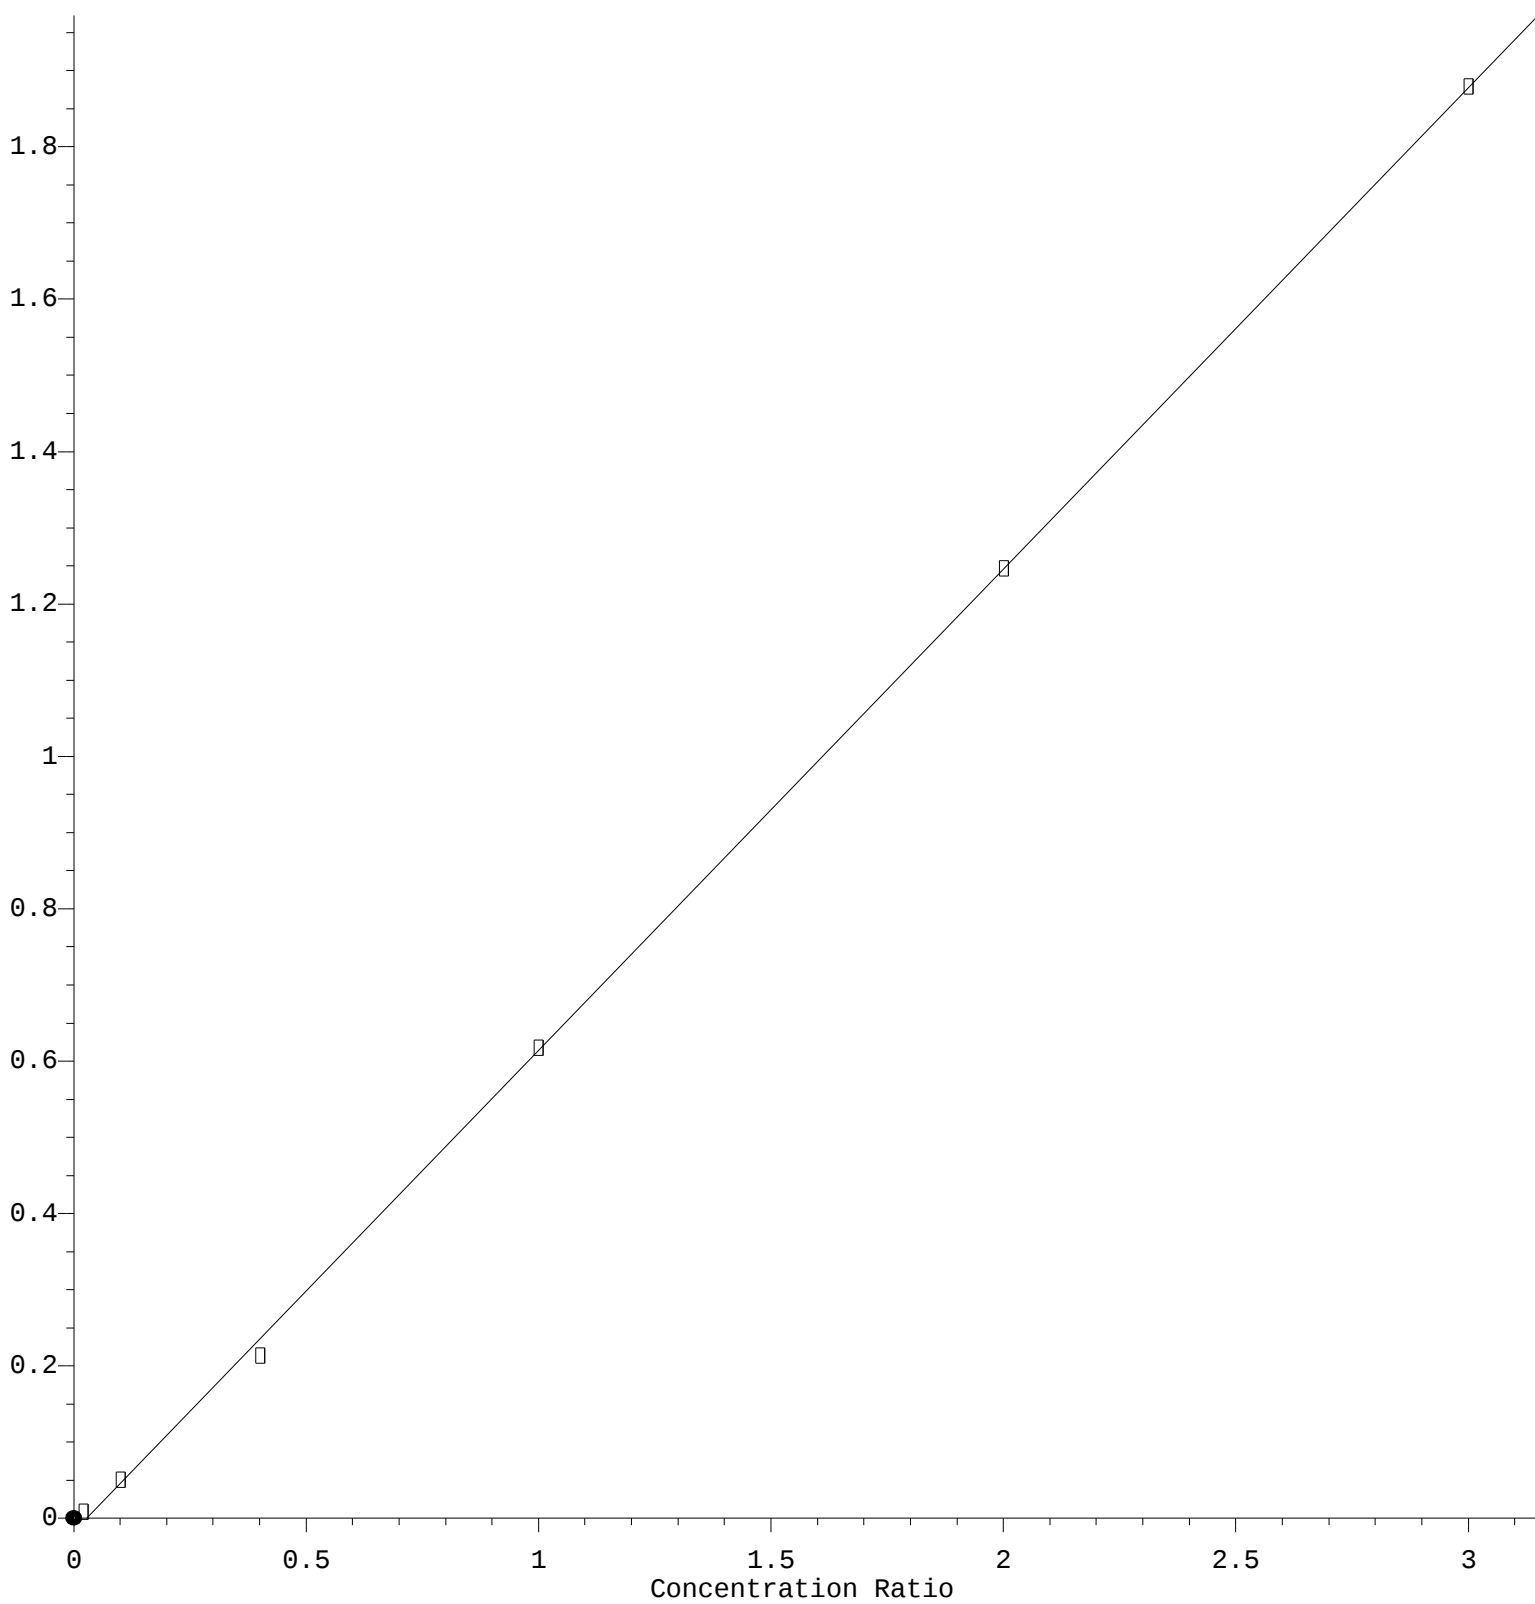

$$\text{Response} = 6.315\text{e-}001 * \text{Amt} - 1.721\text{e-}002$$


Coef of Det (r^2) = 0.999763 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Calibration Table Last Updated: Tue Sep 14 12:18:04 2021

Dibromochloromethane

Response Ratio

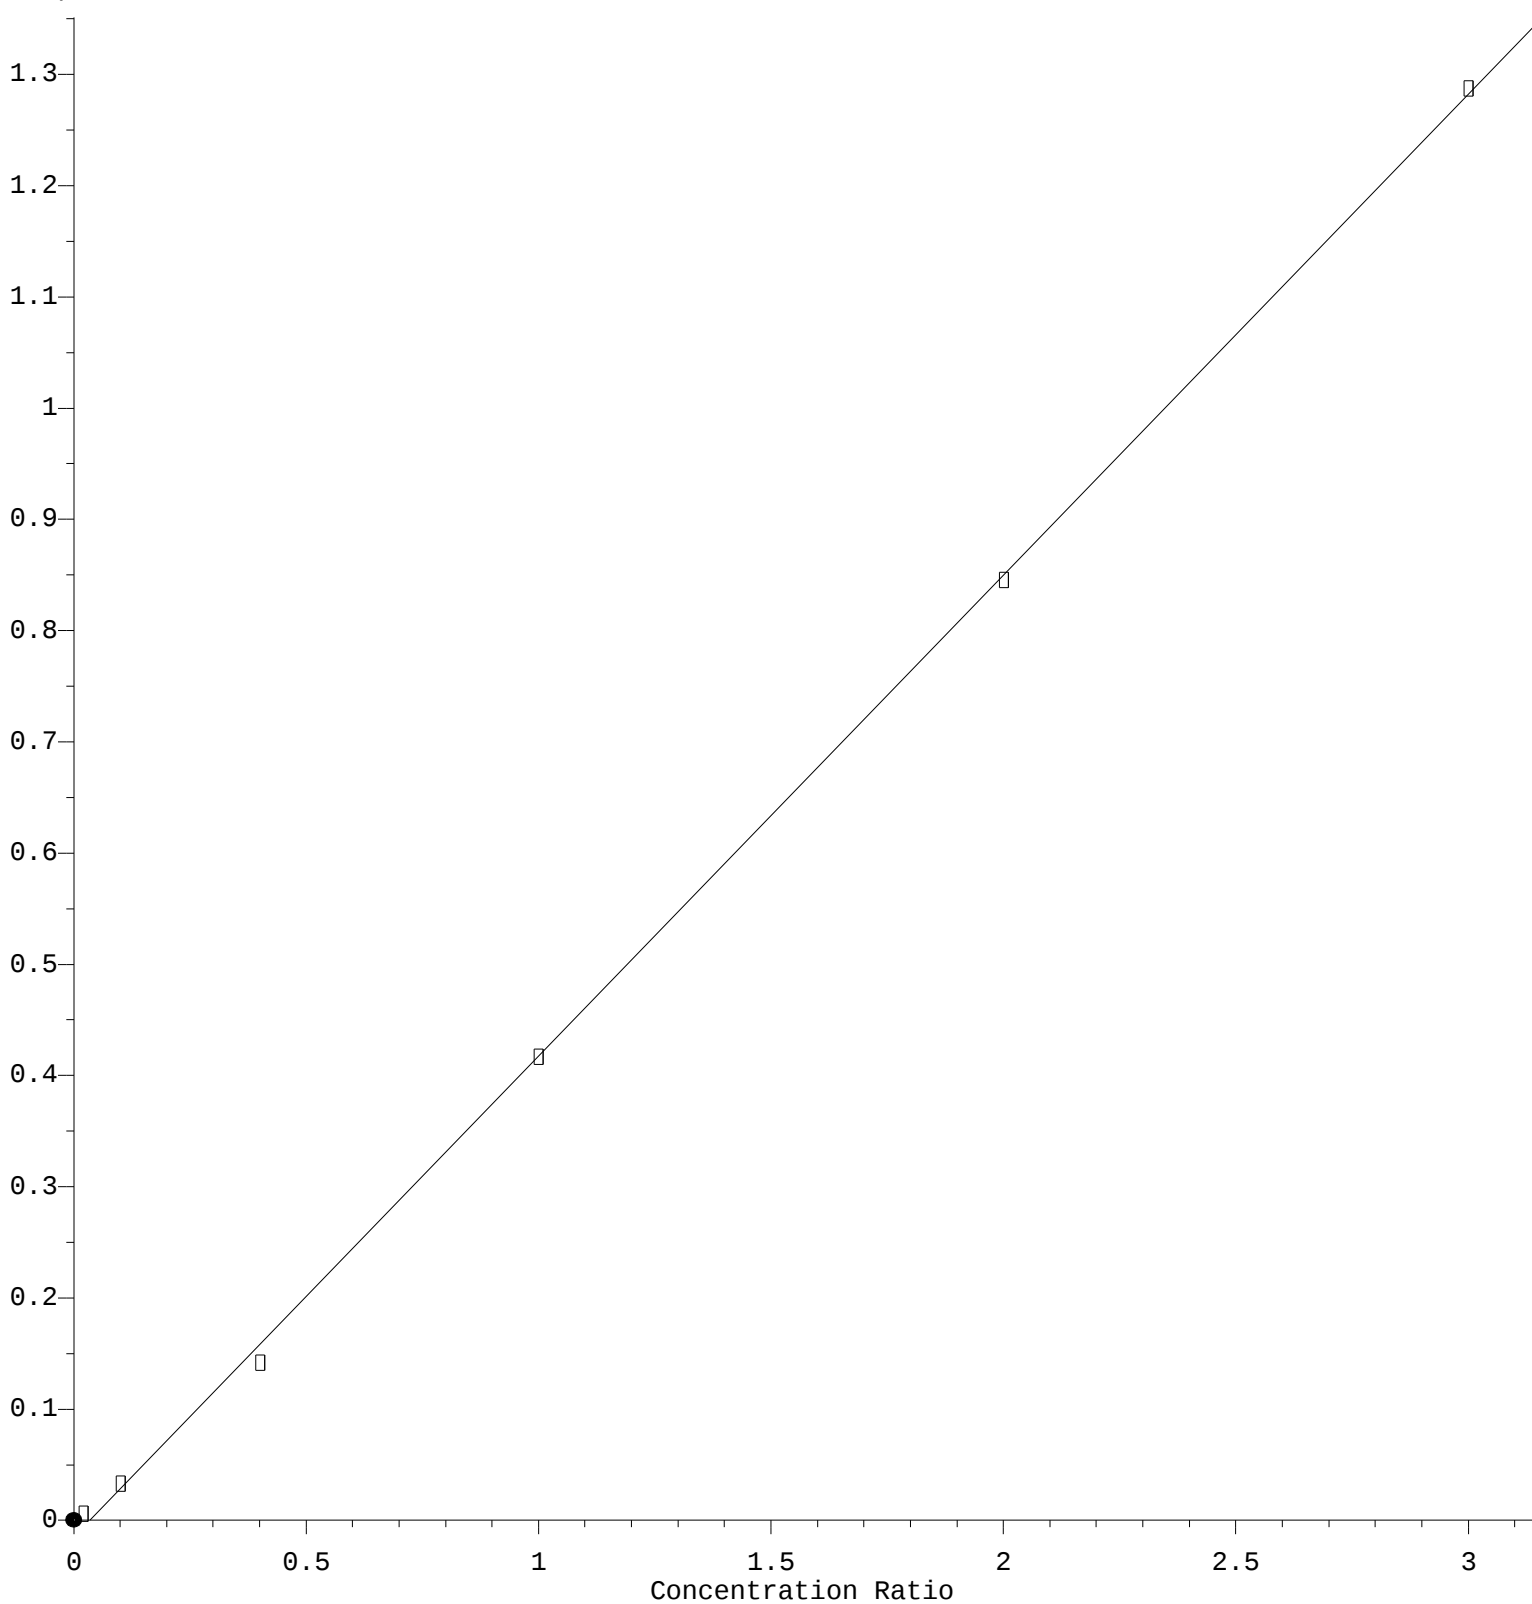

$$\text{Response} = 4.323\text{e-}001 * \text{Amt} - 1.492\text{e-}002$$


Coef of Det (r^2) = 0.999642 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Calibration Table Last Updated: Tue Sep 14 12:18:04 2021

Bromoform

Response Ratio

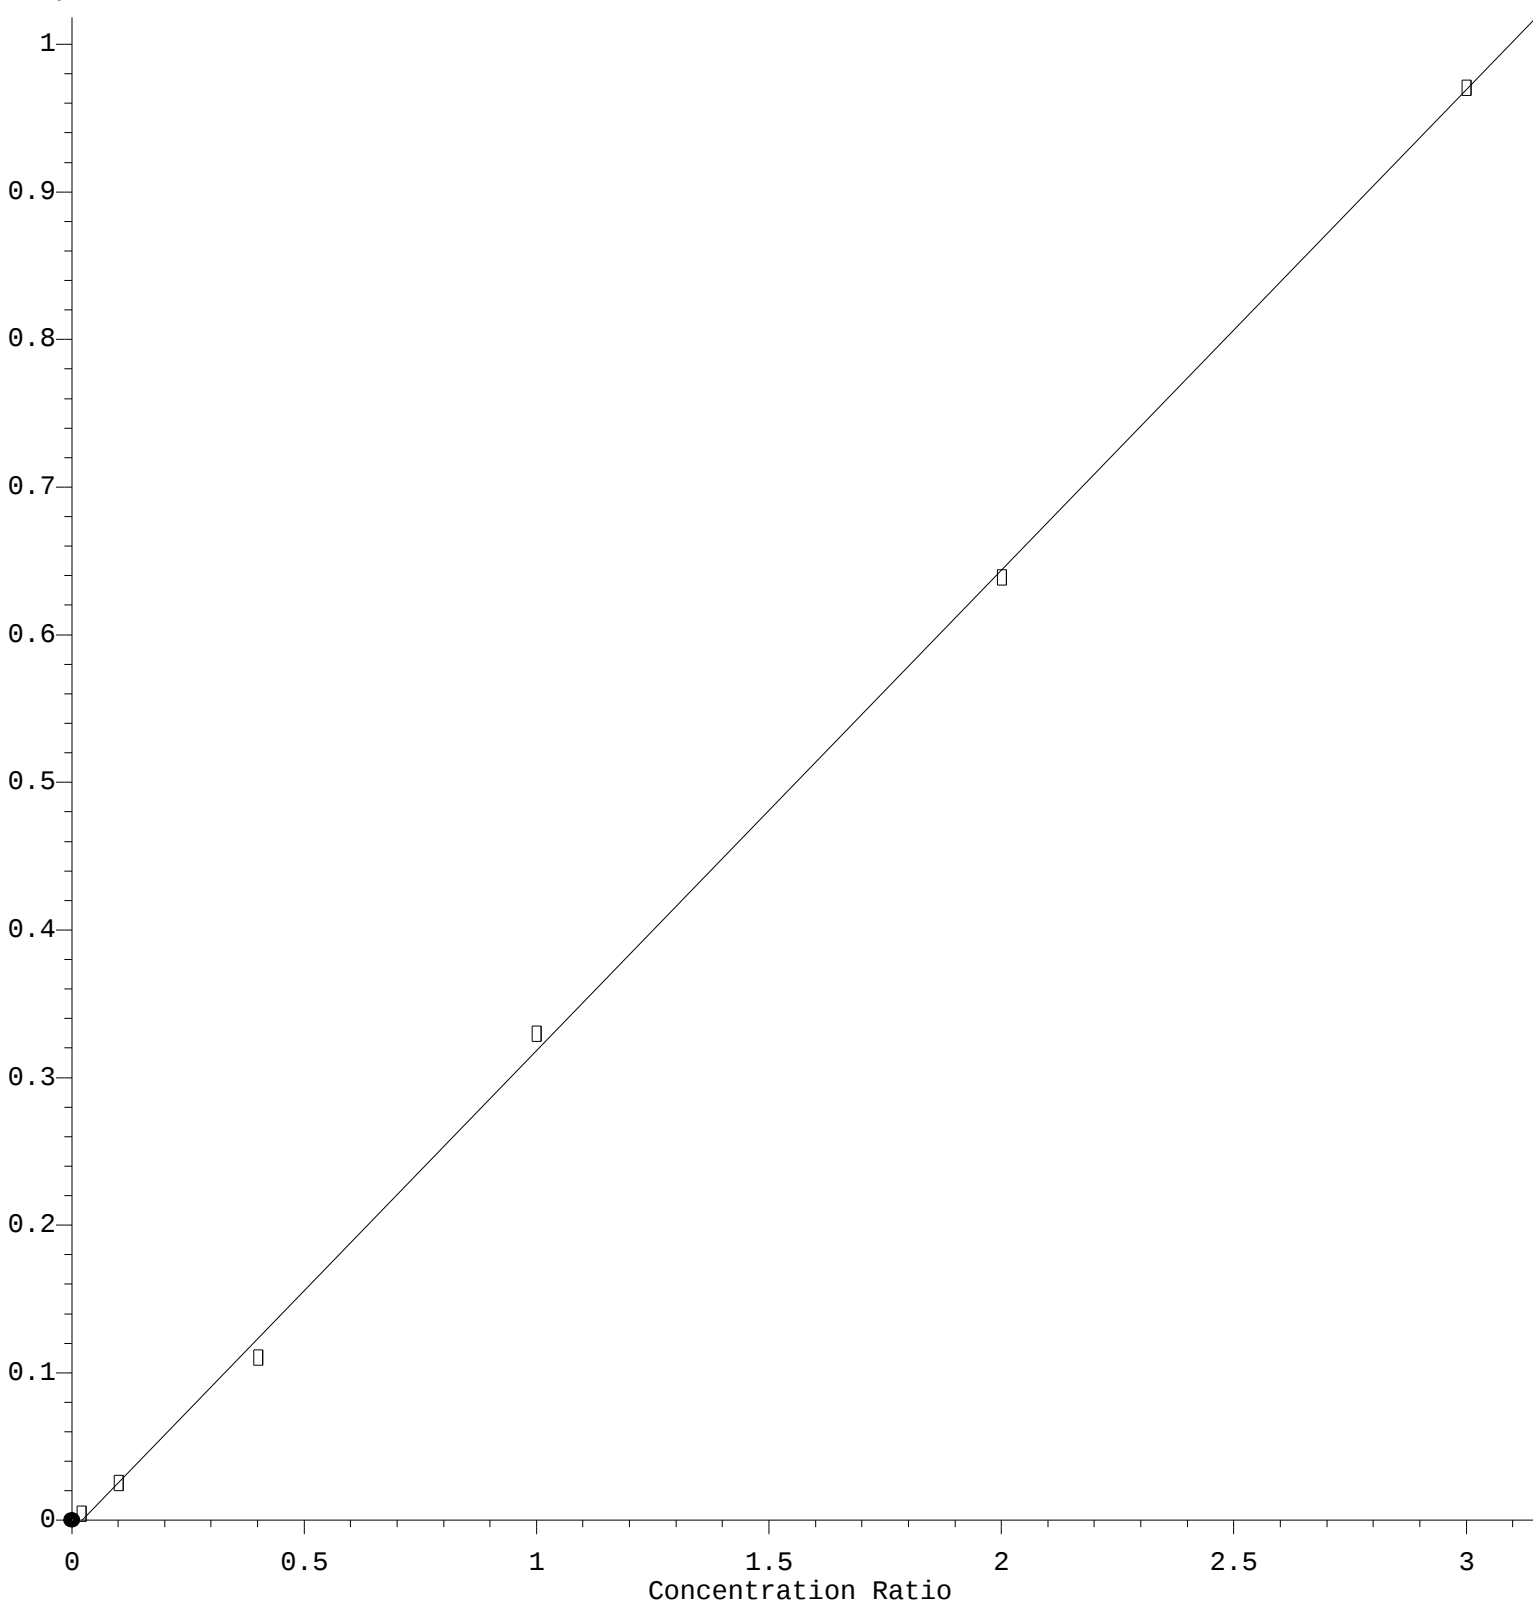

$$\text{Response} = 3.254\text{e-}001 * \text{Amt} - 7.317\text{e-}003$$


Coef of Det (r^2) = 0.999539 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Calibration Table Last Updated: Tue Sep 14 12:18:04 2021

Naphthalene

Response Ratio

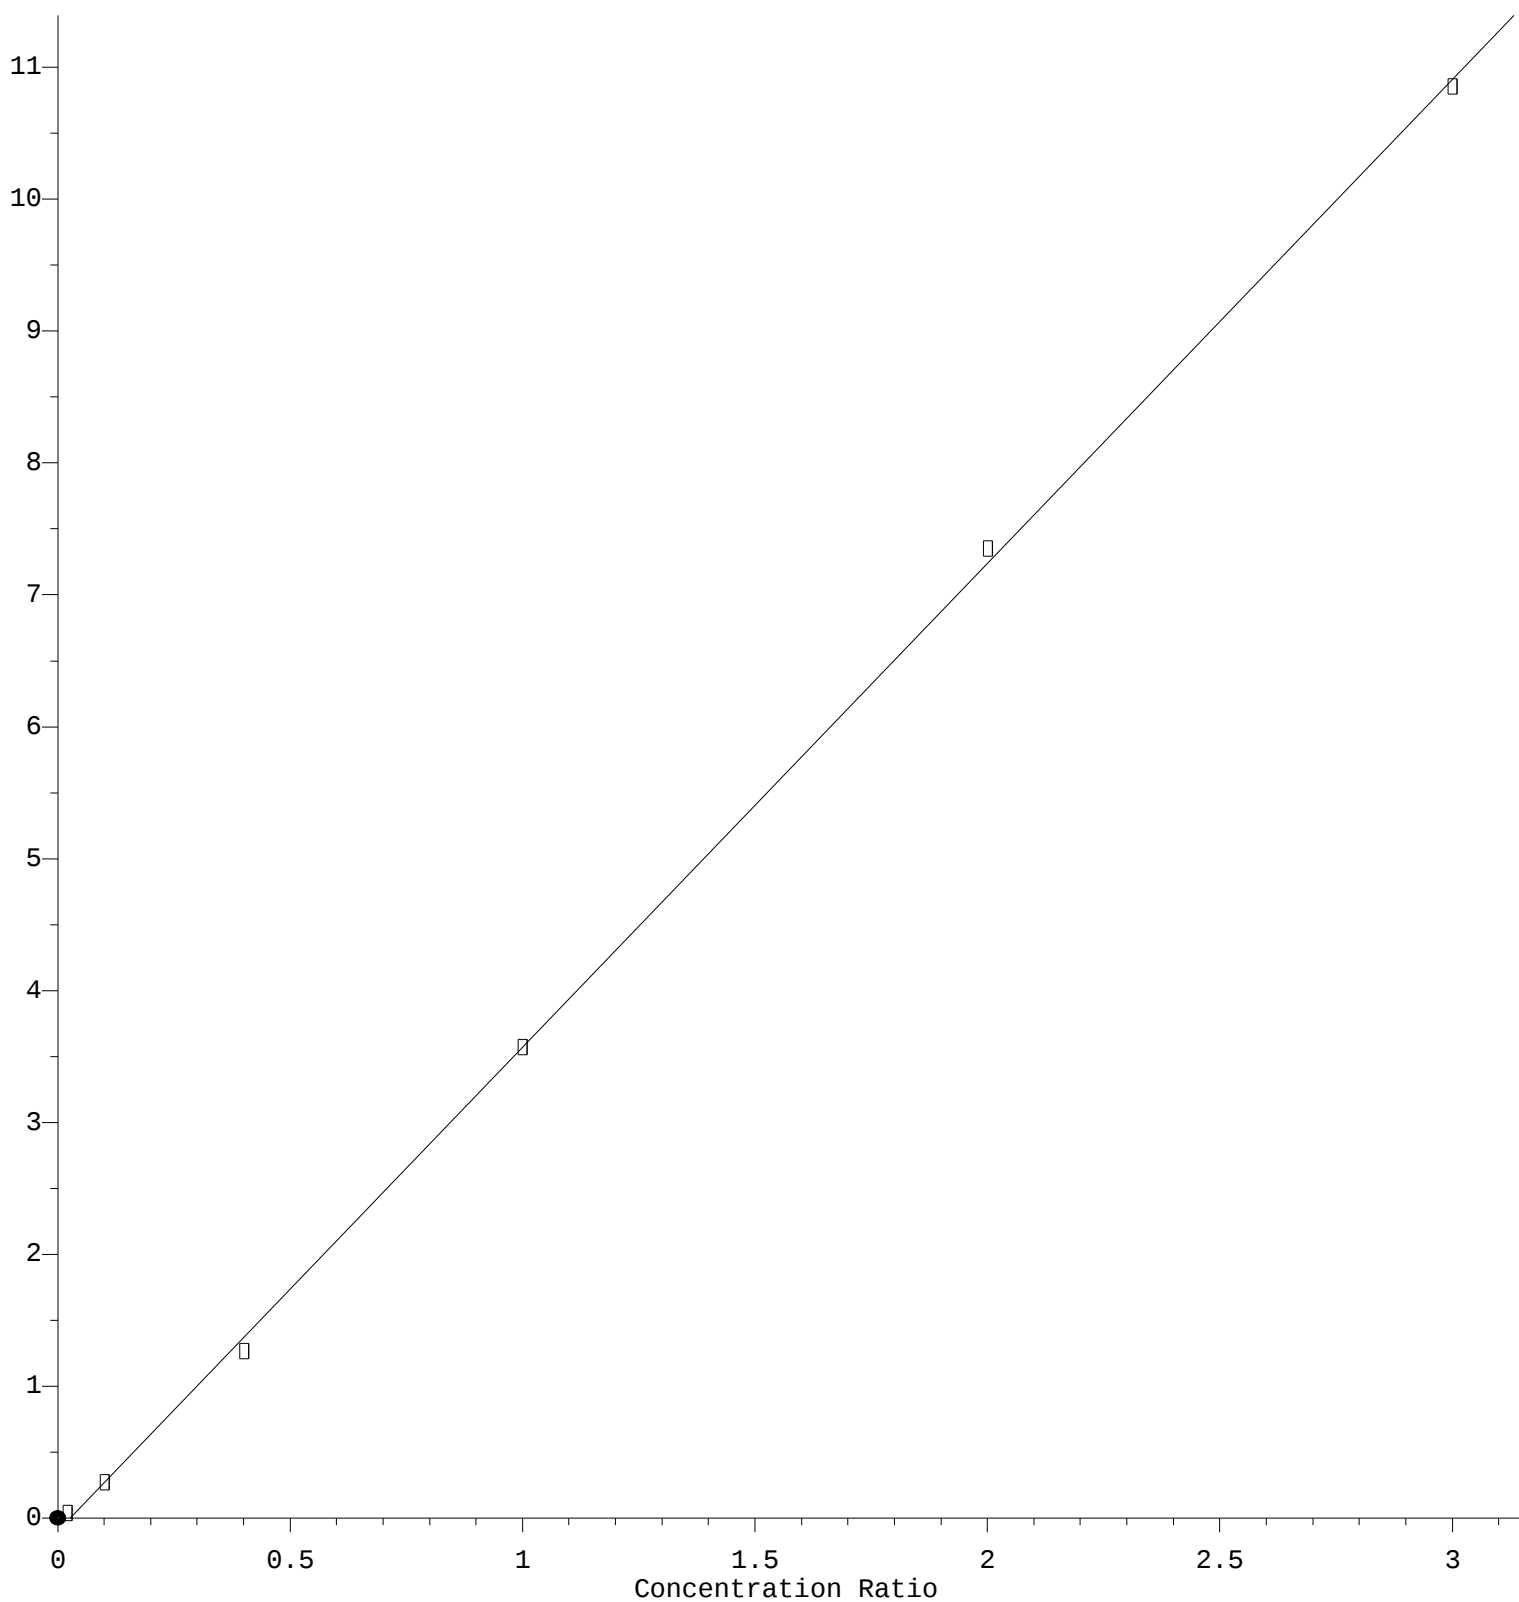

$$\text{Response} = 3.668\text{e}+000 * \text{Amt} - 9.441\text{e}-002$$

Coef of Det (r^2) = 0.999678 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Calibration Table Last Updated: Tue Sep 14 12:18:04 2021