

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
 Data File : VX024207.D
 Acq On : 14 Sep 2021 15:07
 Operator : JC/MD
 Sample : M3702-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Title : SW846 8260

Signal : TIC: VX024207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	44	47	56	rVB	238532	243359	6.43%	0.576%
2	1.892	126	132	147	rVB	479638	689592	18.21%	1.632%
3	2.386	207	213	223	rBV	122867	198052	5.23%	0.469%
4	2.794	272	280	299	rVB	530179	976075	25.77%	2.309%
5	3.123	322	334	352	rBV	776383	1779549	46.99%	4.210%
6	3.617	404	415	430	rVB	247092	574889	15.18%	1.360%
7	4.568	563	571	589	rVB	64323	177095	4.68%	0.419%
8	5.105	645	659	674	rBV	240763	719592	19.00%	1.703%
9	5.397	695	707	723	rBV2	118525	350666	9.26%	0.830%
10	5.562	723	734	744	rVV	204768	584424	15.43%	1.383%
11	5.684	744	754	773	rVB	405022	1201417	31.72%	2.843%
12	5.964	788	800	807	rBV	138212	370895	9.79%	0.878%
13	6.044	807	813	817	rVV	246095	630329	16.64%	1.491%
14	6.098	817	822	834	rVB	348558	883480	23.33%	2.090%
15	6.769	921	932	944	rBV	311301	725046	19.14%	1.715%
16	7.135	982	992	1004	rBV	212965	467035	12.33%	1.105%
17	7.440	1031	1042	1052	rBV	498326	1033223	27.28%	2.445%
18	7.586	1060	1066	1079	rVB	157316	315705	8.34%	0.747%
19	7.830	1098	1106	1115	rBV	103068	188772	4.98%	0.447%
20	8.372	1187	1195	1207	rBV	713569	1116355	29.47%	2.641%
21	8.653	1234	1241	1247	rBV	674112	1034124	27.30%	2.447%
22	8.720	1247	1252	1263	rVB	883847	1392108	36.76%	3.294%
23	8.982	1289	1295	1307	rBV	483291	680028	17.95%	1.609%
24	9.275	1337	1343	1354	rVB	708572	1057113	27.91%	2.501%
25	9.433	1363	1369	1378	rBV	700874	923781	24.39%	2.186%
26	9.525	1378	1384	1393	rVV	360285	513981	13.57%	1.216%
27	9.616	1393	1399	1407	rVB	133549	198271	5.23%	0.469%
28	10.055	1465	1471	1474	rBV	655093	1040846	27.48%	2.463%
29	10.305	1506	1512	1523	rBV	1240723	1662795	43.90%	3.934%
30	10.652	1562	1569	1585	rBV2	2221484	3787482	100.00%	8.961%
31	10.805	1588	1594	1603	rVB	174016	237350	6.27%	0.562%
32	11.085	1634	1640	1652	rVB	583311	743224	19.62%	1.758%
33	11.213	1656	1661	1664	rBV	1233985	1766495	46.64%	4.179%
34	11.244	1664	1666	1674	rVB	1058183	1102995	29.12%	2.610%
35	11.457	1695	1701	1709	rVB	2052375	2586194	68.28%	6.119%
36	11.756	1745	1750	1756	rVB	2125805	2484159	65.59%	5.877%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
Data File : VX024207.D
Acq On : 14 Sep 2021 15:07
Operator : JC/MD
Sample : M3702-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Title : SW846 8260

37	11.969	1780	1785	1790	rBV	526860	677716	17.89%	1.603%
38	12.042	1790	1797	1804	rVB2	1815469	3036415	80.17%	7.184%
39	12.335	1840	1845	1852	rBV	1792276	2240313	59.15%	5.301%
40	12.945	1939	1945	1961	rBV	565322	707991	18.69%	1.675%
41	13.780	2076	2082	2091	rBV	958099	1166817	30.81%	2.761%




Sum of corrected areas: 42265748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
Data File : VX024207.D
Acq On : 14 Sep 2021 15:07
Operator : JC/MD
Sample : M3702-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

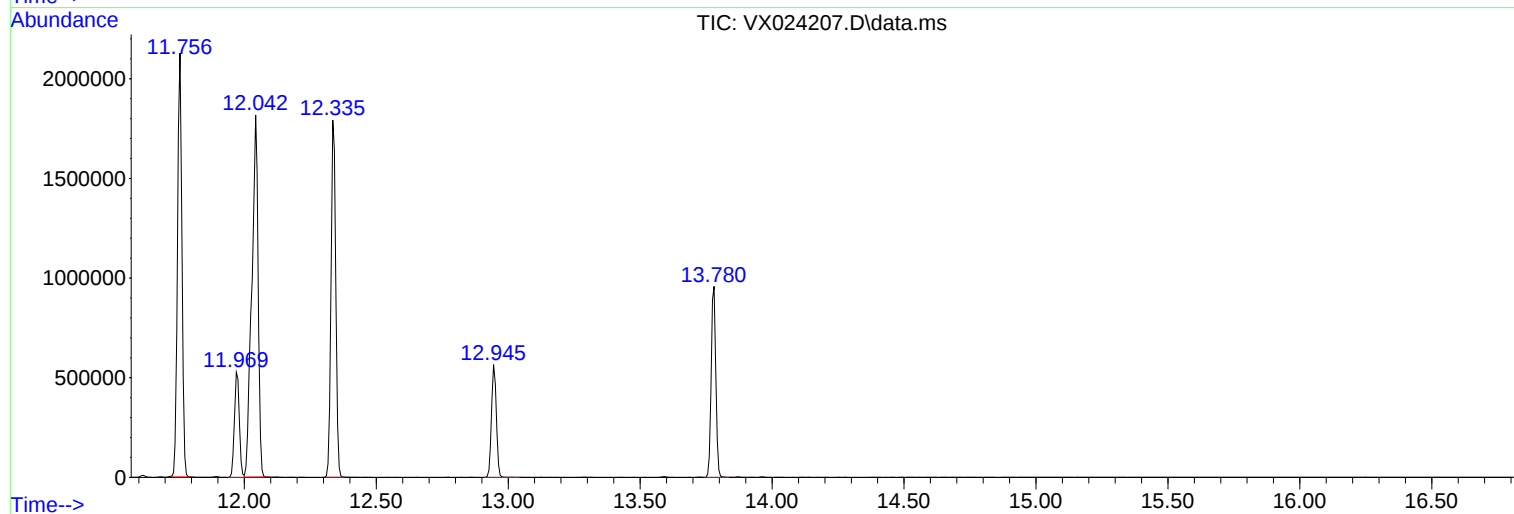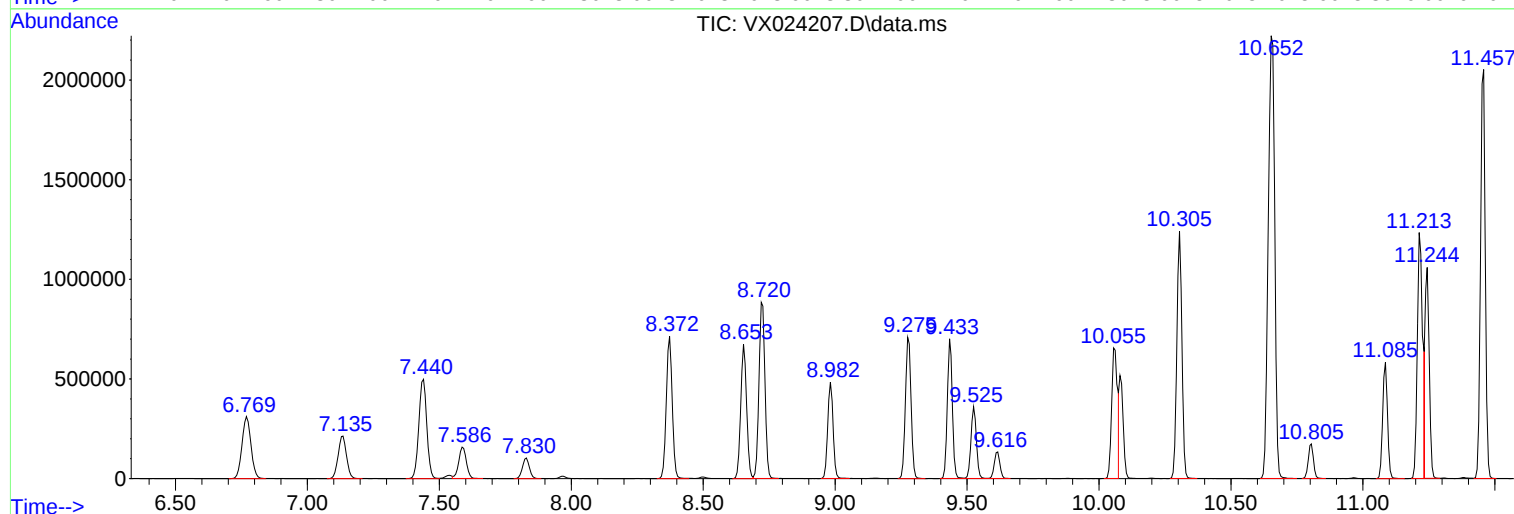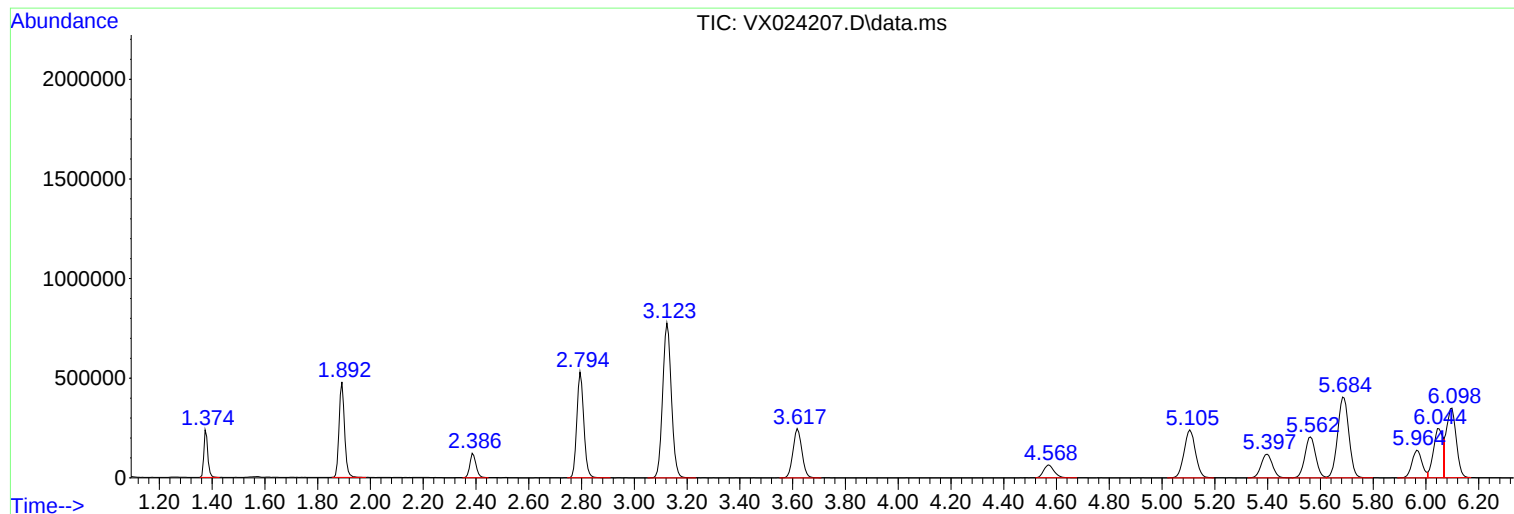

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
Data File : VX024207.D
Acq On : 14 Sep 2021 15:07
Operator : JC/MD
Sample : M3702-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
Data File : VX024207.D
Acq On : 14 Sep 2021 15:07
Operator : JC/MD
Sample : M3702-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------