
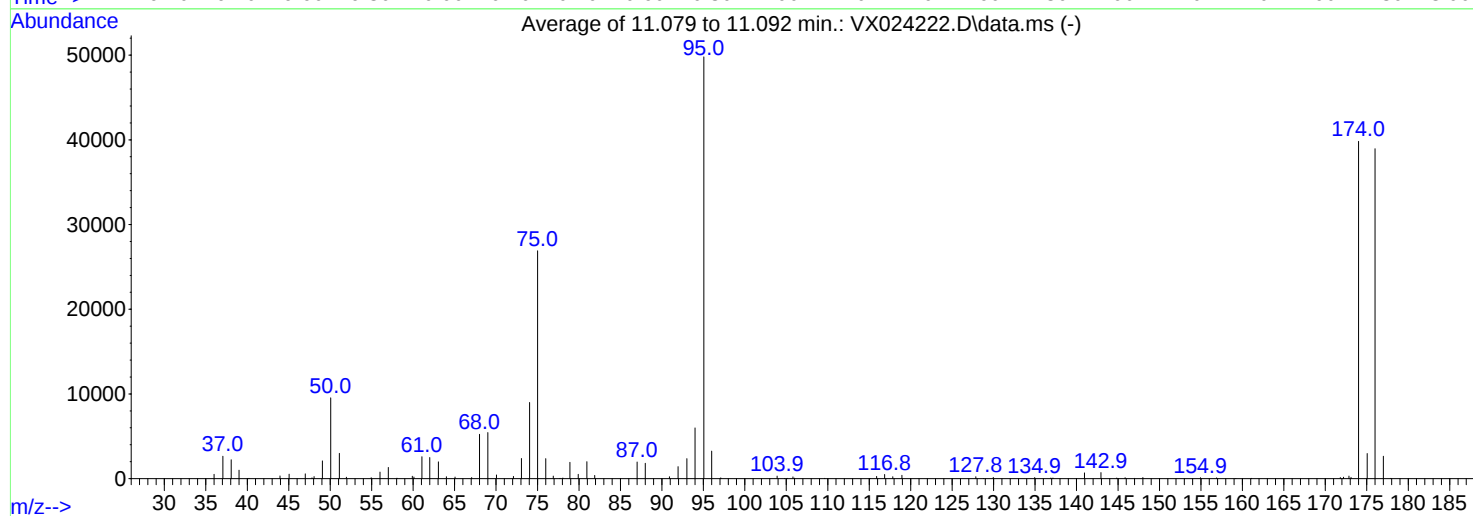


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091421\
 Data File : VX024222.D
 Acq On : 14 Sep 2021 21:24
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Title : SW846 8260
 Last Update : Tue Sep 14 12:18:04 2021

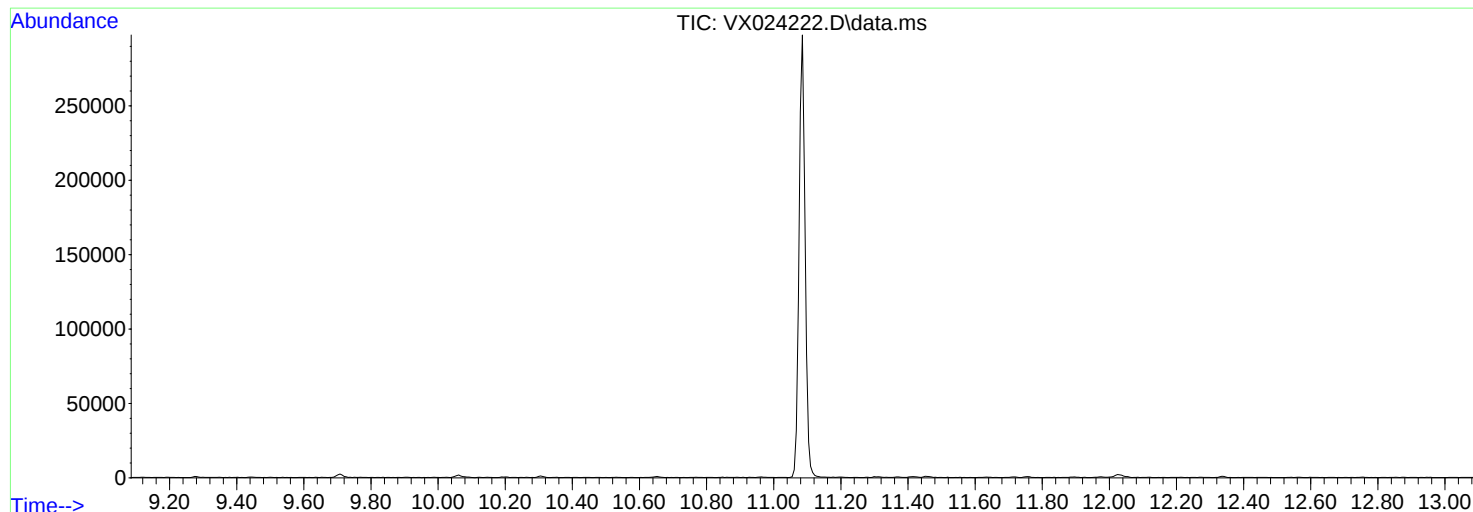

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	9540	PASS
75	95	30	60	54.0	26893	PASS
95	95	100	100	100.0	49800	PASS
96	95	5	9	6.5	3247	PASS
173	174	0.00	2	0.8	300	PASS
174	95	50	100	80.0	39827	PASS
175	174	5	9	7.5	2970	PASS
176	174	95	101	97.8	38947	PASS
177	176	5	9	6.8	2639	PASS