

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
 Data File : VX031319.D
 Acq On : 14 Sep 2022 20:38
 Operator : JC/MD
 Sample : N4492-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB01-090122

Quant Time: Sep 15 06:05:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 01:50:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	63617	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	114688	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	102402	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	42674	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	66083	42.320	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	84.640%
35) Dibromofluoromethane	5.385	113	47818	38.788	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	77.580%
50) Toluene-d8	8.653	98	186361	40.299	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	80.600%#
62) 4-Bromofluorobenzene	11.079	95	61992	36.607	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	73.220%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031319.D
Acq On : 14 Sep 2022 20:38
Operator : JC/MD
Sample : N4492-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB01-090122

Quant Time: Sep 15 06:05:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 01:50:07 2022
Response via : Initial Calibration




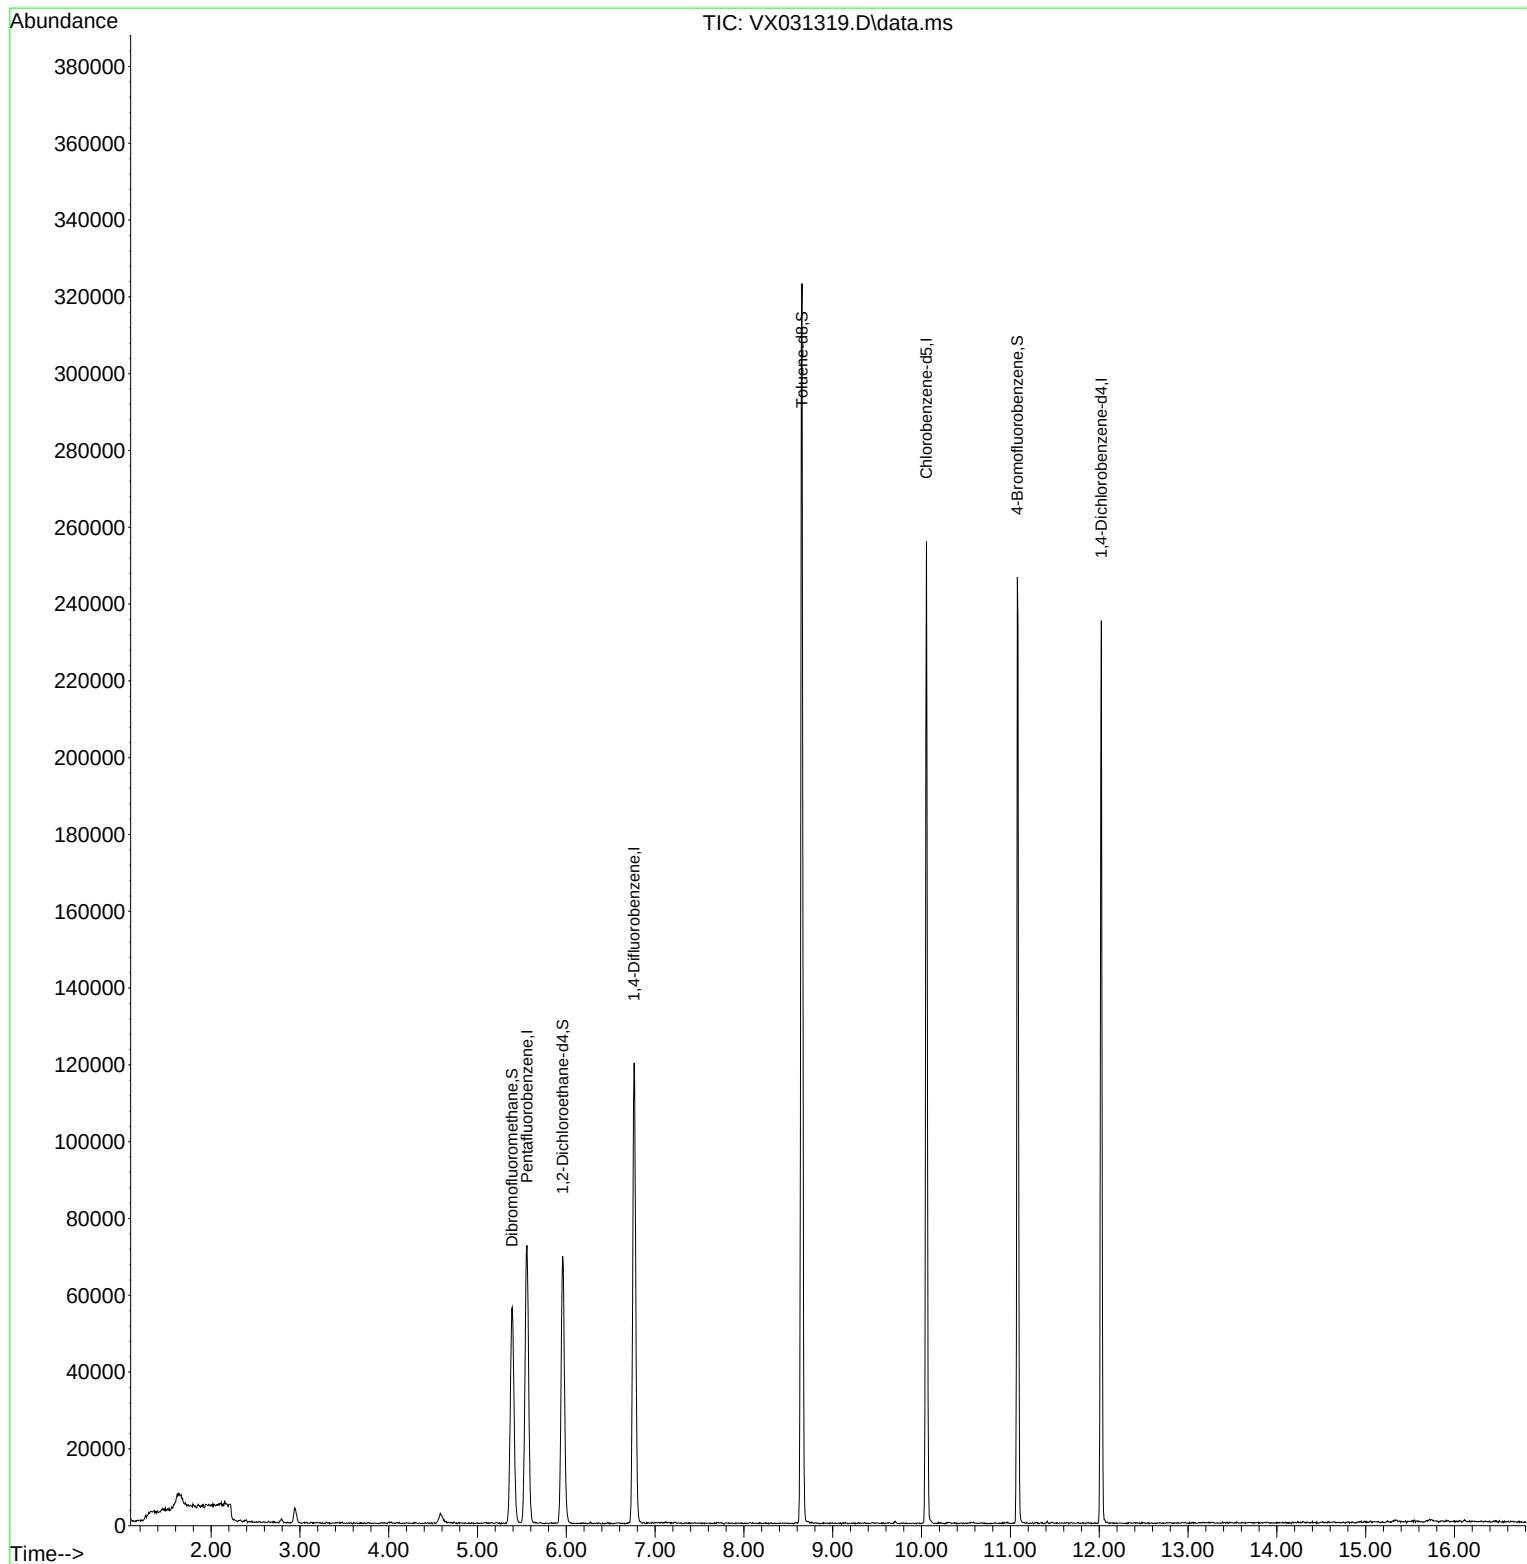


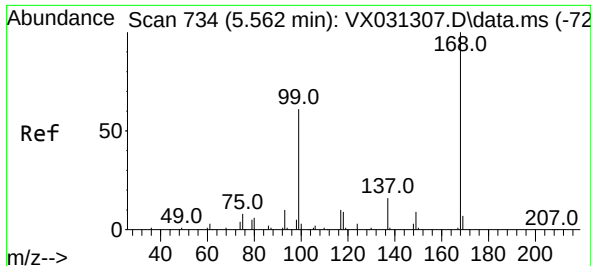

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.006 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38




Instrument :
MSVOA_X
ClientSampleId :
EB01-090122


Tgt Ion:168 Resp: 63617
Ion Ratio Lower Upper
168 100
99 63.9 48.8 73.2

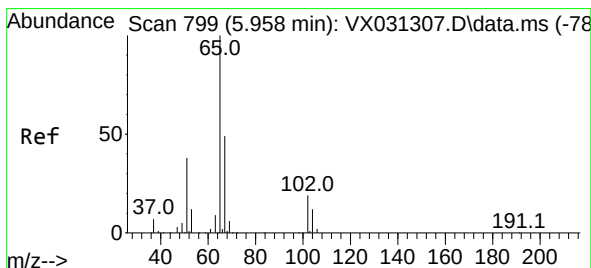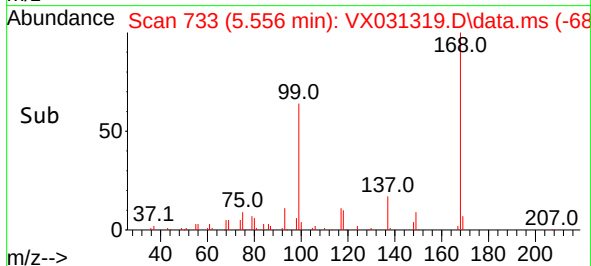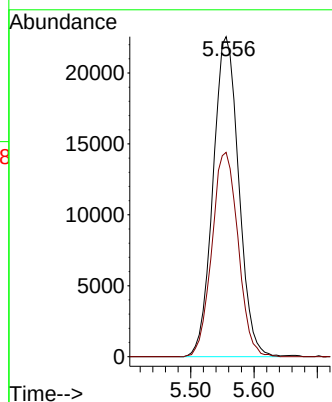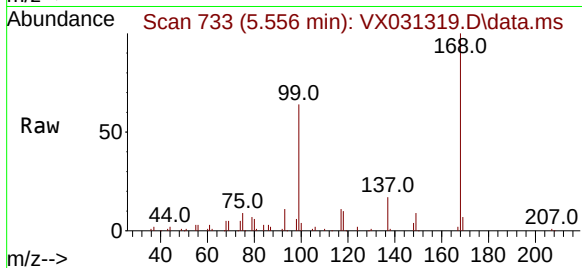

#33
1,2-Dichloroethane-d4
Concen: 42.320 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38

Tgt Ion: 65 Resp: 66083
Ion Ratio Lower Upper
65 100
67 50.1 0.0 102.4


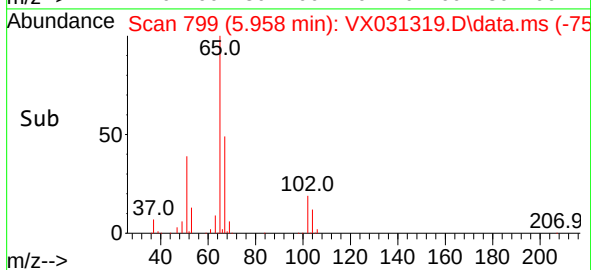
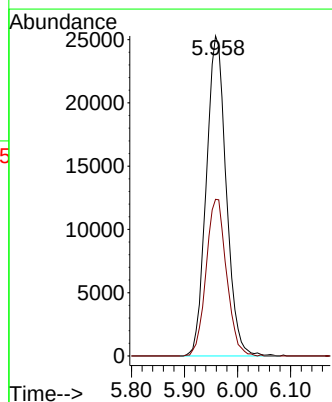
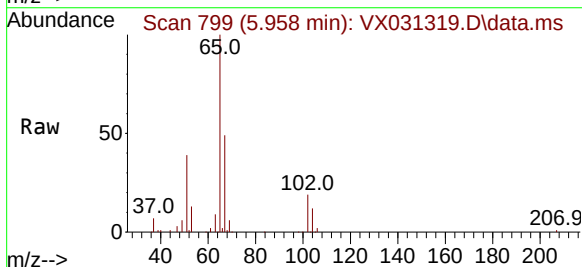


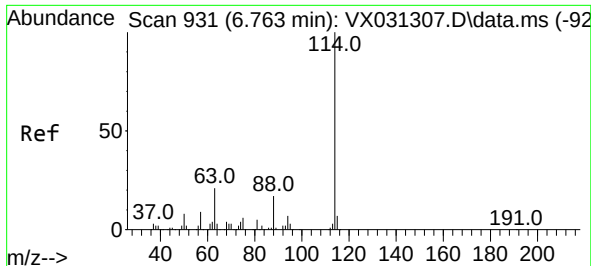

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38




Instrument :
MSVOA_X
ClientSampleId :
EB01-090122


Tgt Ion:114 Resp: 114688
Ion Ratio Lower Upper
114 100
63 22.2 0.0 42.6
88 16.0 0.0 33.0

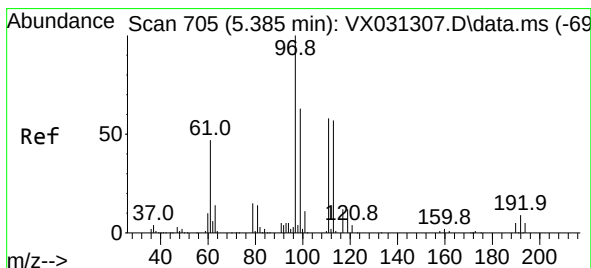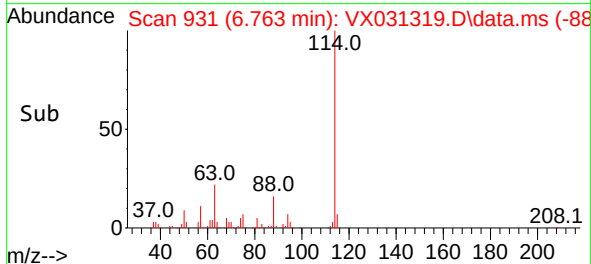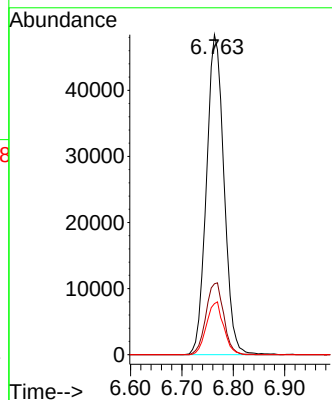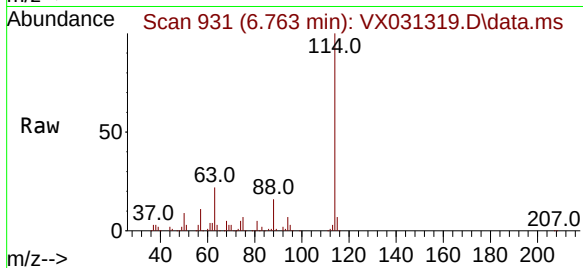

#35
Dibromofluoromethane
Concen: 38.788 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38

Tgt Ion:113 Resp: 47818
Ion Ratio Lower Upper
113 100
111 102.6 82.4 123.6
192 16.7 14.1 21.1


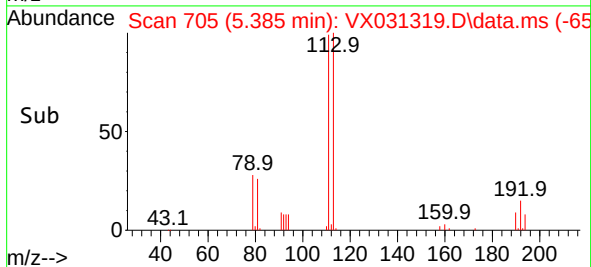
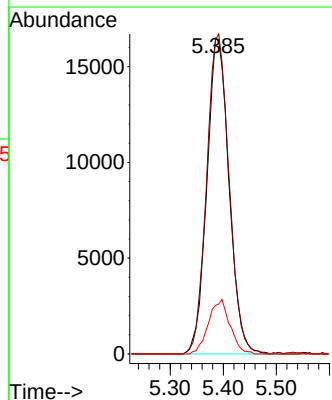
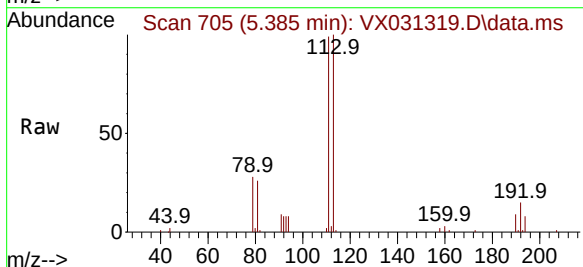


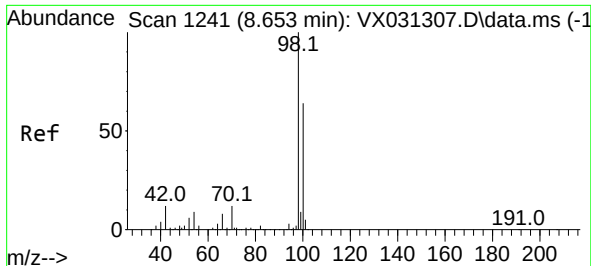

#50
Toluene-d8
Concen: 40.299 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38




Instrument :
MSVOA_X
ClientSampleId :
EB01-090122


Tgt Ion: 98 Resp: 186361
Ion Ratio Lower Upper
98 100
100 64.0 52.5 78.7

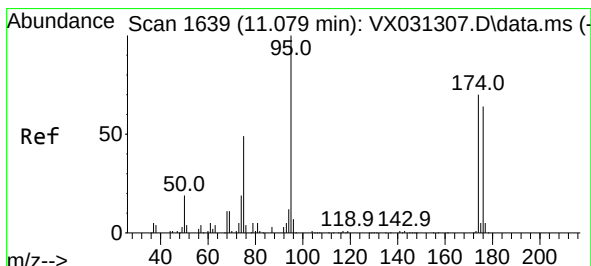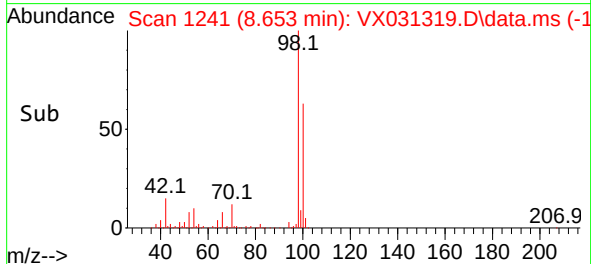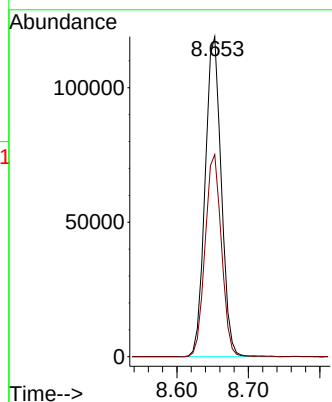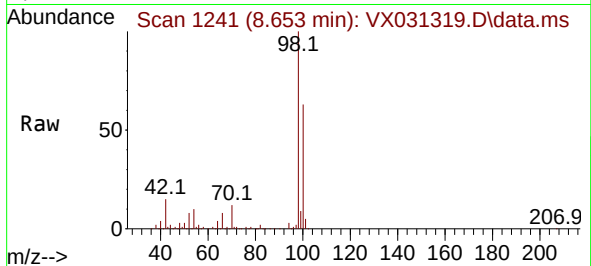

#62
4-Bromofluorobenzene
Concen: 36.607 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031319.D
Acq: 14 Sep 2022 20:38

Tgt Ion: 95 Resp: 61992
Ion Ratio Lower Upper
95 100
174 71.6 0.0 153.2
176 70.7 0.0 144.0

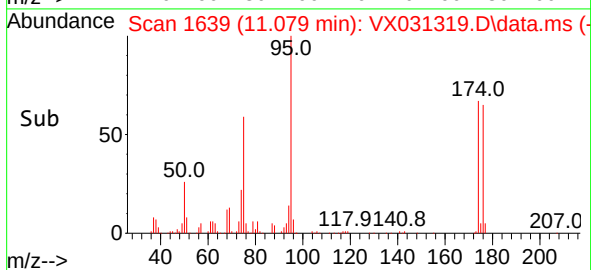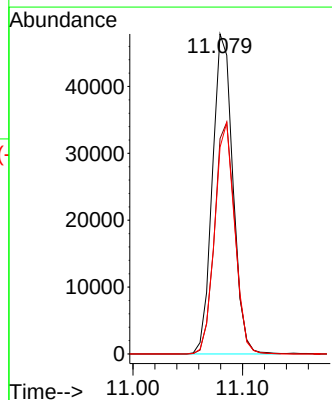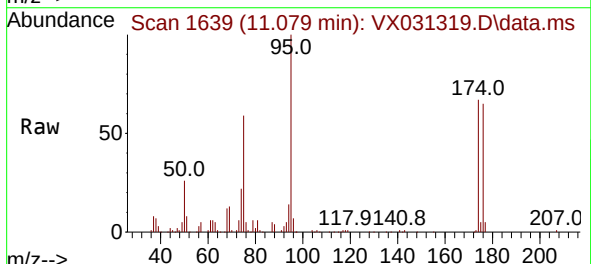

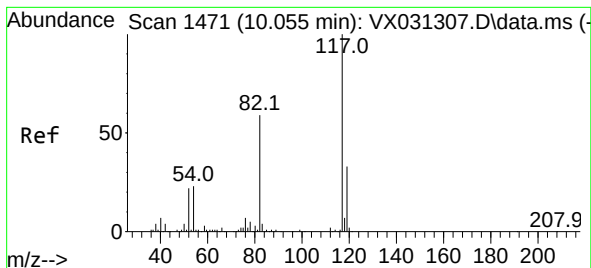

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX031319.D

Acq: 14 Sep 2022 20:38

Instrument :

MSVOA_X

ClientSampleId :

EB01-090122





Tgt Ion:117 Resp: 102402

Ion Ratio Lower Upper

117 100

82 59.6 46.8 70.2

119 32.8 26.4 39.6

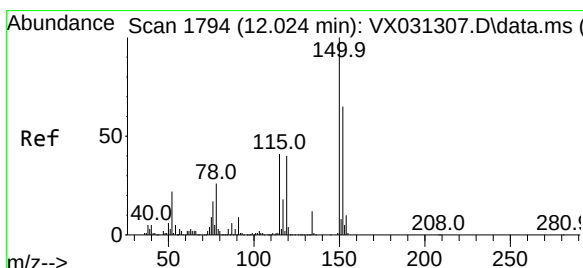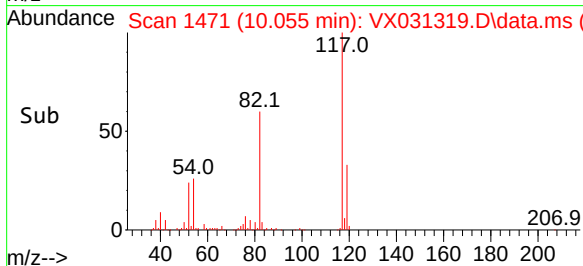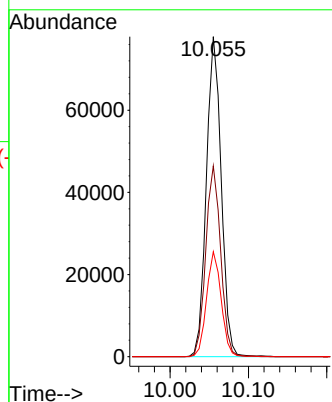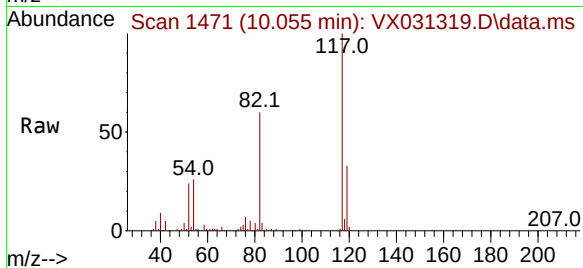

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX031319.D

Acq: 14 Sep 2022 20:38

Tgt Ion:152 Resp: 42674

Ion Ratio Lower Upper

152 100

115 62.6 43.4 130.1

150 157.6 0.0 346.8

