

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
 Data File : VX031327.D
 Acq On : 14 Sep 2022 23:45
 Operator : JC/MD
 Sample : N4446-08RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-YRE

Quant Time: Sep 15 06:08:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 01:50:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	60887	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	109765	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	97875	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	40878	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	69422	46.452	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.900%
35) Dibromofluoromethane	5.391	113	46580	39.478	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	78.960%
50) Toluene-d8	8.652	98	142475	32.191	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	64.380%#
62) 4-Bromofluorobenzene	11.079	95	46180	28.493	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	56.980%#


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031327.D
Acq On : 14 Sep 2022 23:45
Operator : JC/MD
Sample : N4446-08RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-YRE

Quant Time: Sep 15 06:08:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 01:50:07 2022
Response via : Initial Calibration




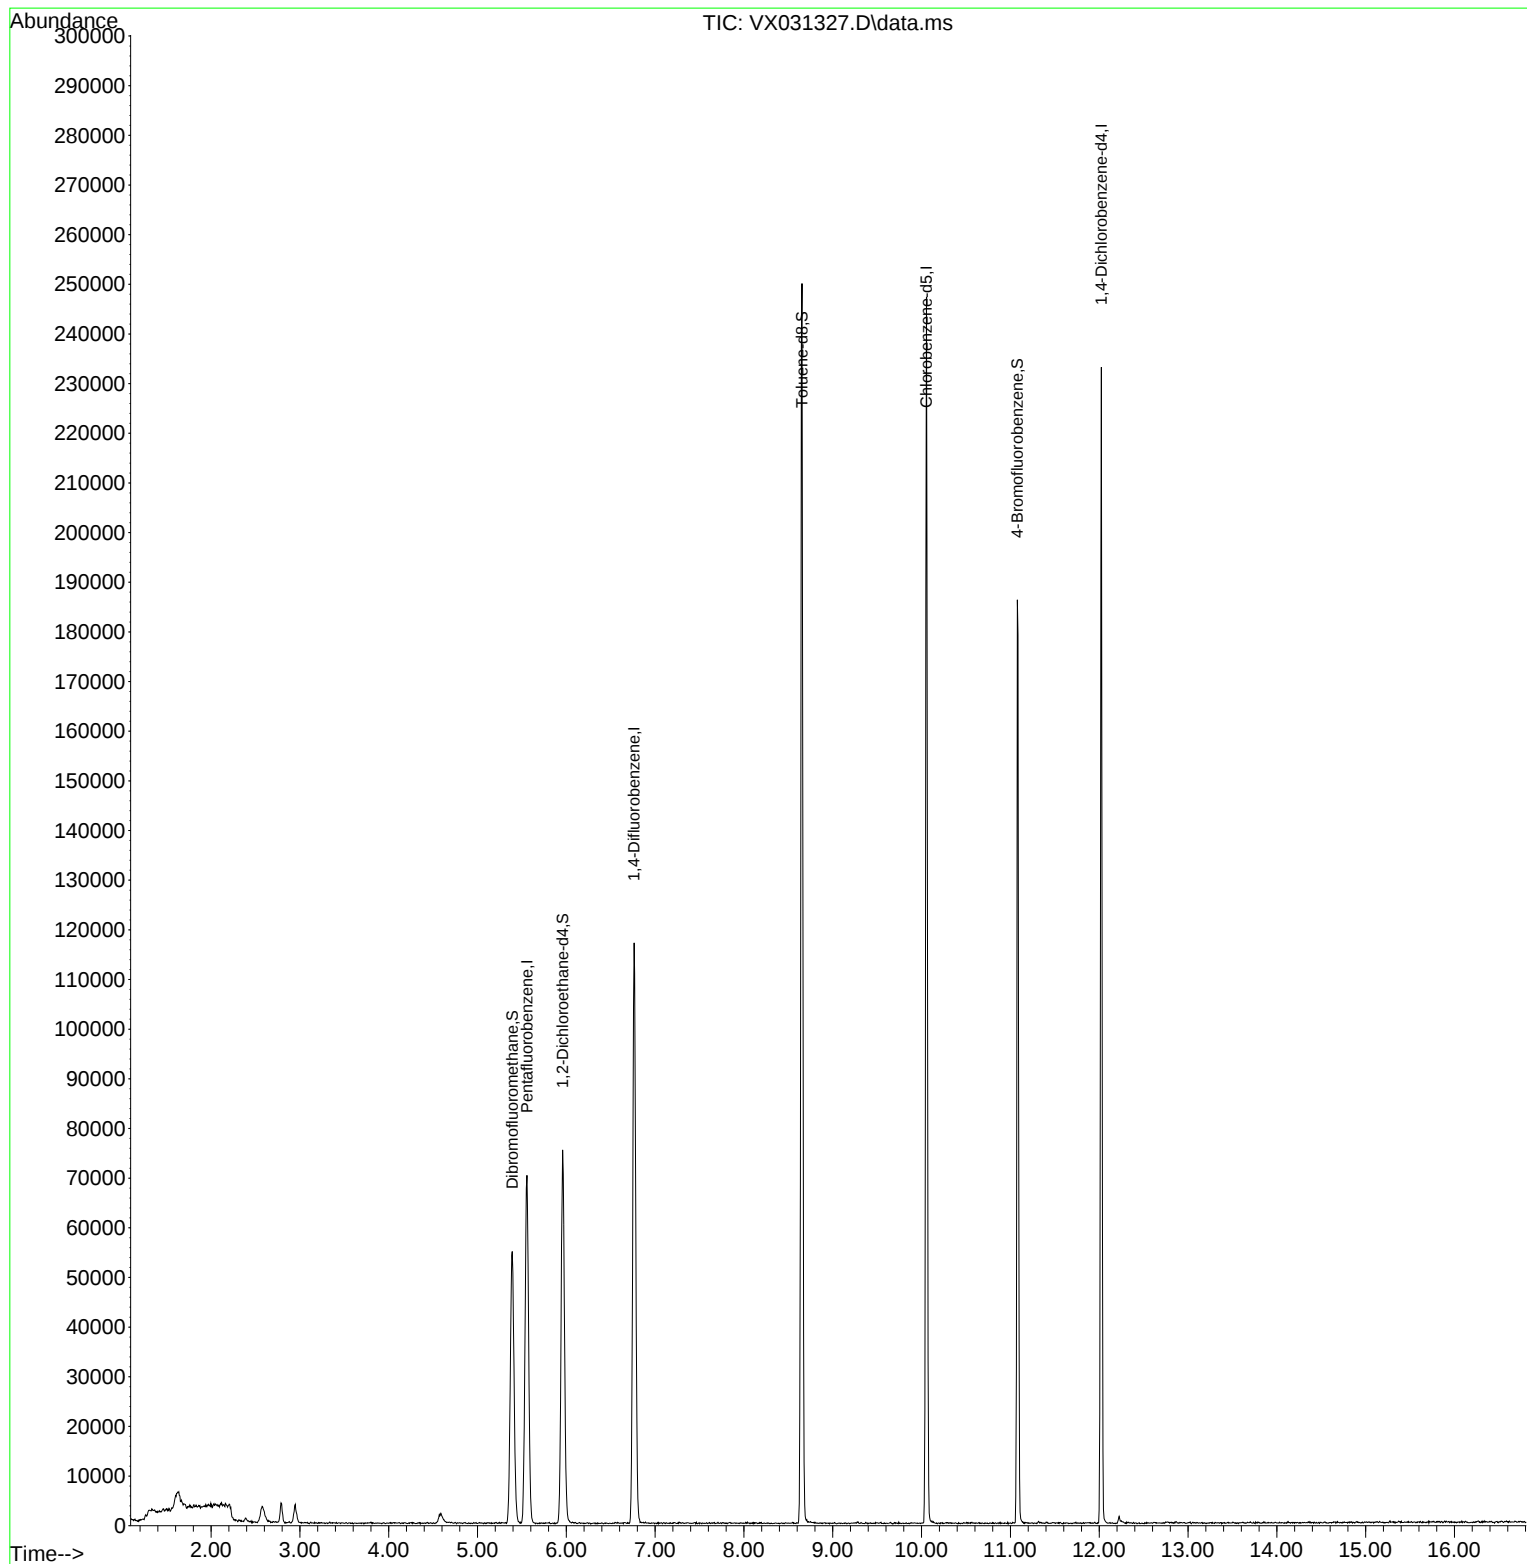




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.006 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45




Instrument :
MSVOA_X
ClientSampleId :
DUP-YRE


Tgt Ion:168 Resp: 60887
Ion Ratio Lower Upper
168 100
99 64.7 48.8 73.2

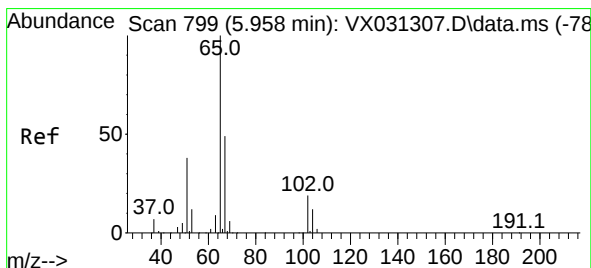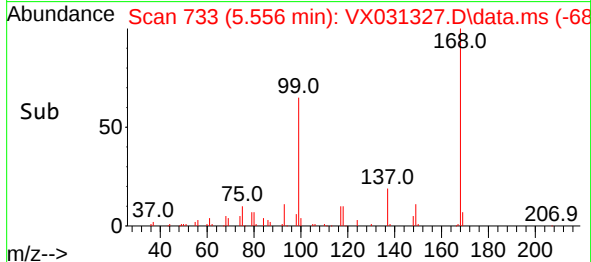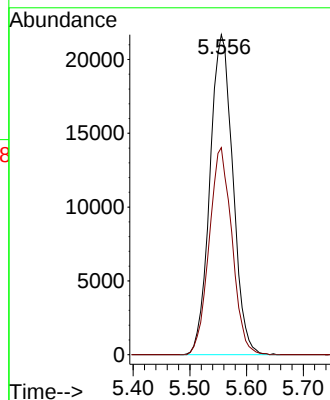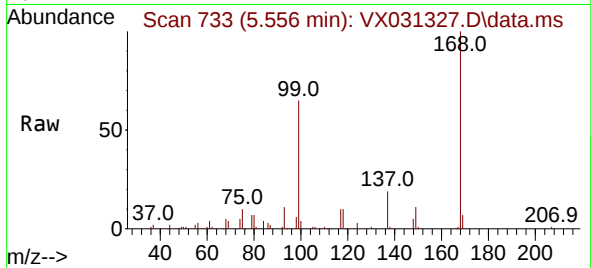

#33
1,2-Dichloroethane-d4
Concen: 46.452 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45

Tgt Ion: 65 Resp: 69422
Ion Ratio Lower Upper
65 100
67 51.0 0.0 102.4


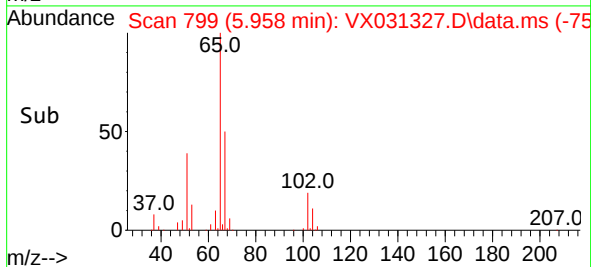
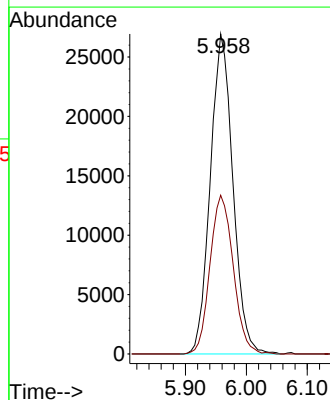
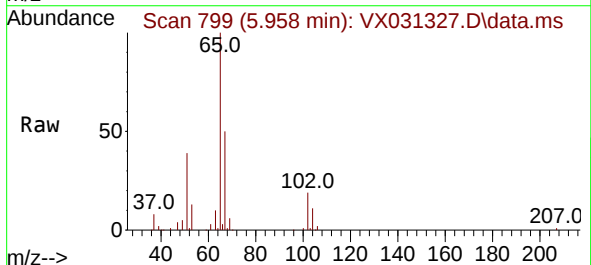


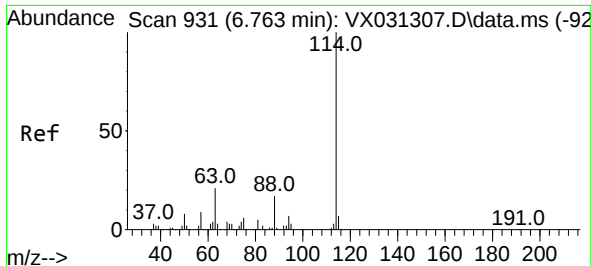

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45




Instrument :
MSVOA_X
ClientSampleId :
DUP-YRE


Tgt Ion:114 Resp: 109765
Ion Ratio Lower Upper
114 100
63 22.8 0.0 42.6
88 15.2 0.0 33.0

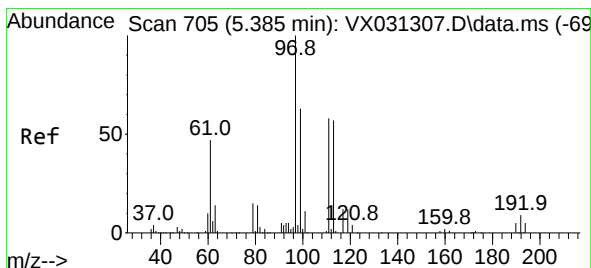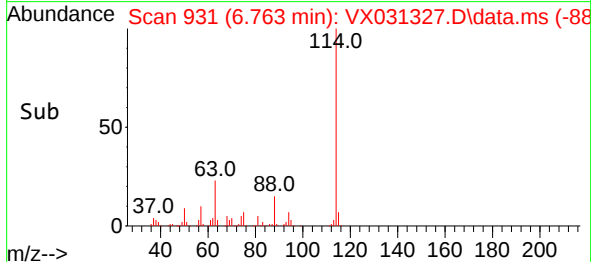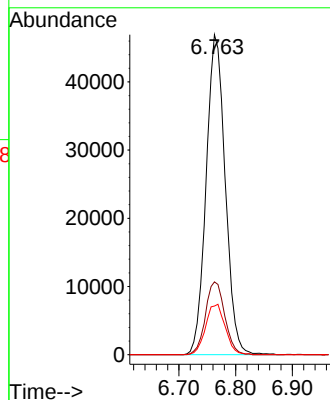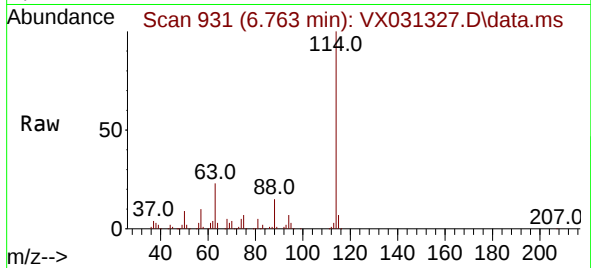

#35
Dibromofluoromethane
Concen: 39.478 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45

Tgt Ion:113 Resp: 46580
Ion Ratio Lower Upper
113 100
111 101.8 82.4 123.6
192 17.0 14.1 21.1


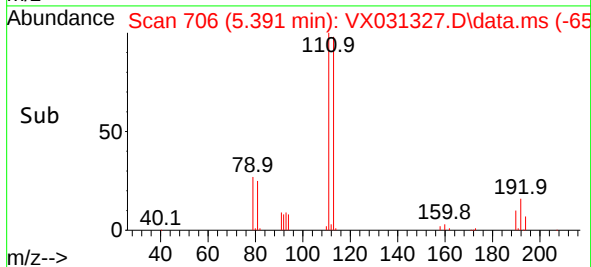
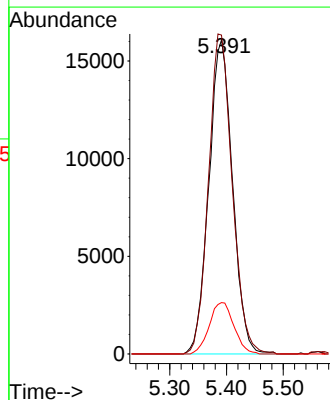
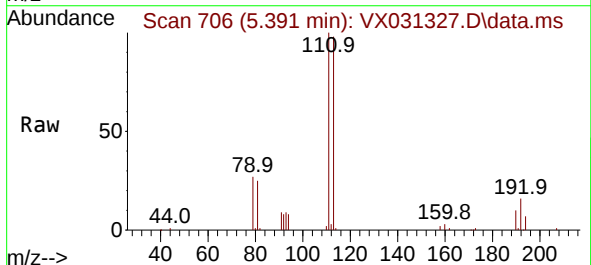


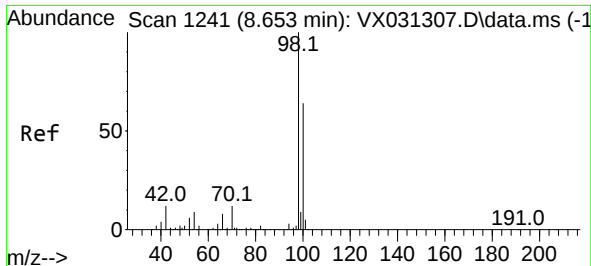

#50
Toluene-d8
Concen: 32.191 ug/l
RT: 8.652 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45




Instrument :
MSVOA_X
ClientSampleId :
DUP-YRE


Tgt Ion: 98 Resp: 142475
Ion Ratio Lower Upper
98 100
100 64.3 52.5 78.7

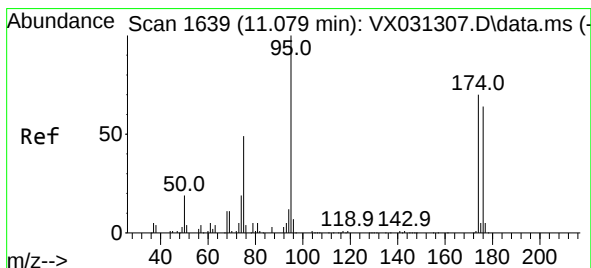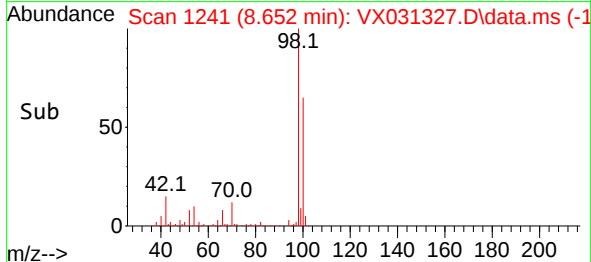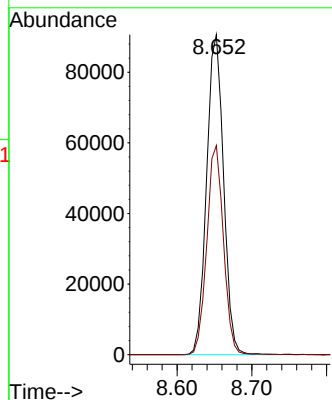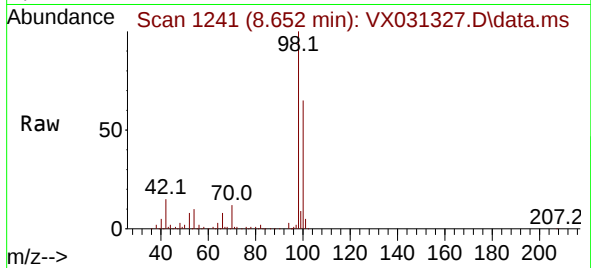

#62
4-Bromofluorobenzene
Concen: 28.493 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX031327.D
Acq: 14 Sep 2022 23:45

Tgt Ion: 95 Resp: 46180
Ion Ratio Lower Upper
95 100
174 72.7 0.0 153.2
176 70.7 0.0 144.0

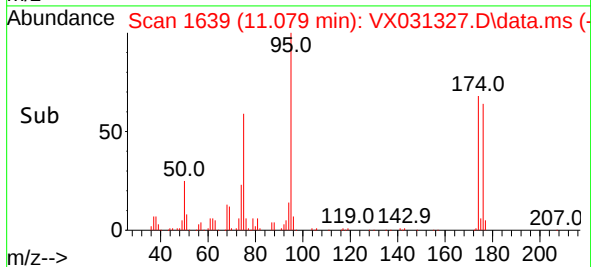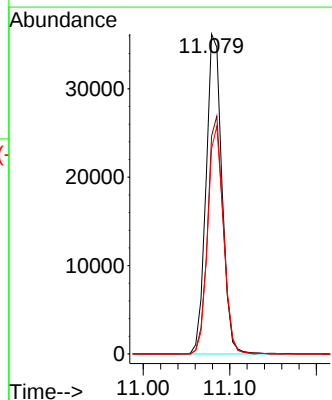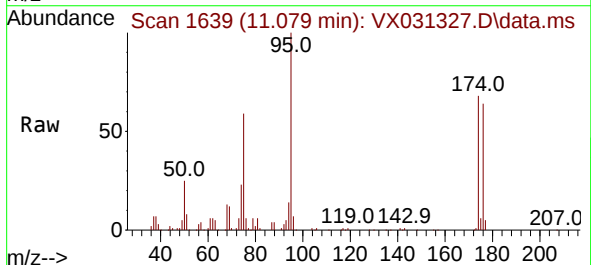

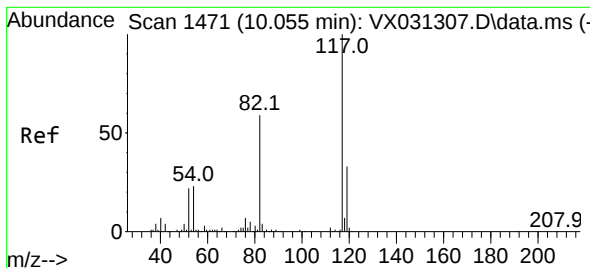

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX031327.D

Acq: 14 Sep 2022 23:45

Instrument :

MSVOA_X

ClientSampleId :

DUP-YRE





Tgt Ion:117 Resp: 97875

Ion Ratio Lower Upper

117 100

82 60.4 46.8 70.2

119 33.7 26.4 39.6

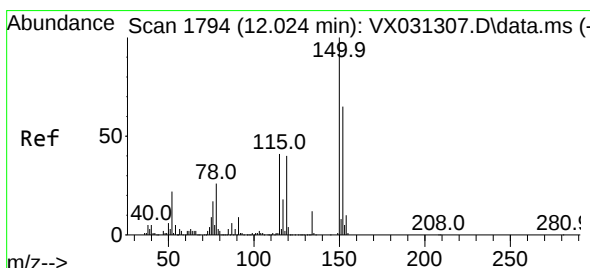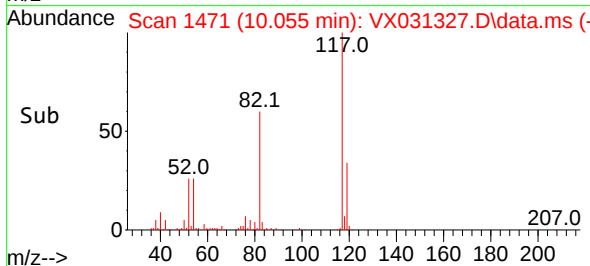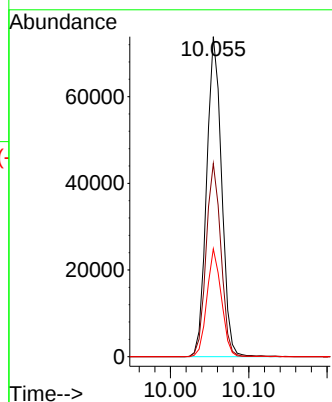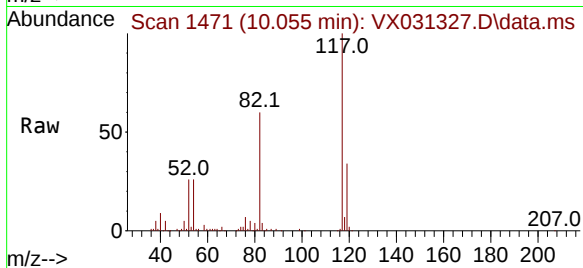

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX031327.D

Acq: 14 Sep 2022 23:45

Tgt Ion:152 Resp: 40878

Ion Ratio Lower Upper

152 100

115 62.3 43.4 130.1

150 157.6 0.0 346.8

