

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
 Data File : VX031316.D
 Acq On : 14 Sep 2022 19:27
 Operator : JC/MD
 Sample : N4588-04 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1666

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Title : SW846 8260

Signal : TIC: VX031316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.422	210	219	225	rBV4	6579	12867	2.26%	0.493%
2	2.947	298	305	312	rBV	11429	26940	4.74%	1.033%
3	4.581	564	573	588	rBV2	9794	34852	6.13%	1.336%
4	5.391	694	706	719	rBV	61369	178314	31.38%	6.835%
5	5.556	723	733	744	rBV2	73042	205705	36.20%	7.885%
6	5.958	789	799	812	rBV	76099	201293	35.42%	7.716%
7	6.763	920	931	942	rBV	122551	290883	51.19%	11.150%
8	8.653	1234	1241	1250	rBV	369762	568255	100.00%	21.781%
9	10.055	1465	1471	1482	rBV	264810	351673	61.89%	13.480%
10	11.085	1634	1640	1647	rBV	270653	351889	61.92%	13.488%
11	12.024	1788	1794	1801	rBV	248243	306487	53.93%	11.748%
12	12.104	1803	1807	1814	rVB2	7746	10066	1.77%	0.386%
13	12.225	1822	1827	1835	rBV2	4736	9861	1.74%	0.378%
14	13.268	1995	1998	2005	rVB2	6075	7317	1.29%	0.280%
15	14.042	2121	2125	2128	rBV	5021	5947	1.05%	0.228%
16	14.201	2146	2151	2159	rBV7	3060	7724	1.36%	0.296%
17	14.756	2238	2242	2246	rBV	11809	12086	2.13%	0.463%
18	15.213	2308	2317	2321	rVB5	4379	7025	1.24%	0.269%
19	15.493	2358	2363	2367	rBV2	6724	8511	1.50%	0.326%
20	16.377	2503	2508	2514	rVB4	6655	11232	1.98%	0.431%




Sum of corrected areas: 2608927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031316.D
Acq On : 14 Sep 2022 19:27
Operator : JC/MD
Sample : N4588-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

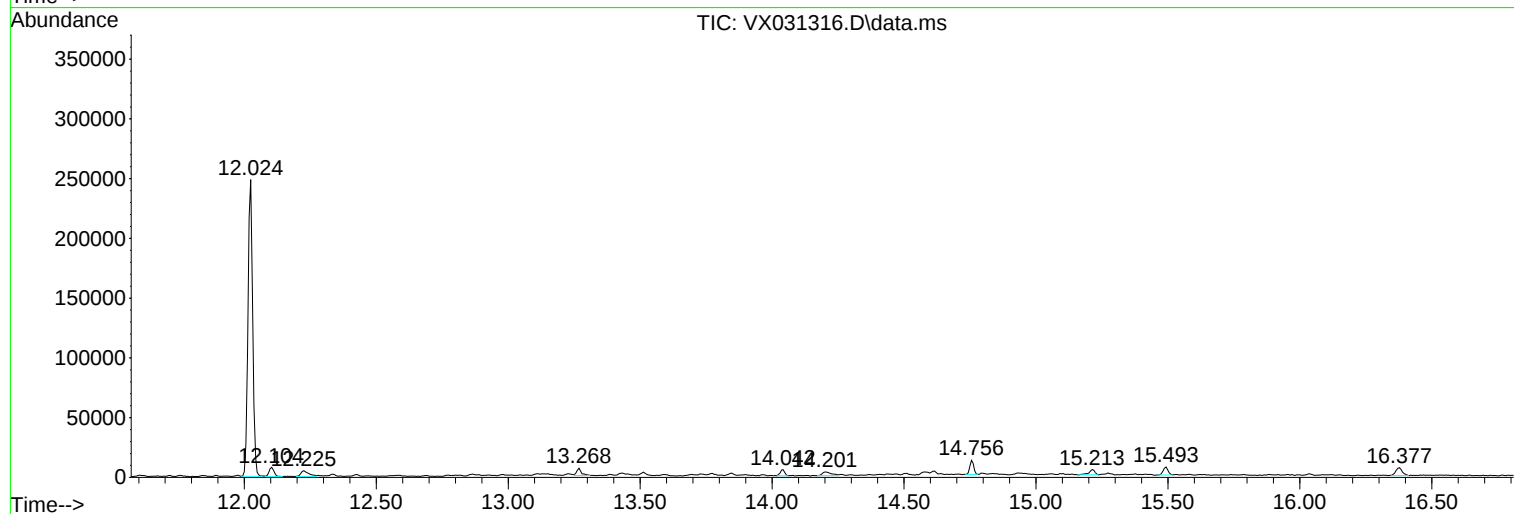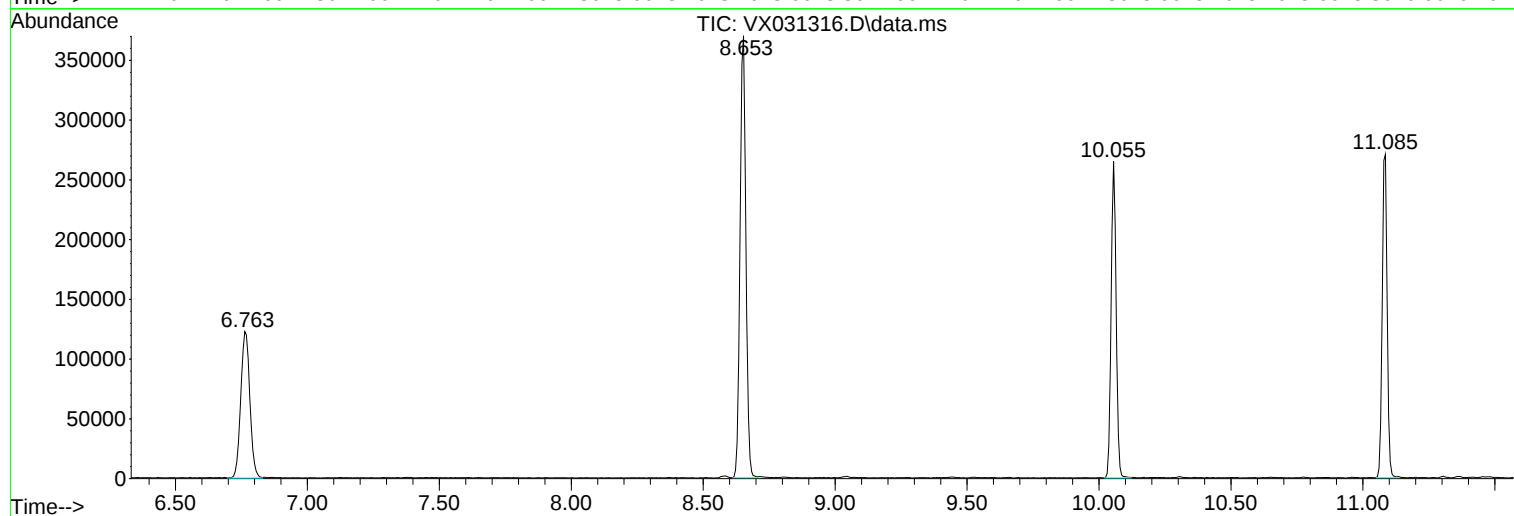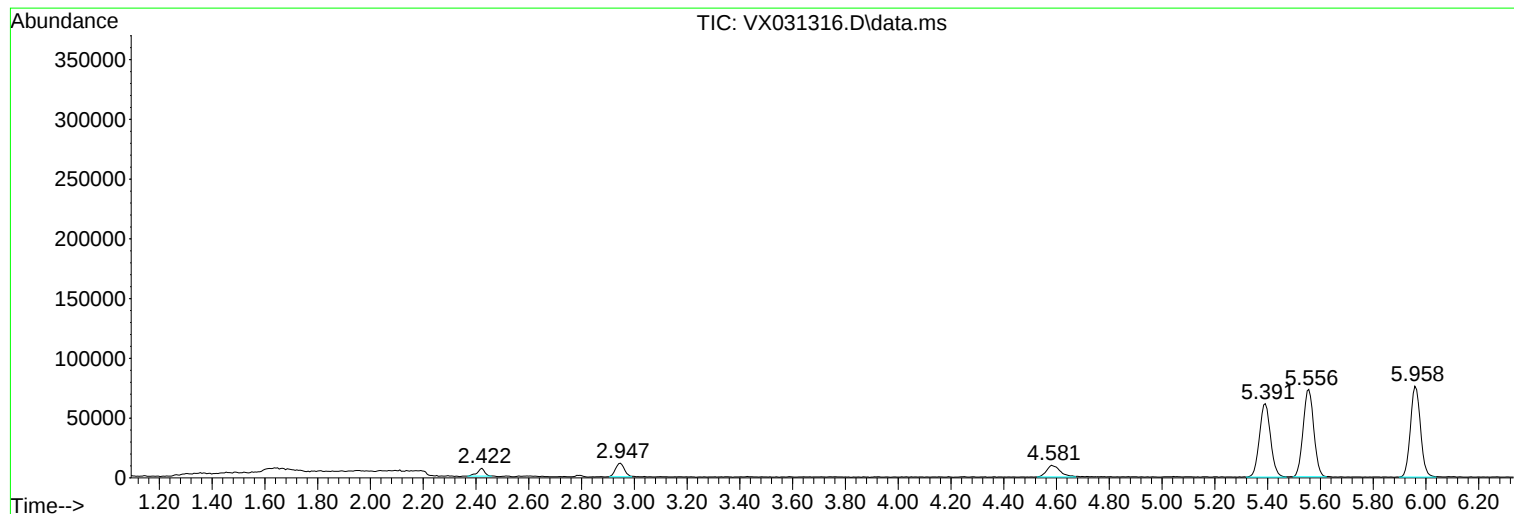

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031316.D
Acq On : 14 Sep 2022 19:27
Operator : JC/MD
Sample : N4588-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031316.D
Acq On : 14 Sep 2022 19:27
Operator : JC/MD
Sample : N4588-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------