

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
 Data File : VX031318.D
 Acq On : 14 Sep 2022 20:14
 Operator : JC/MD
 Sample : N4492-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BR-02-133-143-090122

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	296	305	315	rBV	10869	25227	4.85%	1.046%
2	4.580	563	573	587	rBV2	8010	27177	5.23%	1.126%
3	5.391	696	706	719	rVB2	57431	165395	31.83%	6.855%
4	5.556	723	733	747	rVB	73771	208496	40.12%	8.642%
5	5.958	788	799	814	rBV	70487	188729	36.32%	7.822%
6	6.763	922	931	943	rBV	122982	291055	56.01%	12.064%
7	8.653	1234	1241	1249	rBV	323364	519660	100.00%	21.539%
8	10.055	1465	1471	1481	rVB	261506	349026	67.16%	14.467%
9	11.079	1634	1639	1651	rBV	244994	323458	62.24%	13.407%
10	12.024	1789	1794	1800	rBV	247589	295703	56.90%	12.256%
11	12.219	1822	1826	1838	rBV	8442	18723	3.60%	0.776%




Sum of corrected areas: 2412649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031318.D
Acq On : 14 Sep 2022 20:14
Operator : JC/MD
Sample : N4492-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-02-133-143-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

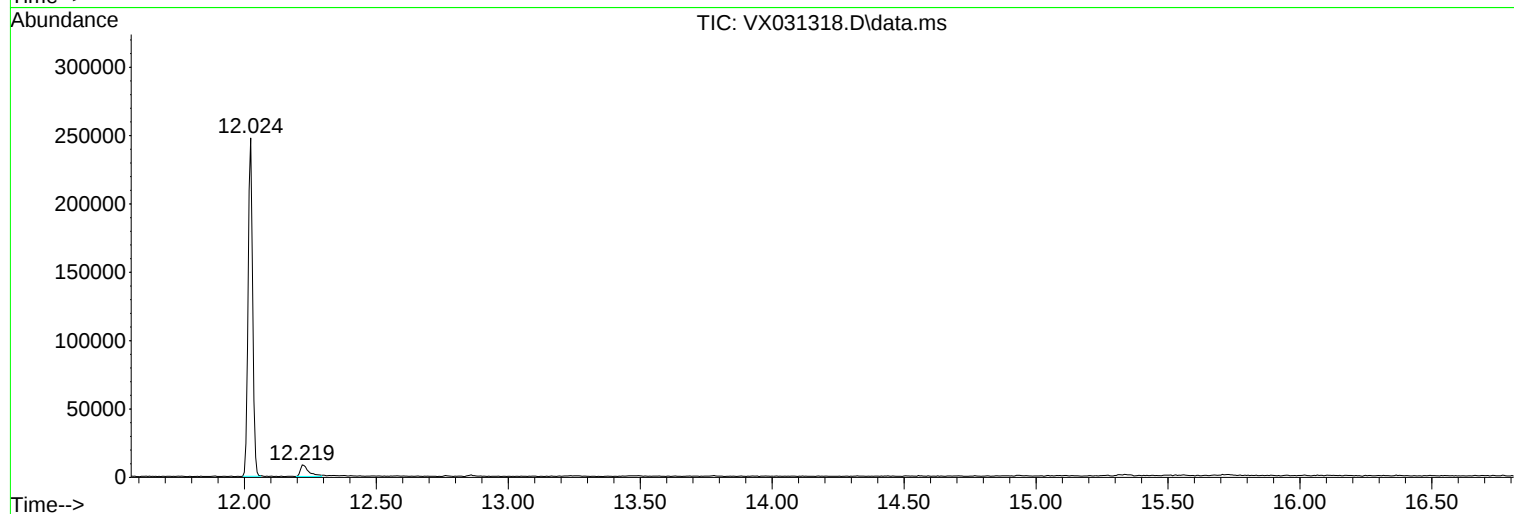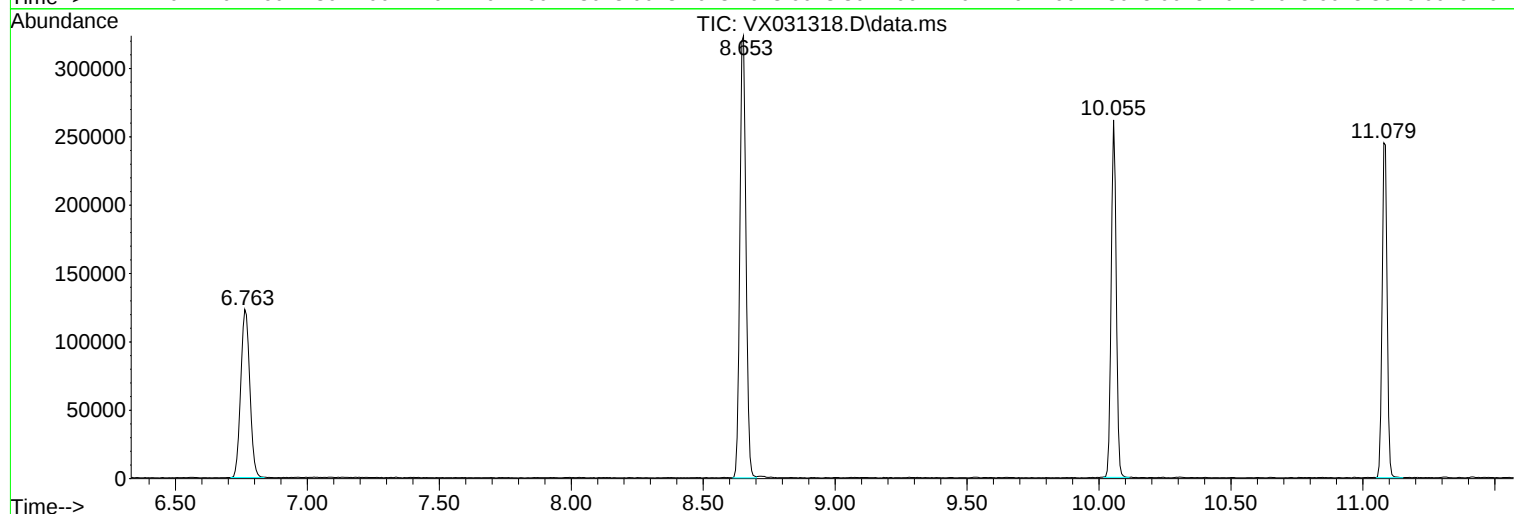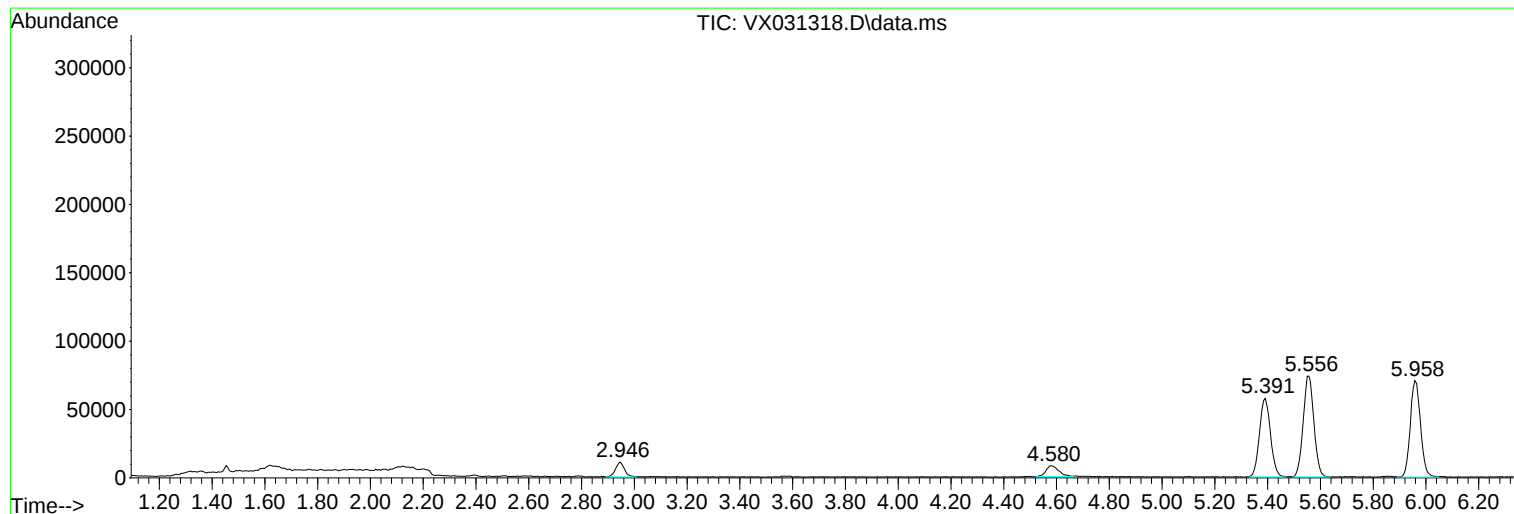

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031318.D
Acq On : 14 Sep 2022 20:14
Operator : JC/MD
Sample : N4492-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-02-133-143-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031318.D
Acq On : 14 Sep 2022 20:14
Operator : JC/MD
Sample : N4492-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-02-133-143-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------