

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
 Data File : VX031326.D
 Acq On : 14 Sep 2022 23:22
 Operator : JC/MD
 Sample : N4446-07RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-WATER-LIQUIDRE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.624	81	88	89	rBV6	2778	4364	1.12%	0.211%
2	2.392	209	214	226	rBV	4012	8281	2.12%	0.400%
3	2.788	274	279	288	rVB4	2983	5861	1.50%	0.283%
4	4.580	564	573	584	rBV3	2301	7300	1.87%	0.353%
5	5.385	694	705	719	rBV2	55789	161240	41.27%	7.795%
6	5.556	723	733	745	rVV	67646	190661	48.80%	9.217%
7	5.958	789	799	812	rBV	73200	193404	49.50%	9.350%
8	6.763	921	931	949	rBV	113415	268024	68.60%	12.957%
9	8.653	1234	1241	1250	rBV	247068	390703	100.00%	18.888%
10	10.055	1465	1471	1481	rBV	245079	322669	82.59%	15.599%
11	11.079	1634	1639	1645	rBV	181779	236654	60.57%	11.441%
12	12.024	1788	1794	1802	rBV	219878	275265	70.45%	13.307%
13	12.219	1821	1826	1832	rBV3	2155	4086	1.05%	0.198%




Sum of corrected areas: 2068512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031326.D
Acq On : 14 Sep 2022 23:22
Operator : JC/MD
Sample : N4446-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUIDRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

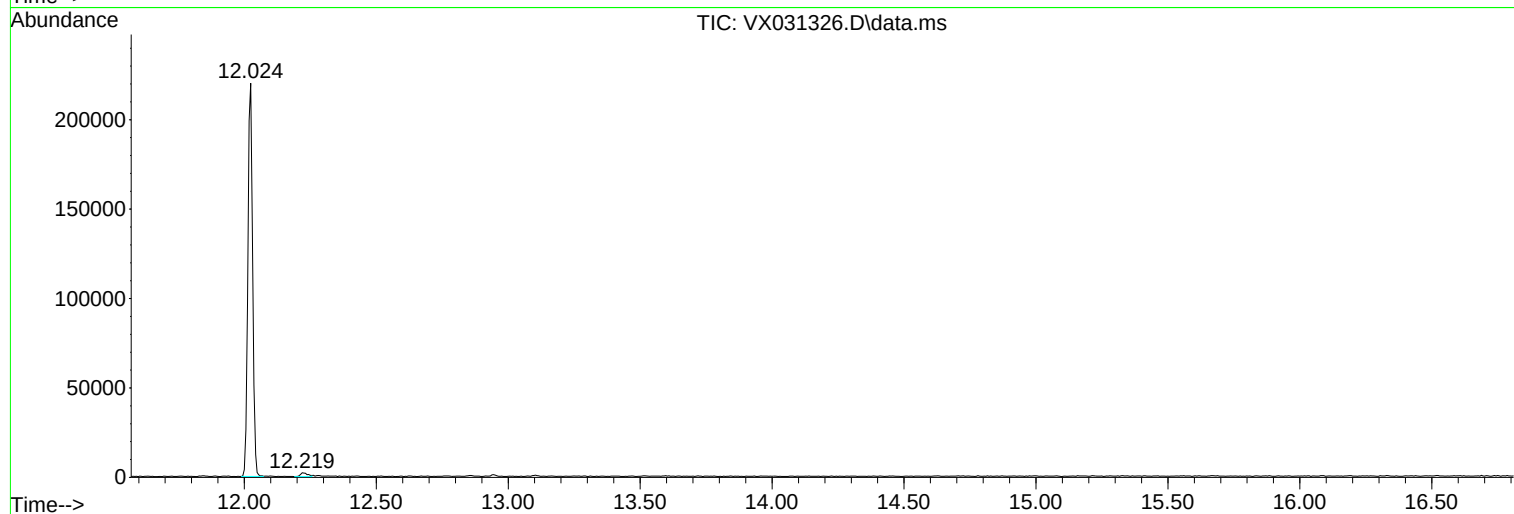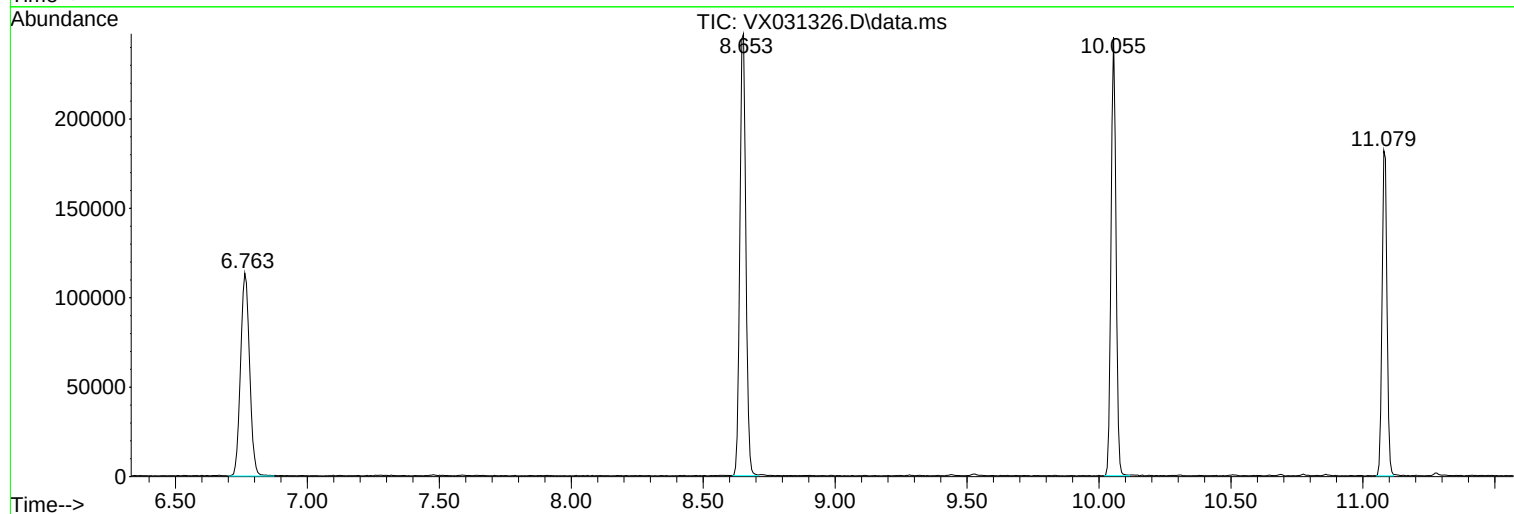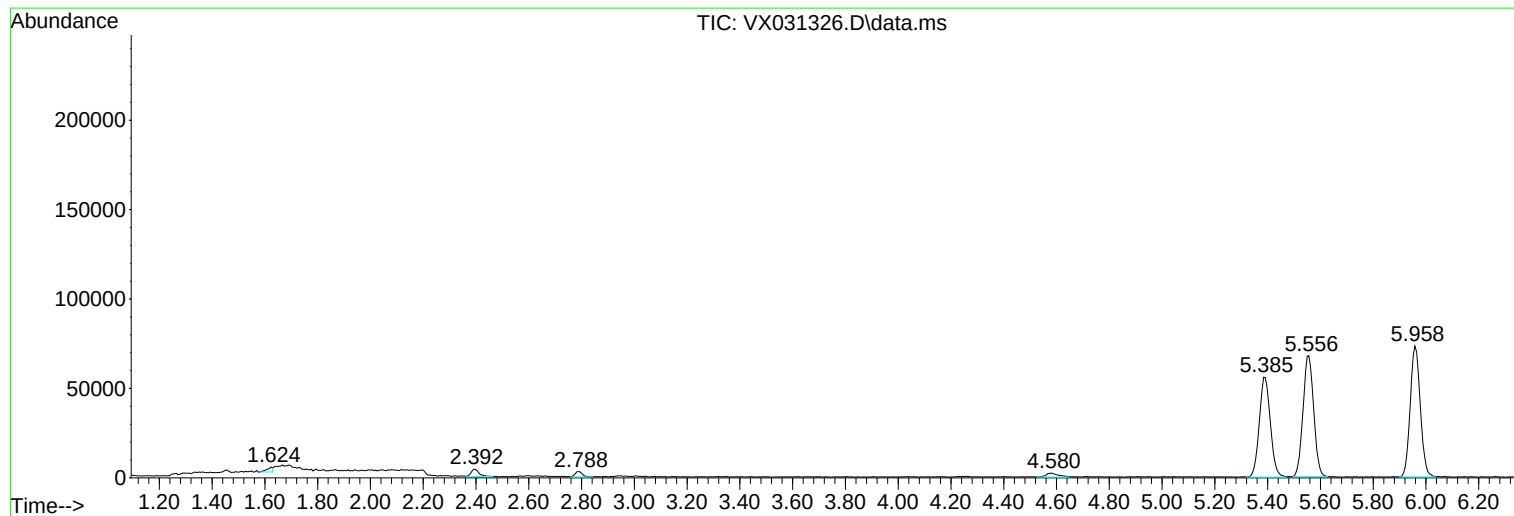

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031326.D
Acq On : 14 Sep 2022 23:22
Operator : JC/MD
Sample : N4446-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUIDRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031326.D
Acq On : 14 Sep 2022 23:22
Operator : JC/MD
Sample : N4446-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUIDRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------