


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091422\
Data File : VX031336.D
Acq On : 15 Sep 2022 03:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Title : SW846 8260
Last Update : Thu Sep 15 01:50:07 2022

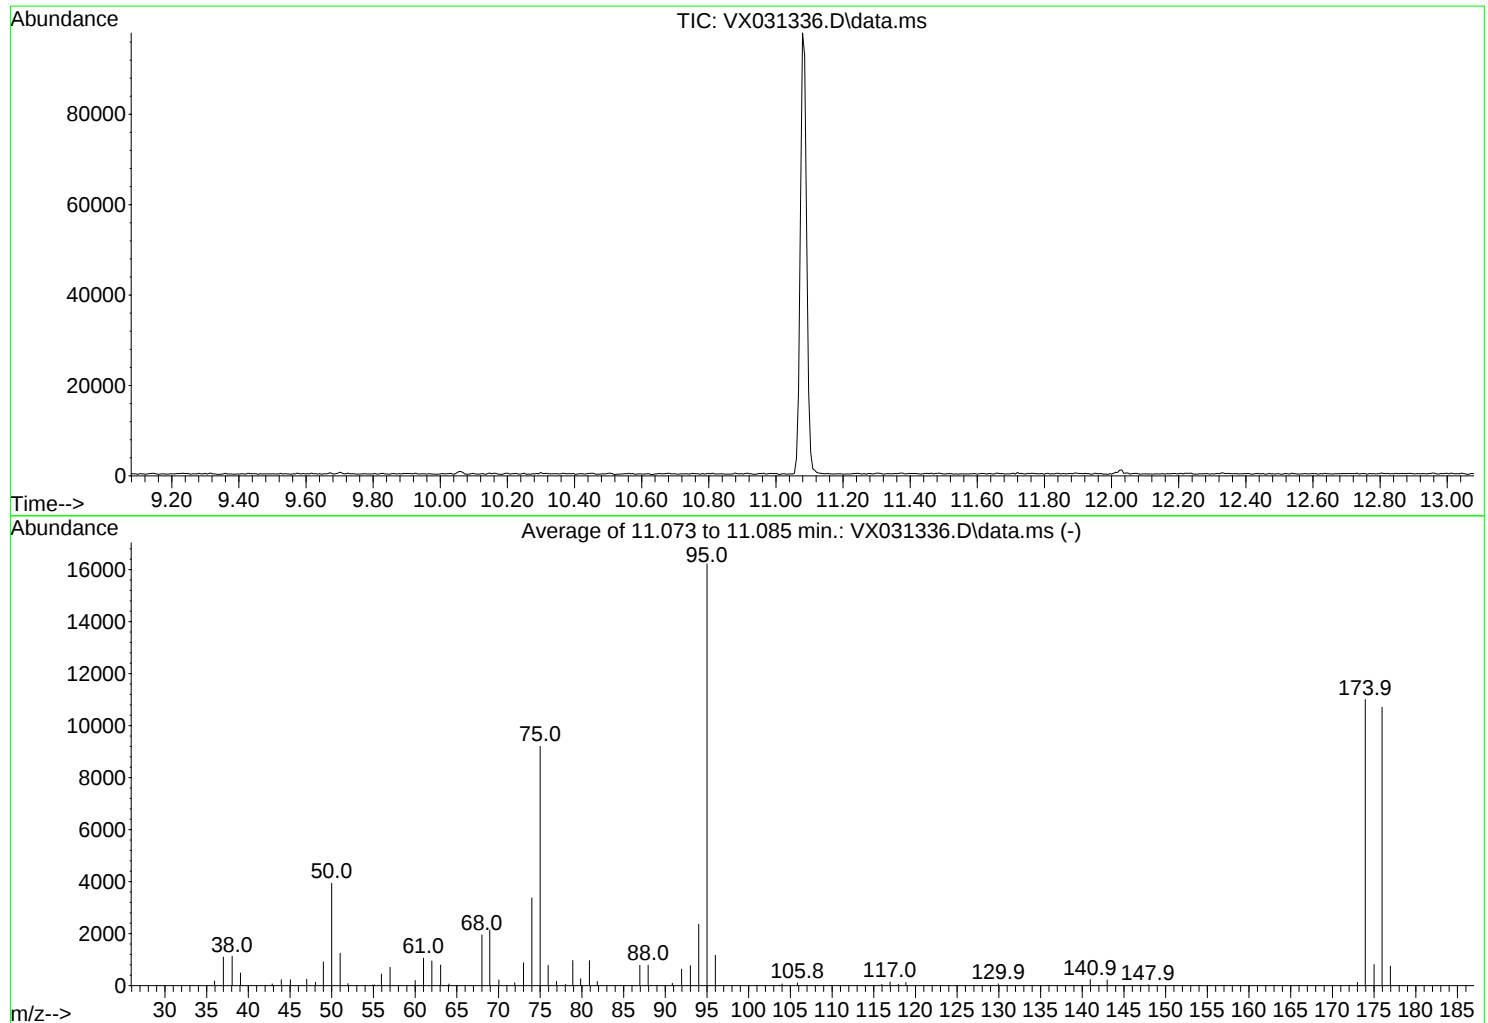

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	3938	PASS
75	95	30	60	56.8	9206	PASS
95	95	100	100	100.0	16220	PASS
96	95	5	9	7.2	1170	PASS
173	174	0.00	2	1.2	129	PASS
174	95	50	100	67.9	11006	PASS
175	174	5	9	7.4	814	PASS
176	174	95	101	97.3	10708	PASS
177	176	5	9	7.0	749	PASS