


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091522\
 Data File : BM036547.D
 Acq On : 15 Sep 2022 10:32
 Operator : CG/JU
 Sample : DFTPP075
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DFTPP075

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION
 Last Update : Fri Sep 16 02:39:54 2022

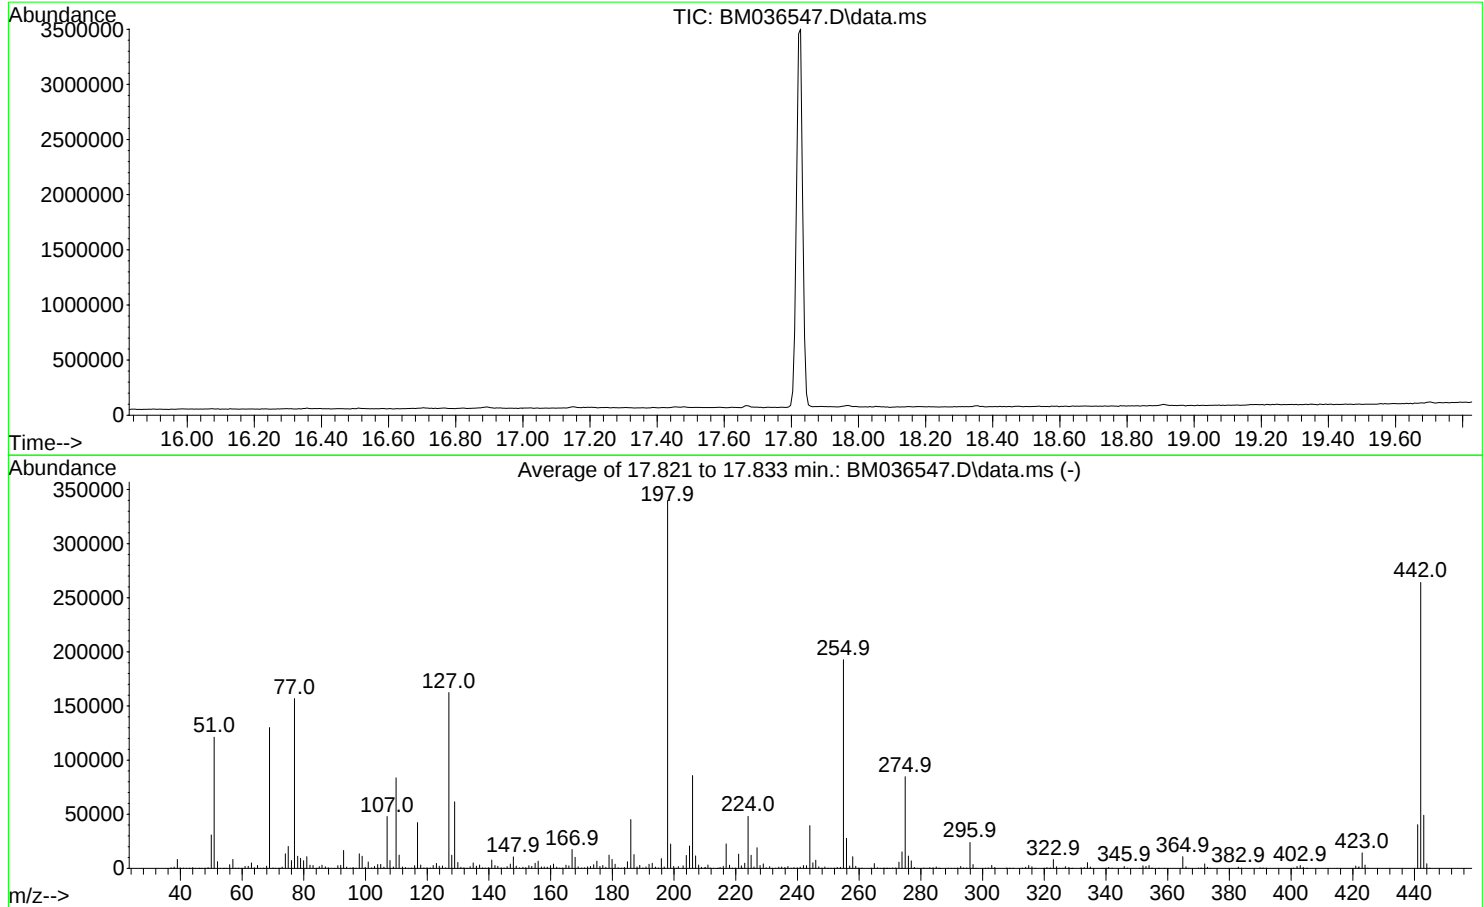

Spectrum Information: Average of 17.821 to 17.833 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	121200	PASS
68	69	0.00	2	1.7	2158	PASS
69	198	0.00	100	38.3	130136	PASS
70	69	0.00	2	0.4	517	PASS
127	198	10	80	47.8	162507	PASS
197	198	0.00	2	0.4	1285	PASS
198	198	100	100	100.0	339840	PASS
199	198	5	9	6.6	22447	PASS
275	198	10	60	24.9	84717	PASS
365	198	1	100	3.2	10825	PASS
441	198	0.01	100	11.9	40427	PASS
442	198	50	100	77.7	264213	PASS
443	442	15	24	18.6	49149	PASS