

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031359.D
 Acq On : 15 Sep 2022 17:22
 Operator : JC/MD
 Sample : N4502-02 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DEACON-WATER-COMP

Quant Time: Sep 16 04:55:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 01:50:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	96313	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	161179	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	141193	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	63567	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	101592	42.974	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.940%
35) Dibromofluoromethane	5.391	113	83206	48.025	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.040%
50) Toluene-d8	8.652	98	313751	48.276	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.560%
62) 4-Bromofluorobenzene	11.079	95	99884	41.970	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	83.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031359.D
Acq On : 15 Sep 2022 17:22
Operator : JC/MD
Sample : N4502-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEACON-WATER-COMP

Quant Time: Sep 16 04:55:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 01:50:07 2022
Response via : Initial Calibration




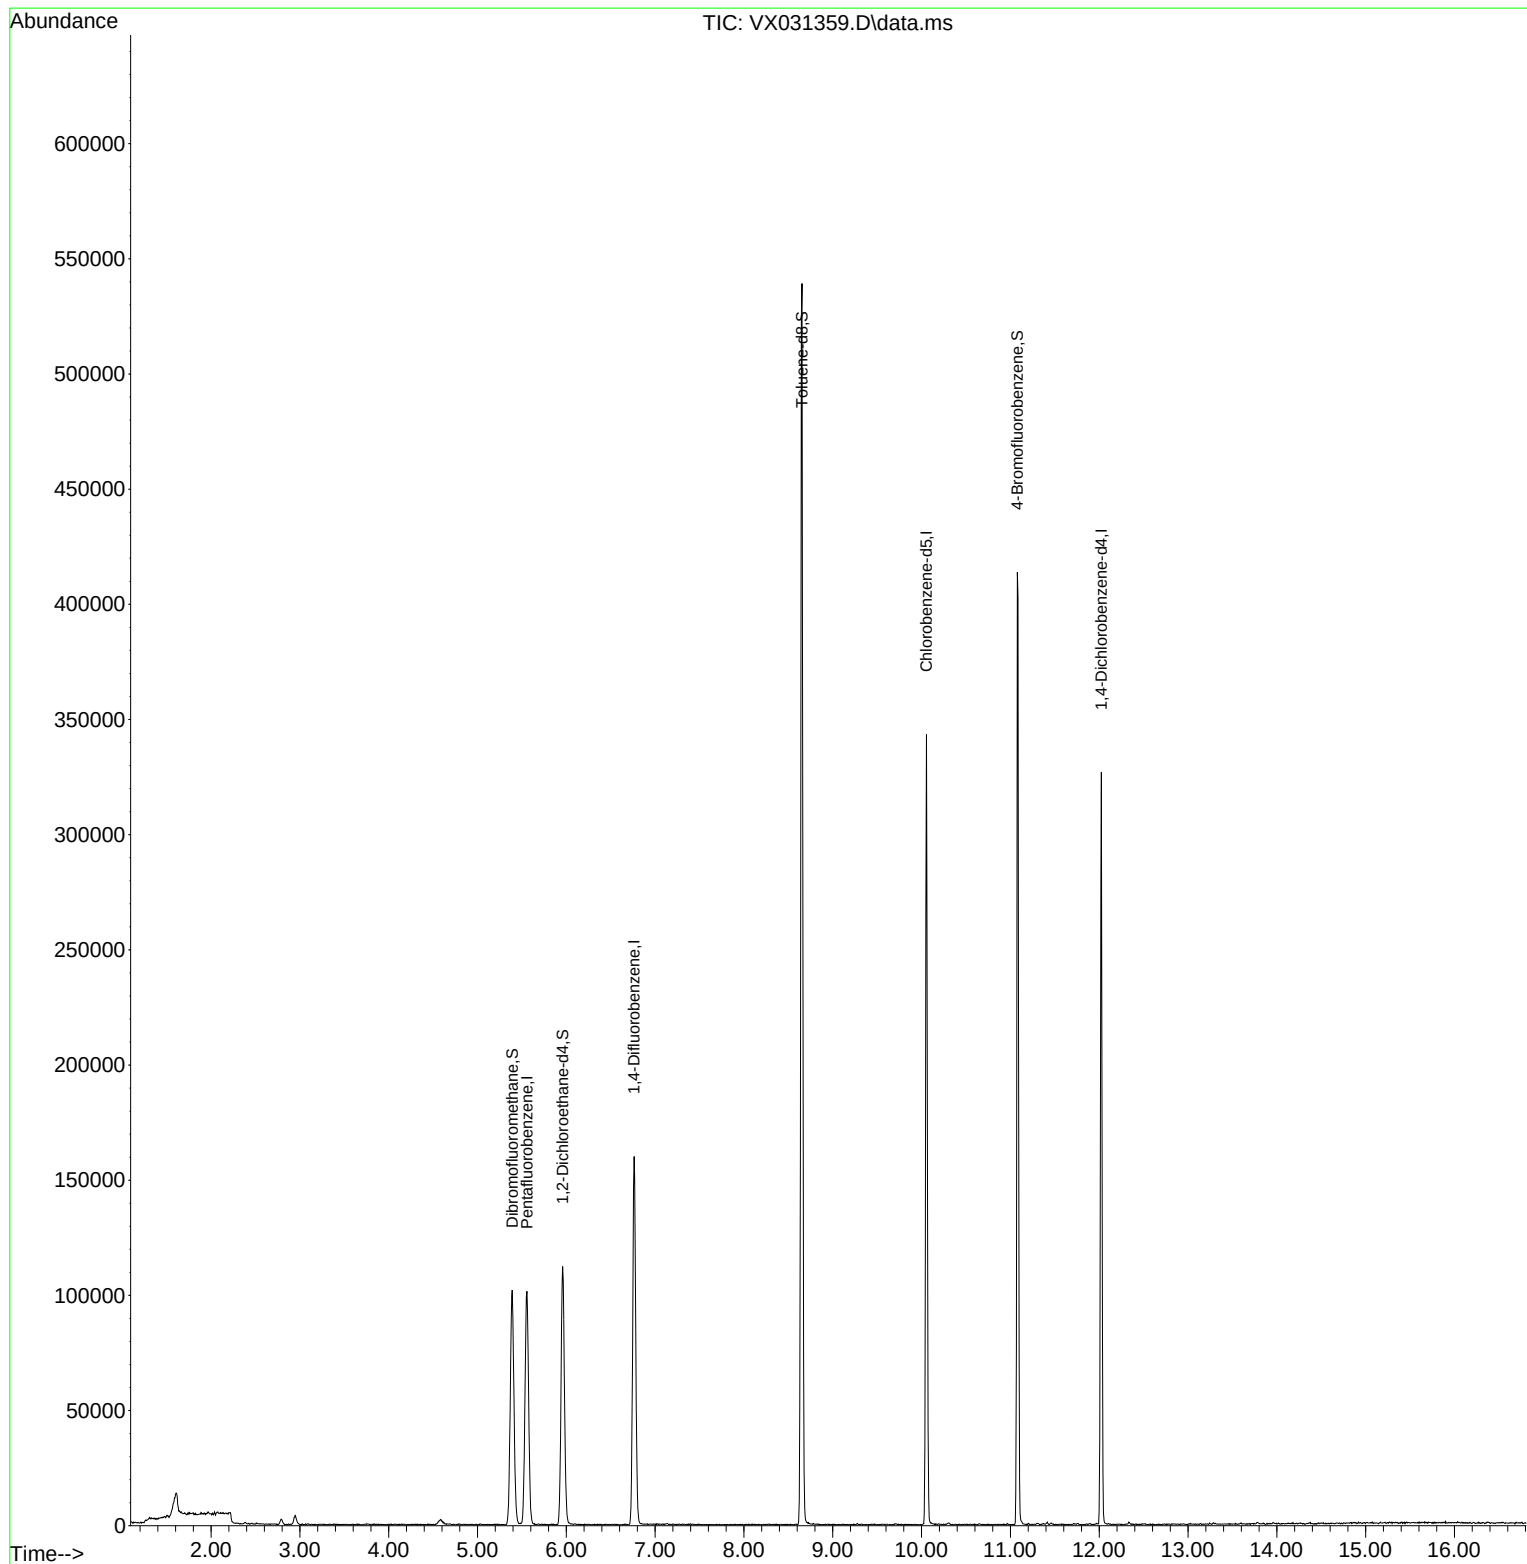


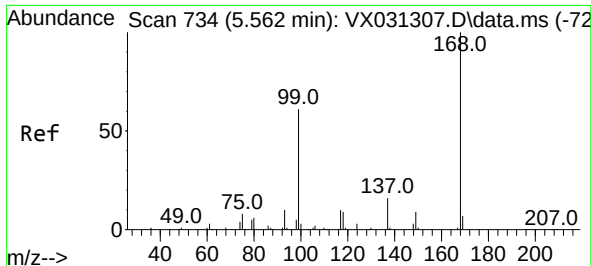

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22




Instrument :
MSVOA_X
ClientSampleId :
DEACON-WATER-COMP


Tgt Ion:168 Resp: 96313
Ion Ratio Lower Upper
168 100
99 53.8 48.8 73.2

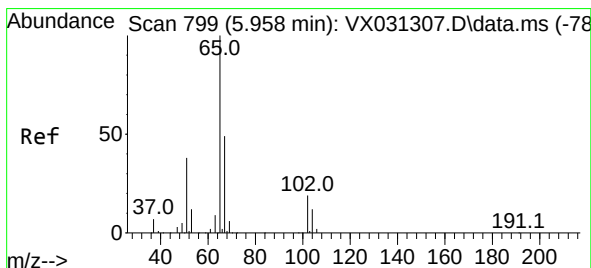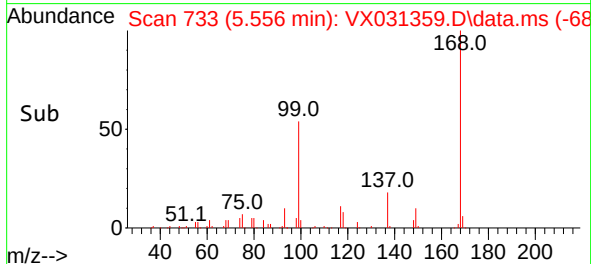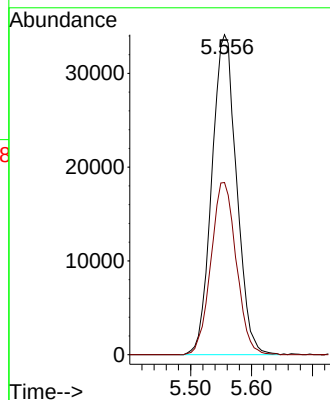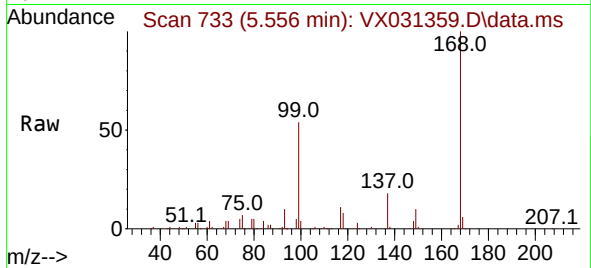

#33
1,2-Dichloroethane-d4
Concen: 42.974 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22

Tgt Ion: 65 Resp: 101592
Ion Ratio Lower Upper
65 100
67 51.6 0.0 102.4


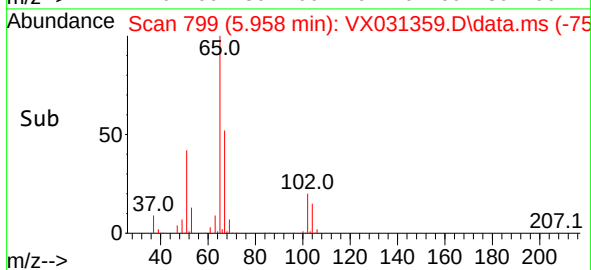
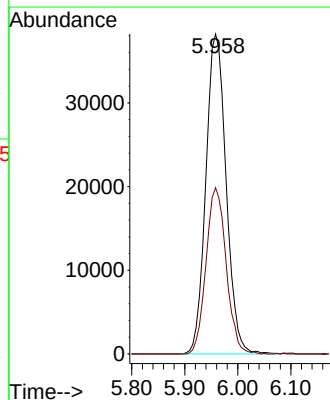
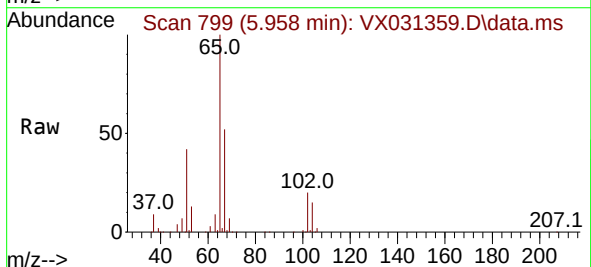


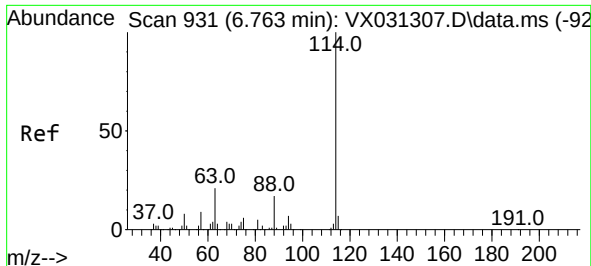

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22




Instrument :
MSVOA_X
ClientSampleId :
DEACON-WATER-COMP


Tgt Ion:114 Resp: 161179
Ion Ratio Lower Upper
114 100
63 21.6 0.0 42.6
88 14.8 0.0 33.0

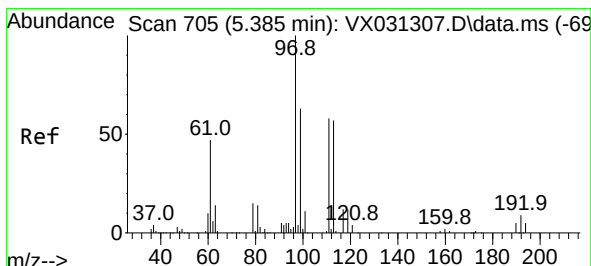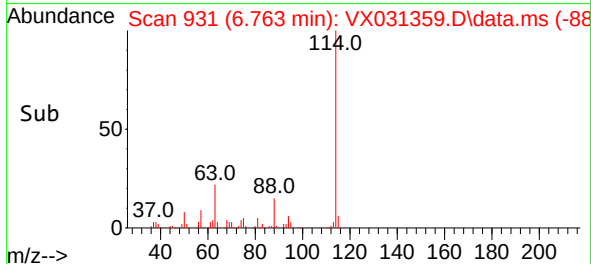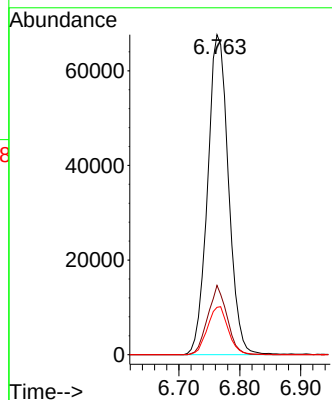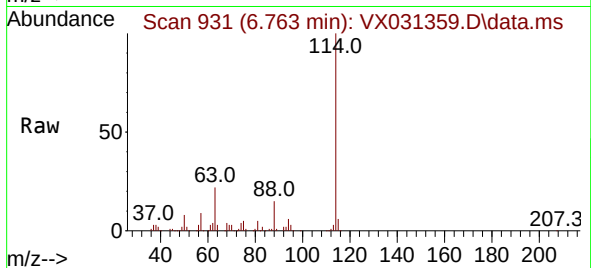

#35
Dibromofluoromethane
Concen: 48.025 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22

Tgt Ion:113 Resp: 83206
Ion Ratio Lower Upper
113 100
111 102.7 82.4 123.6
192 18.8 14.1 21.1


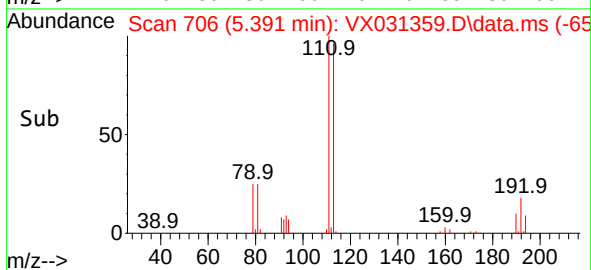
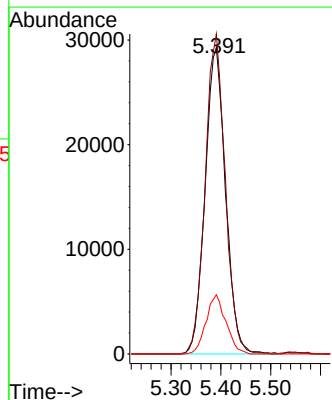
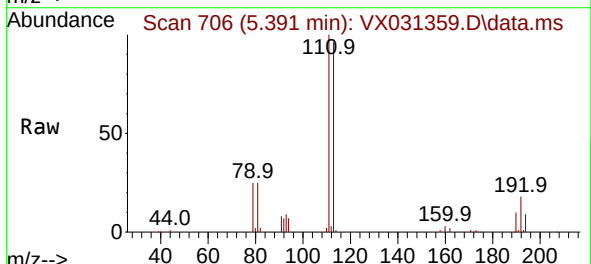


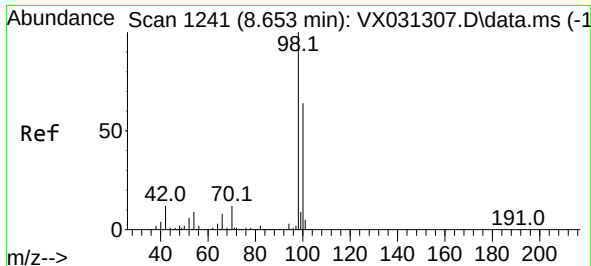

#50
Toluene-d8
Concen: 48.276 ug/l
RT: 8.652 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22




Instrument :
MSVOA_X
ClientSampleId :
DEACON-WATER-COMP


Tgt Ion: 98 Resp: 313751
Ion Ratio Lower Upper
98 100
100 65.8 52.5 78.7

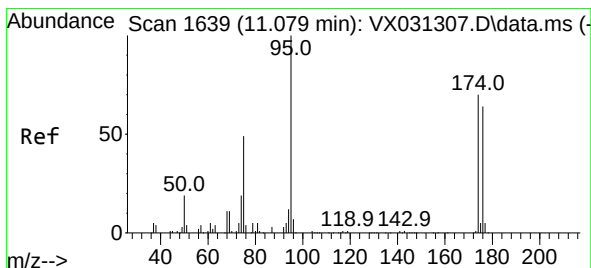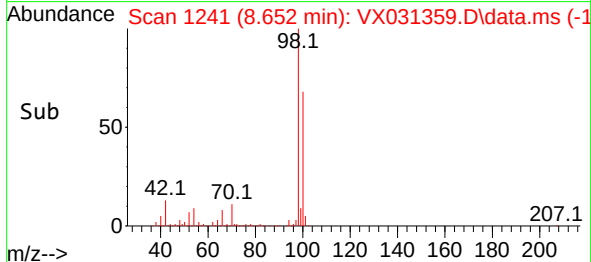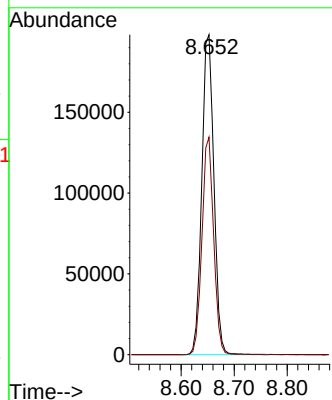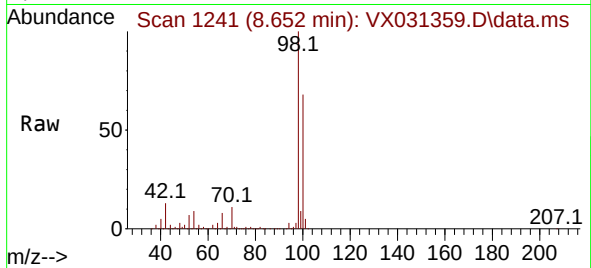

#62
4-Bromofluorobenzene
Concen: 41.970 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX031359.D
Acq: 15 Sep 2022 17:22

Tgt Ion: 95 Resp: 99884
Ion Ratio Lower Upper
95 100
174 84.6 0.0 153.2
176 81.3 0.0 144.0

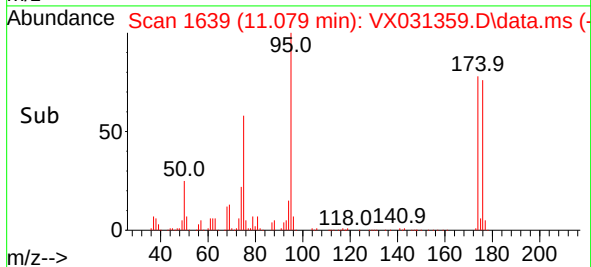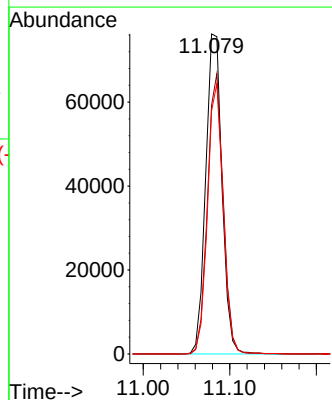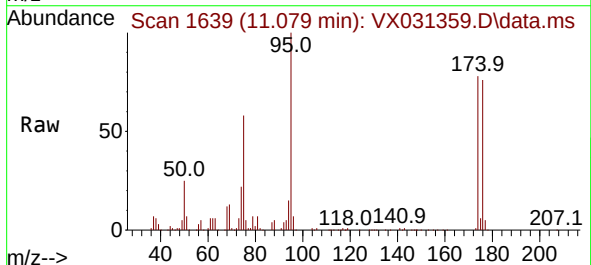

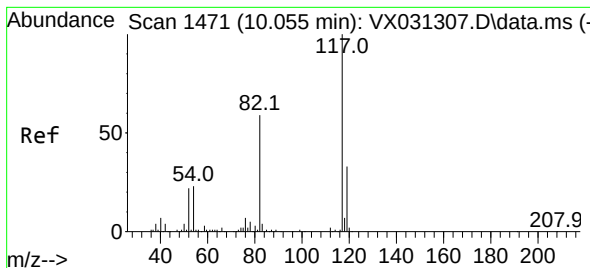

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX031359.D

Acq: 15 Sep 2022 17:22

Instrument :

MSVOA_X

ClientSampleId :

DEACON-WATER-COMP





Tgt Ion:117 Resp: 141193

Ion Ratio Lower Upper

117 100

82 55.0 46.8 70.2

119 31.7 26.4 39.6

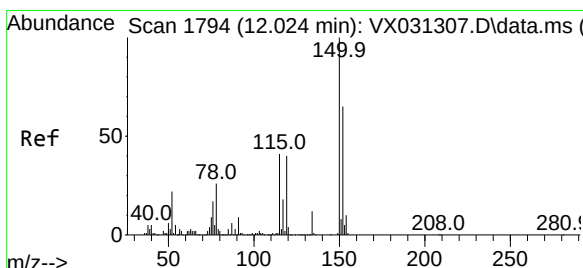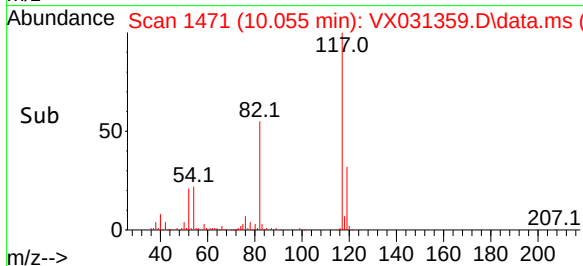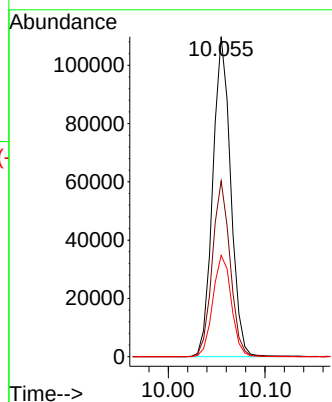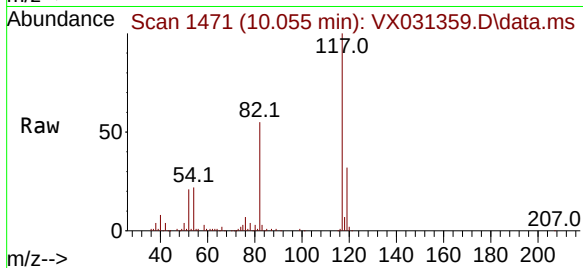

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX031359.D

Acq: 15 Sep 2022 17:22

Tgt Ion:152 Resp: 63567

Ion Ratio Lower Upper

152 100

115 58.9 43.4 130.1

150 156.8 0.0 346.8

