

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031366.D
 Acq On : 15 Sep 2022 20:06
 Operator : JC/MD
 Sample : N4508-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-05-3-13-090122

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.611	73	86	93	rBV7	7012	29682	3.43%	0.825%
2	3.117	325	333	342	rVB2	7702	18737	2.17%	0.521%
3	4.495	551	559	569	rBV2	6204	15877	1.83%	0.441%
4	5.391	692	706	722	rBV	102098	293930	33.97%	8.166%
5	5.556	722	733	747	rVB	103123	285141	32.95%	7.922%
6	5.958	789	799	813	rBV	114223	297679	34.40%	8.271%
7	6.763	920	931	942	rBV	158934	378537	43.75%	10.517%
8	8.653	1234	1241	1250	rBV	546140	865311	100.00%	24.041%
9	10.055	1465	1471	1485	rBV	343943	453868	52.45%	12.610%
10	11.079	1634	1639	1653	rVB	427559	554424	64.07%	15.404%
11	12.024	1788	1794	1802	rBV	328611	406089	46.93%	11.283%




Sum of corrected areas: 3599275

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031366.D
Acq On : 15 Sep 2022 20:06
Operator : JC/MD
Sample : N4508-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05-3-13-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

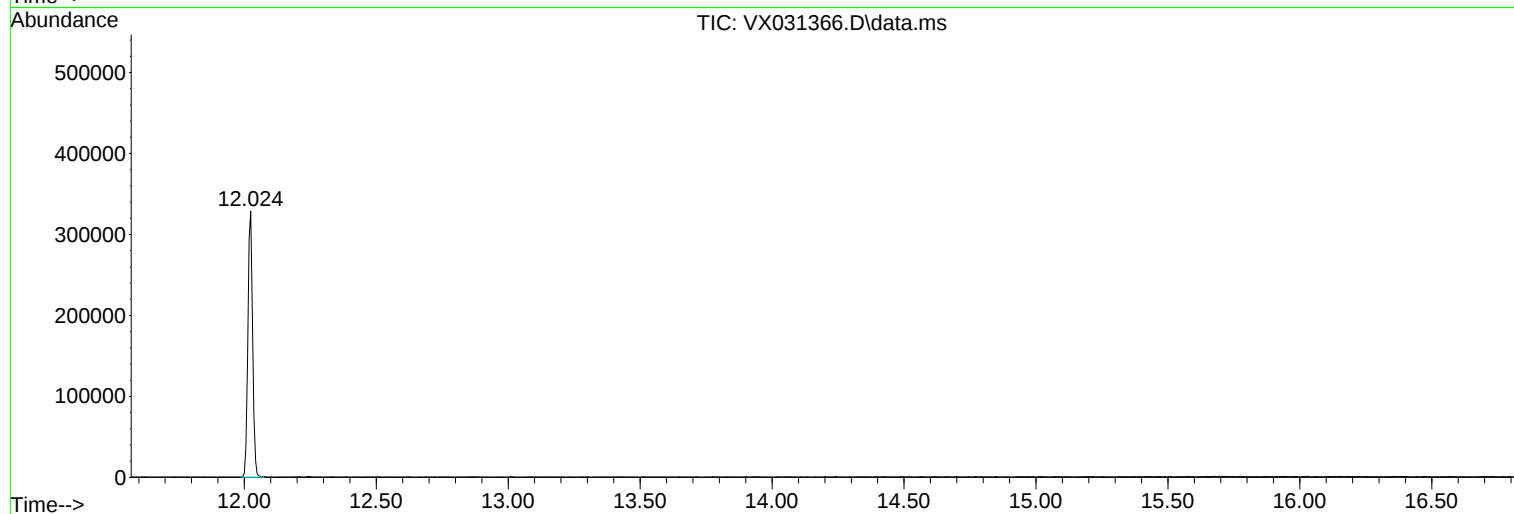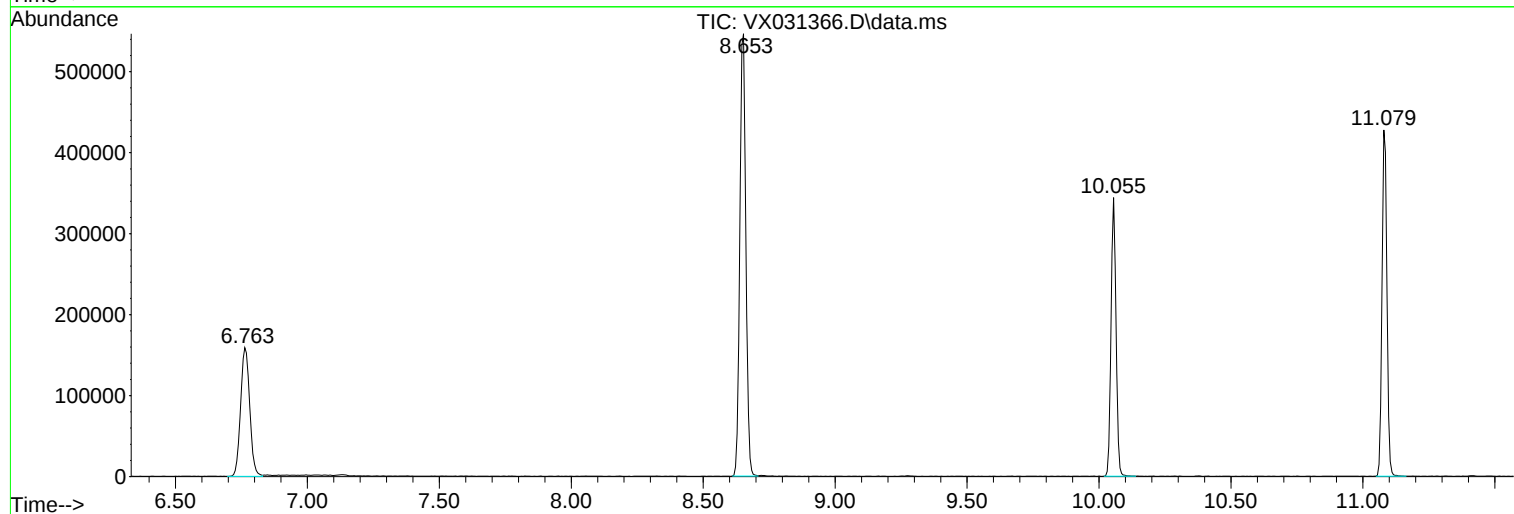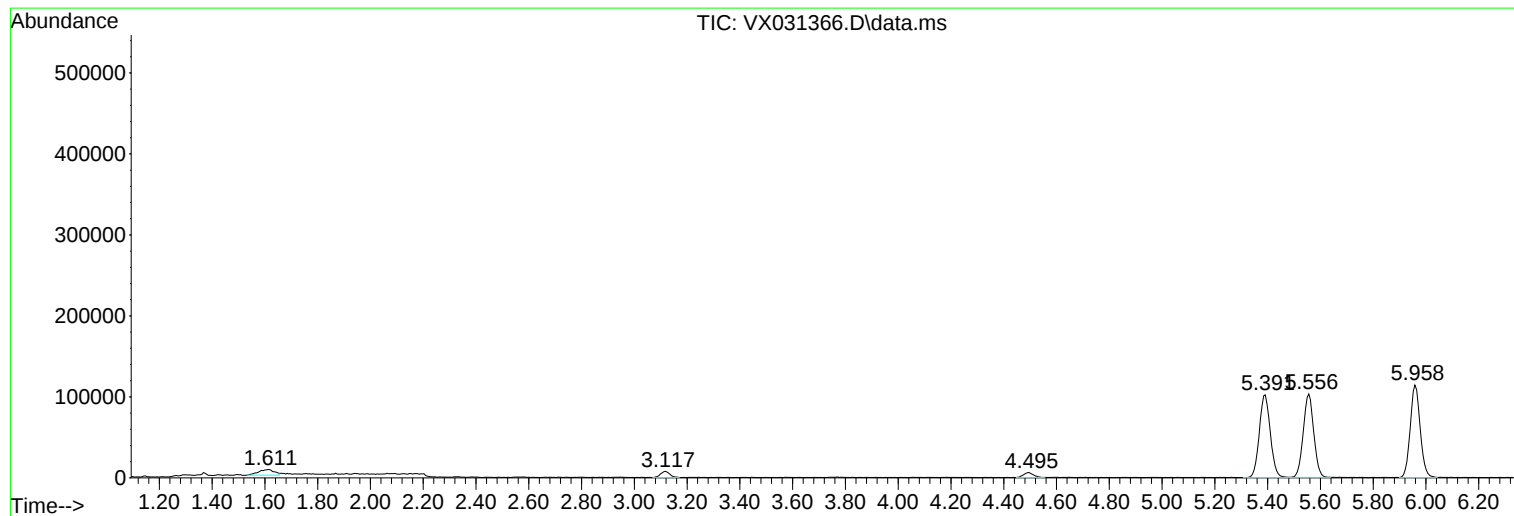

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031366.D
Acq On : 15 Sep 2022 20:06
Operator : JC/MD
Sample : N4508-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05-3-13-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031366.D
Acq On : 15 Sep 2022 20:06
Operator : JC/MD
Sample : N4508-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-05-3-13-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------