

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031369.D
 Acq On : 15 Sep 2022 21:16
 Operator : JC/MD
 Sample : N4508-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB02-090222

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Title : SW846 8260

Signal : TIC: VX031369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	76	87	88	rBV5	6143	13611	1.65%	0.394%
2	2.392	207	214	222	rBV2	5551	10724	1.30%	0.311%
3	2.940	296	304	312	rBV	7888	19002	2.30%	0.551%
4	4.580	562	573	585	rBV3	4535	14878	1.80%	0.431%
5	5.391	693	706	720	rBV	96749	282180	34.17%	8.175%
6	5.556	720	733	747	rVB2	98881	277468	33.60%	8.039%
7	5.958	787	799	816	rBV2	108027	287903	34.86%	8.341%
8	6.763	922	931	943	rBV2	154512	364768	44.17%	10.568%
9	8.653	1234	1241	1258	rBV	525345	825860	100.00%	23.927%
10	10.055	1465	1471	1479	rBV	333956	436510	52.86%	12.647%
11	11.079	1634	1639	1651	rVB	404303	526712	63.78%	15.260%
12	12.024	1788	1794	1801	rBV	319514	391932	47.46%	11.355%




Sum of corrected areas: 3451548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031369.D
Acq On : 15 Sep 2022 21:16
Operator : JC/MD
Sample : N4508-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-090222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

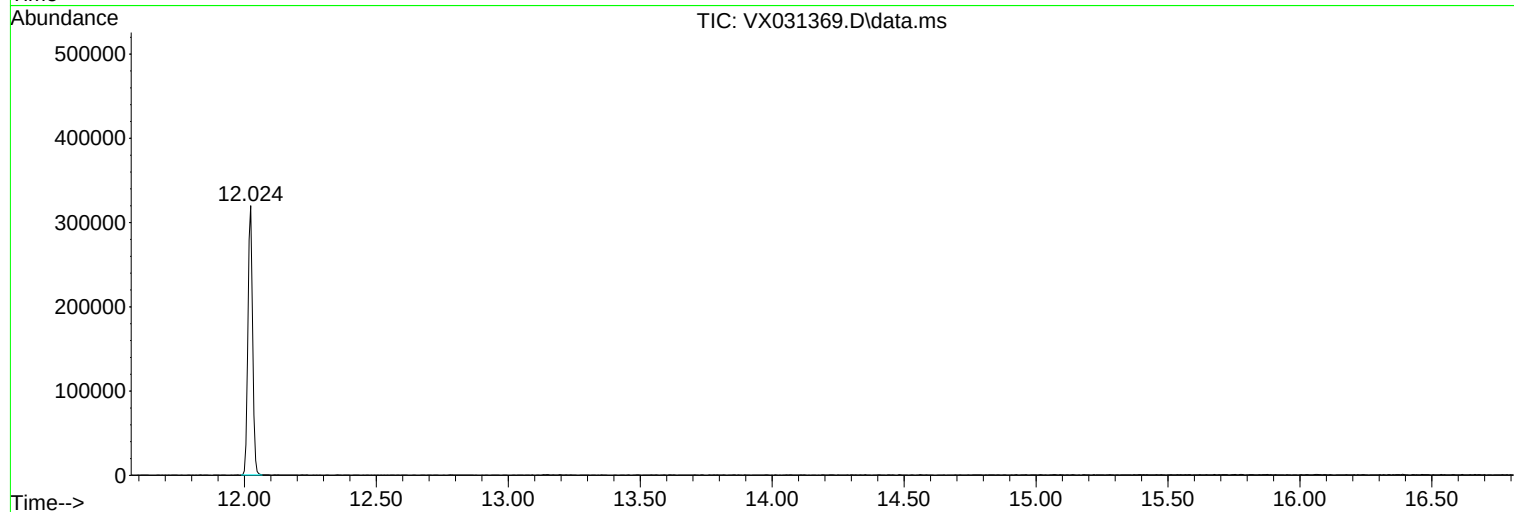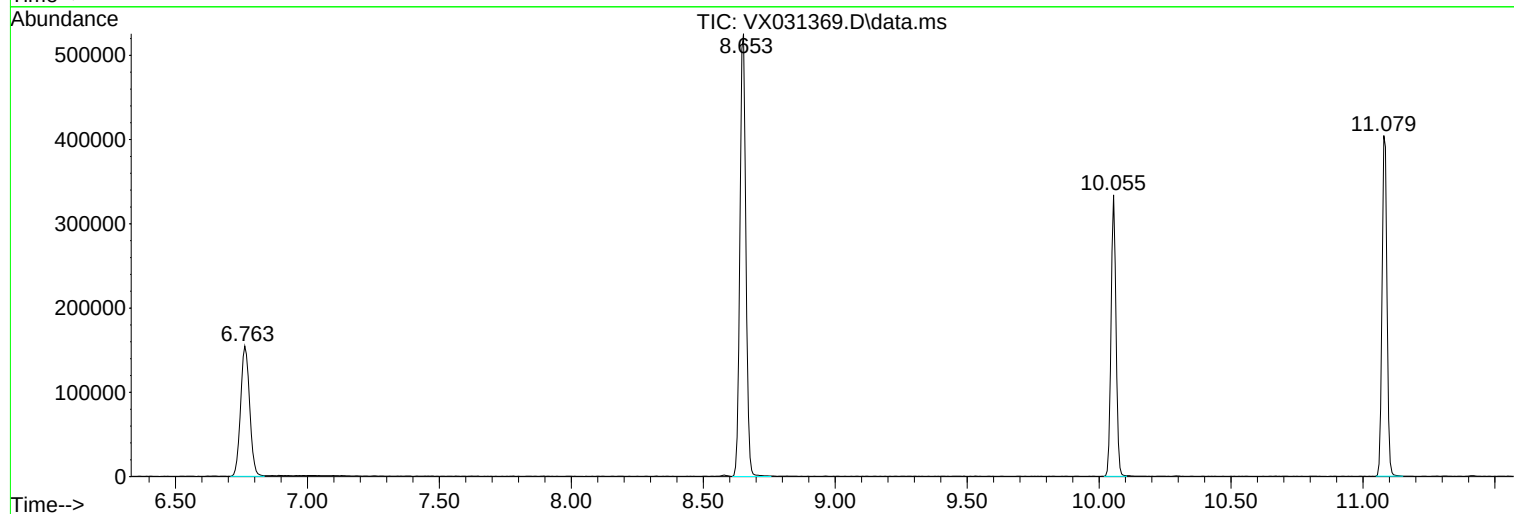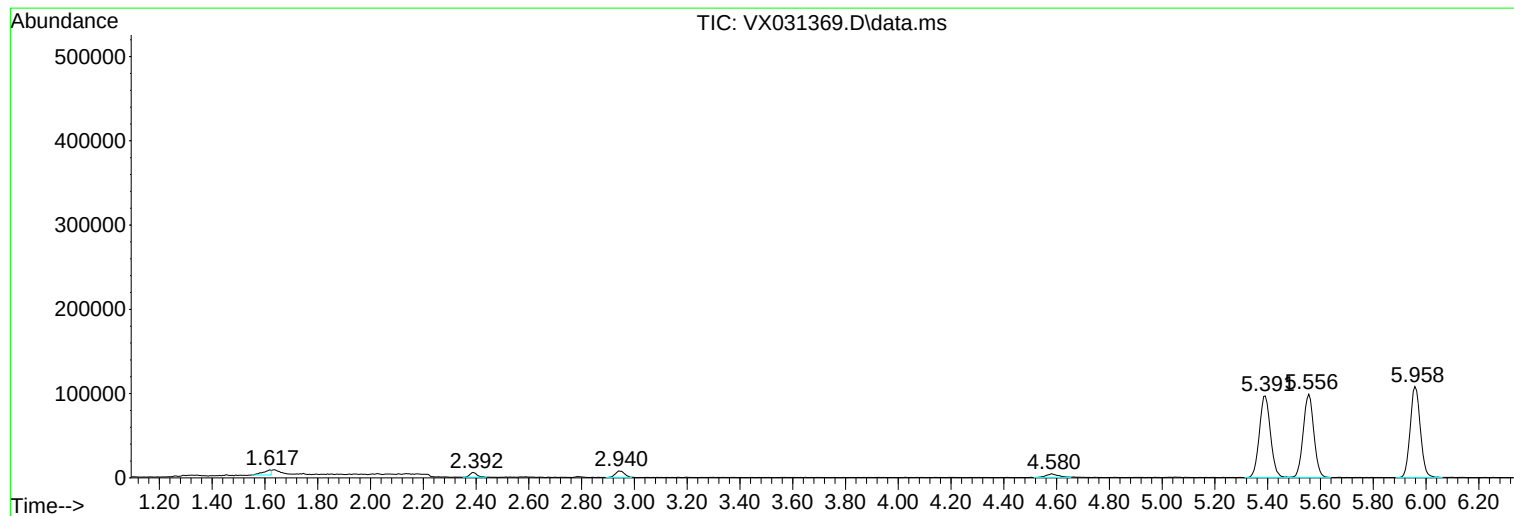

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031369.D
Acq On : 15 Sep 2022 21:16
Operator : JC/MD
Sample : N4508-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-090222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031369.D
Acq On : 15 Sep 2022 21:16
Operator : JC/MD
Sample : N4508-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-090222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc