

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031372.D
 Acq On : 15 Sep 2022 22:26
 Operator : JC/MD
 Sample : N4508-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BR-03-117-137-090222

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	75	83	85	rBV5	5933	14824	1.81%	0.328%
2	2.136	167	172	180	rVB10	3613	8511	1.04%	0.189%
3	2.319	196	202	209	rBV	108555	166773	20.36%	3.695%
4	2.386	209	213	220	rVB	16534	28455	3.47%	0.630%
5	2.563	229	242	255	rVB	10859	31871	3.89%	0.706%
6	3.093	323	329	338	rVB	7171	13865	1.69%	0.307%
7	3.611	408	414	423	rVB	7563	17331	2.12%	0.384%
8	4.489	547	558	571	rBV	49960	136628	16.68%	3.027%
9	5.385	694	705	721	rBV	94879	277394	33.87%	6.145%
10	5.550	721	732	746	rVB	95412	270607	33.04%	5.995%
11	5.958	788	799	811	rBV2	108169	284092	34.68%	6.294%
12	6.092	814	821	833	rVB3	5250	13807	1.69%	0.306%
13	6.763	922	931	944	rBV	150282	355500	43.40%	7.876%
14	7.129	980	991	1002	rBV	337181	724713	88.48%	16.055%
15	8.653	1233	1241	1251	rBV	517141	819106	100.00%	18.146%
16	10.055	1465	1471	1483	rBV	324248	430498	52.56%	9.537%
17	11.079	1634	1639	1652	rBV	413764	526191	64.24%	11.657%
18	12.024	1788	1794	1804	rBV	318278	393705	48.07%	8.722%




Sum of corrected areas: 4513871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031372.D
Acq On : 15 Sep 2022 22:26
Operator : JC/MD
Sample : N4508-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-03-117-137-090222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

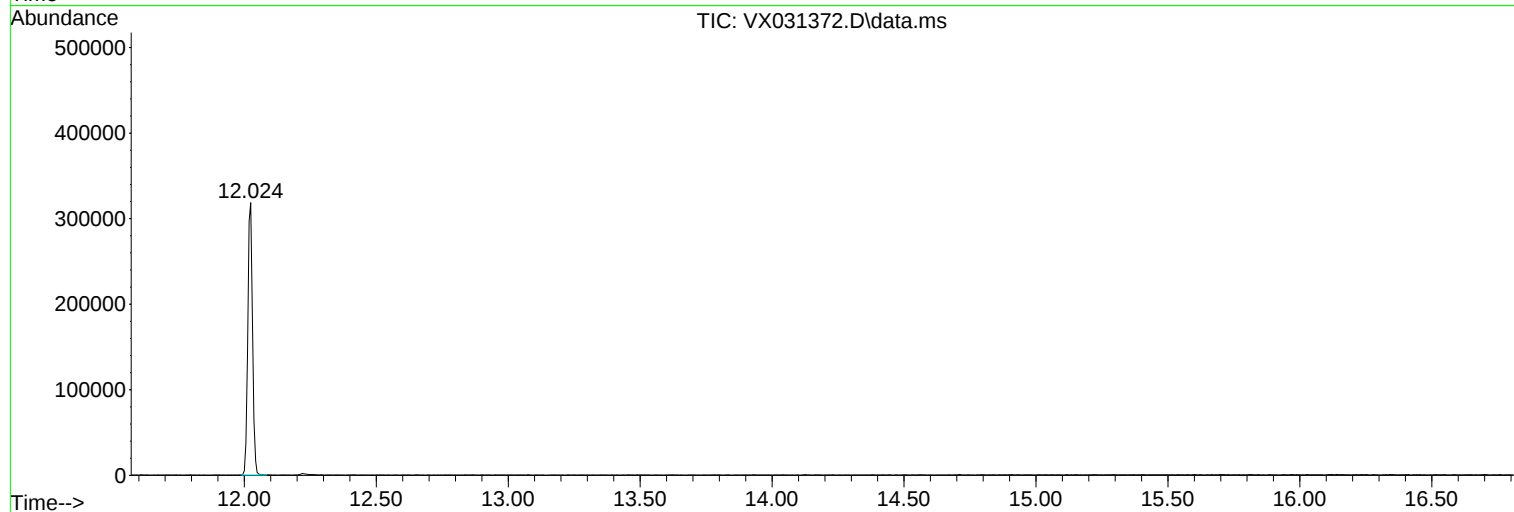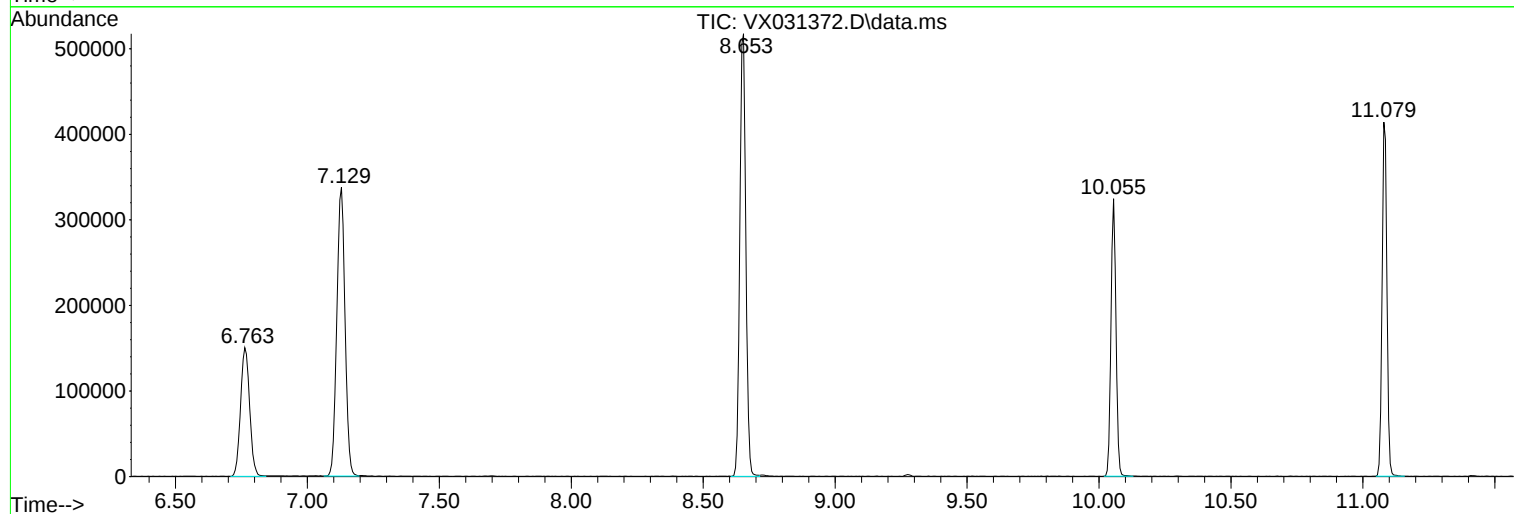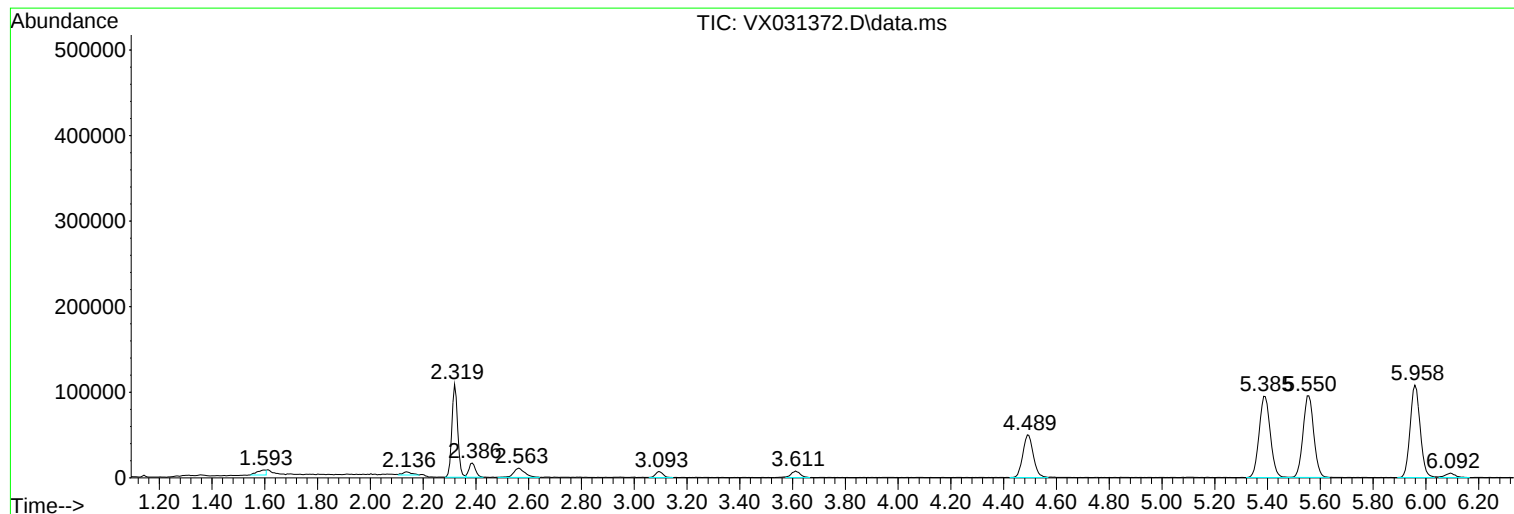

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031372.D
Acq On : 15 Sep 2022 22:26
Operator : JC/MD
Sample : N4508-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-03-117-137-090222










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.563	5.89 ug/l	31871	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	74
2			4-Penten-2-ol	86	C5H10O	000625-31-0	9
3			Ethylamine	45	C2H7N	000075-04-7	5
4			Formamide	45	CH3NO	000075-12-7	4
5			2-Pentanol, 3-methyl-	102	C6H14O	000565-60-6	4

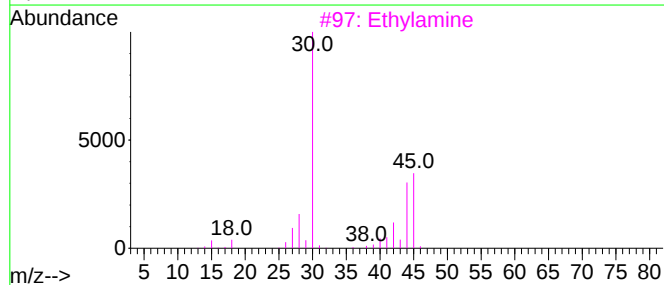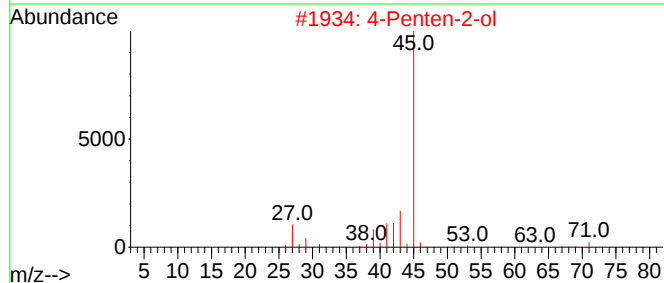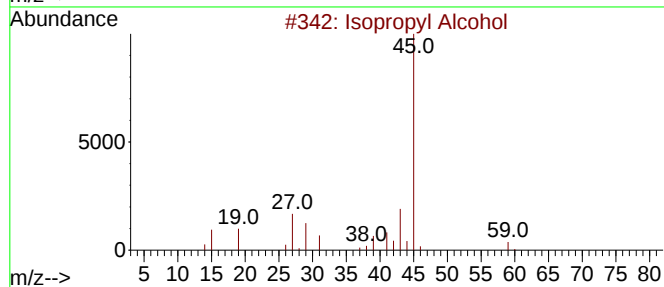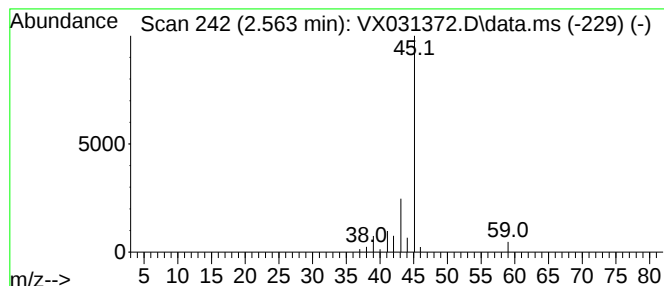

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031372.D
Acq On : 15 Sep 2022 22:26
Operator : JC/MD
Sample : N4508-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BR-03-117-137-090222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.563	5.9	ug/l	31871	1	5.550	270607	50.0