

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031395.D
 Acq On : 16 Sep 2022 08:32
 Operator : JC/MD
 Sample : N4537-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	24	32	42	rBV3	5337	19886	2.53%	0.583%
2	1.617	77	87	88	rBV6	4366	10338	1.32%	0.303%
3	2.946	296	305	319	rVB	16822	38747	4.94%	1.136%
4	4.580	561	573	582	rBV2	5612	20399	2.60%	0.598%
5	5.391	695	706	718	rBV	93852	267213	34.05%	7.834%
6	5.556	723	733	750	rVB	93237	264877	33.75%	7.765%
7	5.958	788	799	812	rBV	104431	272328	34.70%	7.984%
8	6.763	920	931	943	rBV	146410	345522	44.03%	10.130%
9	8.647	1234	1240	1251	rBV	497821	784774	100.00%	23.007%
10	10.055	1465	1471	1483	rBV	328968	419087	53.40%	12.286%
11	11.079	1634	1639	1653	rBV	401012	517548	65.95%	15.173%
12	12.024	1788	1794	1802	rVB	303776	389950	49.69%	11.432%
13	12.244	1825	1830	1834	rBV2	18166	23479	2.99%	0.688%
14	14.371	2176	2179	2184	rVB4	5989	8399	1.07%	0.246%
15	14.780	2241	2246	2250	rBV2	7684	11532	1.47%	0.338%
16	15.182	2307	2312	2315	rBV6	4916	8111	1.03%	0.238%
17	15.377	2337	2344	2347	rBV9	3983	8823	1.12%	0.259%




Sum of corrected areas: 3411013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031395.D
Acq On : 16 Sep 2022 08:32
Operator : JC/MD
Sample : N4537-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

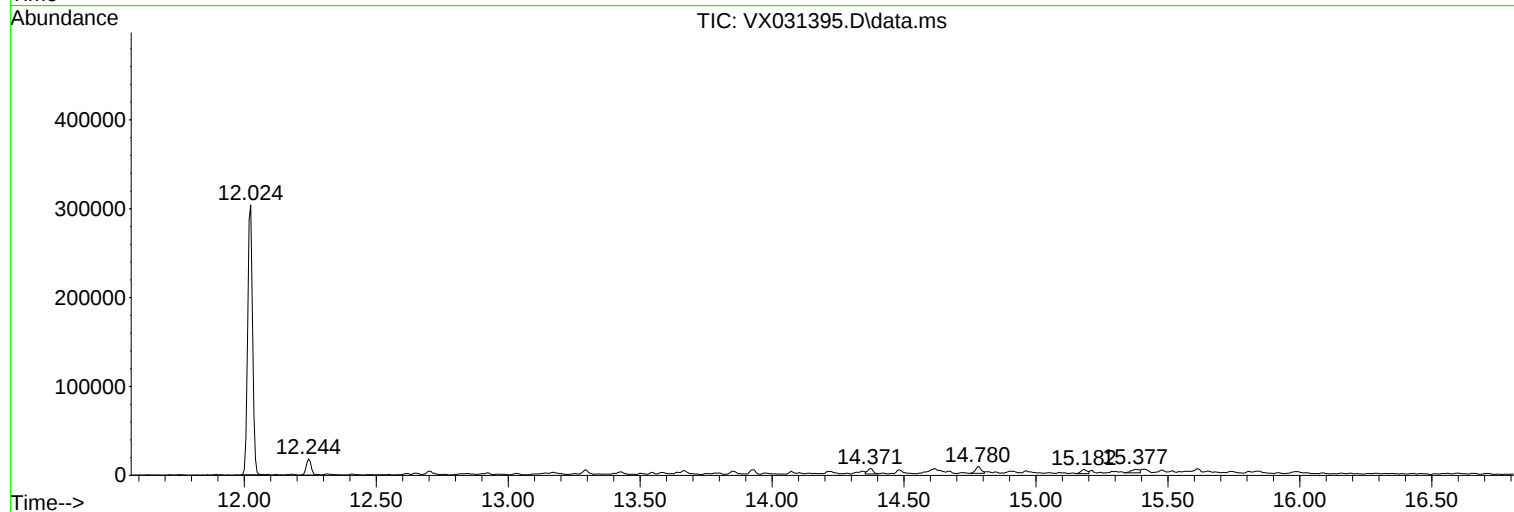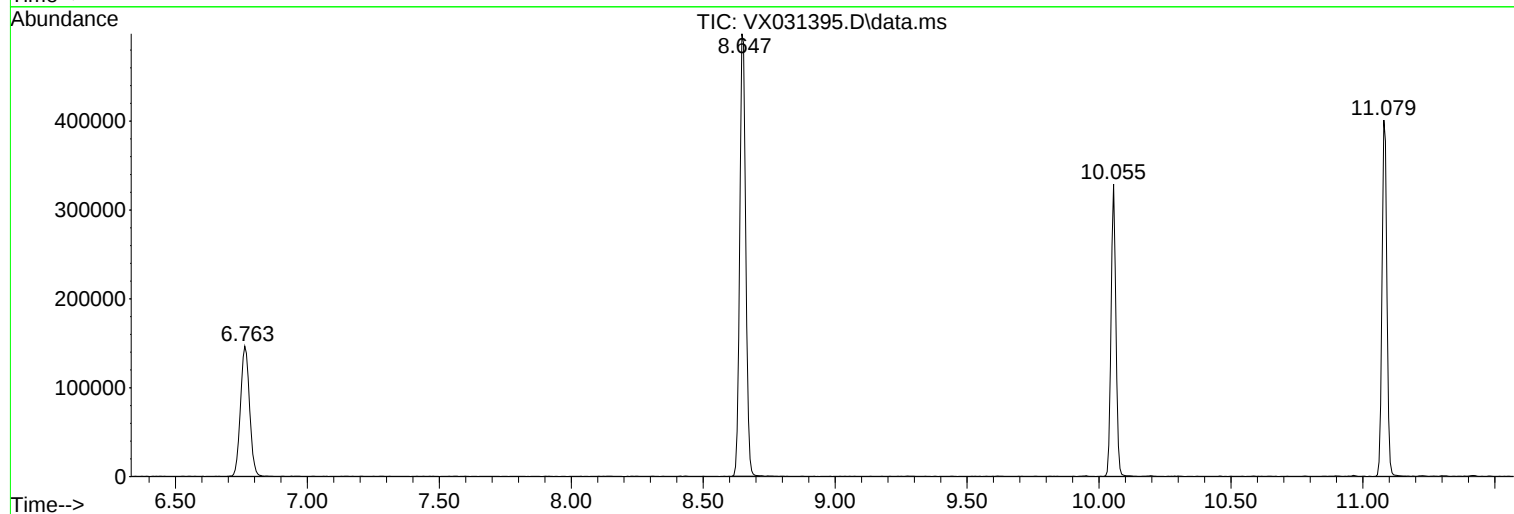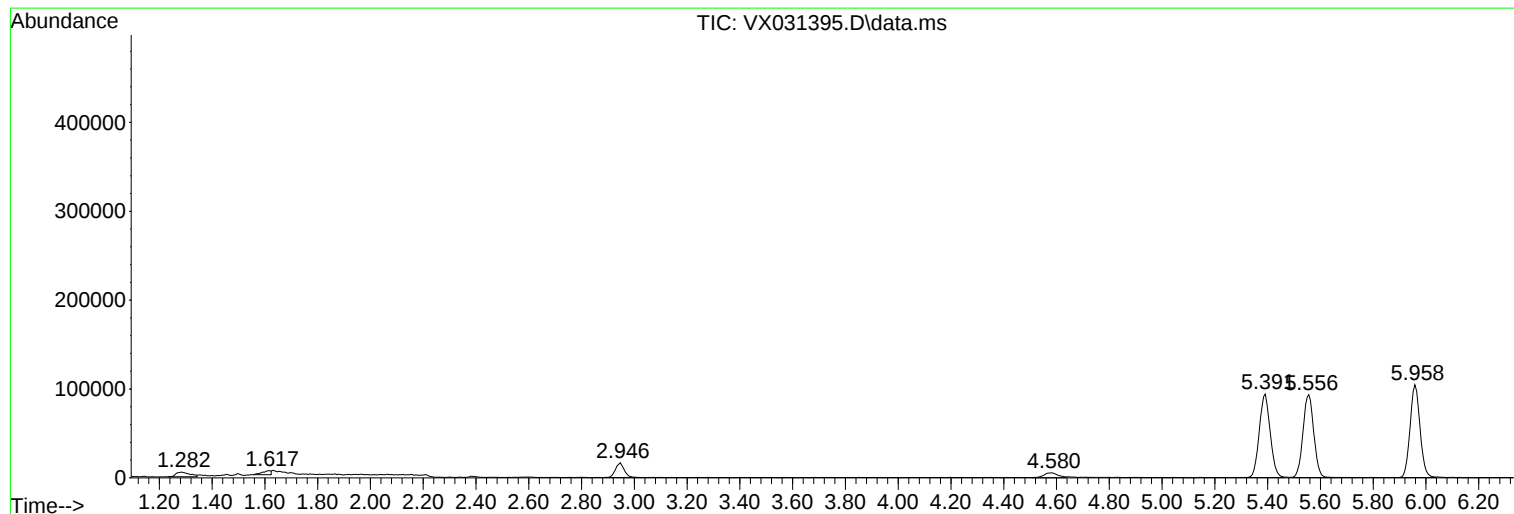

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031395.D
Acq On : 16 Sep 2022 08:32
Operator : JC/MD
Sample : N4537-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Methanol, TMS derivative Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.946	7.31 ug/l	38747	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methanol, TMS derivative	104	C4H12OSi	001825-61-2	91
2			Methanol, TBDMS derivative	146	C7H18OSi	1000364-10-7	83
3			Silane, (2-methoxyethyl)trimethyl-	132	C6H16OSi	018173-63-2	78
4			Ethyl(dimethyl)methoxysilane	118	C5H14OSi	052686-75-6	64
5			Methanethioamide, N,N-dimethyl-	89	C3H7NS	000758-16-7	9

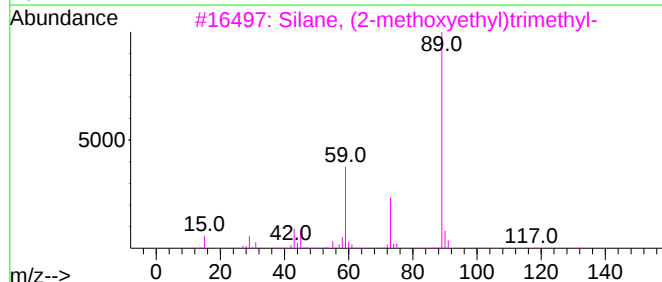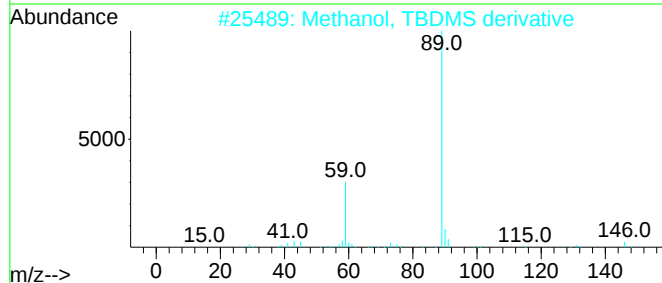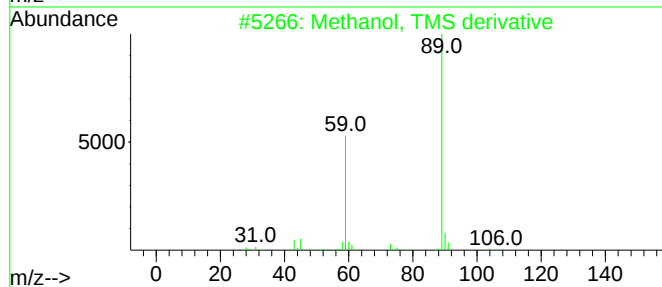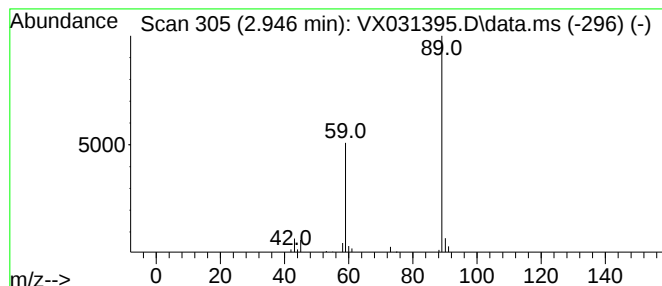

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031395.D
Acq On : 16 Sep 2022 08:32
Operator : JC/MD
Sample : N4537-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methanol, TMS d...	2.946	7.3	ug/l	38747	1	5.556	264877	50.0