

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
 Data File : VX031396.D
 Acq On : 16 Sep 2022 08:55
 Operator : JC/MD
 Sample : N4537-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M

Title : SW846 8260

Signal : TIC: VX031396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	26	32	36	rBV4	4971	11666	1.49%	0.340%
2	1.618	76	87	88	rBV7	5711	12820	1.64%	0.374%
3	2.148	169	174	178	rVB4	4898	8292	1.06%	0.242%
4	2.941	297	304	313	rBV2	8165	18924	2.42%	0.552%
5	5.093	647	657	668	rBV	14861	42880	5.49%	1.251%
6	5.391	694	706	722	rBV2	97180	292734	37.50%	8.542%
7	5.556	722	733	750	rVB	94655	263929	33.81%	7.701%
8	5.958	788	799	814	rBV	103092	271276	34.75%	7.916%
9	6.641	902	911	920	rBV2	3652	9303	1.19%	0.271%
10	6.763	920	931	944	rVB	147538	348634	44.66%	10.173%
11	7.275	1007	1015	1025	rVB5	3282	8177	1.05%	0.239%
12	8.580	1223	1229	1234	rBV	9827	16071	2.06%	0.469%
13	8.647	1234	1240	1250	rBV	487910	780615	100.00%	22.778%
14	10.055	1465	1471	1484	rVB	329210	427011	54.70%	12.460%
15	11.079	1634	1639	1648	rBV	403723	510847	65.44%	14.906%
16	12.024	1788	1794	1799	rBV	317131	403881	51.74%	11.785%




Sum of corrected areas: 3427060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031396.D
Acq On : 16 Sep 2022 08:55
Operator : JC/MD
Sample : N4537-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

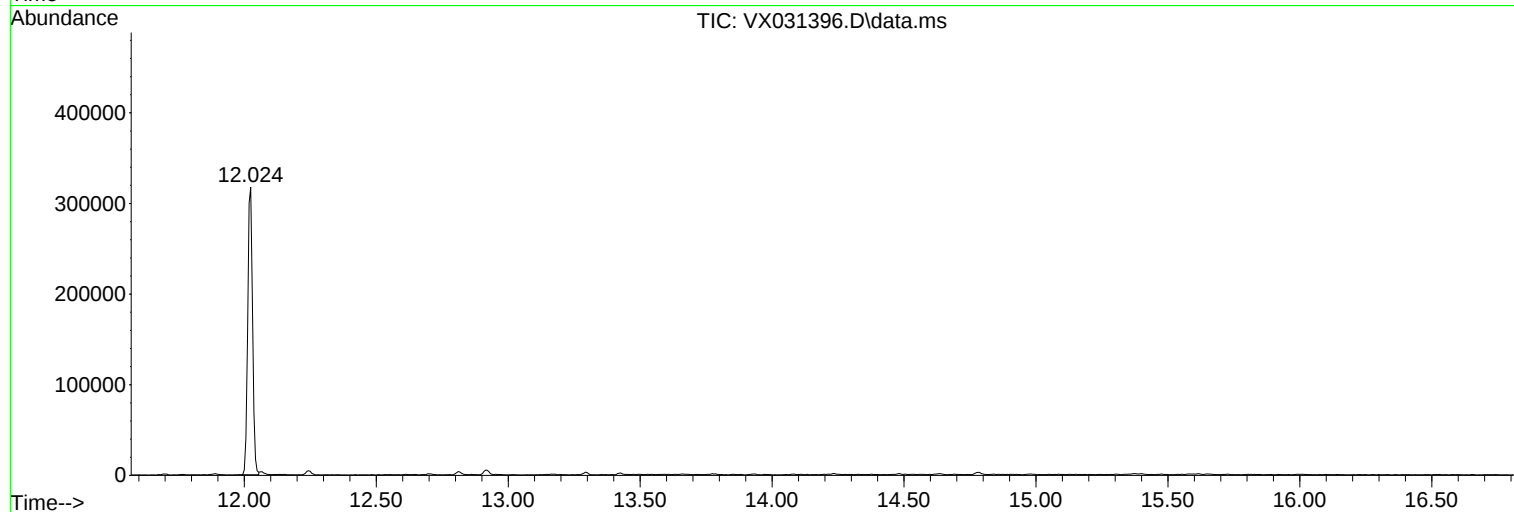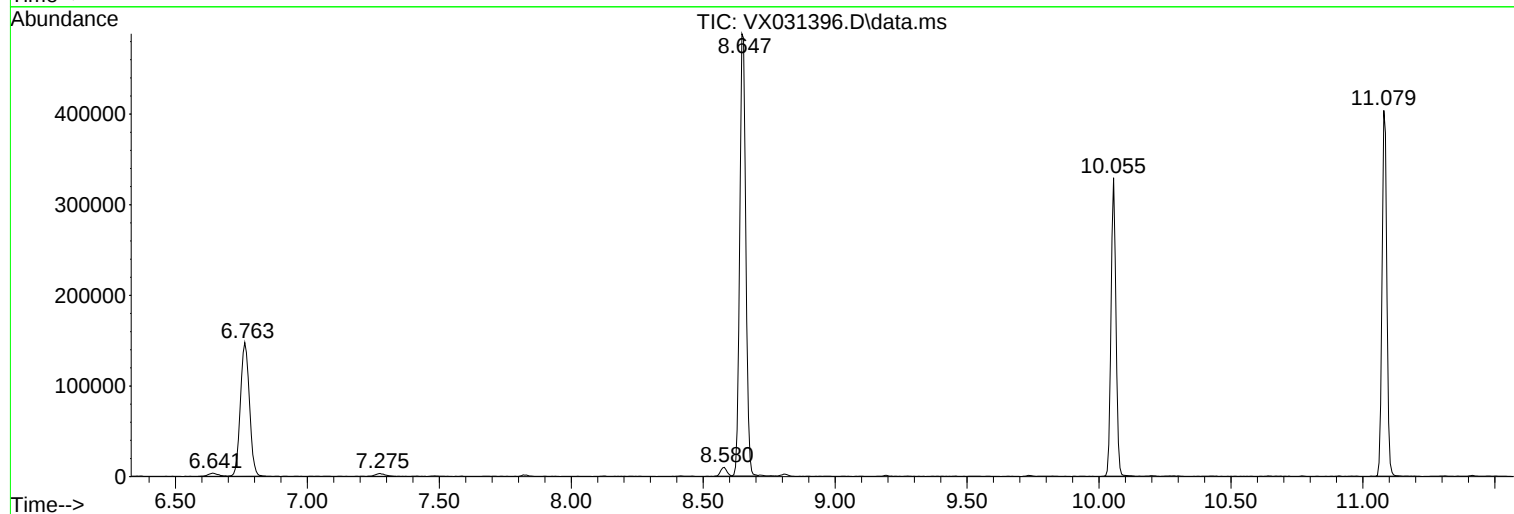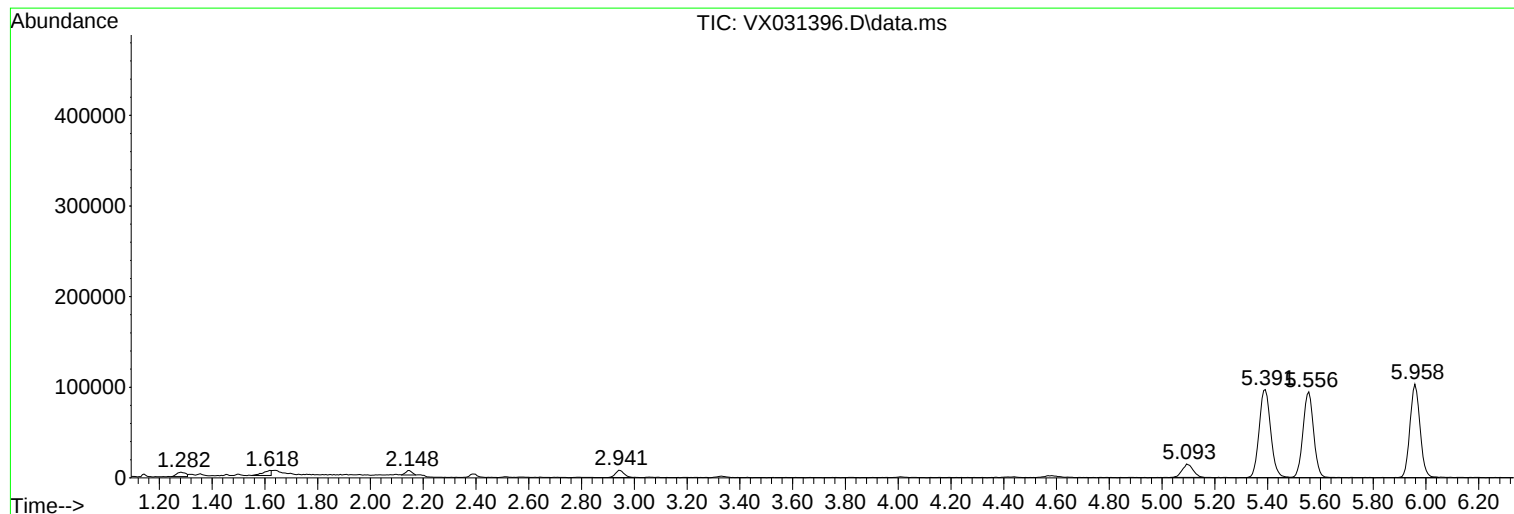

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031396.D
Acq On : 16 Sep 2022 08:55
Operator : JC/MD
Sample : N4537-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031396.D
Acq On : 16 Sep 2022 08:55
Operator : JC/MD
Sample : N4537-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc