
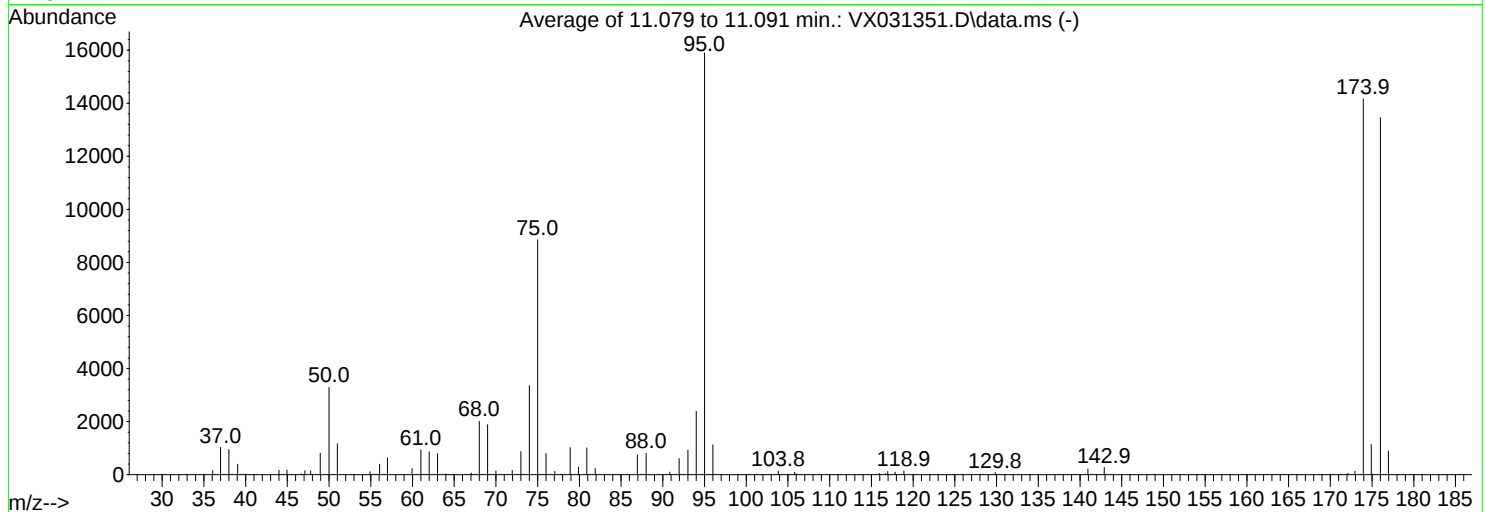


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091522\
Data File : VX031351.D
Acq On : 15 Sep 2022 12:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Title : SW846 8260
Last Update : Thu Sep 15 01:50:07 2022

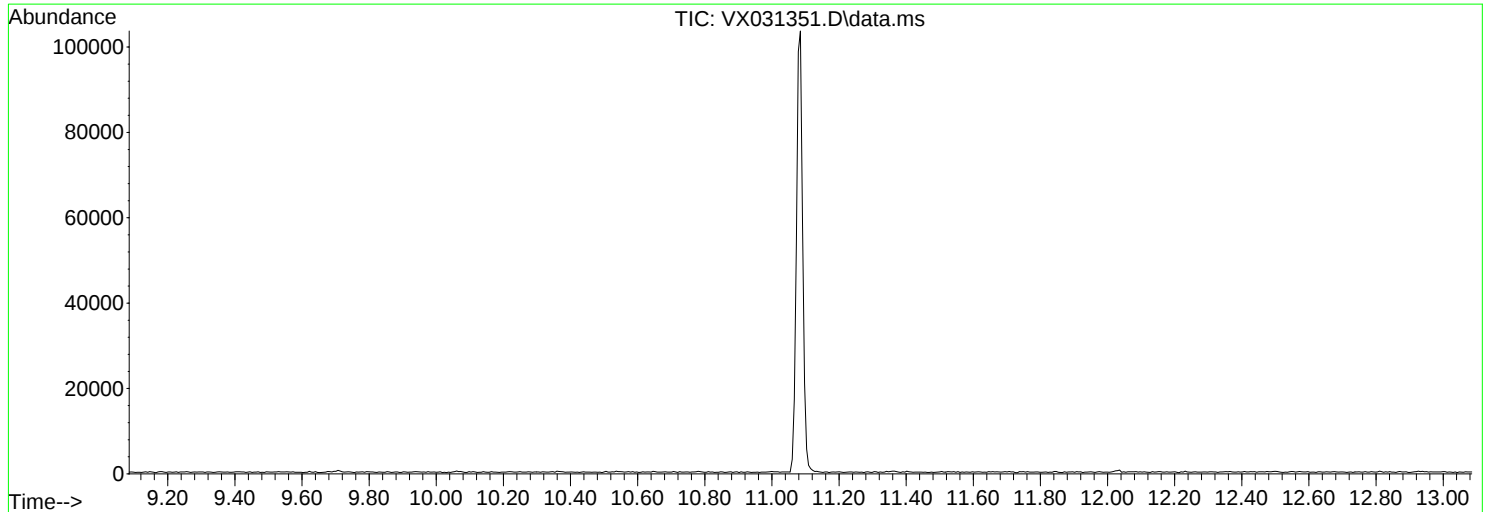

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	3290	PASS
75	95	30	60	55.7	8856	PASS
95	95	100	100	100.0	15900	PASS
96	95	5	9	7.1	1121	PASS
173	174	0.00	2	1.0	135	PASS
174	95	50	100	89.1	14162	PASS
175	174	5	9	8.0	1137	PASS
176	174	95	101	95.0	13458	PASS
177	176	5	9	6.7	895	PASS