

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
 Data File : VX037749.D
 Acq On : 15 Sep 2023 12:36
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Sep 16 05:40:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	211350	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	337912	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	298294	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	129773	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	120547	43.412	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	86.820%
35) Dibromofluoromethane	5.385	113	105090	46.480	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.960%
50) Toluene-d8	8.647	98	404369	48.134	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.260%
62) 4-Bromofluorobenzene	11.079	95	137355	44.994	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037749.D
Acq On : 15 Sep 2023 12:36
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Sep 16 05:40:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




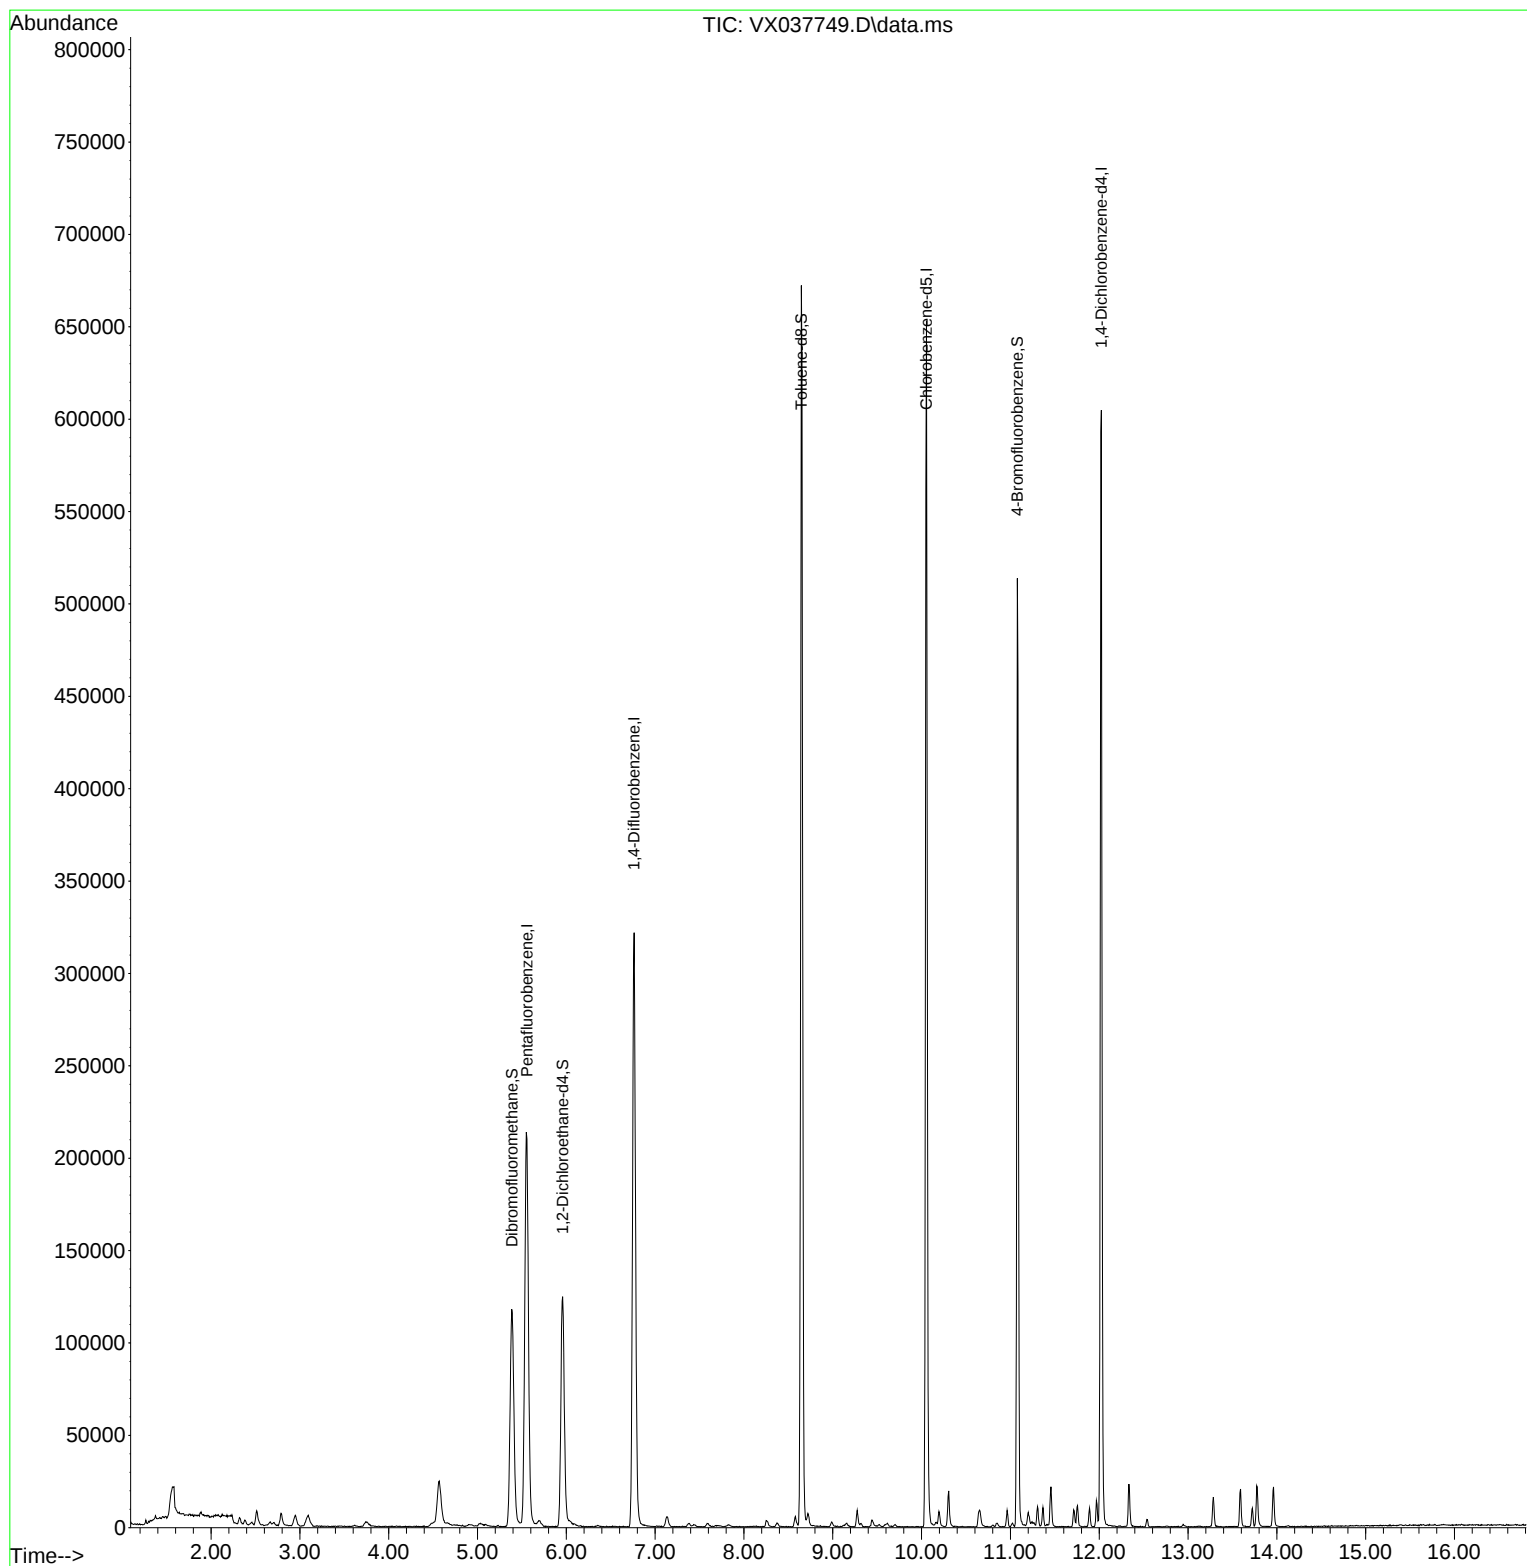


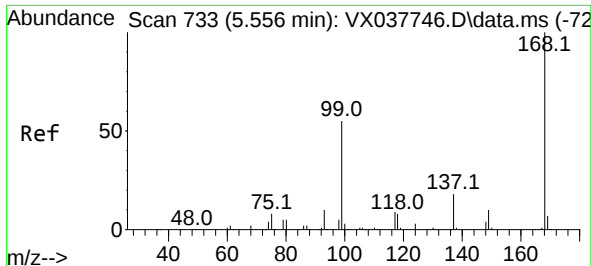

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 211350
Ion Ratio Lower Upper
168 100
99 55.7 56.6 85.0#

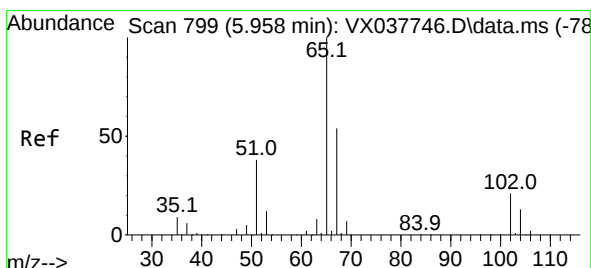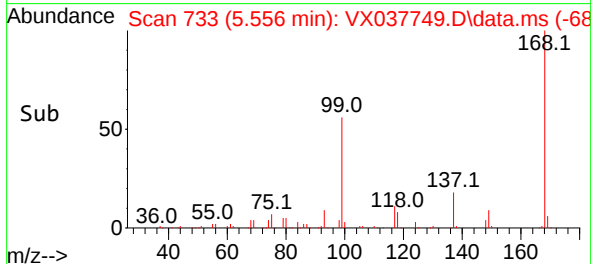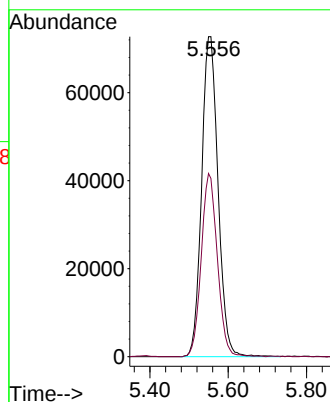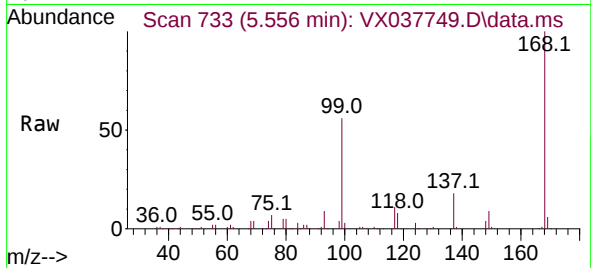

#33
1,2-Dichloroethane-d4
Concen: 43.412 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36

Tgt Ion: 65 Resp: 120547
Ion Ratio Lower Upper
65 100
67 53.5 0.0 100.2


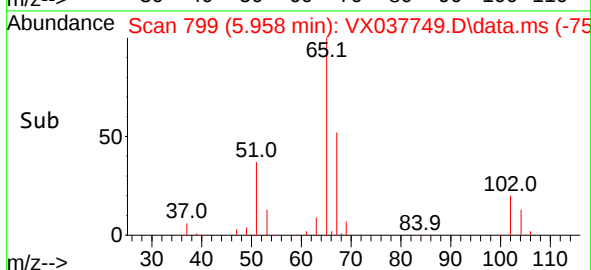
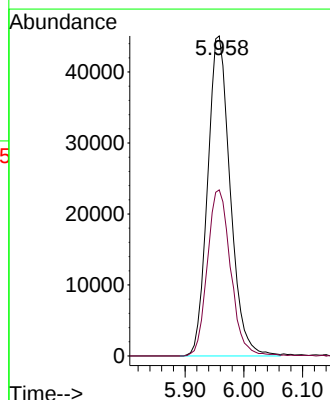
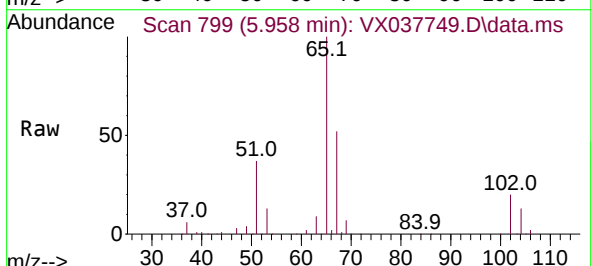


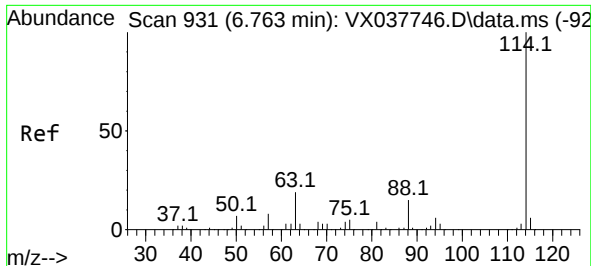

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 337912
Ion Ratio Lower Upper
114 100
63 19.6 0.0 45.0
88 15.5 0.0 36.6

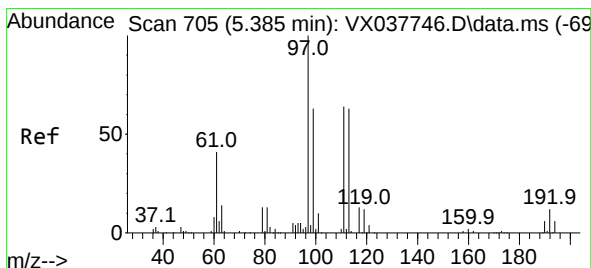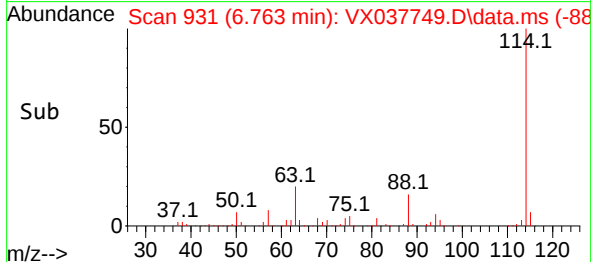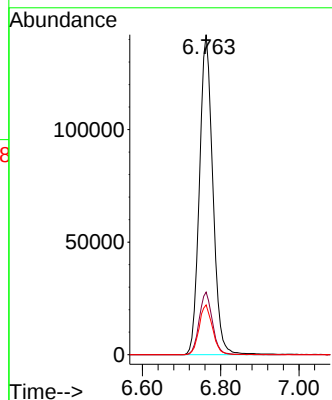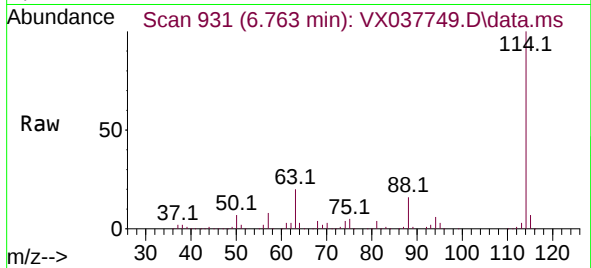

#35
Dibromofluoromethane
Concen: 46.480 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36

Tgt Ion:113 Resp: 105090
Ion Ratio Lower Upper
113 100
111 103.1 82.9 124.3
192 19.7 13.3 19.9


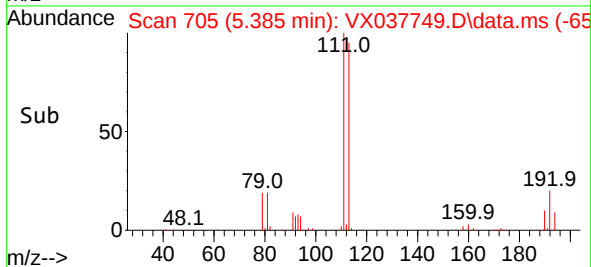
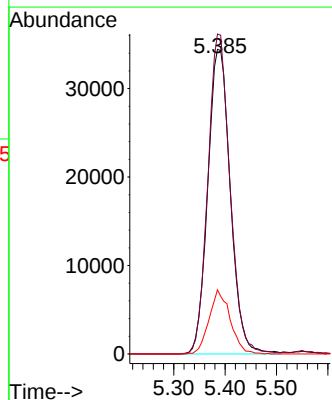
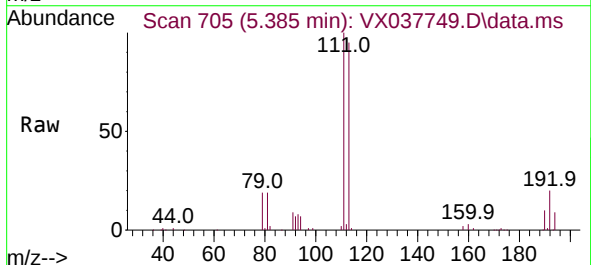


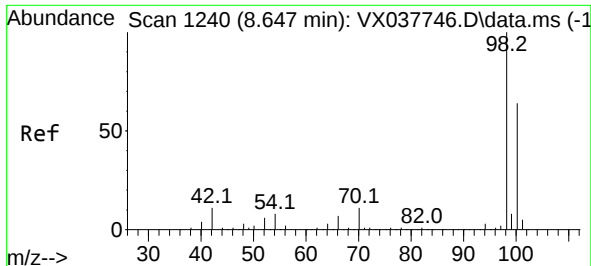

#50
Toluene-d8
Concen: 48.134 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 404369
Ion Ratio Lower Upper
98 100
100 63.8 53.1 79.7

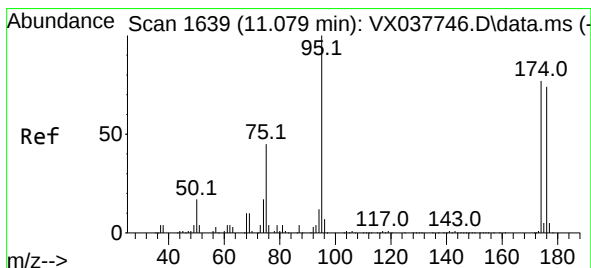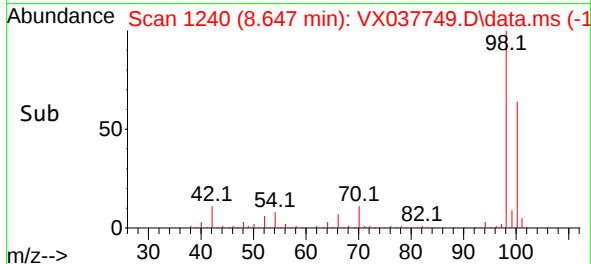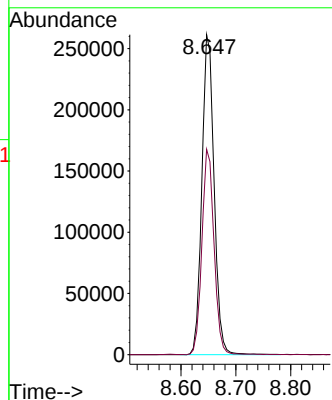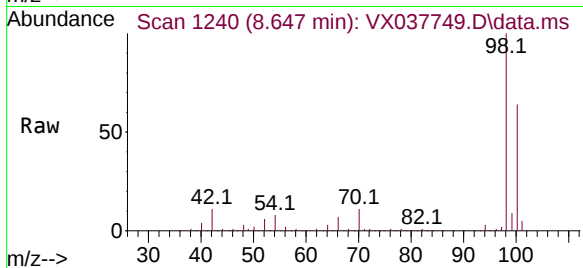

#62
4-Bromofluorobenzene
Concen: 44.994 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037749.D
Acq: 15 Sep 2023 12:36

Tgt Ion: 95 Resp: 137355
Ion Ratio Lower Upper
95 100
174 80.7 0.0 135.6
176 78.3 0.0 131.0

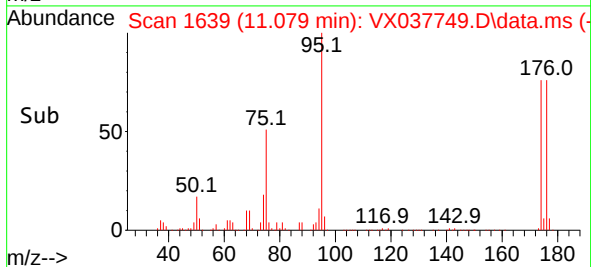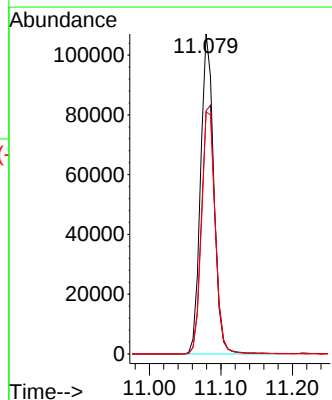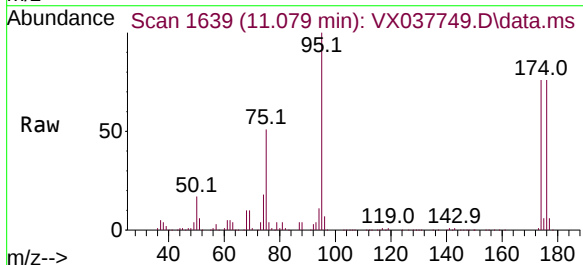

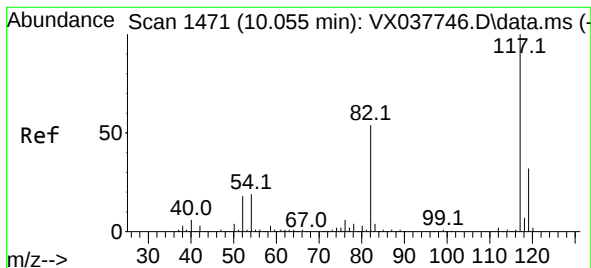

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX037749.D

Acq: 15 Sep 2023 12:36

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:117 Resp: 298294

Ion Ratio Lower Upper

117 100

82 53.9 46.2 69.4

119 32.9 25.5 38.3

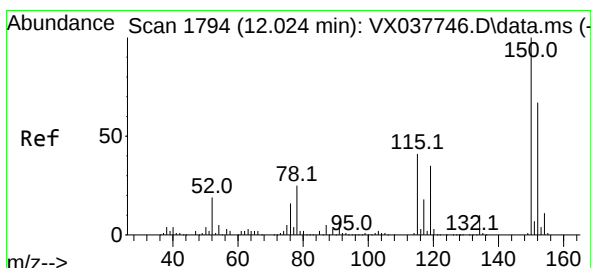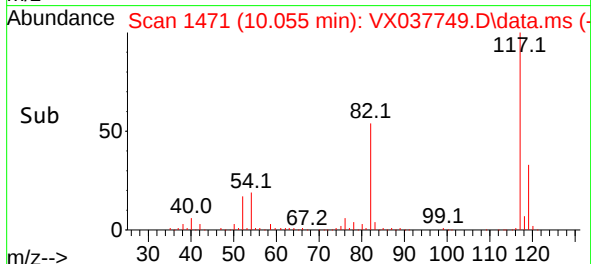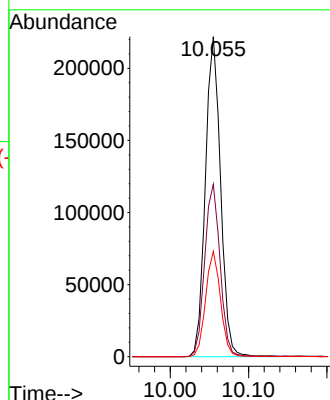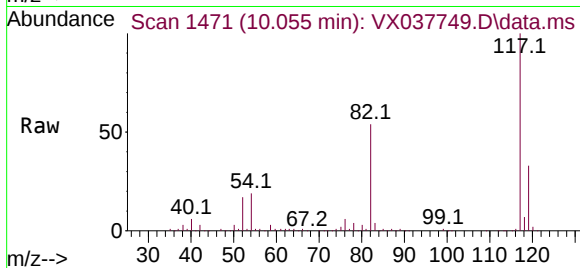

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX037749.D

Acq: 15 Sep 2023 12:36

Tgt Ion:152 Resp: 129773

Ion Ratio Lower Upper

152 100

115 59.5 43.3 129.9

150 156.7 0.0 345.0

