

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
 Data File : VX037756.D
 Acq On : 15 Sep 2023 15:40
 Operator : JC/MD
 Sample : 04390-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10A-TB-20230906

Quant Time: Sep 16 05:45:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	222123	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	365240	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	320666	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	133317	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	132962	45.561	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.120%
35) Dibromofluoromethane	5.385	113	111184	45.496	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.000%
50) Toluene-d8	8.647	98	431643	47.536	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.080%
62) 4-Bromofluorobenzene	11.079	95	142122	43.072	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.140%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037756.D
Acq On : 15 Sep 2023 15:40
Operator : JC/MD
Sample : 04390-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-TB-20230906

Quant Time: Sep 16 05:45:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




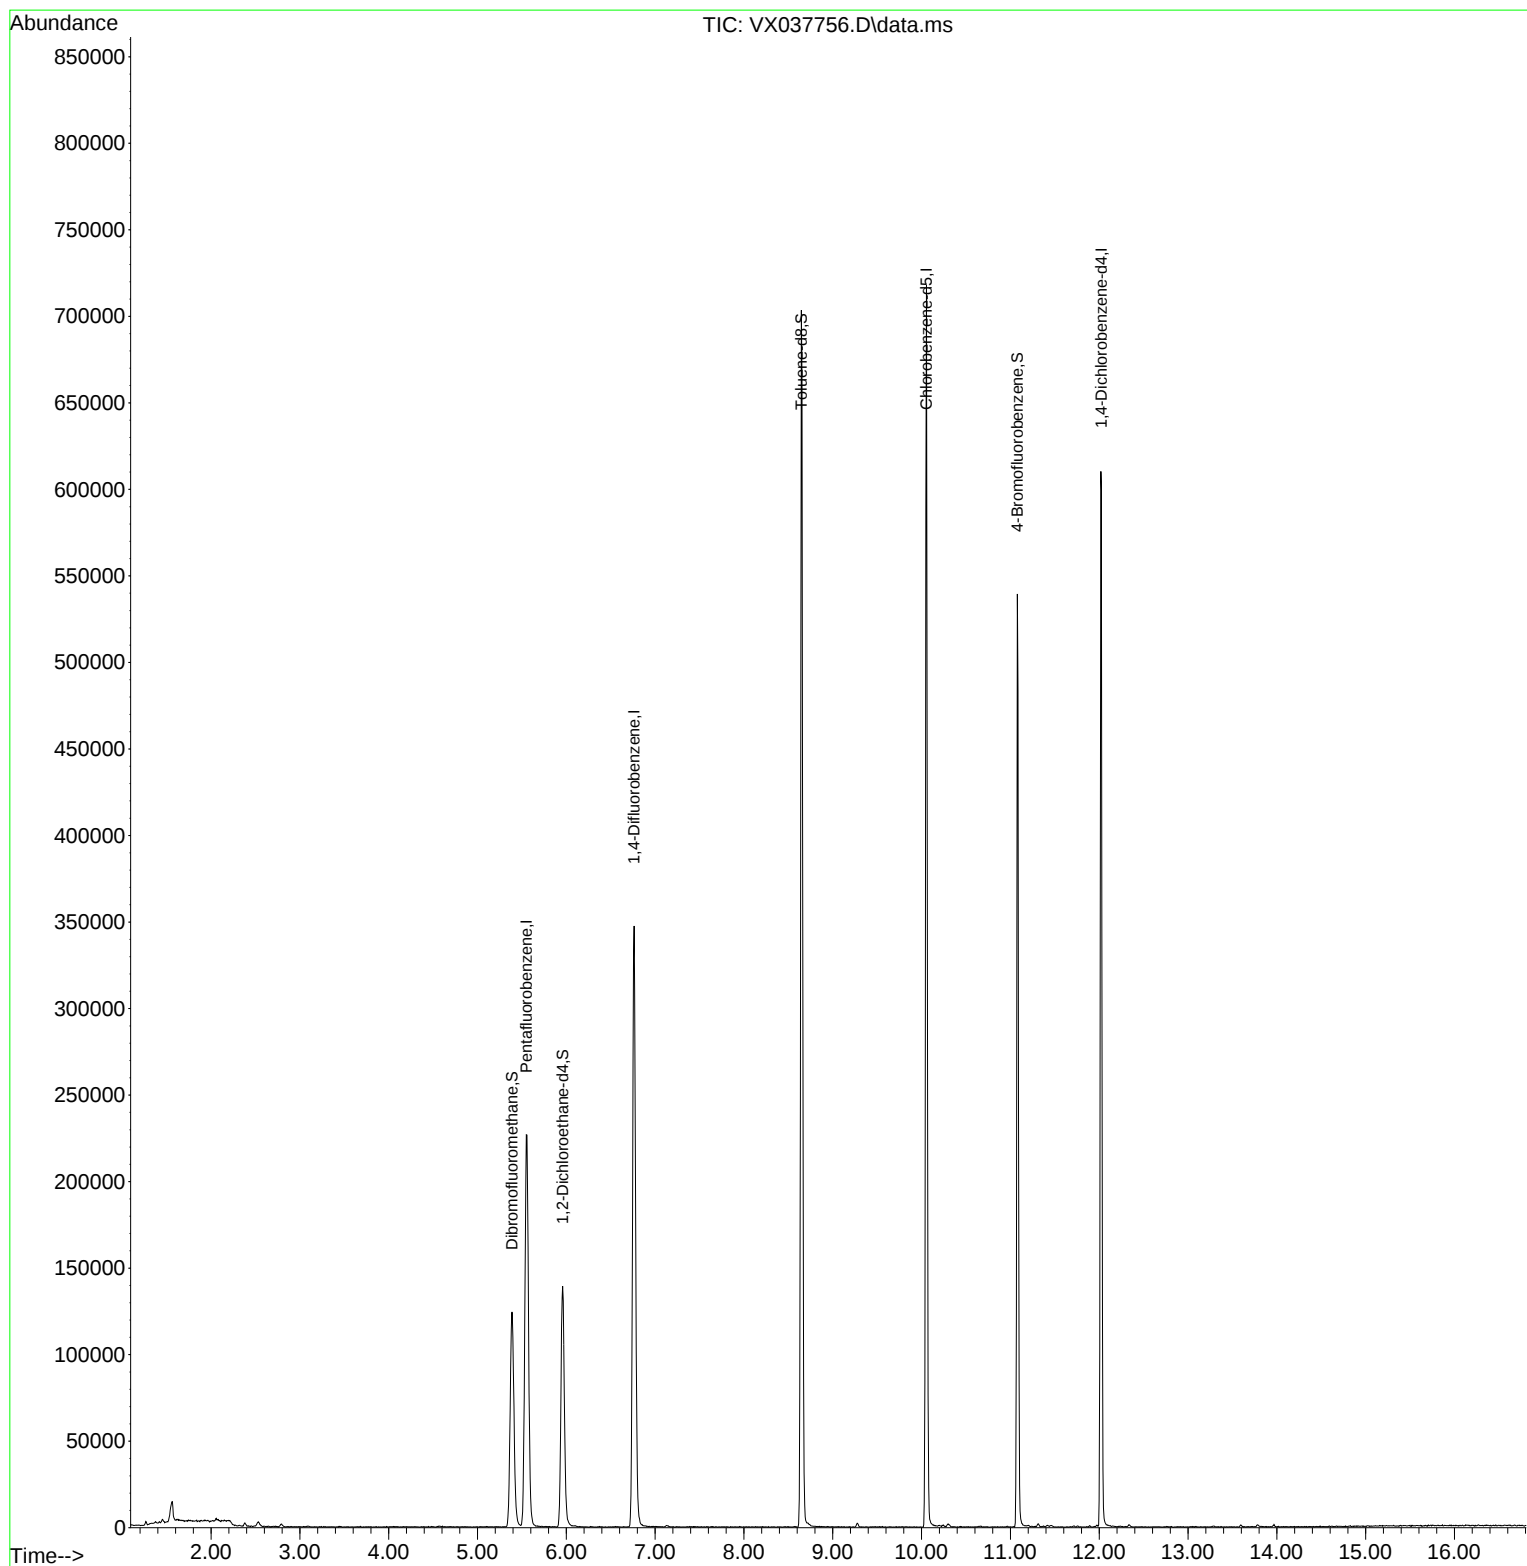




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-TB-20230906

Tgt Ion:168 Resp: 222123
Ion Ratio Lower Upper
168 100
99 55.5 56.6 85.0#

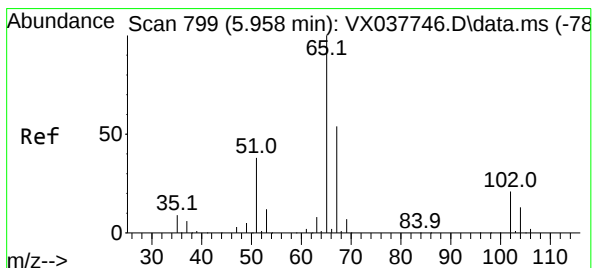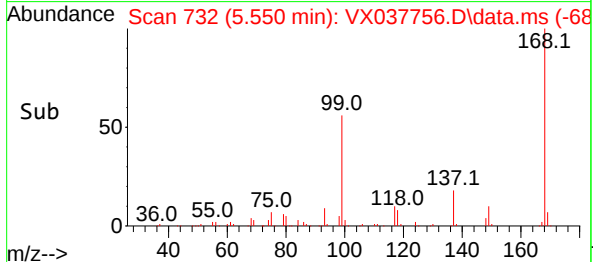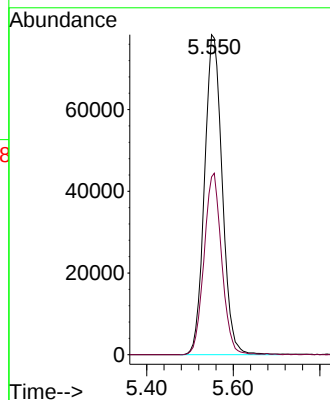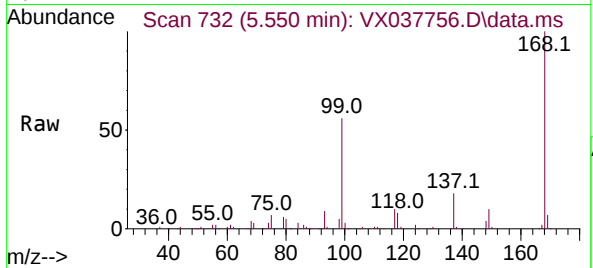

#33
1,2-Dichloroethane-d4
Concen: 45.561 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40

Tgt Ion: 65 Resp: 132962
Ion Ratio Lower Upper
65 100
67 53.4 0.0 100.2


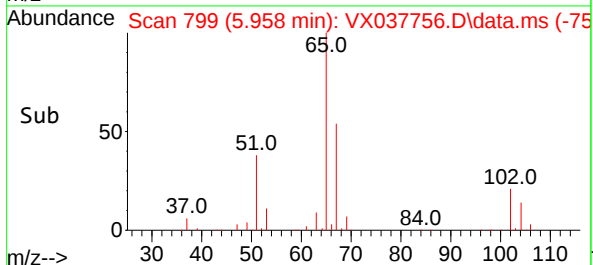
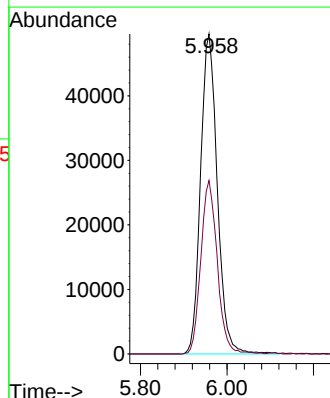
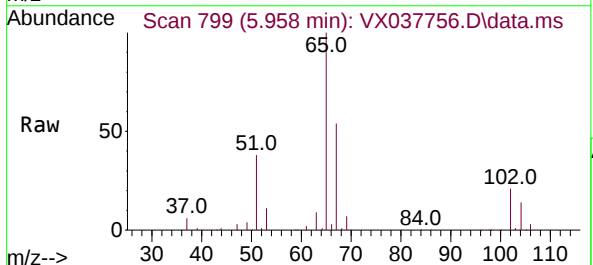




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-TB-20230906


Tgt Ion:114 Resp: 365240
Ion Ratio Lower Upper
114 100
63 18.9 0.0 45.0
88 14.6 0.0 36.6

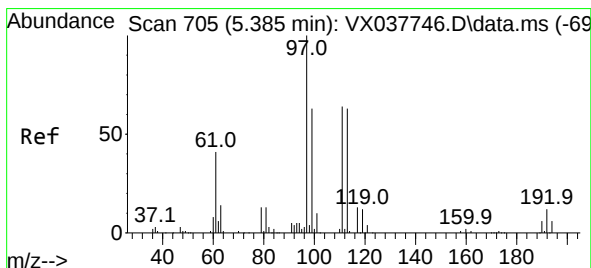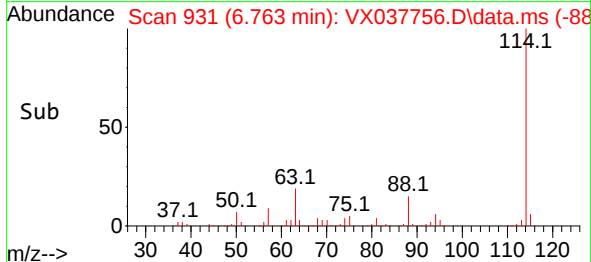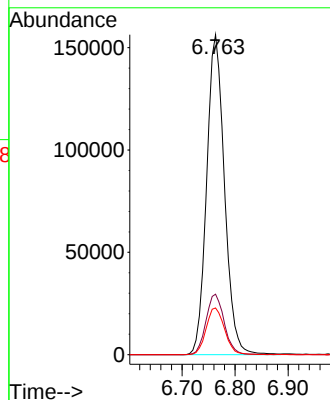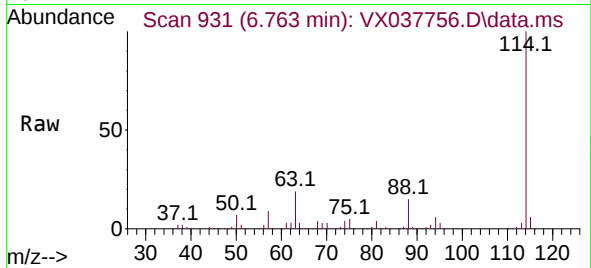

#35
Dibromofluoromethane
Concen: 45.496 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40

Tgt Ion:113 Resp: 111184
Ion Ratio Lower Upper
113 100
111 102.8 82.9 124.3
192 18.7 13.3 19.9

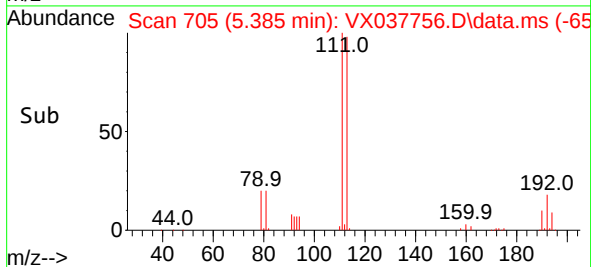
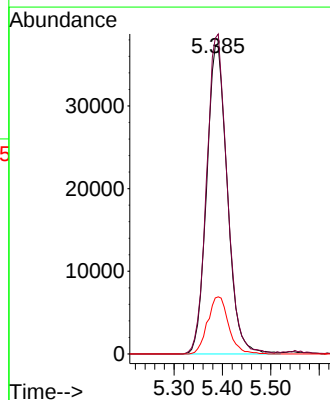
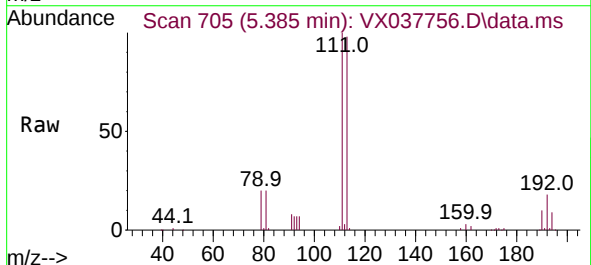


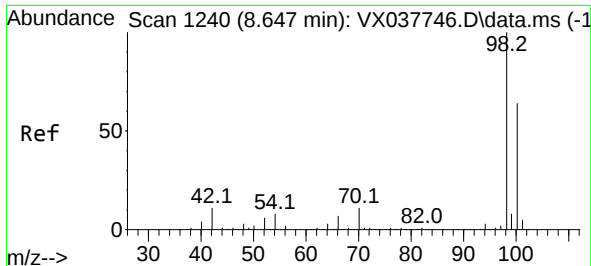

#50
Toluene-d8
Concen: 47.536 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-TB-20230906


Tgt Ion: 98 Resp: 431643
Ion Ratio Lower Upper
98 100
100 63.4 53.1 79.7

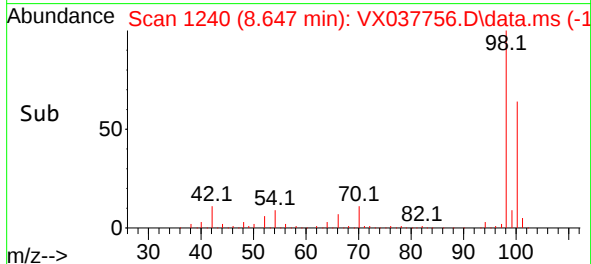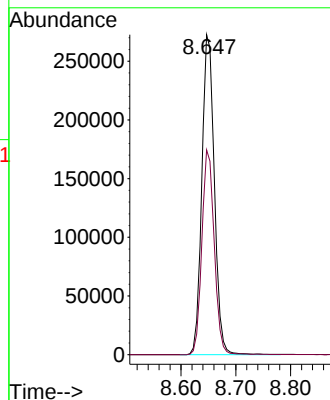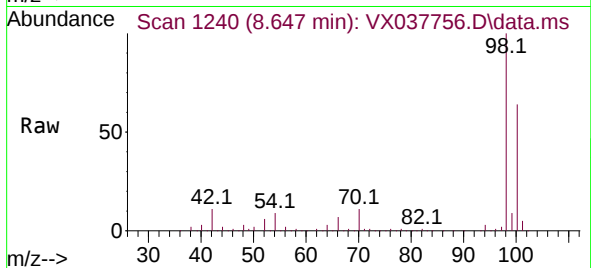

#62
4-Bromofluorobenzene
Concen: 43.072 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40

Tgt Ion: 95 Resp: 142122
Ion Ratio Lower Upper
95 100
174 81.4 0.0 135.6
176 78.9 0.0 131.0


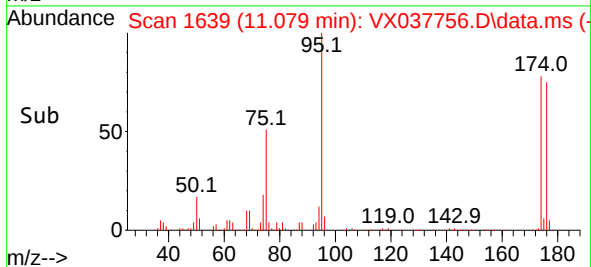
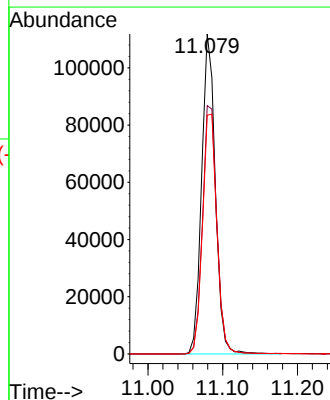
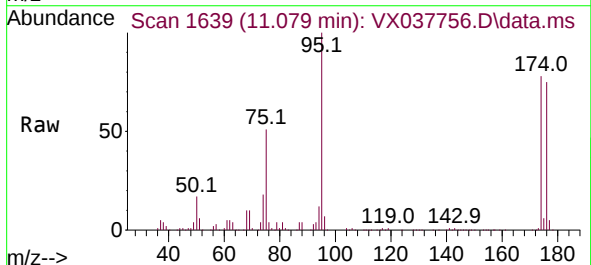


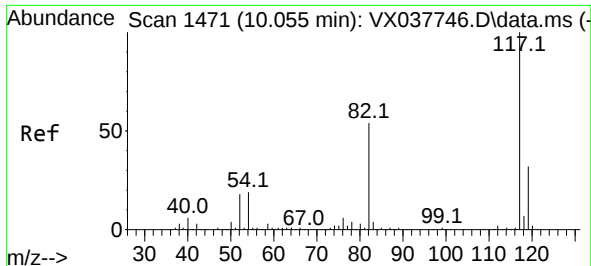

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-TB-20230906

Tgt Ion:117 Resp: 320666
Ion Ratio Lower Upper
117 100
82 54.9 46.2 69.4
119 32.2 25.5 38.3

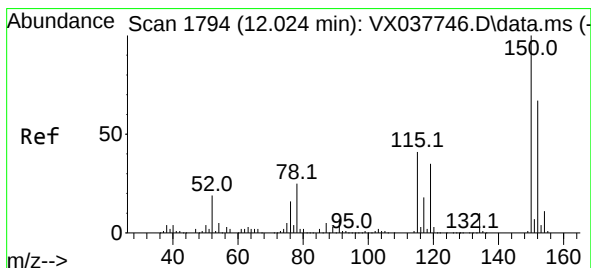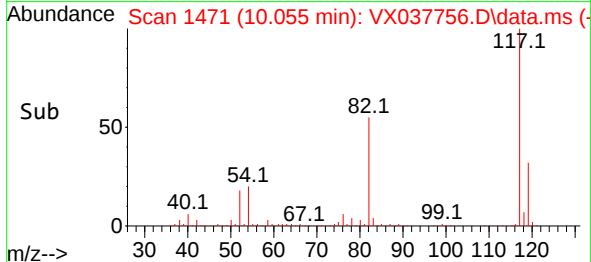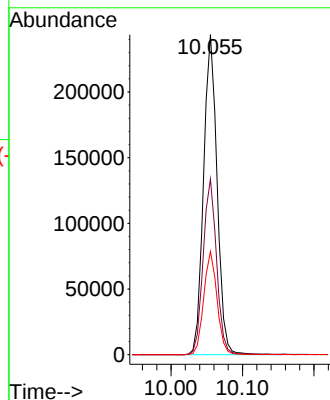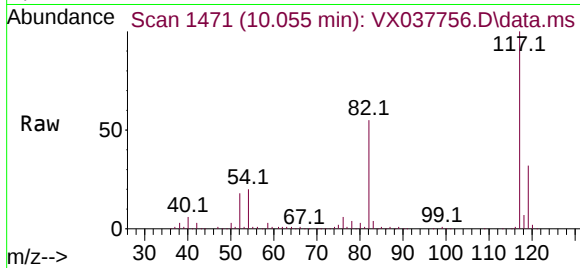

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037756.D
Acq: 15 Sep 2023 15:40

Tgt Ion:152 Resp: 133317
Ion Ratio Lower Upper
152 100
115 59.6 43.3 129.9
150 156.0 0.0 345.0

