

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
 Data File : VX037749.D
 Acq On : 15 Sep 2023 12:36
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Title : SW846 8260

Signal : TIC: VX037749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	68	79	80	rBV4	16899	42985	4.14%	0.711%
2	2.514	229	234	243	rVB3	7634	14652	1.41%	0.242%
3	2.788	274	279	287	rBV2	6638	12850	1.24%	0.212%
4	2.946	298	305	314	rVB2	5886	13996	1.35%	0.231%
5	3.093	320	329	340	rVB7	6036	18437	1.77%	0.305%
6	4.568	559	571	583	rBV	22820	70714	6.81%	1.169%
7	5.385	694	705	721	rBV	117578	354473	34.12%	5.860%
8	5.550	722	732	751	rVV	213379	619880	59.67%	10.248%
9	5.958	788	799	810	rBV	124534	338111	32.55%	5.590%
10	6.763	921	931	948	rBV	321572	762385	73.39%	12.604%
11	7.135	984	992	1000	rBV5	5454	12921	1.24%	0.214%
12	8.647	1234	1240	1249	rVV	671682	1038792	100.00%	17.173%
13	8.720	1249	1252	1260	rVB	6694	11603	1.12%	0.192%
14	9.275	1338	1343	1348	rBV2	8909	13089	1.26%	0.216%
15	10.055	1465	1471	1485	rBV	652558	893890	86.05%	14.778%
16	10.195	1491	1494	1505	rVB	8218	12571	1.21%	0.208%
17	10.305	1505	1512	1521	rVB	19478	28766	2.77%	0.476%
18	10.652	1563	1569	1580	rVB3	8947	19688	1.90%	0.325%
19	10.963	1614	1620	1625	rBV	8869	11048	1.06%	0.183%
20	11.079	1634	1639	1651	rBV	513135	665570	64.07%	11.003%
21	11.201	1654	1659	1664	rBV2	7033	11892	1.14%	0.197%
22	11.305	1673	1676	1681	rVB	10569	13666	1.32%	0.226%
23	11.366	1681	1686	1690	rBV	10021	11950	1.15%	0.198%
24	11.457	1696	1701	1711	rVB3	21784	31630	3.04%	0.523%
25	11.713	1738	1743	1747	rBV2	9150	13216	1.27%	0.218%
26	11.756	1747	1750	1761	rVB	11459	15176	1.46%	0.251%
27	11.890	1766	1772	1778	rBV	10140	13094	1.26%	0.216%
28	11.969	1781	1785	1788	rBV	14180	17750	1.71%	0.293%
29	12.024	1788	1794	1804	rVB	603191	808947	77.87%	13.373%
30	12.335	1840	1845	1851	rVB2	22911	30023	2.89%	0.496%
31	13.286	1994	2001	2006	rBV2	16082	20796	2.00%	0.344%
32	13.591	2045	2051	2057	rBV	20458	27887	2.68%	0.461%
33	13.725	2066	2073	2077	rBV2	10078	13382	1.29%	0.221%
34	13.774	2077	2081	2092	rVB	22047	32702	3.15%	0.541%
35	13.963	2107	2112	2123	rVB	21571	30434	2.93%	0.503%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037749.D
Acq On : 15 Sep 2023 12:36
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Title : SW846 8260


Sum of corrected areas: 6048966

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037749.D
Acq On : 15 Sep 2023 12:36
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

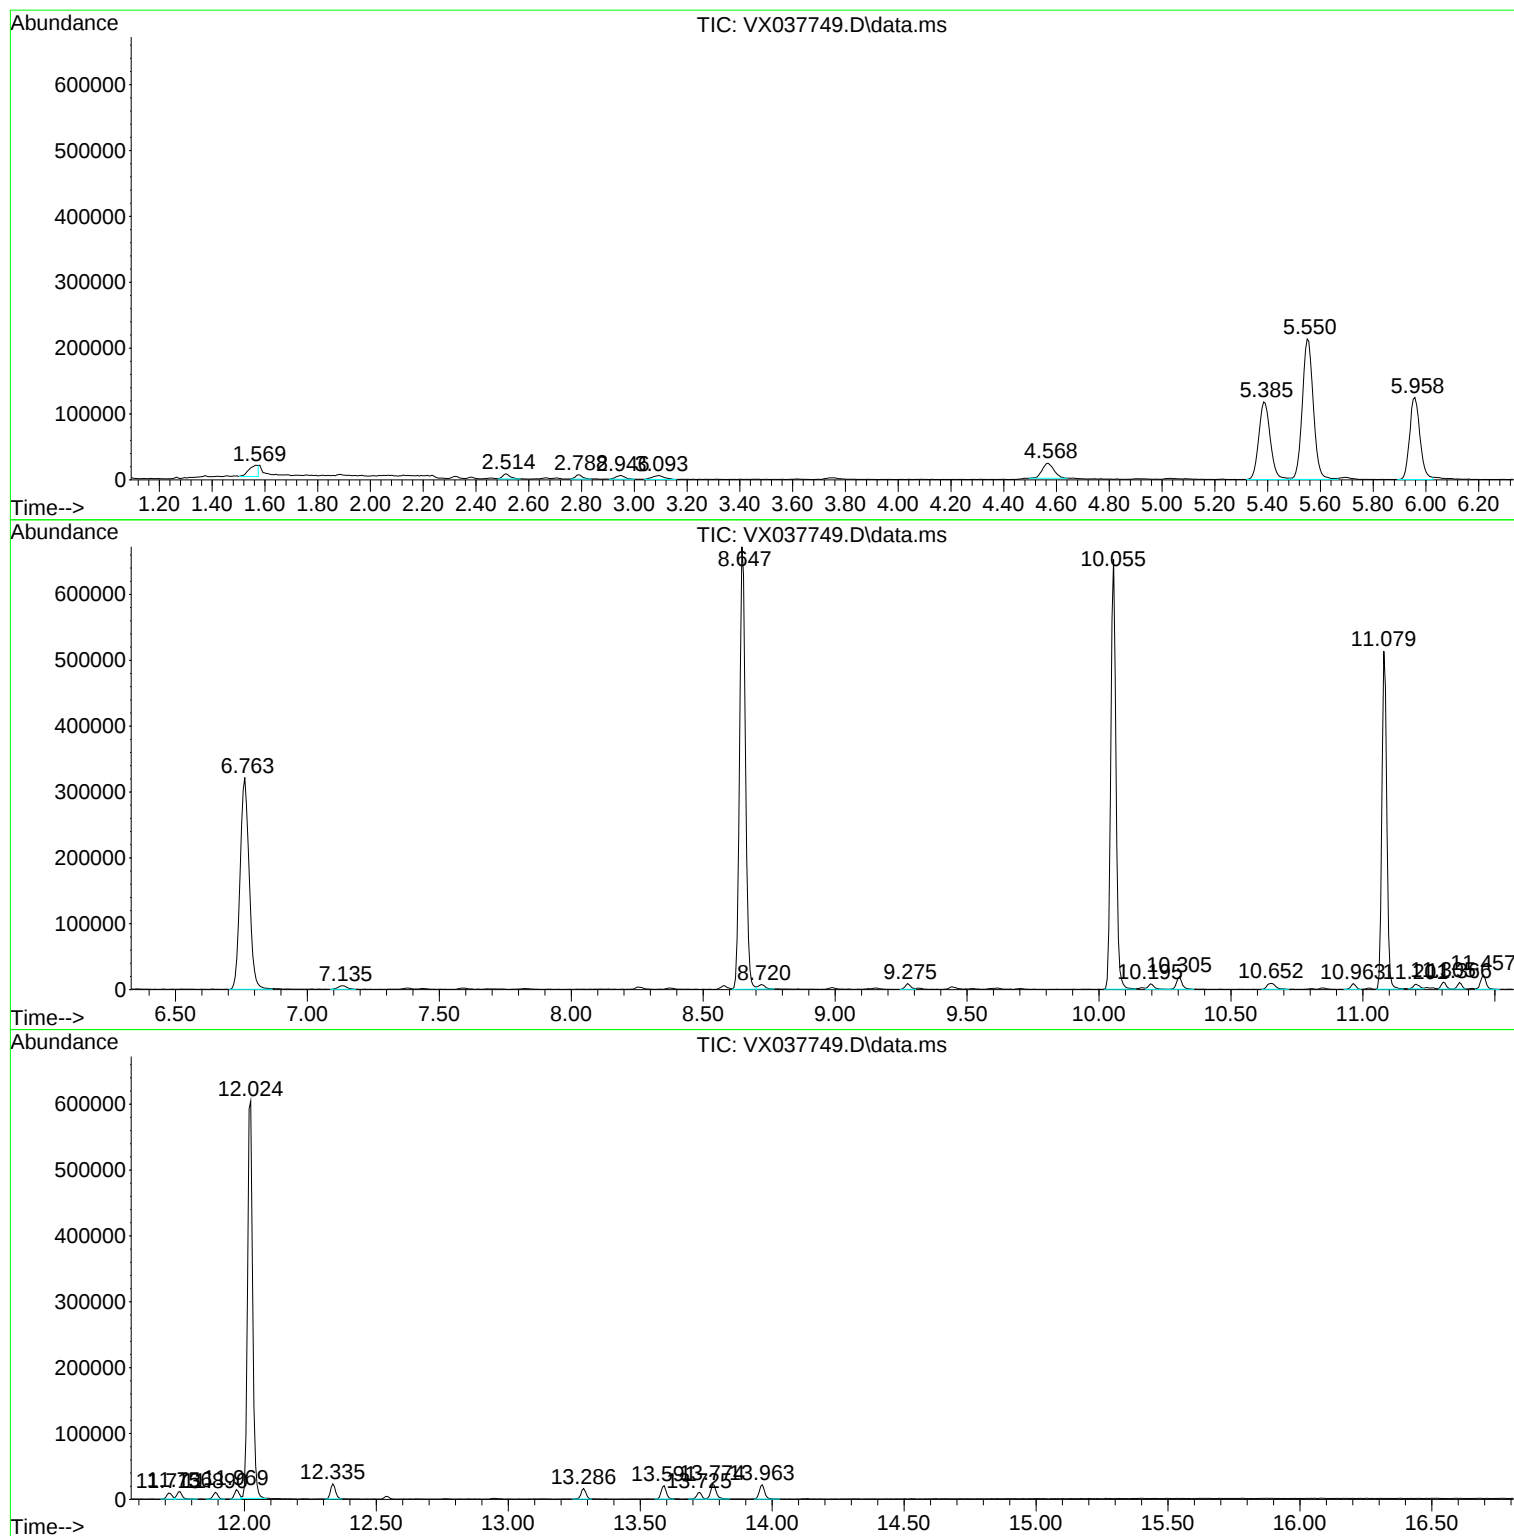

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037749.D
Acq On : 15 Sep 2023 12:36
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037749.D
Acq On : 15 Sep 2023 12:36
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc