
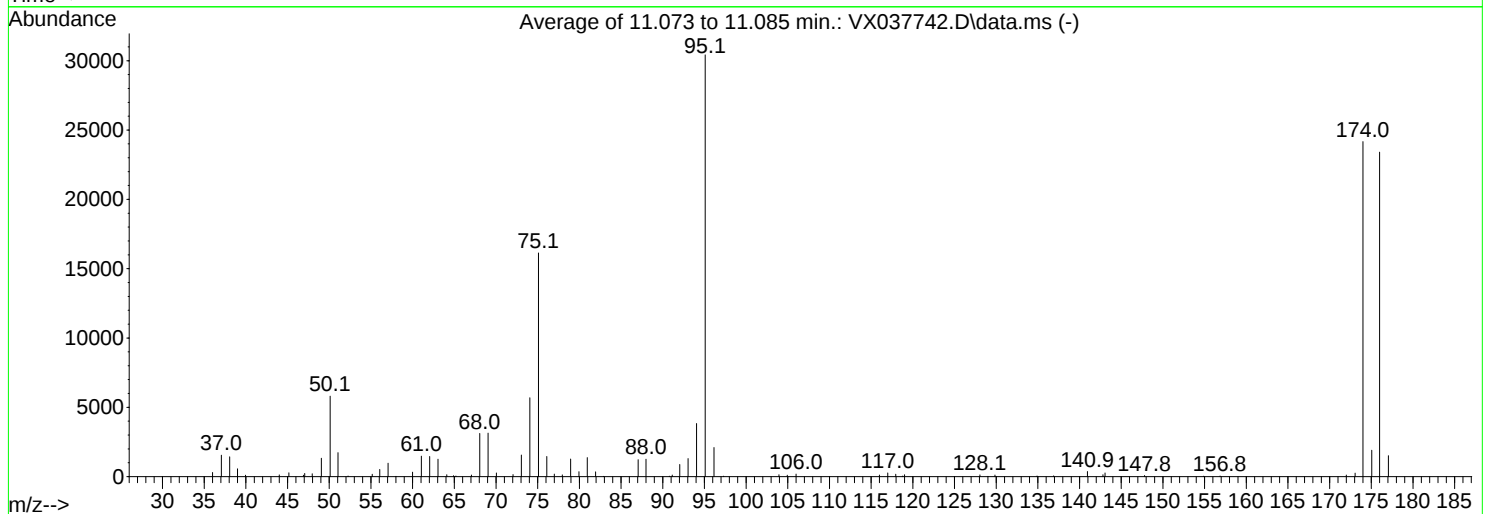


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091523\
Data File : VX037742.D
Acq On : 15 Sep 2023 08:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Title : SW846 8260
Last Update : Sat Sep 16 04:55:44 2023

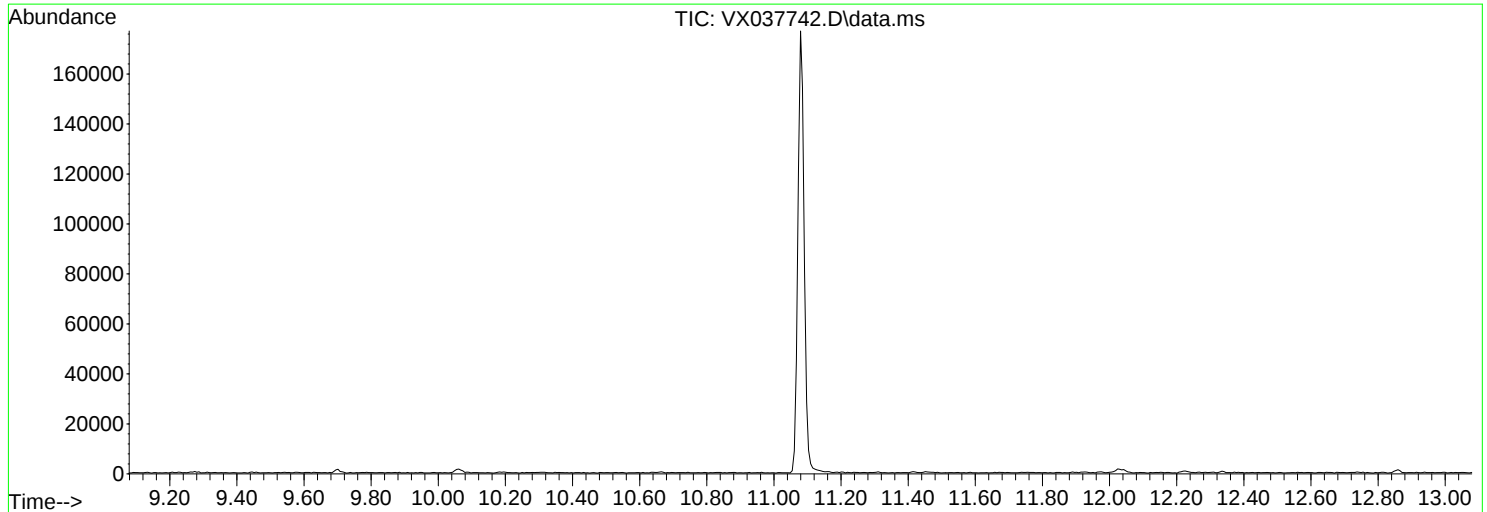

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	5800	PASS
75	95	30	60	53.0	16134	PASS
95	95	100	100	100.0	30424	PASS
96	95	5	9	6.9	2104	PASS
173	174	0.00	2	1.1	256	PASS
174	95	50	100	79.4	24163	PASS
175	174	5	9	7.9	1906	PASS
176	174	95	101	96.8	23400	PASS
177	176	5	9	6.5	1511	PASS