




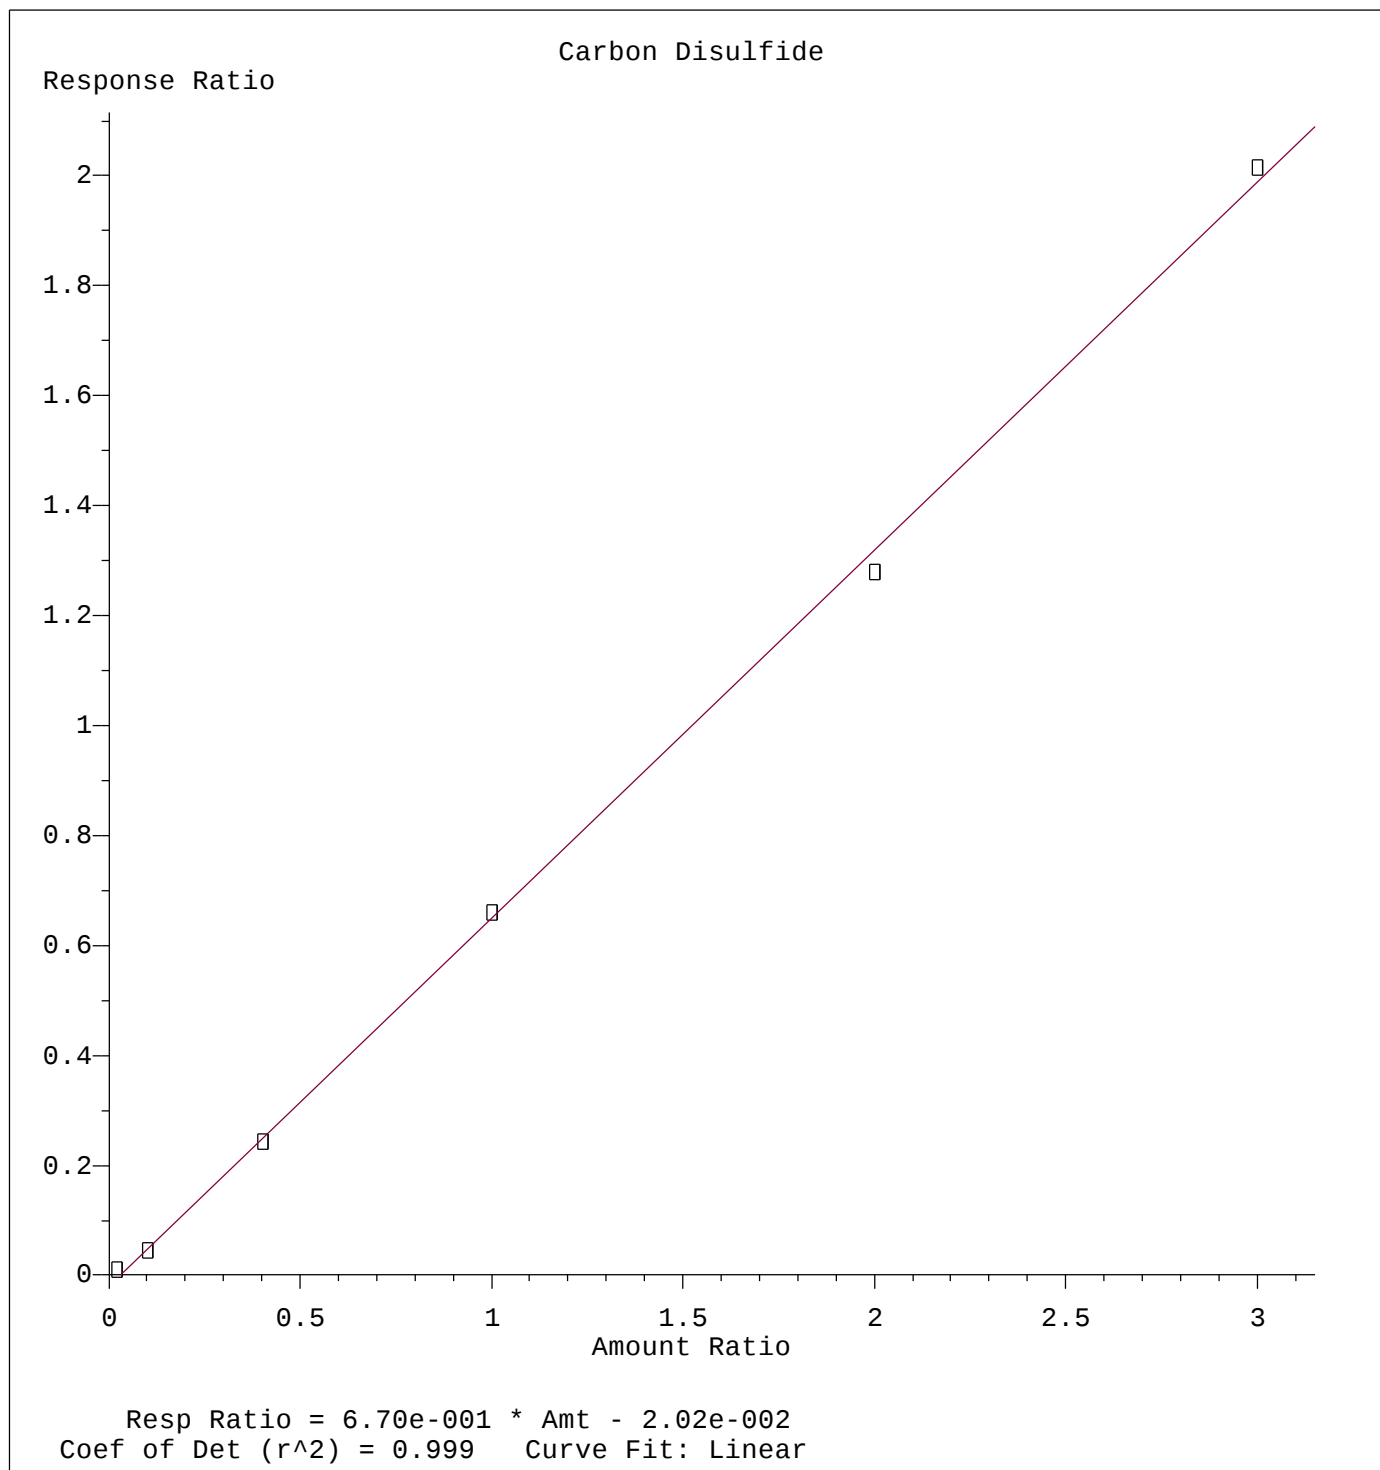


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019

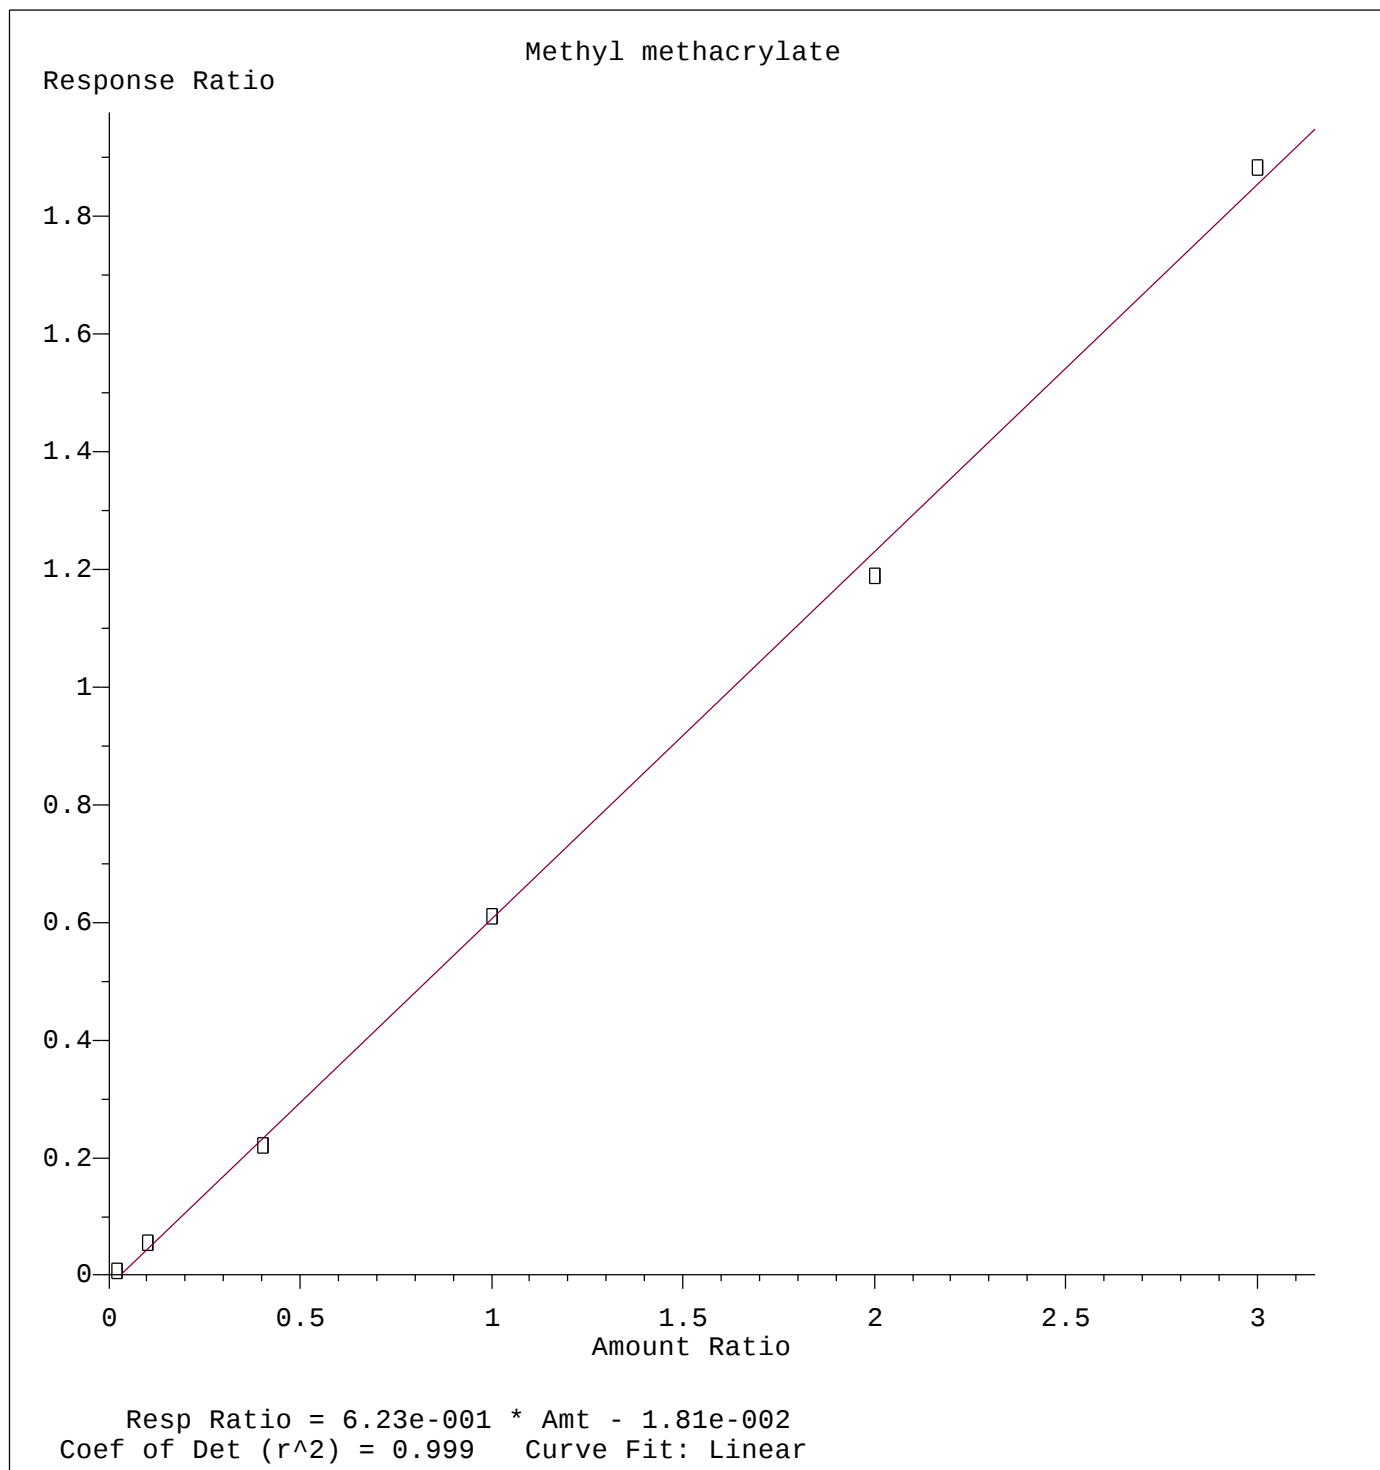


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019

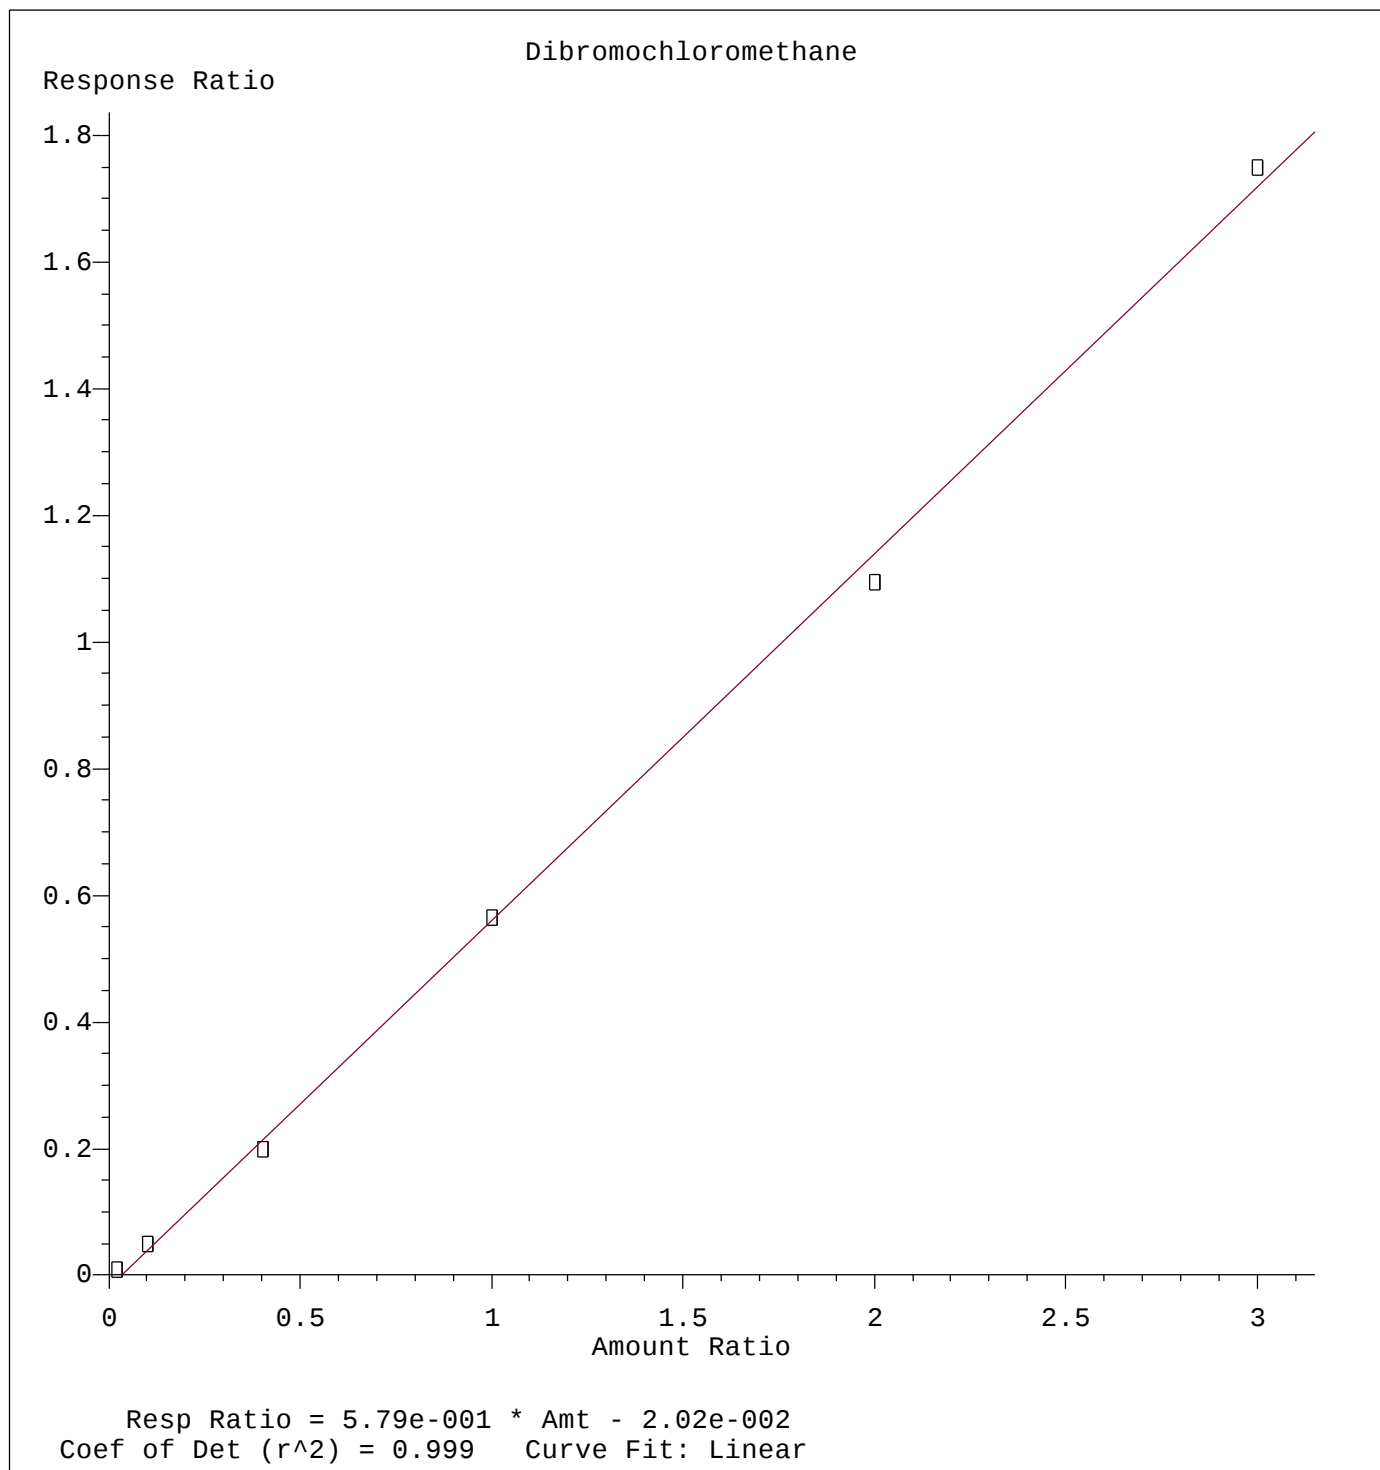

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019

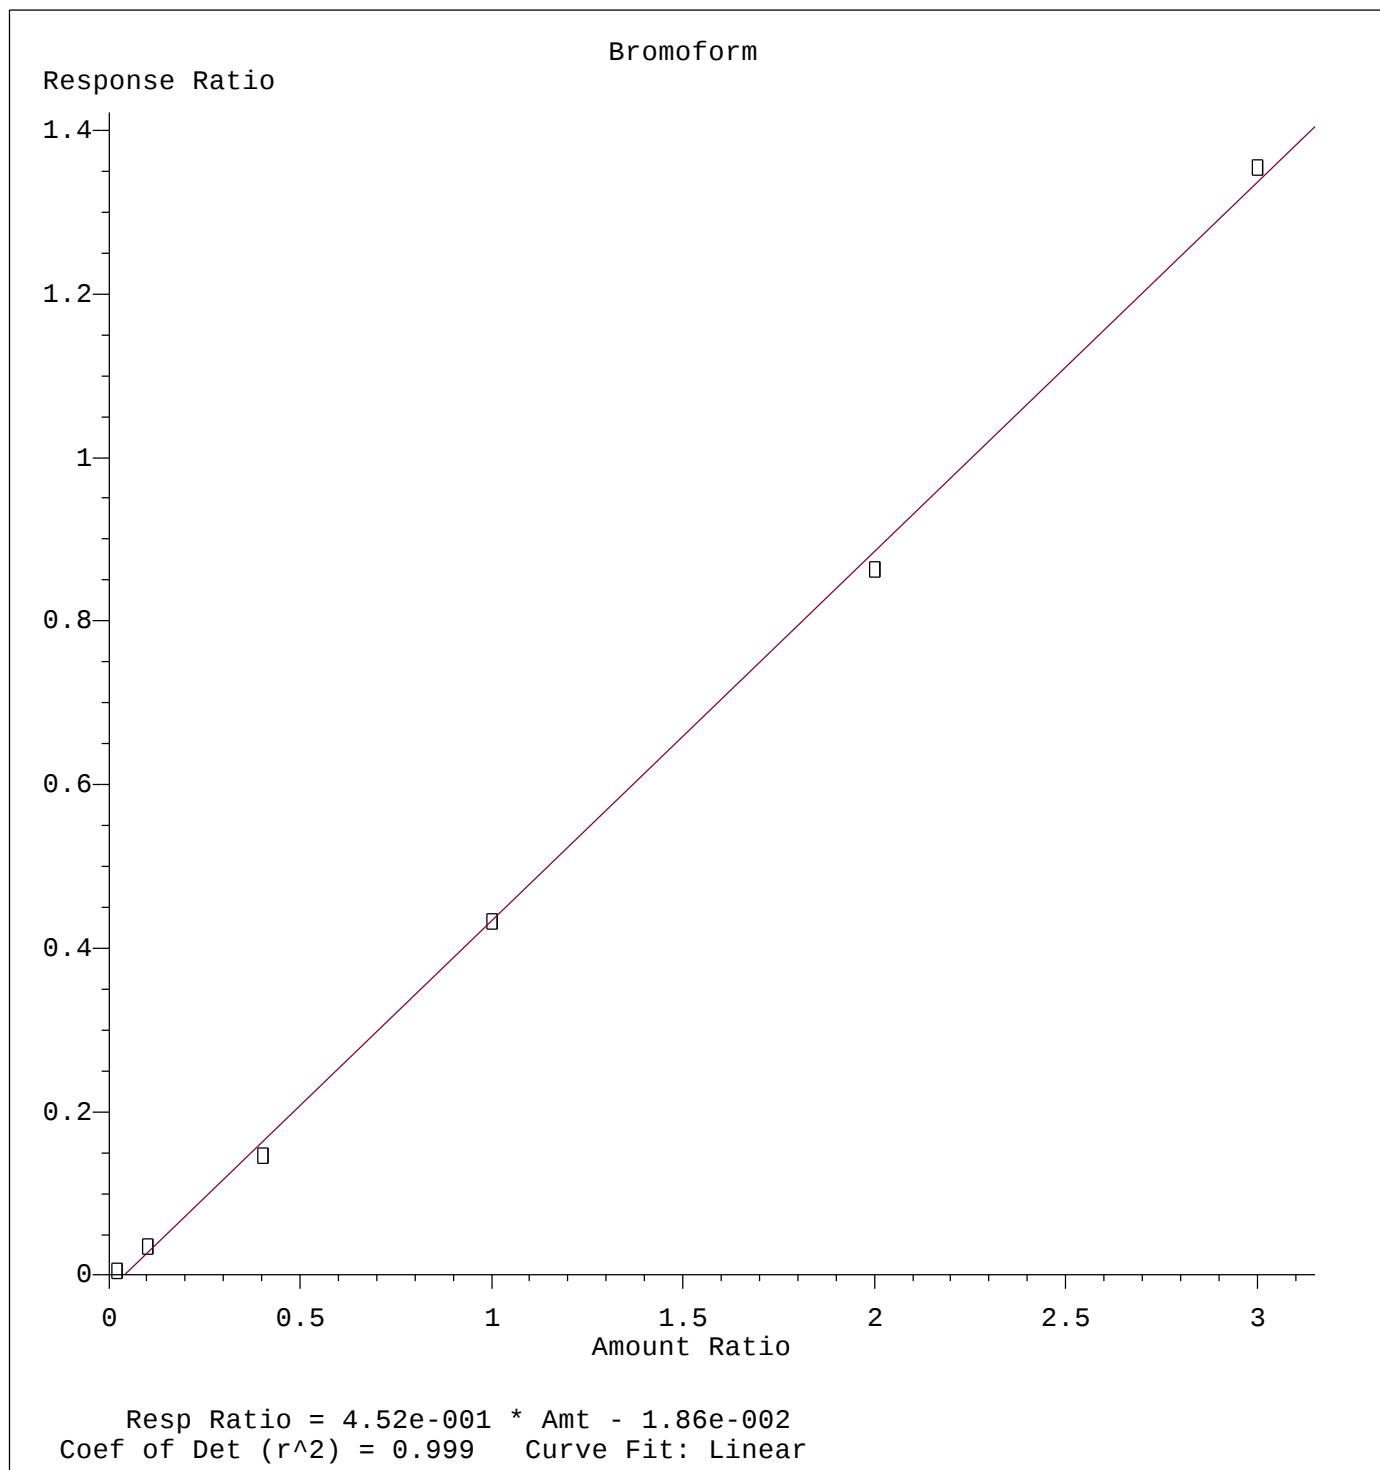


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019

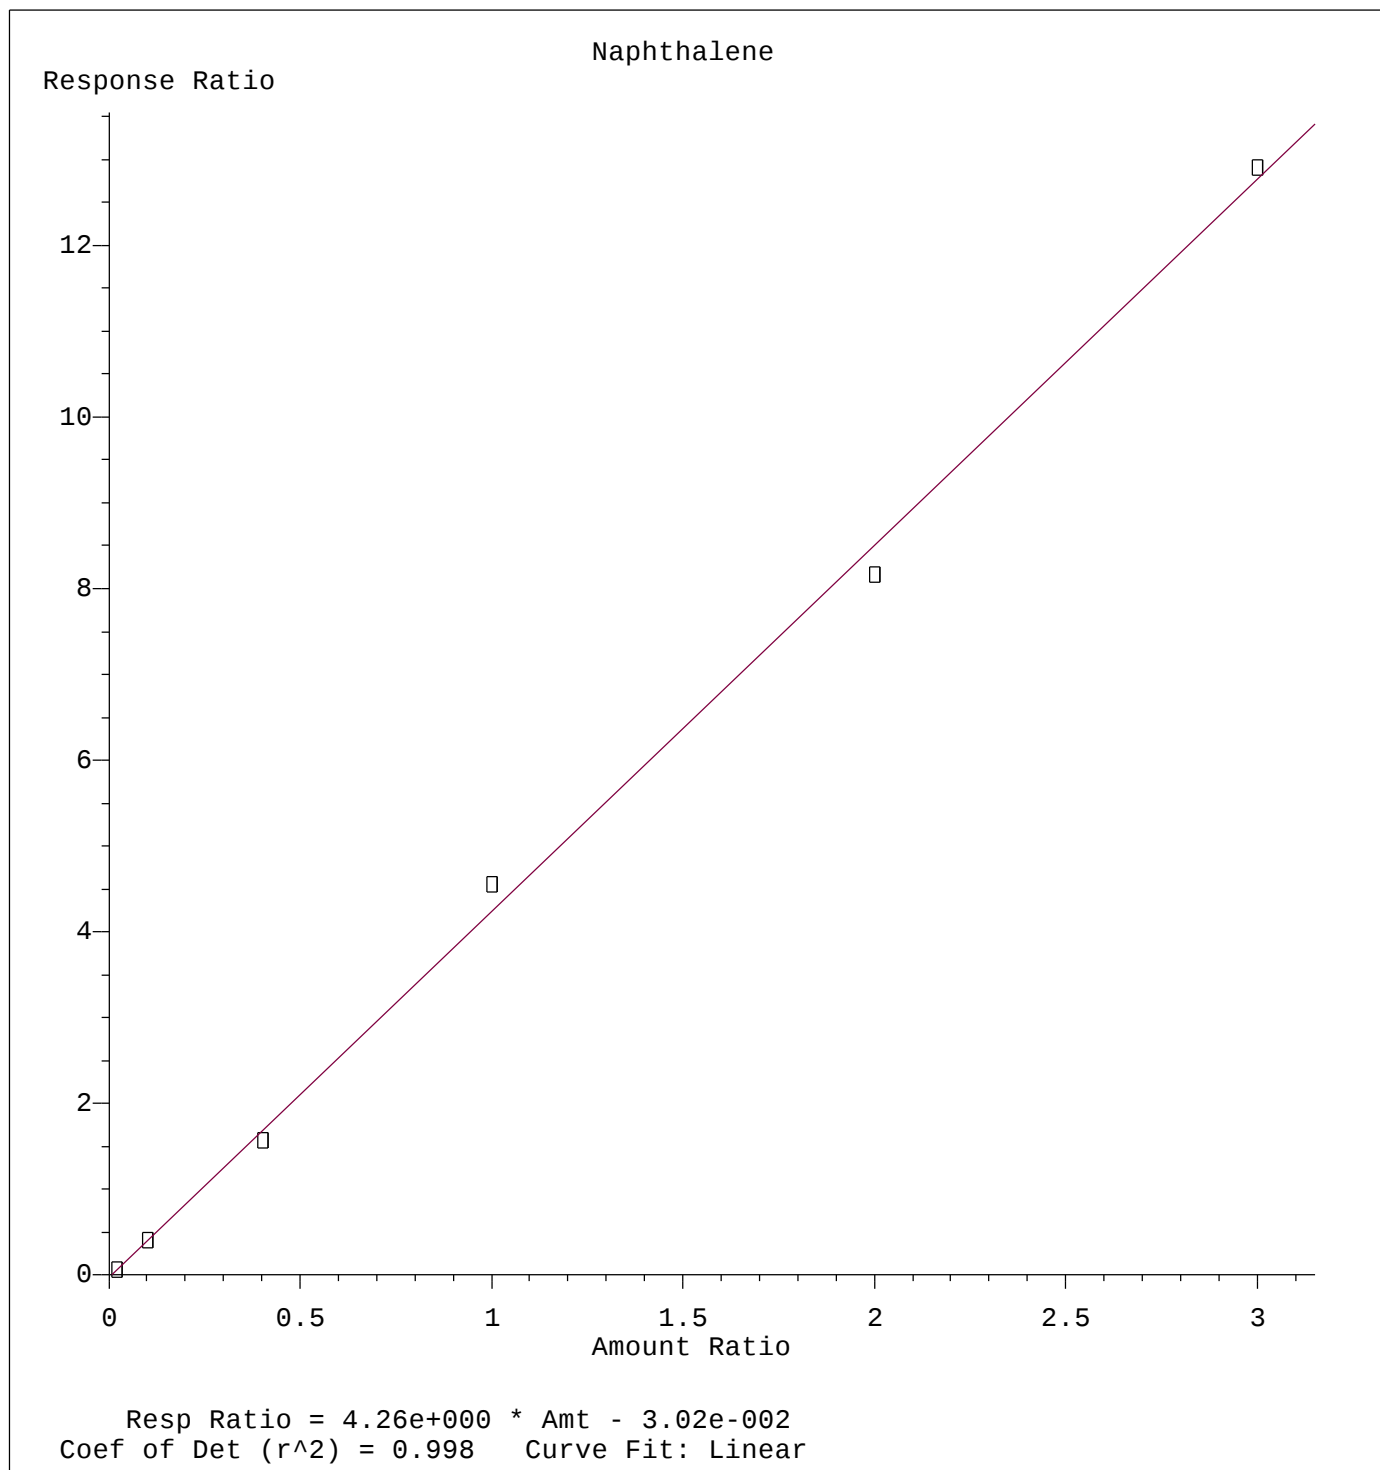

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019

Dichlorodifluoromethane

Response Ratio

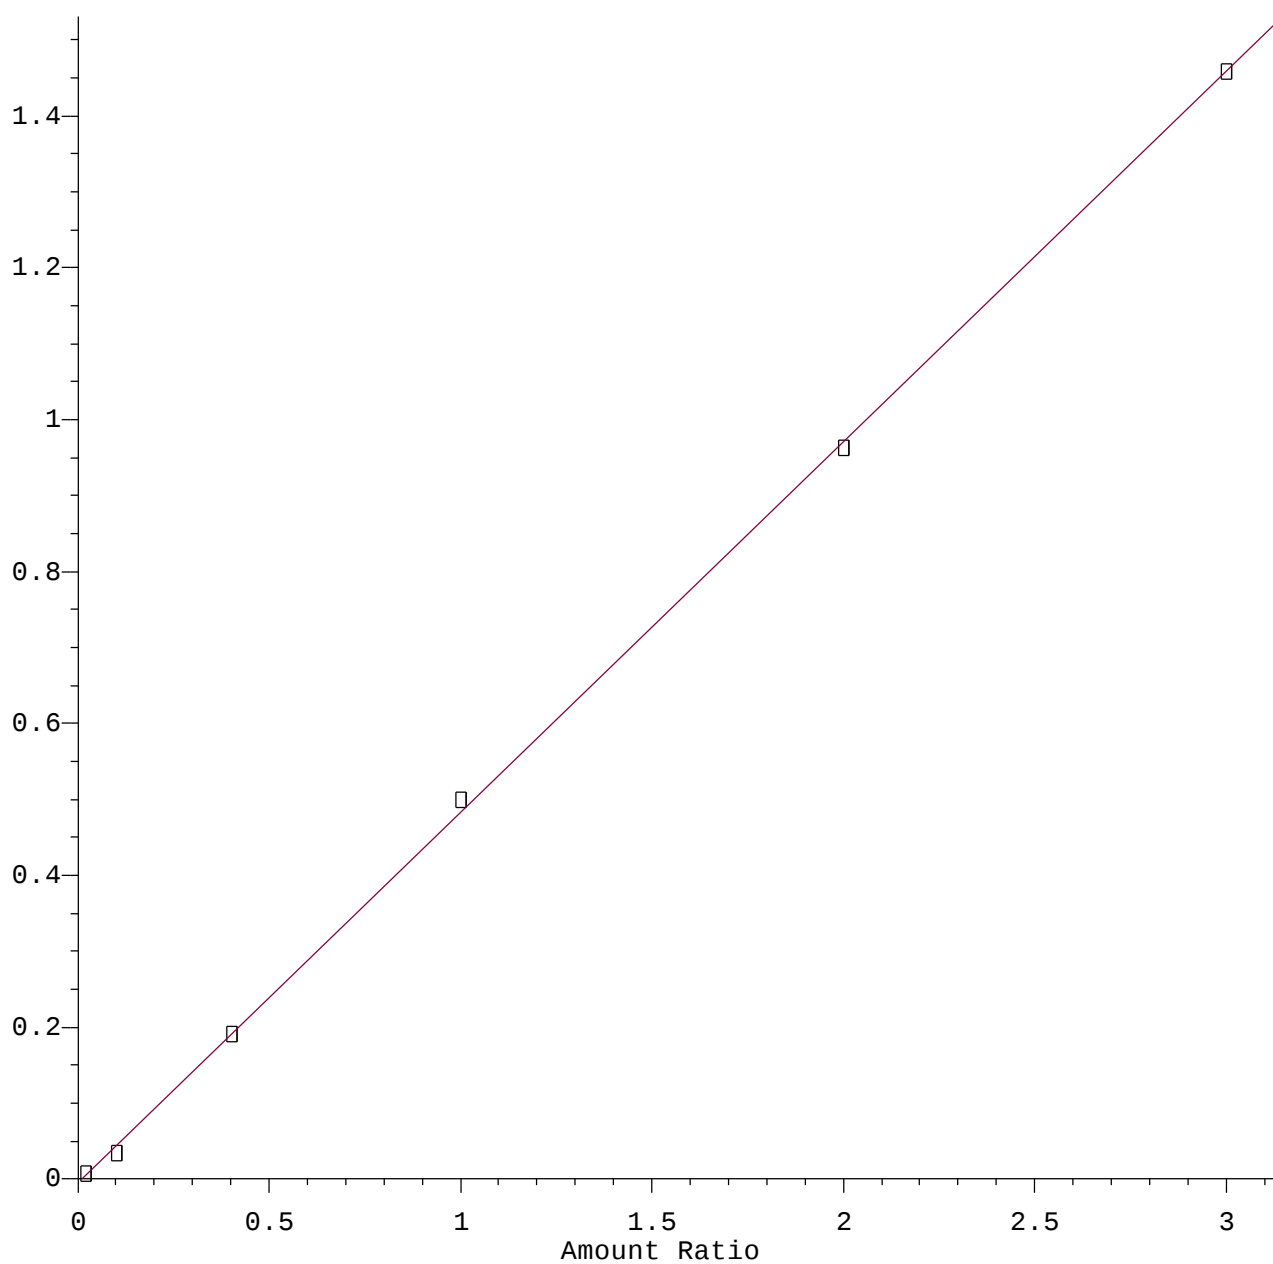

Resp Ratio = $4.87 \times 10^{-1} \times \text{Amt} - 4.75 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091619W.M
Calibration Table Last Updated: Tue Sep 17 04:36:38 2019