

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
 Data File : VX024293.D
 Acq On : 16 Sep 2021 17:16
 Operator : JC/MD
 Sample : M3774-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-02-(1.0)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.397	693	707	723	rBV2	93732	270575	33.34%	6.138%
2	5.562	723	734	748	rVB	150083	431105	53.12%	9.780%
3	5.970	790	801	810	rBV	102966	276382	34.05%	6.270%
4	6.050	810	814	824	rVB3	4481	11560	1.42%	0.262%
5	6.769	922	932	945	rBV	245804	582063	71.71%	13.205%
6	8.653	1234	1241	1249	rBV	529927	811635	100.00%	18.413%
7	10.055	1466	1471	1482	rBV	520594	747990	92.16%	16.969%
8	11.085	1634	1640	1653	rBV	443118	559776	68.97%	12.699%
9	12.024	1789	1794	1803	rBV	507993	641370	79.02%	14.550%
10	12.341	1842	1846	1851	rVB	9761	12672	1.56%	0.287%
11	13.780	2077	2082	2089	rBV	50611	62873	7.75%	1.426%




Sum of corrected areas: 4408001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024293.D
Acq On : 16 Sep 2021 17:16
Operator : JC/MD
Sample : M3774-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-02-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

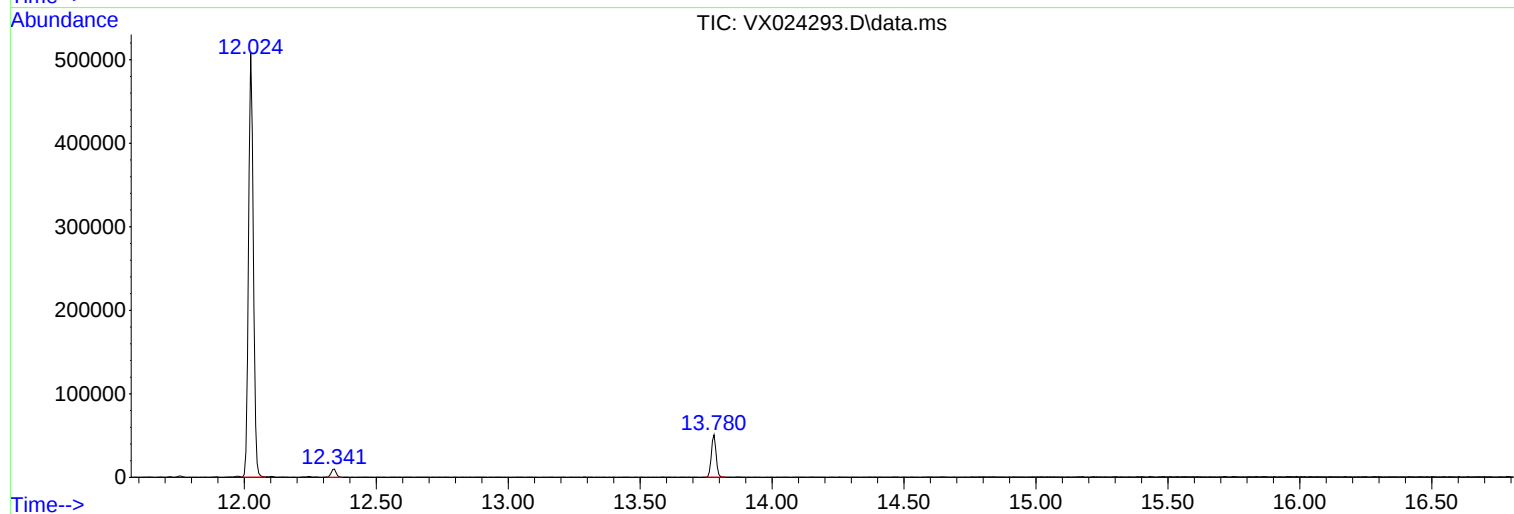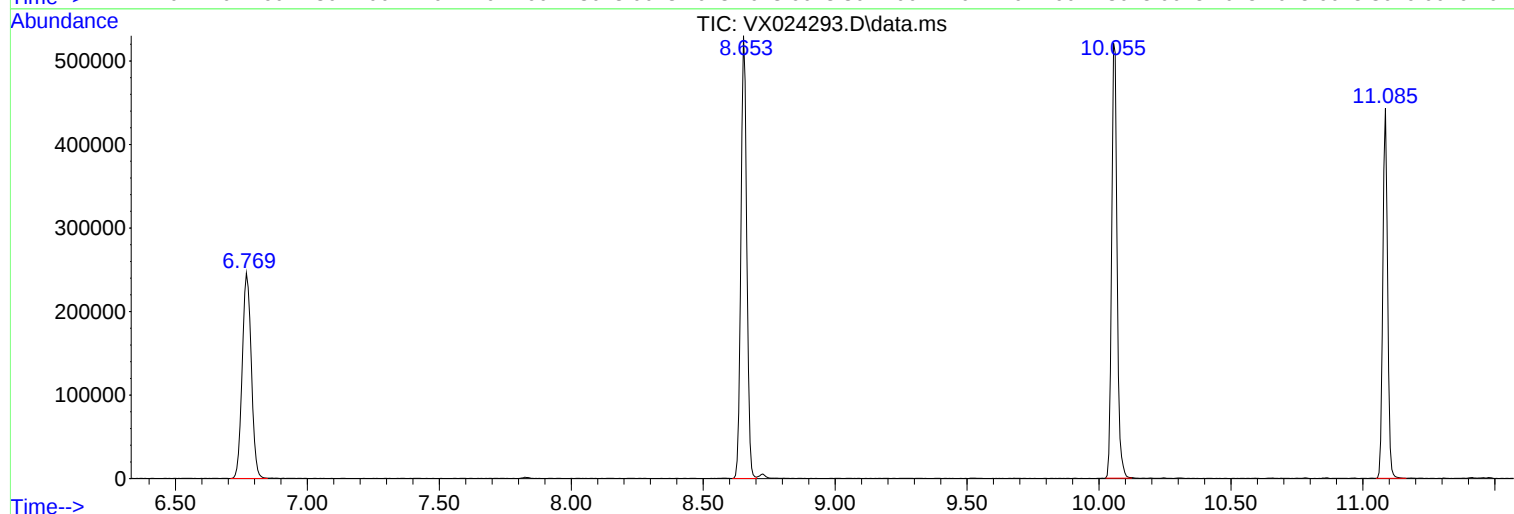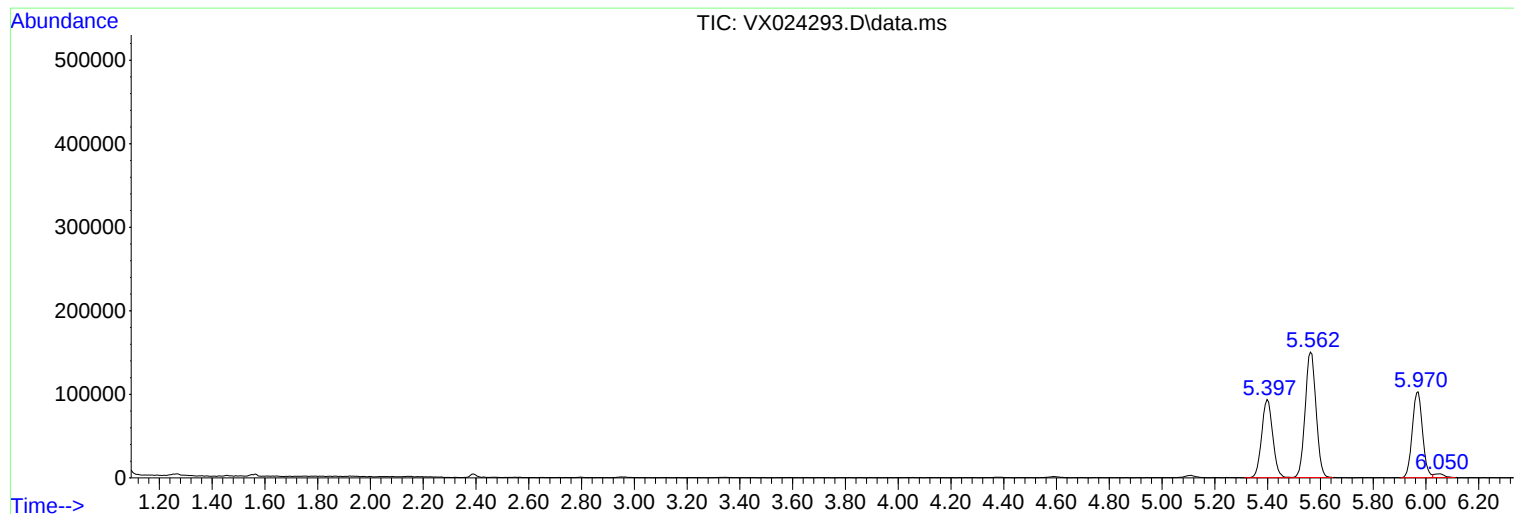

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024293.D
Acq On : 16 Sep 2021 17:16
Operator : JC/MD
Sample : M3774-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-02-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024293.D
Acq On : 16 Sep 2021 17:16
Operator : JC/MD
Sample : M3774-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-02-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------