

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
 Data File : VX024297.D
 Acq On : 16 Sep 2021 18:50
 Operator : JC/MD
 Sample : M3774-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-CB-03-(1.0)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.593	565	575	585	rBV3	2694	9309	1.19%	0.212%
2	5.397	695	707	721	rBV2	90337	262757	33.49%	5.988%
3	5.562	723	734	749	rVV	146468	411533	52.46%	9.378%
4	5.964	790	800	807	rBV	99006	262654	33.48%	5.985%
5	6.050	807	814	831	rVB	106304	280378	35.74%	6.389%
6	6.769	922	932	945	rBV	235934	562471	71.70%	12.818%
7	8.653	1234	1241	1250	rBV	507921	784471	100.00%	17.877%
8	10.055	1465	1471	1475	rBV	466809	768836	98.01%	17.520%
9	11.085	1634	1640	1656	rVB	394018	489187	62.36%	11.148%
10	12.024	1789	1794	1803	rBV	420881	539543	68.78%	12.295%
11	12.341	1838	1846	1853	rVB	12757	17118	2.18%	0.390%




Sum of corrected areas: 4388257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024297.D
Acq On : 16 Sep 2021 18:50
Operator : JC/MD
Sample : M3774-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

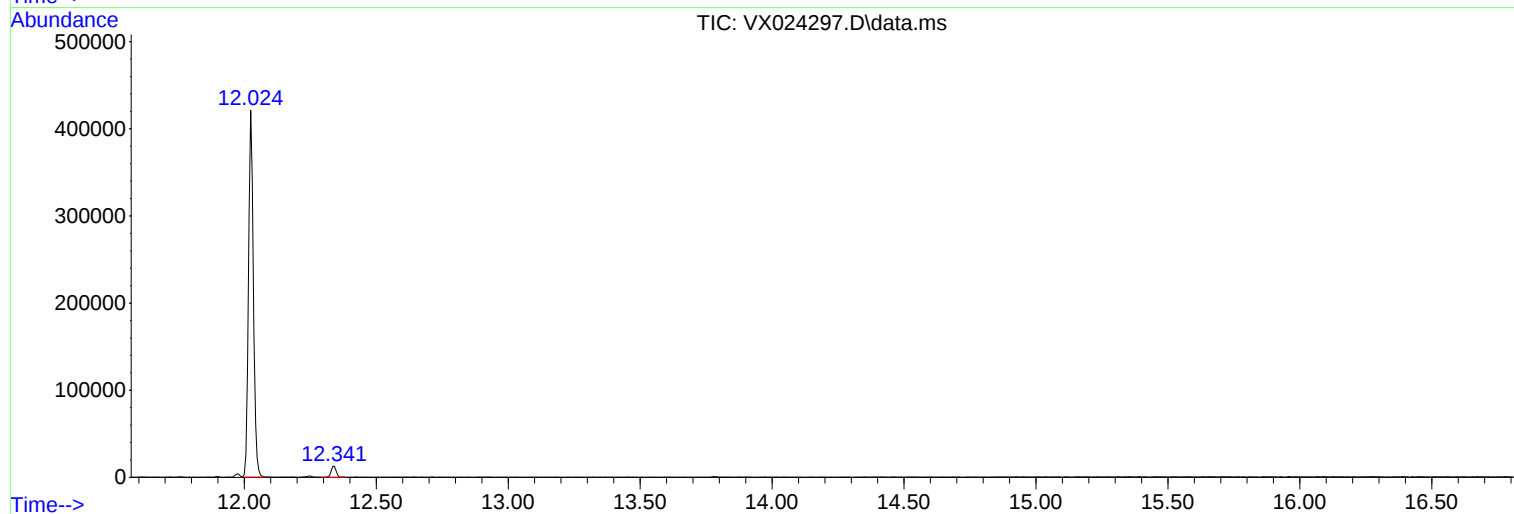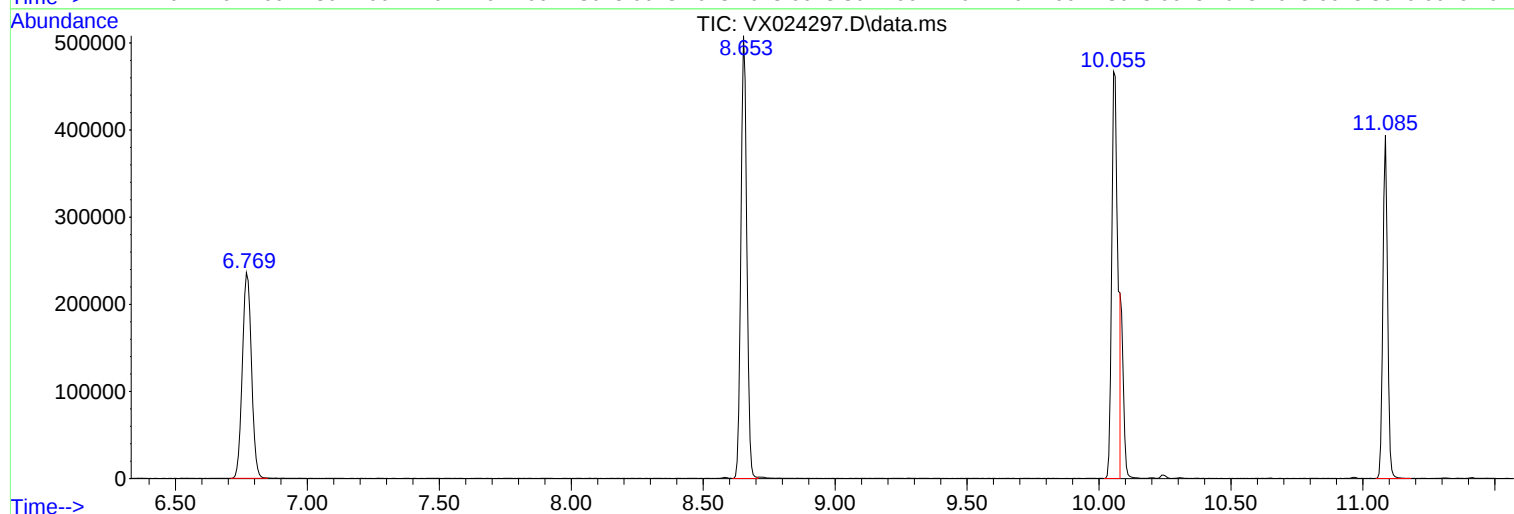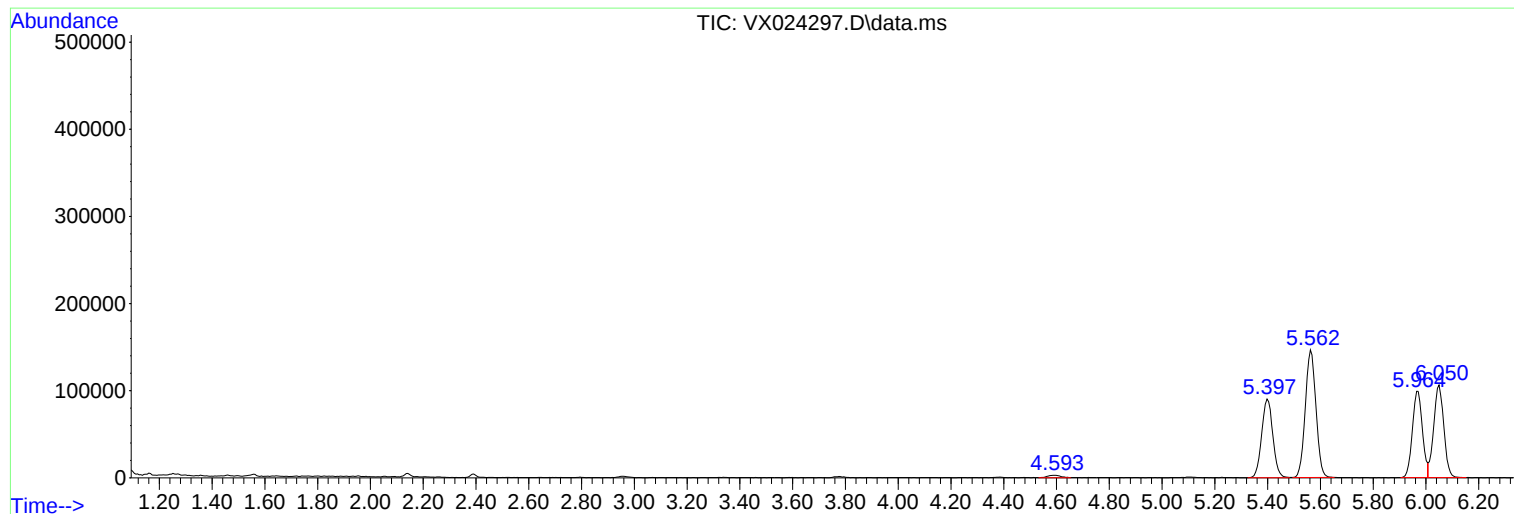

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024297.D
Acq On : 16 Sep 2021 18:50
Operator : JC/MD
Sample : M3774-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091621\
Data File : VX024297.D
Acq On : 16 Sep 2021 18:50
Operator : JC/MD
Sample : M3774-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
