

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
 Data File : VX031419.D
 Acq On : 16 Sep 2022 18:46
 Operator : JC/MD
 Sample : N4645-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOLL-MW-02

Quant Time: Sep 17 02:07:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 01:50:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	83048	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	134729	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	125308	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58025	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	82147	40.299	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	80.600%		
35) Dibromofluoromethane	5.391	113	68677	47.421	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.840%		
50) Toluene-d8	8.653	98	263763	48.552	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.100%		
62) 4-Bromofluorobenzene	11.085	95	86882	43.673	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	87.340%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.270	85	267	0.298	ug/l	95
3) Chloromethane	1.288	50	387	Below Cal	#	84
4) Vinyl Chloride	1.374	62	472	0.325	ug/l #	43
5) Bromomethane	1.612	94	571	0.525	ug/l	98
6) Chloroethane	1.563	64	3423	2.993	ug/l #	53
10) Methyl Iodide	2.459	142	231	1.077	ug/l #	68
11) Tert butyl alcohol	2.947	59	1536	Below Cal	#	73
13) Acrolein	2.203	56	51	0.217	ug/l #	1
14) Allyl chloride	2.782	41	2240	0.875	ug/l #	70
15) Acrylonitrile	3.099	53	1044	1.110	ug/l #	38
16) Acetone	2.386	43	1325	1.523	ug/l #	83
17) Carbon Disulfide	2.514	76	778	1.155	ug/l #	75
18) Methyl Acetate	2.782	43	4572	1.772	ug/l #	52
19) Methyl tert-butyl Ether	3.117	73	6745	1.256	ug/l #	1
20) Methylene Chloride	2.782	84	91	Below Cal	#	45
21) trans-1,2-Dichloroethene	3.093	96	209	Below Cal	#	48
22) Diisopropyl ether	3.770	45	1298	0.242	ug/l #	66
25) 2-Butanone	4.587	43	789	0.550	ug/l	92
31) Cyclohexane	5.477	56	12904	5.892	ug/l	96
36) 1,1-Dichloropropene	5.544	75	6587	3.323	ug/l #	46
38) Carbon Tetrachloride	5.556	117	8420	3.908	ug/l #	16
39) Methylcyclohexane	7.379	83	3055	1.399	ug/l	99
40) Benzene	6.044	78	2854	0.501	ug/l	97
55) 1,1,2-Trichloroethane	9.104	97	1693	1.065	ug/l #	15
73) Isopropylbenzene	10.964	105	1183	0.276	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	49657	33.960	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	49657	93.967	ug/l #	11
83) tert-Butylbenzene	11.713	119	818	0.228	ug/l	90
85) sec-Butylbenzene	11.890	105	1237	0.275	ug/l #	56
90) Hexachloroethane	12.646	117	150	0.205	ug/l #	15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
Data File : VX031419.D
Acq On : 16 Sep 2022 18:46
Operator : JC/MD
Sample : N4645-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02

Quant Time: Sep 17 02:07:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 01:50:07 2022
Response via : Initial Calibration




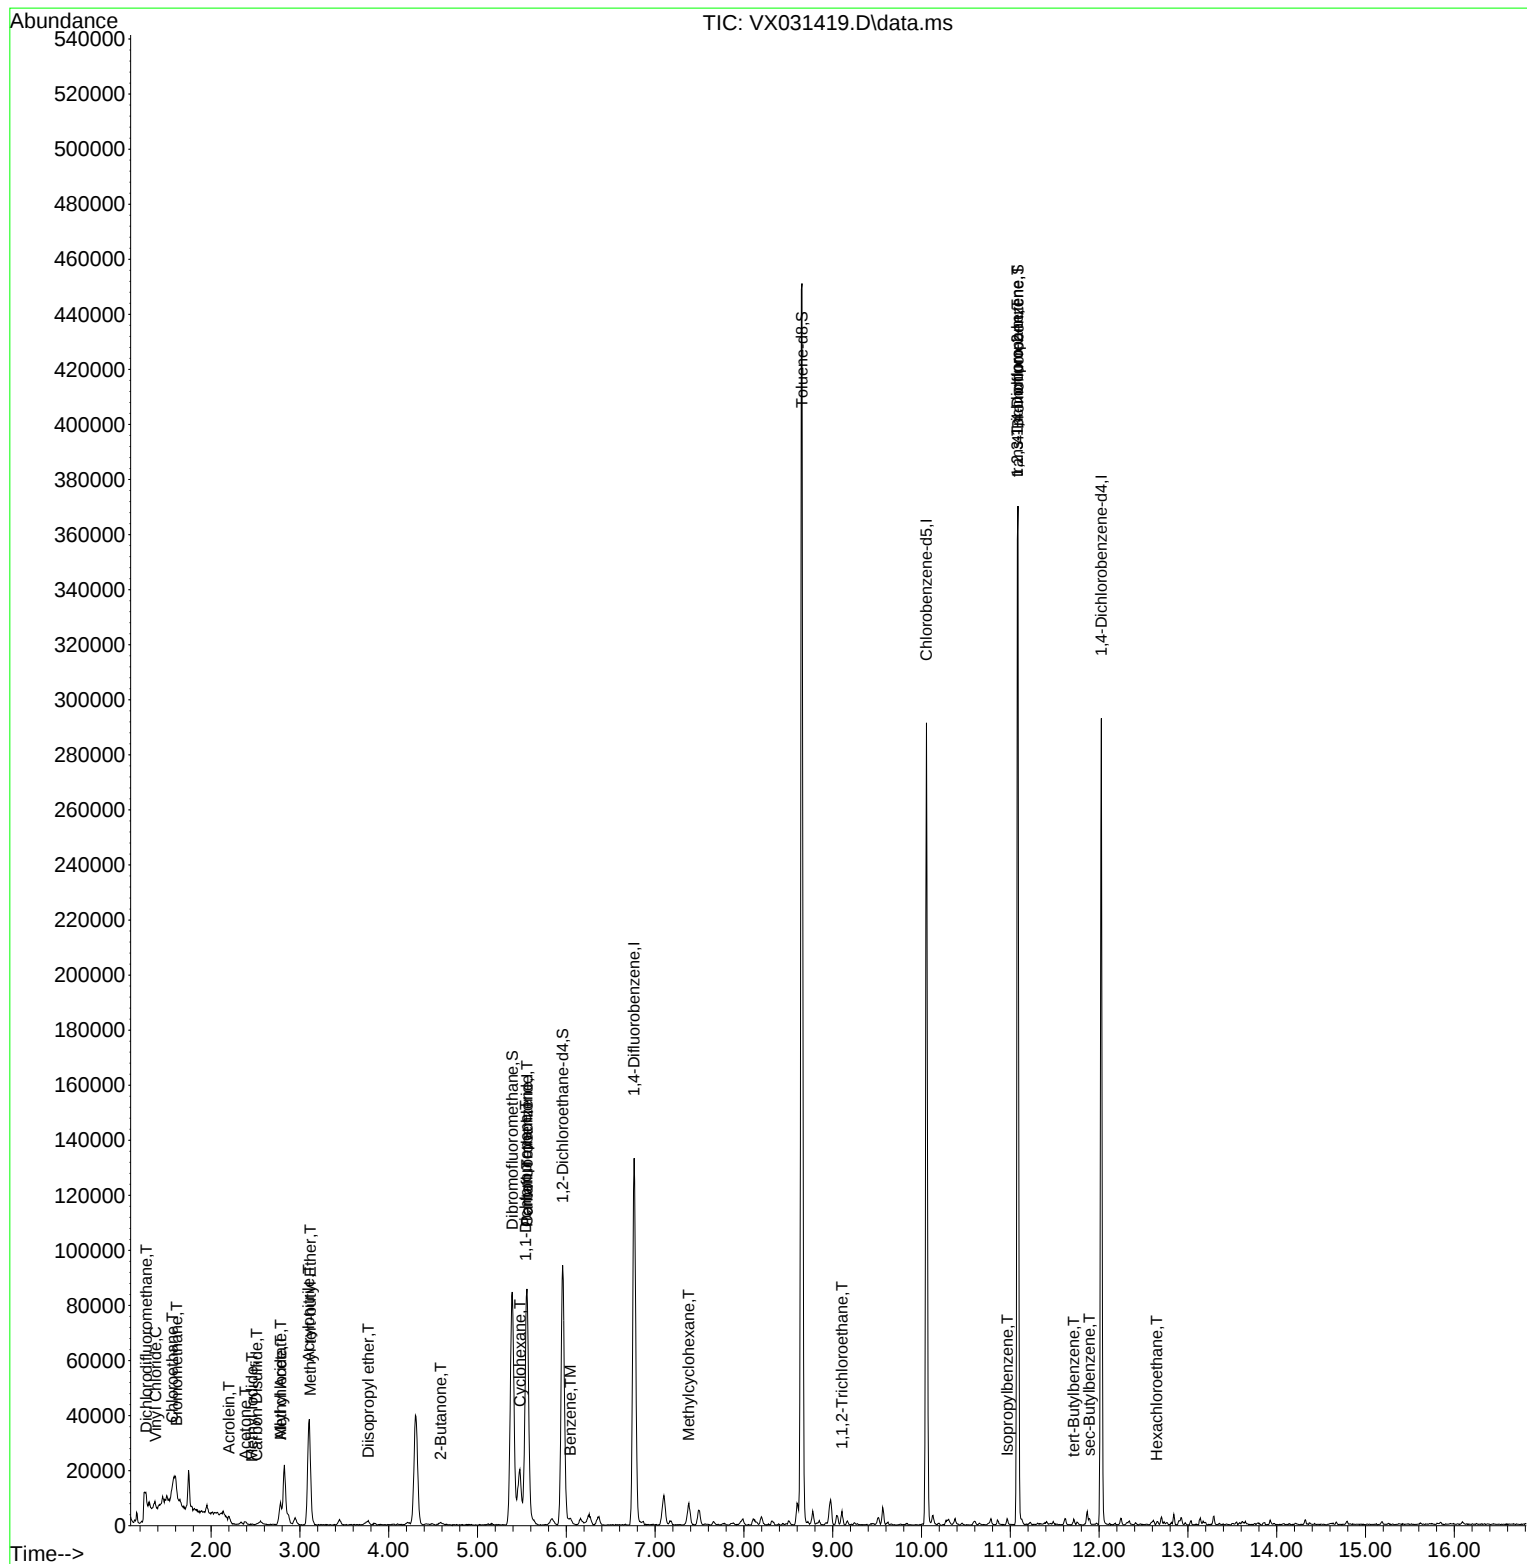




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion:168 Resp: 83048
Ion Ratio Lower Upper
168 100
99 52.3 48.8 73.2

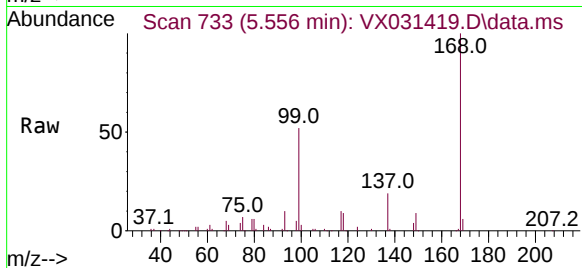

#2
Dichlorodifluoromethane
Concen: 0.298 ug/l
RT: 1.270 min Scan# 30
Delta R.T. 0.104 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 85 Resp: 267
Ion Ratio Lower Upper
85 100
87 28.8 15.8 47.4


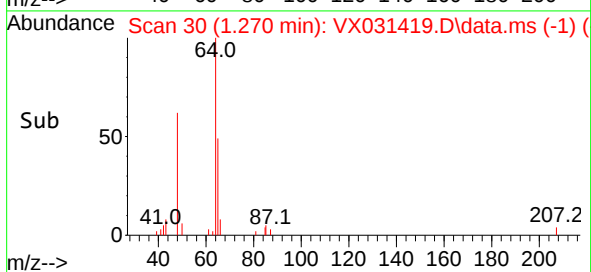

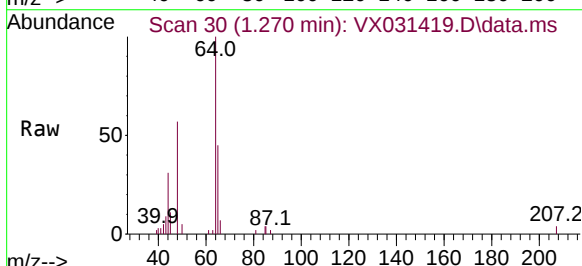


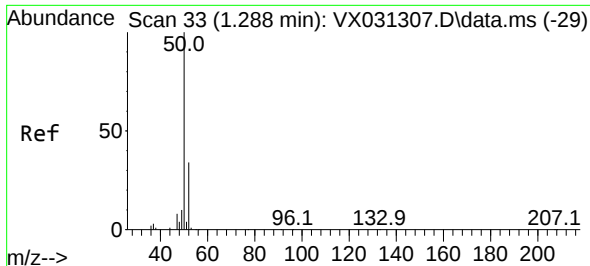

#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 50 Resp: 387
Ion Ratio Lower Upper
50 100
52 24.5 26.9 40.3#

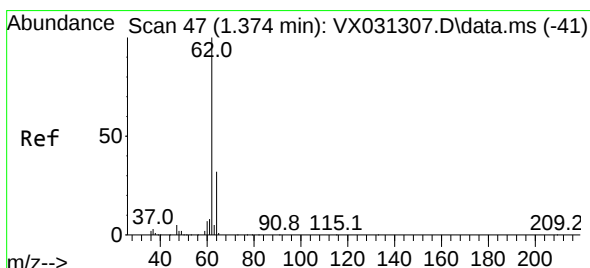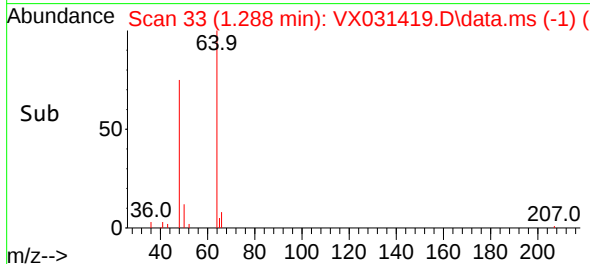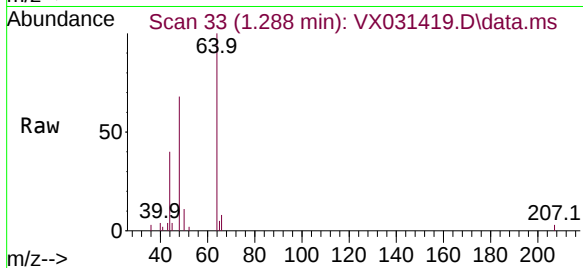

#4
Vinyl Chloride
Concen: 0.325 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 62 Resp: 472
Ion Ratio Lower Upper
62 100
64 0.0 25.3 37.9#


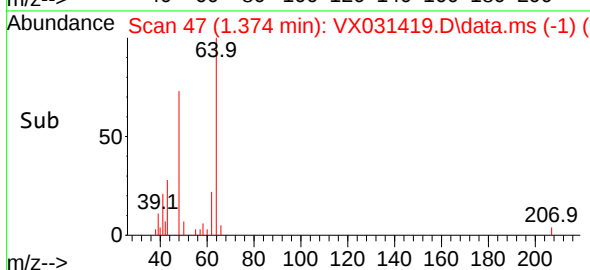

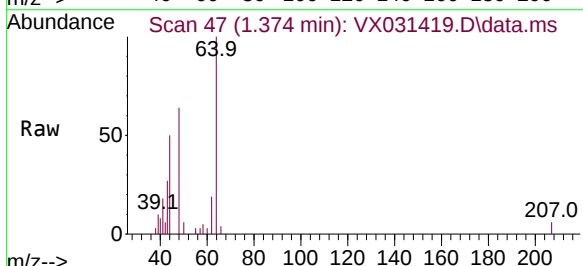


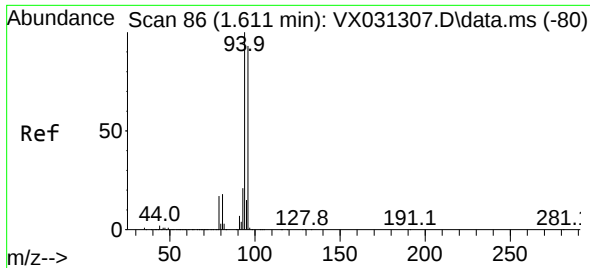

#5
Bromomethane
Concen: 0.525 ug/l
RT: 1.612 min Scan# 80
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 94 Resp: 571
Ion Ratio Lower Upper
94 100
96 94.9 74.4 111.6

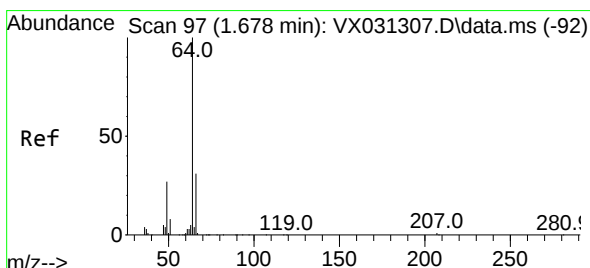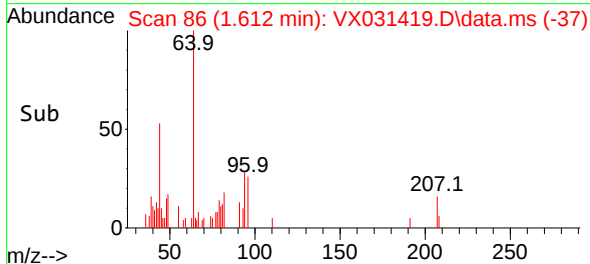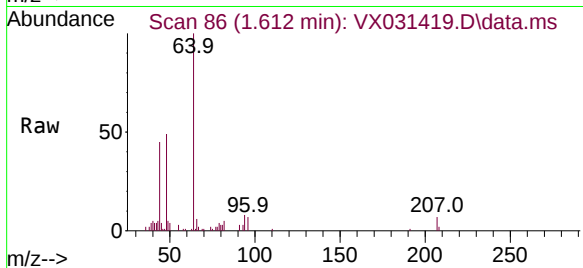

#6
Chloroethane
Concen: 2.993 ug/l
RT: 1.563 min Scan# 78
Delta R.T. -0.115 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 64 Resp: 3423
Ion Ratio Lower Upper
64 100
66 5.0 25.0 37.4#


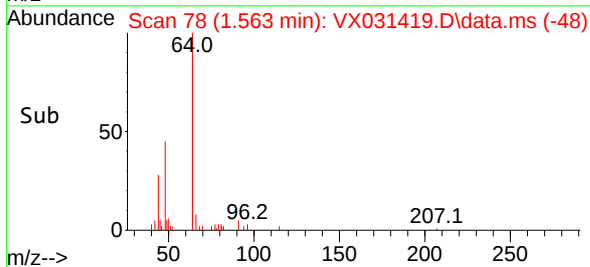

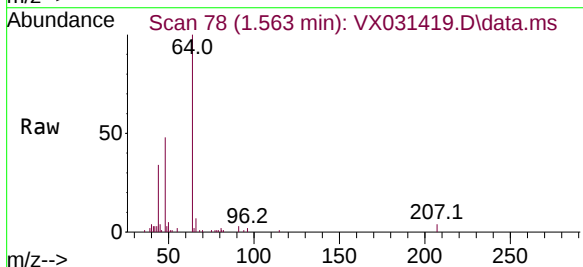




#10
Methyl Iodide
Concen: 1.077 ug/l
RT: 2.459 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion:142 Resp: 231
Ion Ratio Lower Upper
142 100
127 26.0 37.4 56.0#
141 0.0 11.6 17.4#

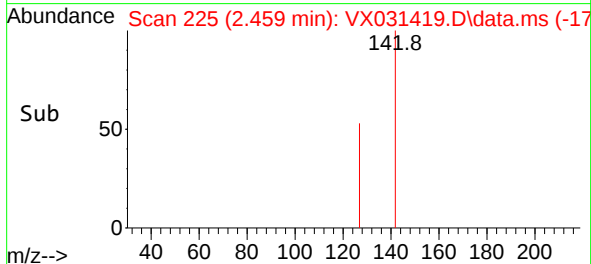

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.947 min Scan# 305
Delta R.T. -0.042 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 59 Resp: 1536
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#


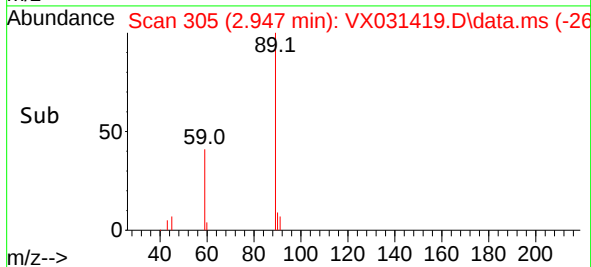

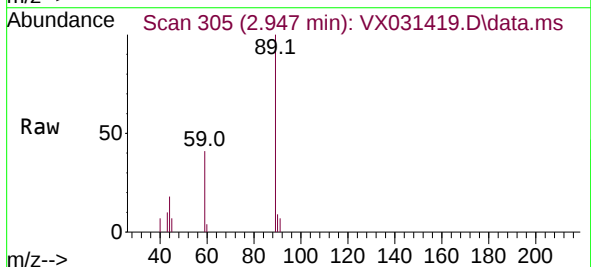


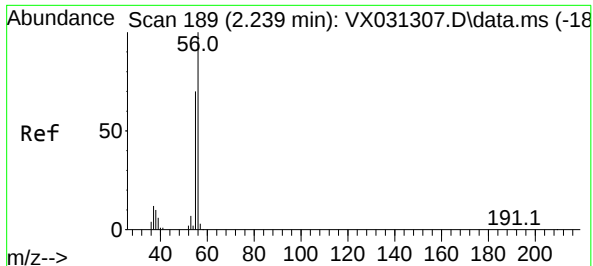

#13
Acrolein
Concen: 0.217 ug/l
RT: 2.203 min Scan# 11
Delta R.T. -0.036 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 56 Resp: 51
Ion Ratio Lower Upper
56 100
55 935.3 56.0 84.0#

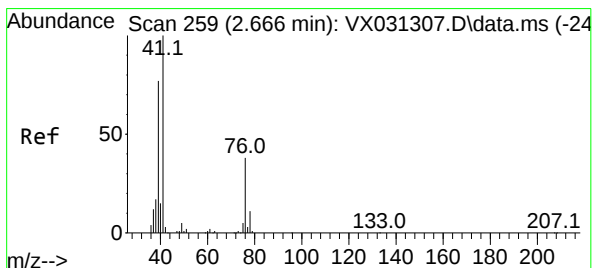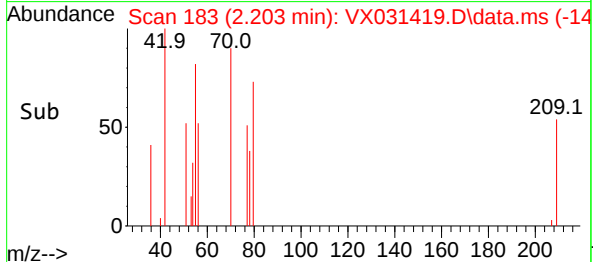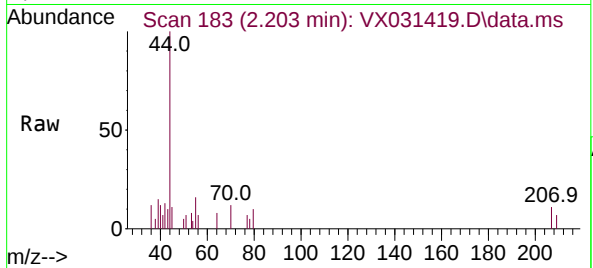

#14
Allyl chloride
Concen: 0.875 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.116 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 41 Resp: 2240
Ion Ratio Lower Upper
41 100
39 57.0 58.2 87.4#
76 2.9 26.9 40.3#

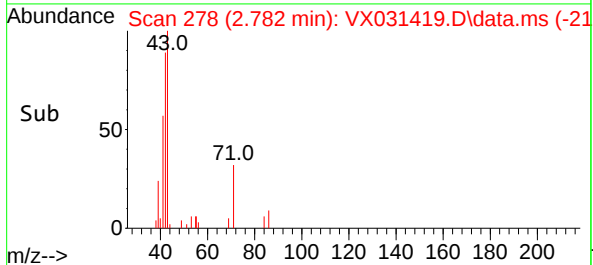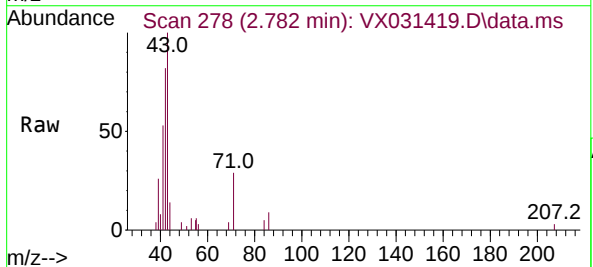



#15

Acrylonitrile

Concen: 1.110 ug/l

RT: 3.099 min Scan# 31

Delta R.T. 0.031 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :

TOLL-MW-02





Tgt Ion: 53 Resp: 1044

Ion Ratio Lower Upper

53 100

52 19.1 66.9 100.3#

51 61.5 30.0 45.0#

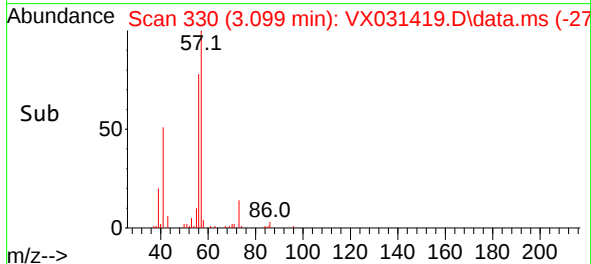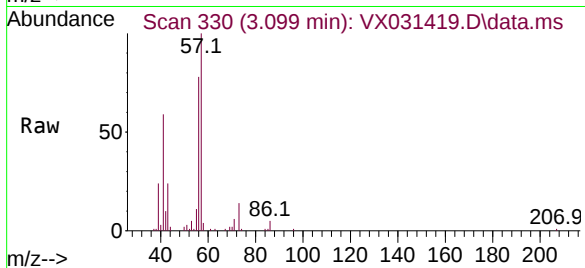

#16

Acetone

Concen: 1.523 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.000 min

Lab File: VX031419.D




Acq: 16 Sep 2022 18:46


Tgt Ion: 43 Resp: 1325

Ion Ratio Lower Upper

43 100

58 20.5 23.8 35.8#


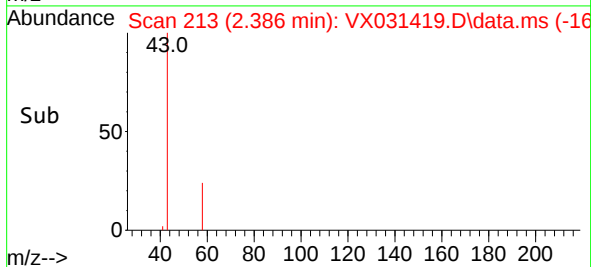

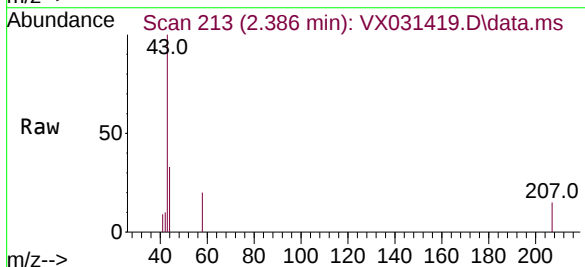




#17
Carbon Disulfide
Concen: 1.155 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.007 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 76 Resp: 778
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

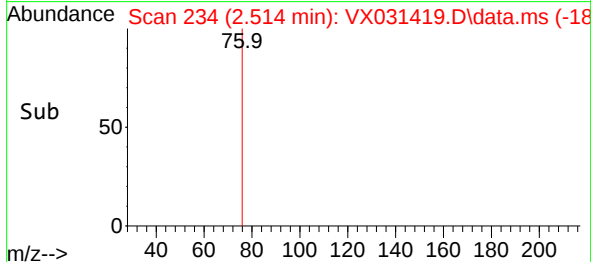

#18
Methyl Acetate
Concen: 1.772 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.079 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 43 Resp: 4572
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#


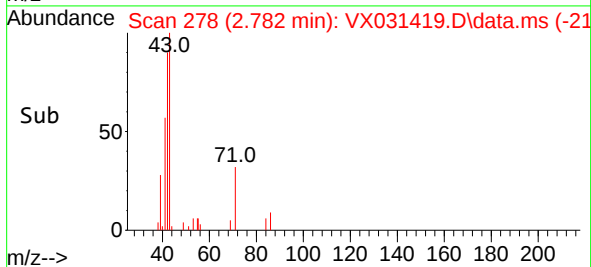

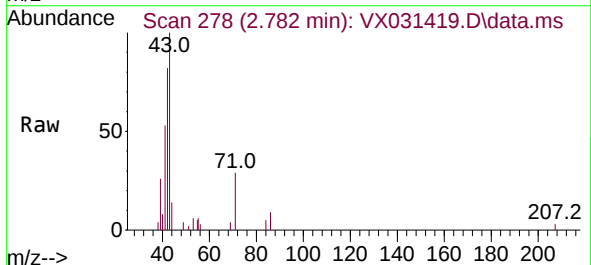




#19
Methyl tert-butyl Ether
Concen: 1.256 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 73 Resp: 6745
Ion Ratio Lower Upper
73 100
57 207.2 17.2 25.8#

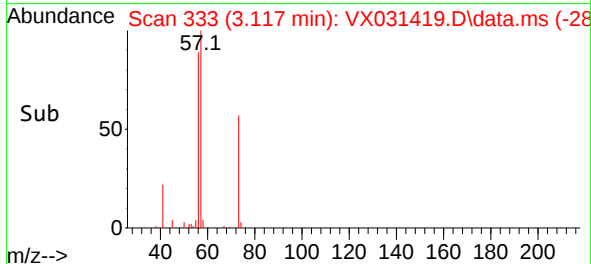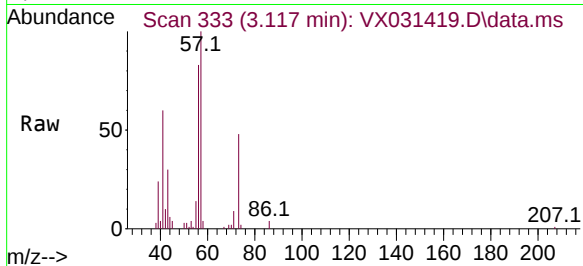

#20
Methylene Chloride
Concen: Below Cal
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 84 Resp: 91
Ion Ratio Lower Upper
84 100
49 69.9 105.9 158.9#
51 0.0 32.2 48.2#
86 104.1 50.8 76.2#


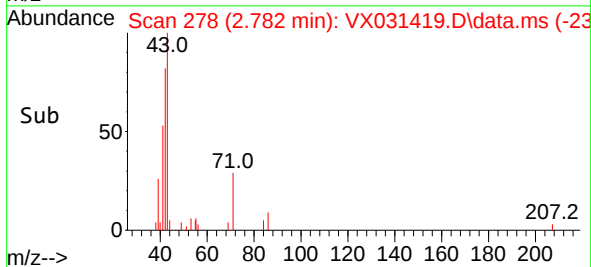

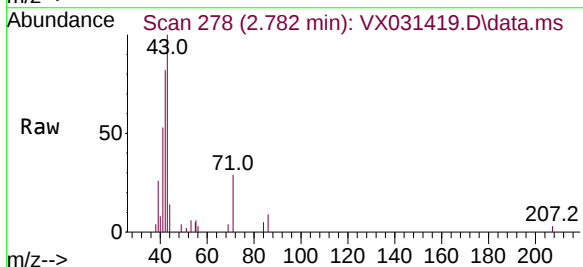




#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 96 Resp: 209
Ion Ratio Lower Upper
96 100
61 87.1 106.7 160.1#
98 0.0 48.7 73.1#

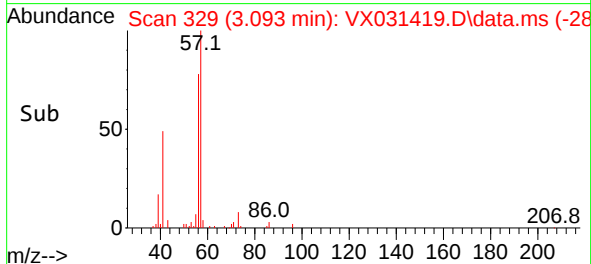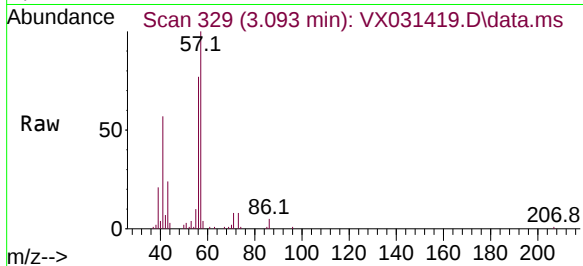

#22
Diisopropyl ether
Concen: 0.242 ug/l
RT: 3.770 min Scan# 440
Delta R.T. 0.006 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 45 Resp: 1298
Ion Ratio Lower Upper
45 100
43 62.9 59.0 88.6
87 69.9 22.6 33.8#
59 34.3 8.8 13.2#

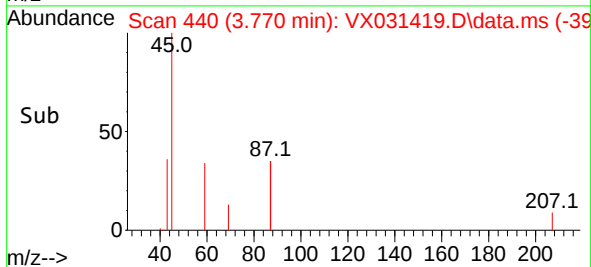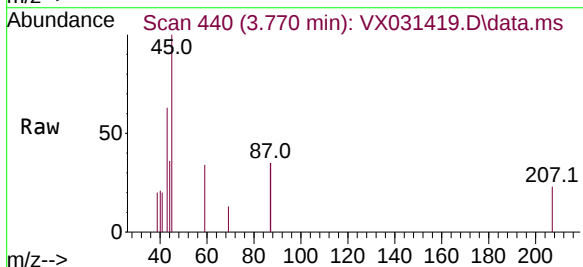



#25

2-Butanone

Concen: 0.550 ug/l

RT: 4.587 min Scan# 51

Delta R.T. 0.025 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :





TOLL-MW-02

Tgt Ion: 43 Resp: 789

Ion Ratio Lower Upper

43 100

72 30.3 21.1 31.7

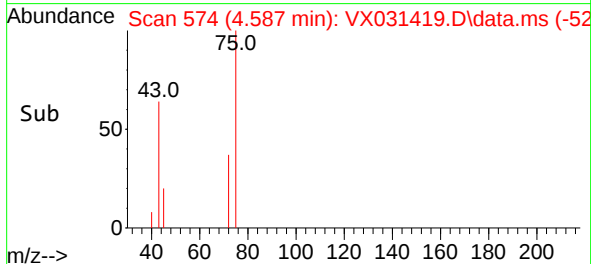

#31

Cyclohexane

Concen: 5.892 ug/l

RT: 5.477 min Scan# 720

Delta R.T. 0.006 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46




Tgt Ion: 56 Resp: 12904


Ion Ratio Lower Upper

56 100

69 29.3 25.1 37.7

84 83.5 70.2 105.4

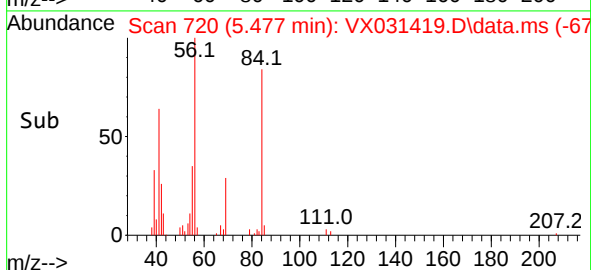

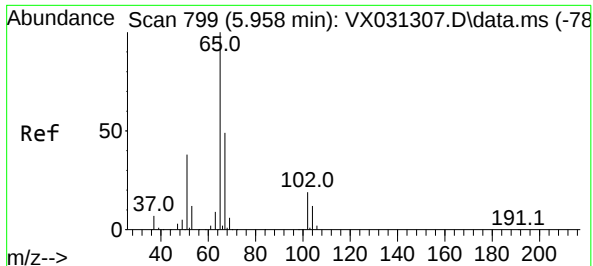

#33

1,2-Dichloroethane-d4

Concen: 40.299 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :





TOLL-MW-02

Tgt Ion: 65 Resp: 82147

Ion Ratio Lower Upper

65 100

67 52.6 0.0 102.4

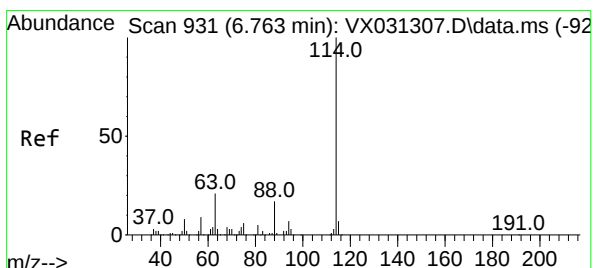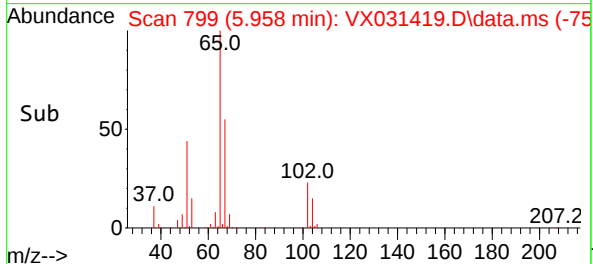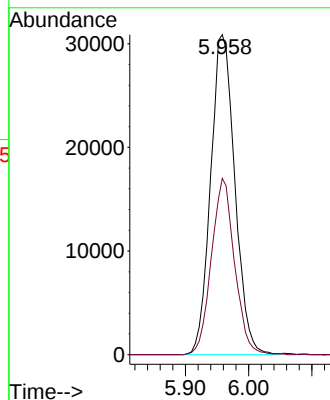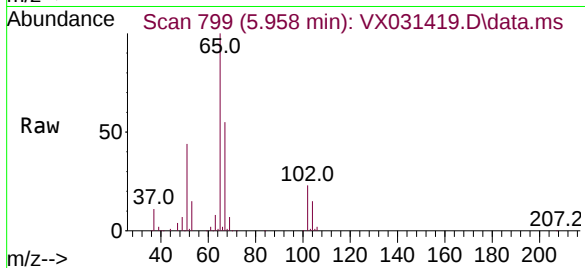

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46




Tgt Ion: 114 Resp: 134729


Ion Ratio Lower Upper

114 100

63 19.7 0.0 42.6

88 14.8 0.0 33.0

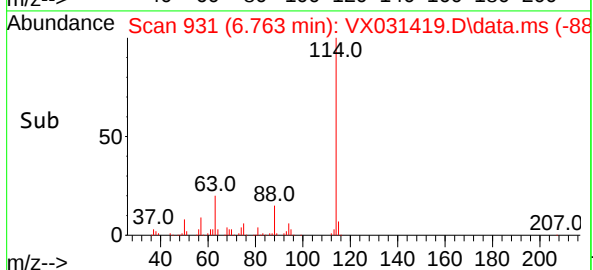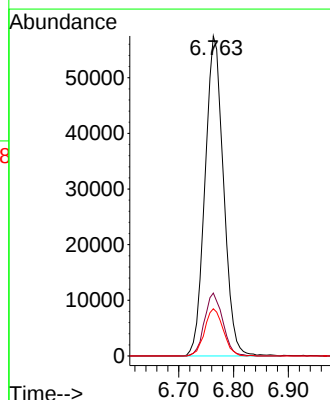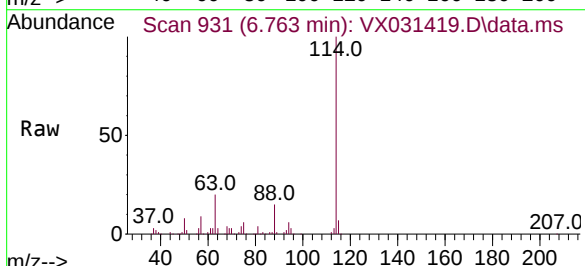

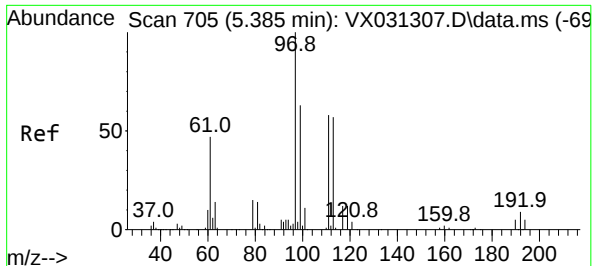

#35

Dibromofluoromethane

Concen: 47.421 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :

TOLL-MW-02





Tgt Ion:113 Resp: 68677

Ion Ratio Lower Upper

113 100

111 104.4 82.4 123.6

192 19.2 14.1 21.1

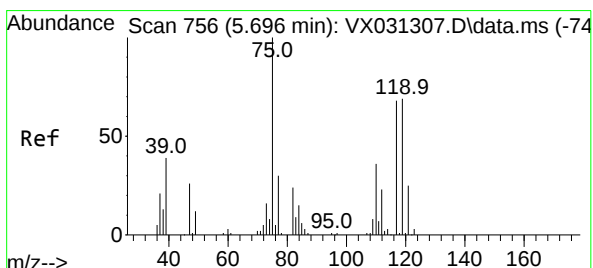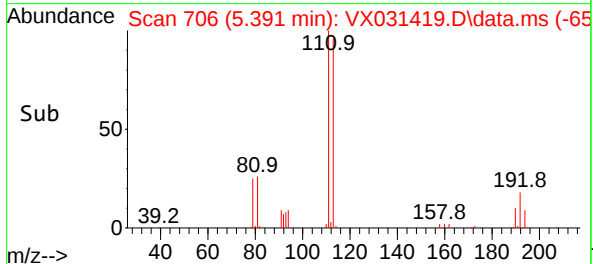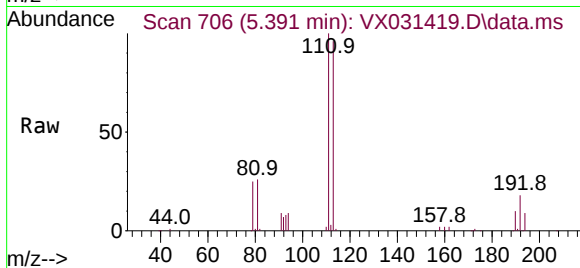

#36

1,1-Dichloropropene

Concen: 3.323 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.152 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46




Tgt Ion: 75 Resp: 6587


Ion Ratio Lower Upper

75 100

110 4.5 17.5 52.5#

77 0.0 24.9 37.3#


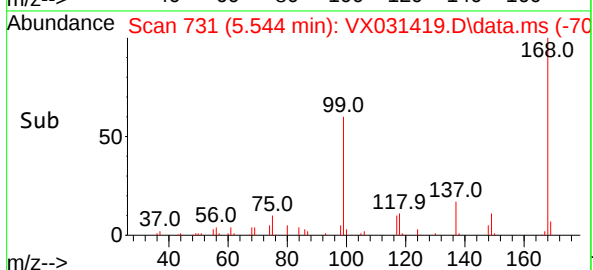

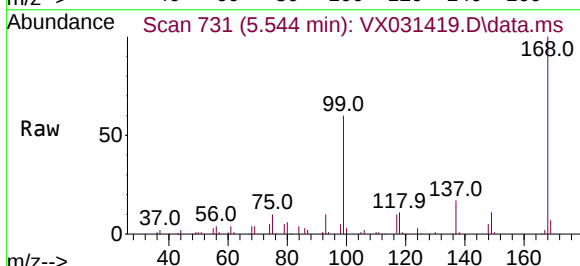




#38
Carbon Tetrachloride
Concen: 3.908 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.122 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion:117 Resp: 8420
Ion Ratio Lower Upper
117 100
119 4.0 74.6 112.0#
121 0.0 25.3 37.9#

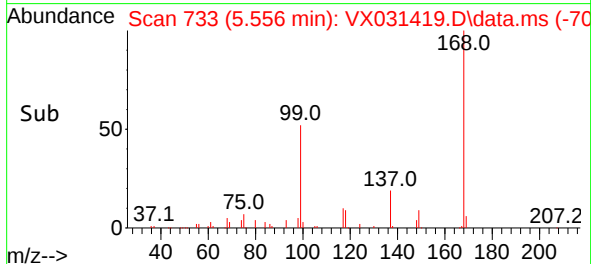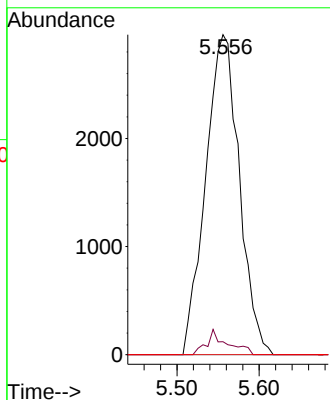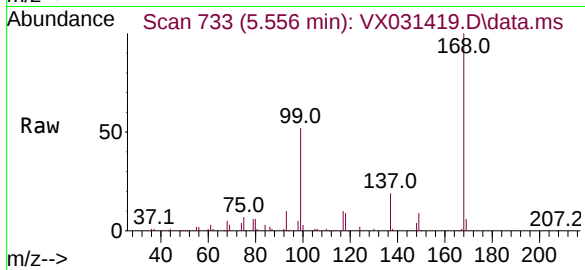

#39
Methylcyclohexane
Concen: 1.399 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 83 Resp: 3055
Ion Ratio Lower Upper
83 100
55 75.6 61.0 91.4
98 47.3 37.7 56.5


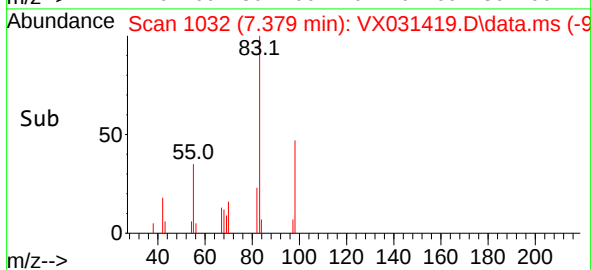
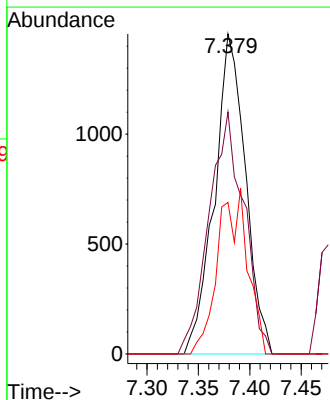
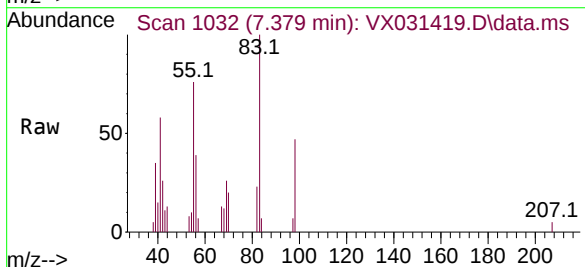


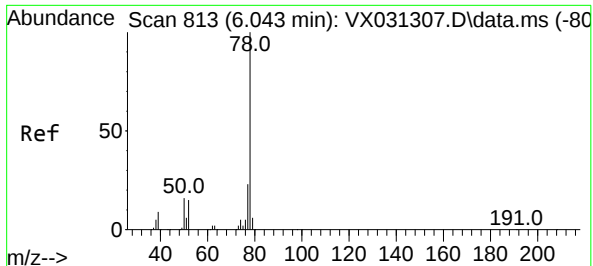

#40
Benzene
Concen: 0.501 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 78 Resp: 2854
Ion Ratio Lower Upper
78 100
77 25.1 18.7 28.1

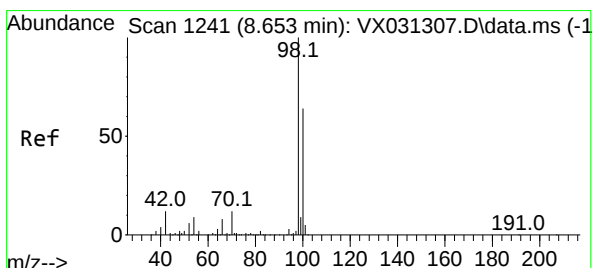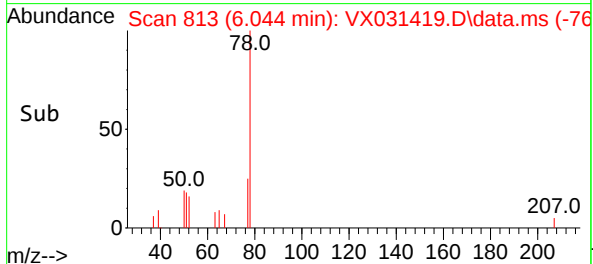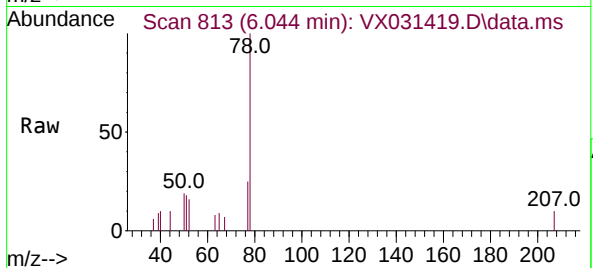

#50
Toluene-d8
Concen: 48.552 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 98 Resp: 263763
Ion Ratio Lower Upper
98 100
100 64.5 52.5 78.7


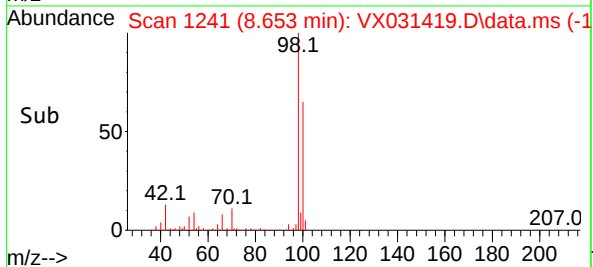

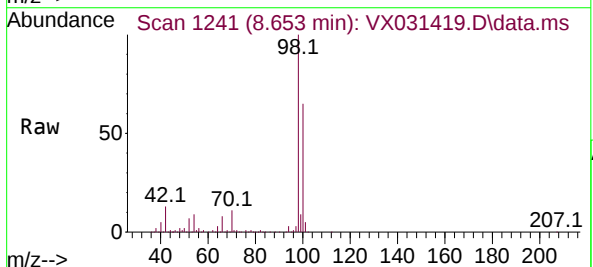




#55
1,1,2-Trichloroethane
Concen: 1.065 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02


Tgt Ion: 97	Resp: 1693
Ion Ratio	Lower Upper
97 100	
83 0.0	69.0 103.6#
85 0.0	44.1 66.1#
99 0.0	51.3 76.9#

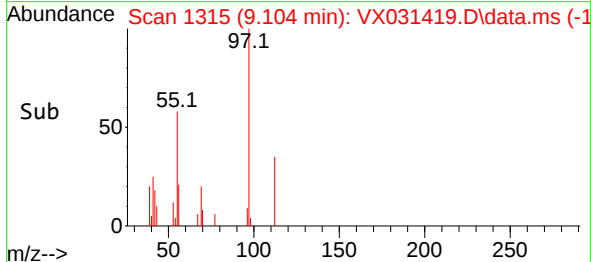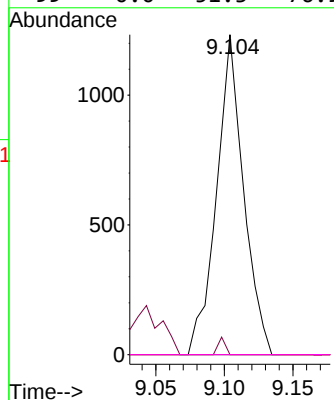

#62
4-Bromofluorobenzene
Concen: 43.673 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion: 95	Resp: 86882
Ion Ratio	Lower Upper
95 100	
174 86.7	0.0 153.2
176 84.6	0.0 144.0

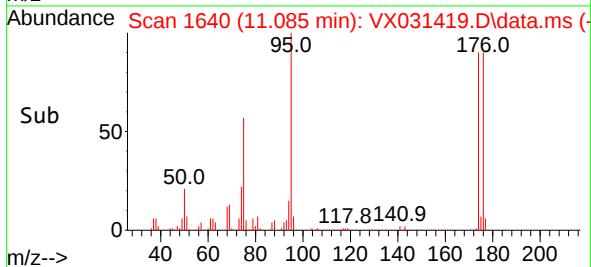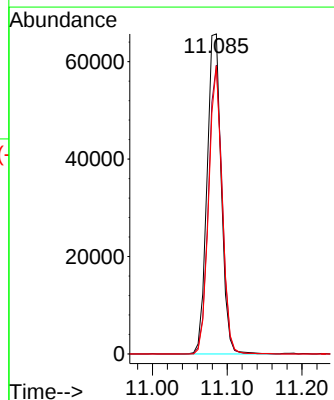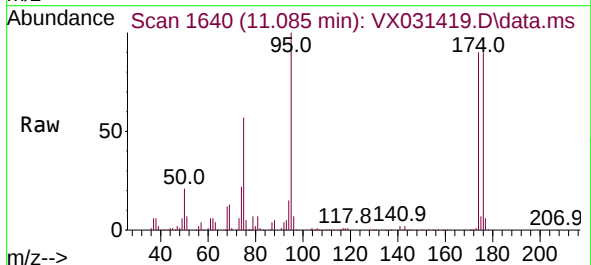



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :

TOLL-MW-02





Tgt Ion:117 Resp: 125308

Ion Ratio Lower Upper

117 100

82 52.0 46.8 70.2

119 30.9 26.4 39.6

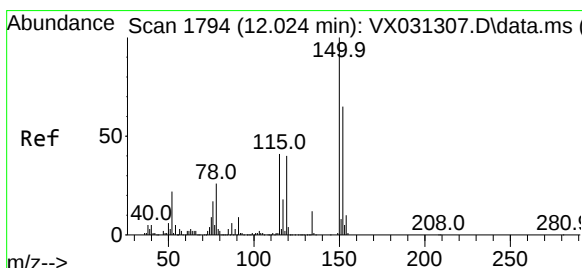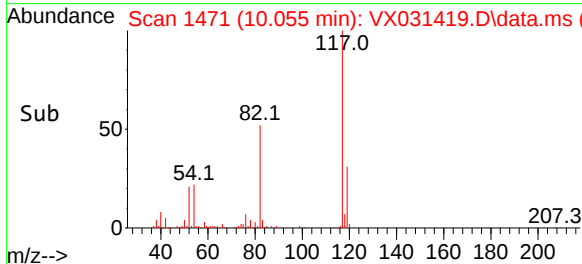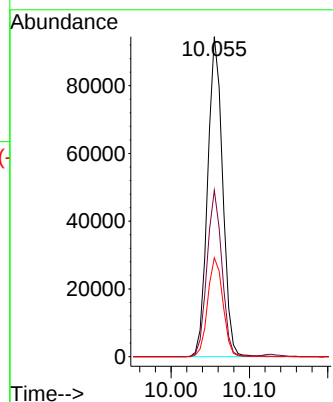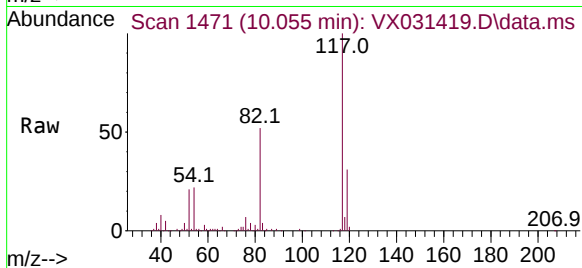

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46




Tgt Ion:152 Resp: 58025


Ion Ratio Lower Upper

152 100

115 55.3 43.4 130.1

150 153.8 0.0 346.8

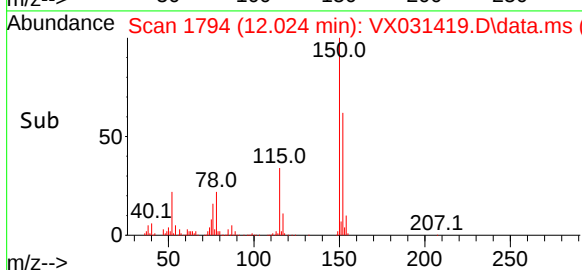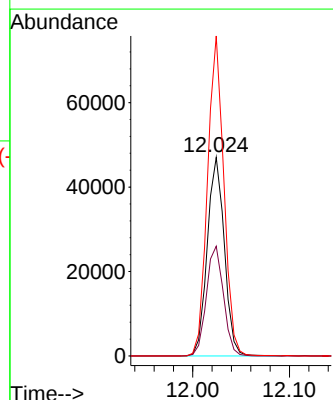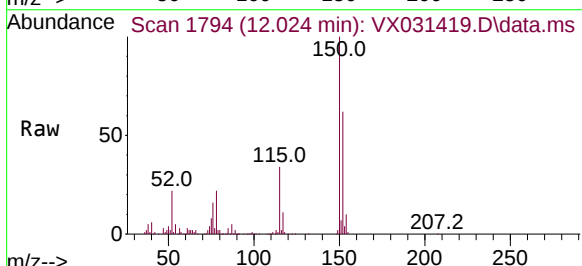



#73

Isopropylbenzene

Concen: 0.276 ug/l

RT: 10.964 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX031419.D

Acq: 16 Sep 2022 18:46

Instrument :

MSVOA_X

ClientSampleId :





TOLL-MW-02

Tgt Ion:105 Resp: 1183

Ion Ratio Lower Upper

105 100

120 24.8 13.7 41.0

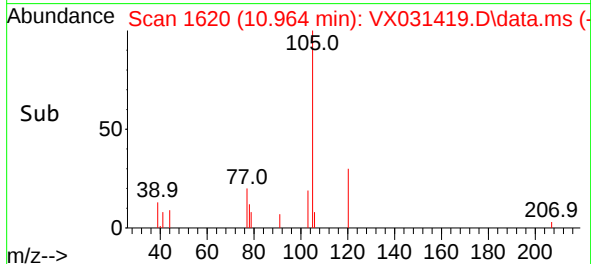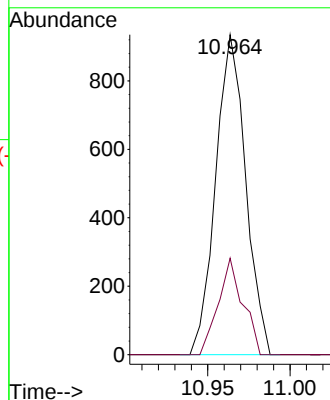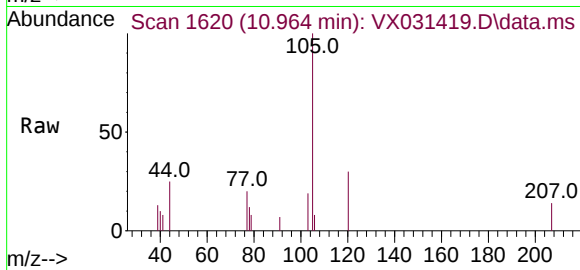

#76

1,2,3-Trichloropropane

Concen: 33.960 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX031419.D




Acq: 16 Sep 2022 18:46


Tgt Ion: 75 Resp: 49657

Ion Ratio Lower Upper

75 100

77 1.4 20.3 60.9#



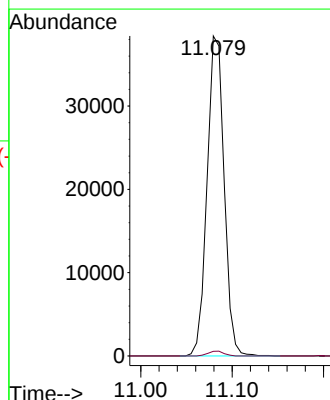
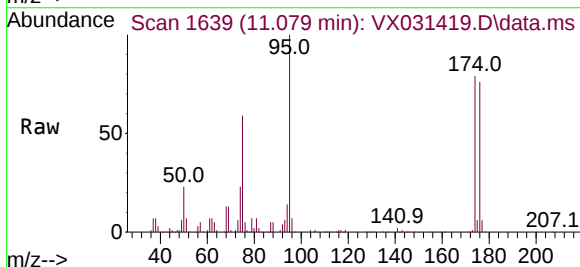




#81
 trans-1,4-Dichloro-2-butene
 Concen: 93.967 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX031419.D
 Acq: 16 Sep 2022 18:46




Instrument :
 MSVOA_X
 ClientSampleId :
 TOLL-MW-02


Tgt Ion: 75 Resp: 49657
 Ion Ratio Lower Upper
 75 100
 53 0.0 77.6 116.4#
 89 0.0 37.4 56.0#

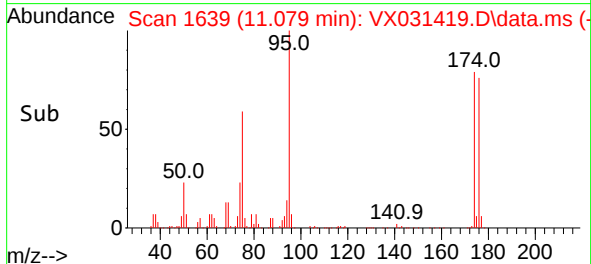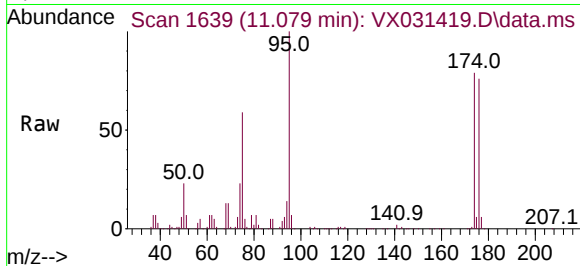

#83
 tert-Butylbenzene
 Concen: 0.228 ug/l
 RT: 11.713 min Scan# 1743
 Delta R.T. -0.006 min
 Lab File: VX031419.D
 Acq: 16 Sep 2022 18:46

Tgt Ion: 119 Resp: 818
 Ion Ratio Lower Upper
 119 100
 91 65.3 29.2 87.6
 134 28.2 11.6 34.8


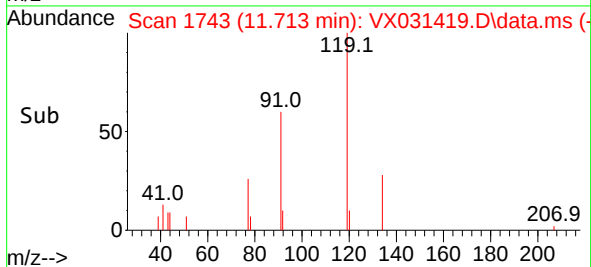

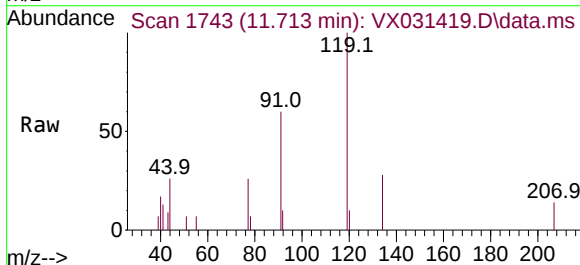




#85
sec-Butylbenzene
Concen: 0.275 ug/l
RT: 11.890 min Scan# 1172
Delta R.T. 0.000 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Instrument :
MSVOA_X
ClientSampleId :
TOLL-MW-02

Tgt Ion:105 Resp: 1237
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

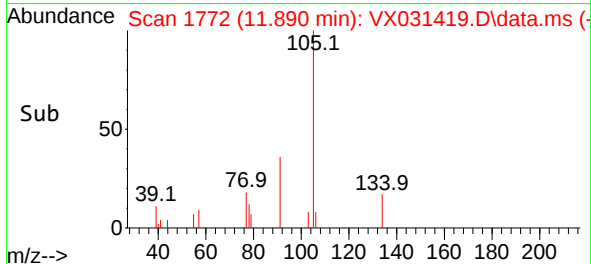

#90
Hexachloroethane
Concen: 0.205 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.104 min
Lab File: VX031419.D
Acq: 16 Sep 2022 18:46

Tgt Ion:117 Resp: 150
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

